

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
 Data File : PP034265.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 10:24
 Operator : DD\AJ
 Sample : M1702-08 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 33021

Manual Integrations
 APPROVED

Ankita
 3/24/2021 2:17:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 02:53:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.848	4.260	351818	201713	4.188	4.558
2)	SA Decachlor...	10.773	9.573	274151	105767	3.493m	4.008
Target Compounds							
16)	L4 AR-1242-1	6.161	5.515	2021720	1003984	1014.575	1102.253m
17)	L4 AR-1242-2	6.184	5.535	2880155	1285558	968.674	979.386m
18)	L4 AR-1242-3	6.249	5.728	1686063	692063	906.080	951.804
19)	L4 AR-1242-4	6.356	5.822	1417527	842941	940.307	1163.613
20)	L4 AR-1242-5	7.136	6.384	1130374	661160	741.453	842.406

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
Data File : PP034265.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 10:24
Operator : DD\AJ
Sample : M1702-08 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
33021


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 02:53:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

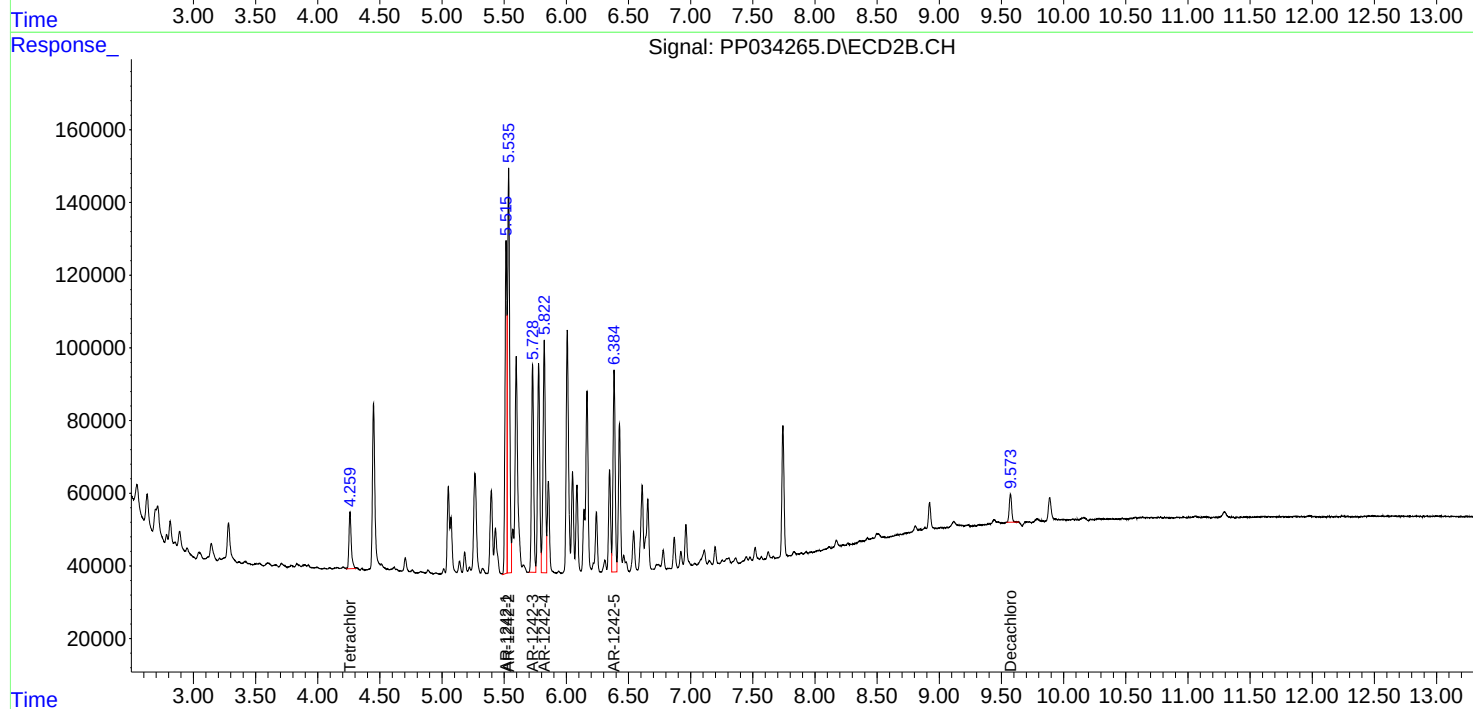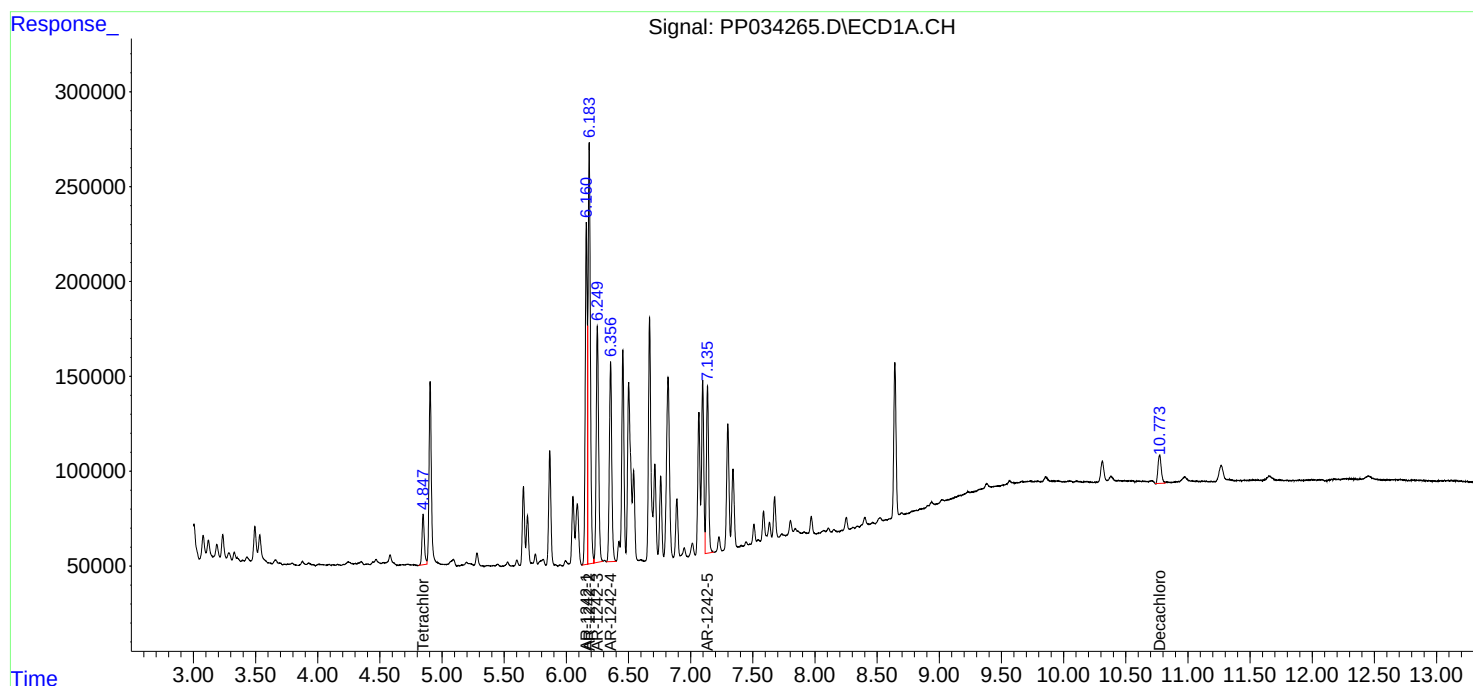

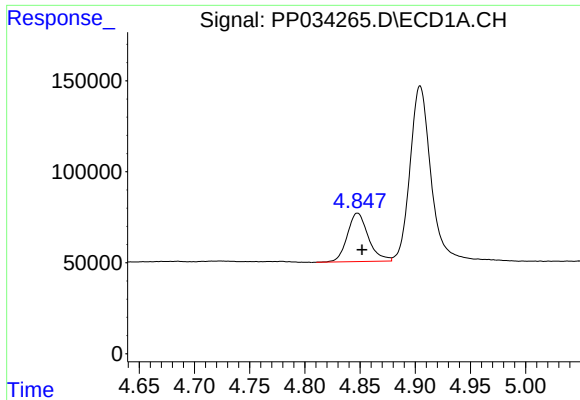


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 351818
Conc: 4.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
33021


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:23 PM

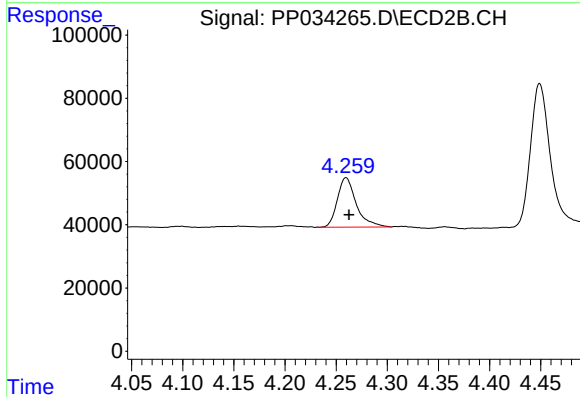


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.003 min
Response: 201713
Conc: 4.56 ng/ml

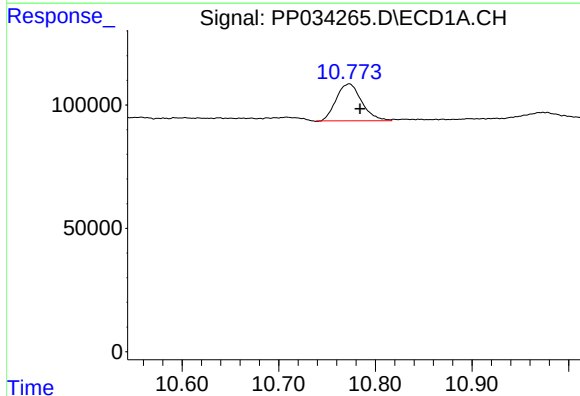


#2 Decachlorobiphenyl

R.T.: 10.773 min
Delta R.T.: -0.011 min
Response: 274151
Conc: 3.49 ng/ml m

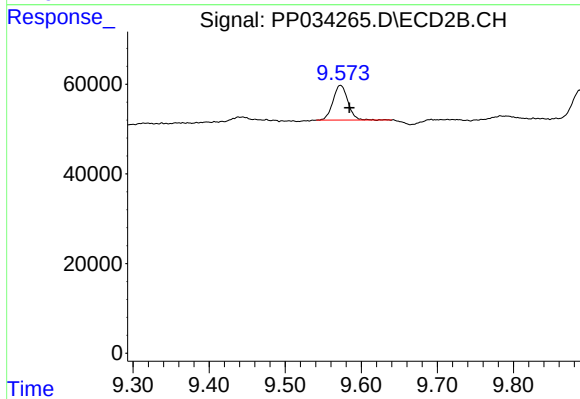

#2 Decachlorobiphenyl

R.T.: 9.573 min
Delta R.T.: -0.012 min
Response: 105767
Conc: 4.01 ng/ml

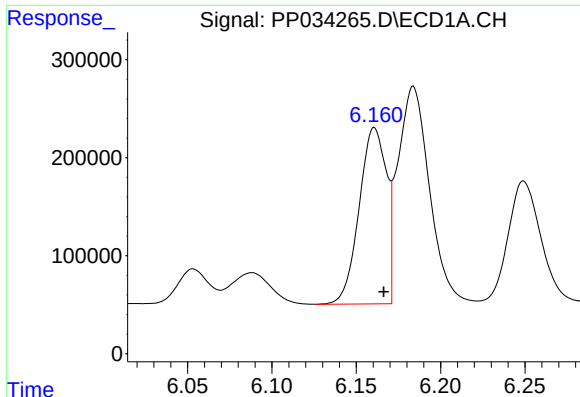


#16 AR-1242-1

R.T.: 6.161 min
Delta R.T.: -0.006 min
Response: 2021720
Conc: 1014.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
33021


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:23 PM

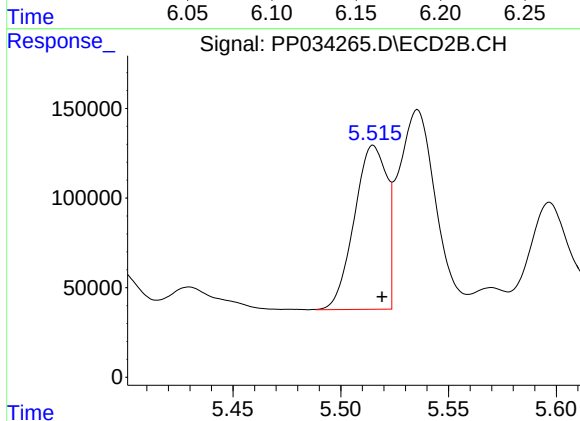


#16 AR-1242-1

R.T.: 5.515 min
Delta R.T.: -0.005 min
Response: 1003984
Conc: 1102.25 ng/ml m

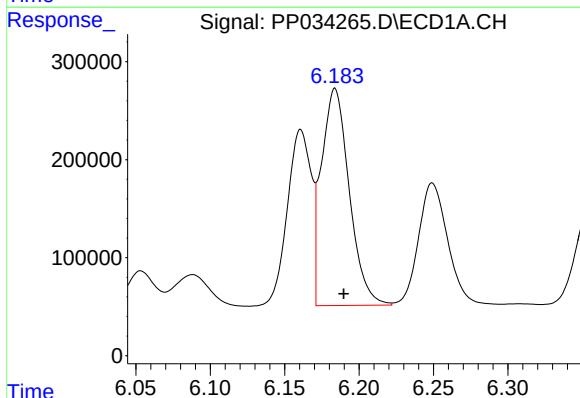


#17 AR-1242-2

R.T.: 6.184 min
Delta R.T.: -0.006 min
Response: 2880155
Conc: 968.67 ng/ml

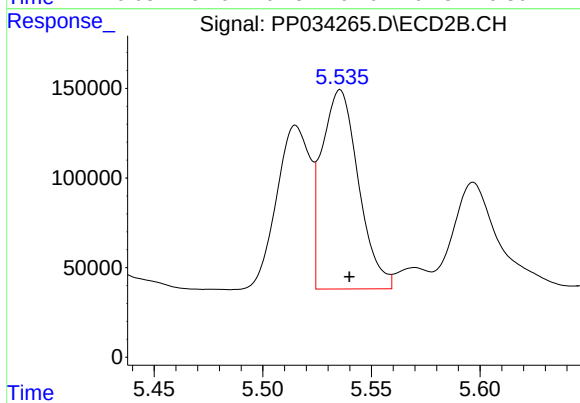

#17 AR-1242-2

R.T.: 5.535 min
Delta R.T.: -0.005 min
Response: 1285558
Conc: 979.39 ng/ml m

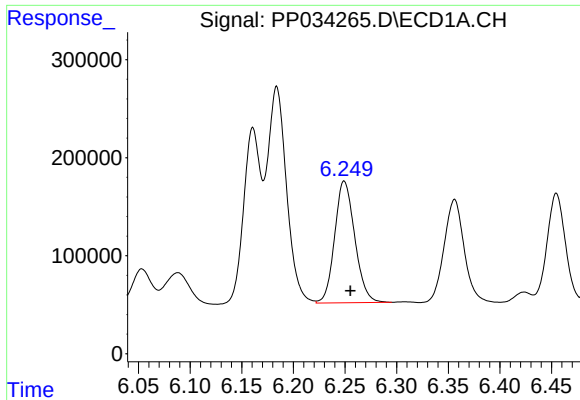


#18 AR-1242-3

R.T.: 6.249 min
Delta R.T.: -0.006 min
Response: 1686063
Conc: 906.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
33021


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:23 PM

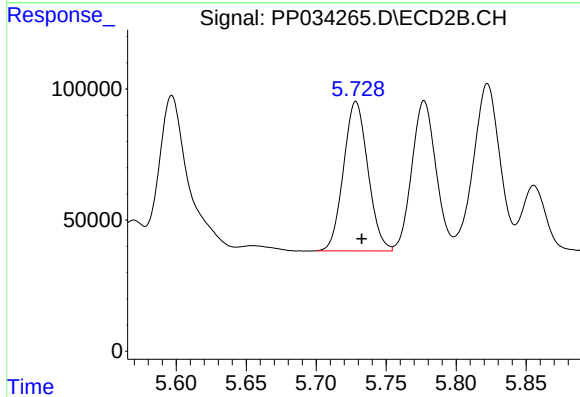


#18 AR-1242-3

R.T.: 5.728 min
Delta R.T.: -0.004 min
Response: 692063
Conc: 951.80 ng/ml

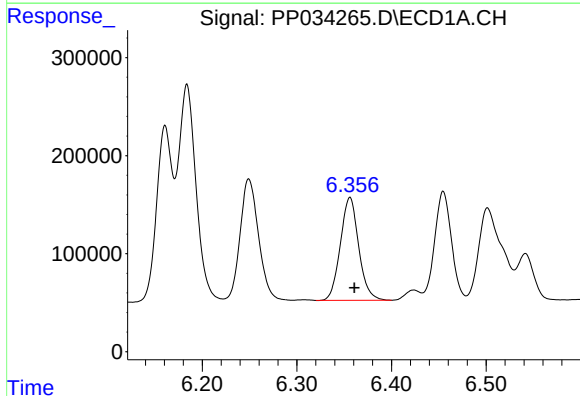


#19 AR-1242-4

R.T.: 6.356 min
Delta R.T.: -0.005 min
Response: 1417527
Conc: 940.31 ng/ml

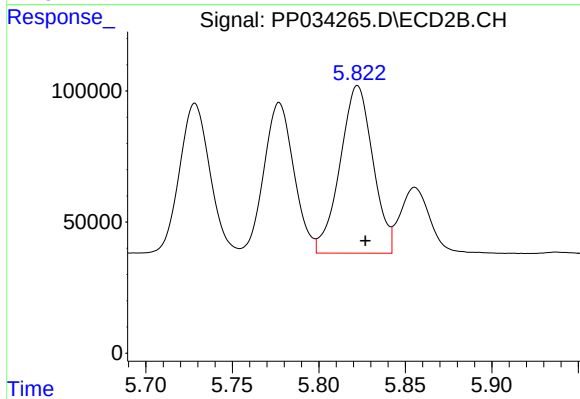

#19 AR-1242-4

R.T.: 5.822 min
Delta R.T.: -0.005 min
Response: 842941
Conc: 1163.61 ng/ml

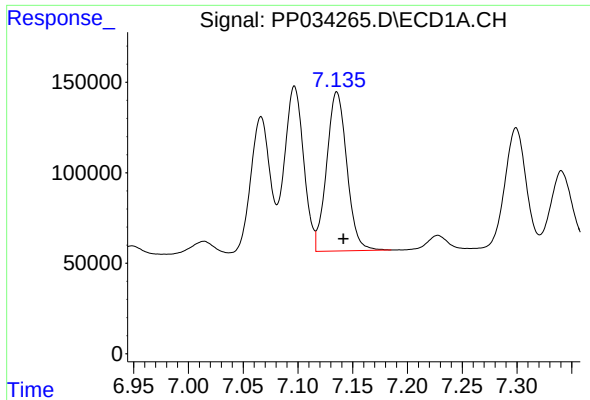


#20 AR-1242-5

R.T.: 7.136 min
Delta R.T.: -0.006 min
Response: 1130374
Conc: 741.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
33021

Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:23 PM

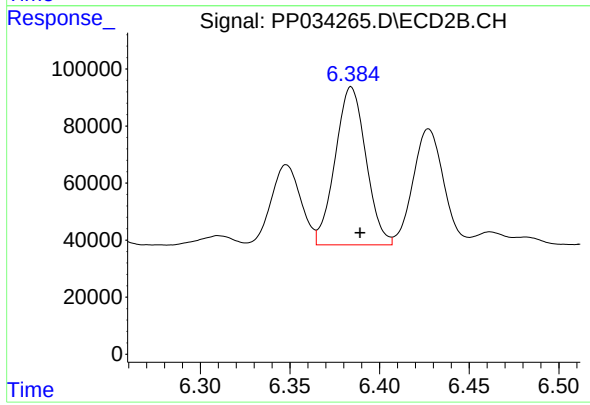

#20 AR-1242-5

R.T.: 6.384 min
Delta R.T.: -0.005 min
Response: 661160
Conc: 842.41 ng/ml