

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
 Data File : PP034266.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 10:41
 Operator : DD\AJ
 Sample : M1660-19RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-6CRE

Manual Integrations
 APPROVED

Ankita
 3/24/2021 2:17:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 02:54:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.260	2529764	1432535	30.114m	32.372
2) SA Decachlor...	10.770	9.574	3054524	1123487	38.923	42.574
Target Compounds						
26) L6 AR-1254-1	7.067	6.385	256009	156137	93.537	93.111
27) L6 AR-1254-2	7.296	6.542	489043	178567	117.444	123.134
28) L6 AR-1254-3	7.676	6.963	886718	587952	204.162	256.734 #
29) L6 AR-1254-4	7.971	7.198	539669	230663	185.892	192.902
30) L6 AR-1254-5	8.398	7.625	1669235	1861777	500.033	1008.298 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
Data File : PP034266.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 10:41
Operator : DD\AJ
Sample : M1660-19RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-6CRE


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 02:54:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

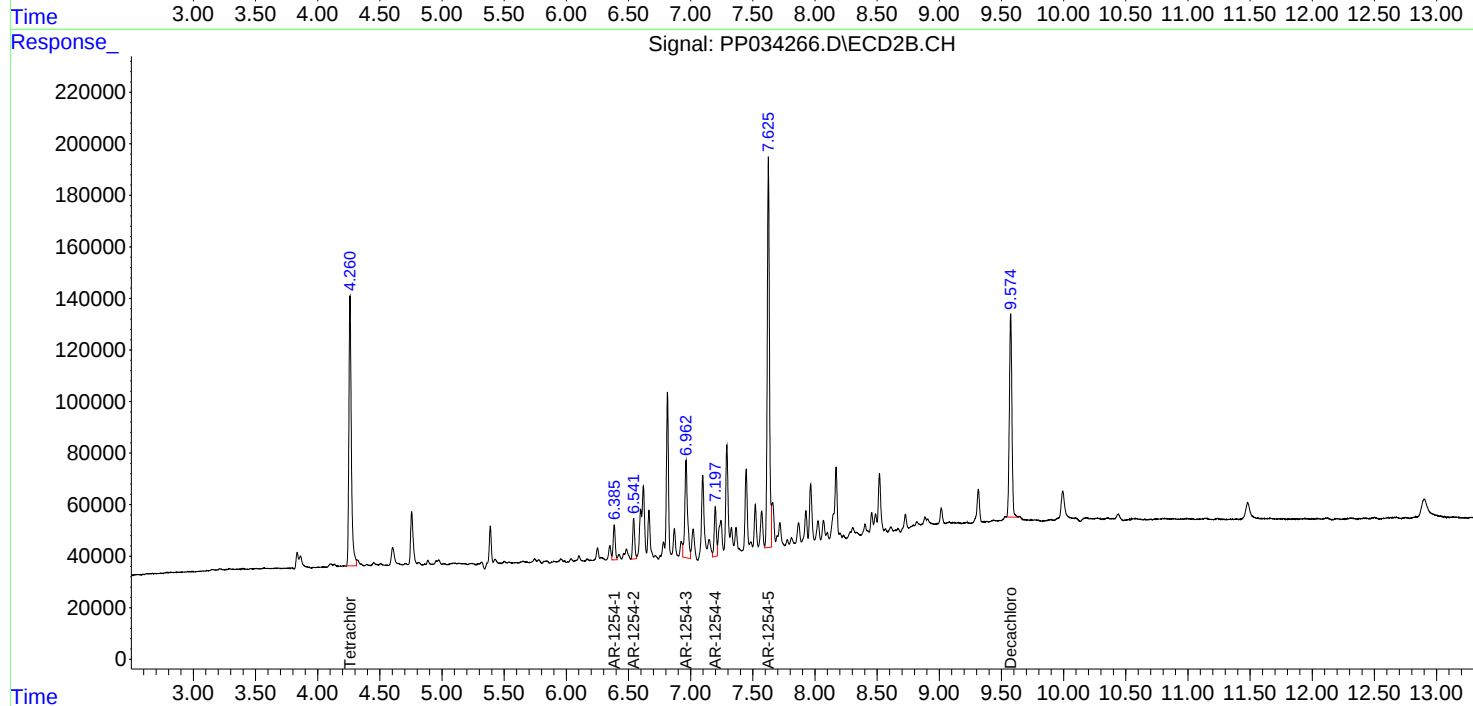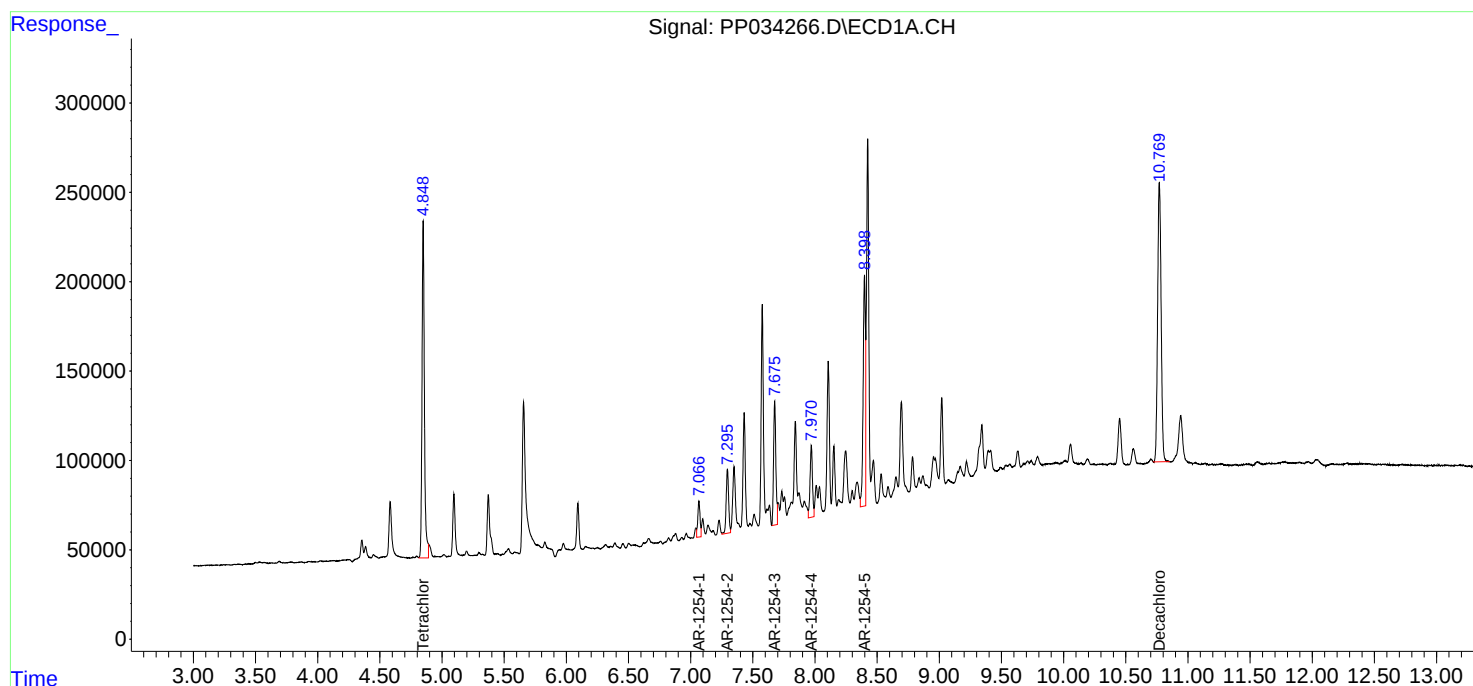

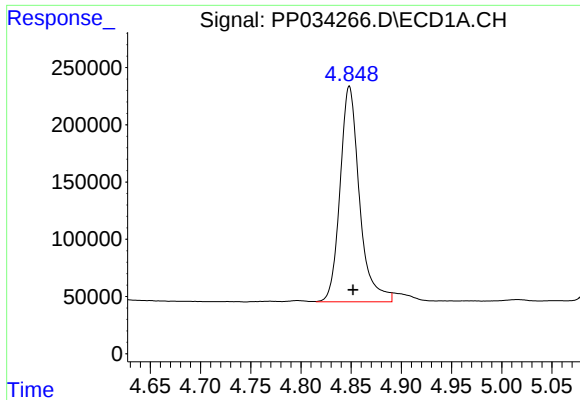


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 2529764
Conc: 30.11 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-6CRE


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:25 PM

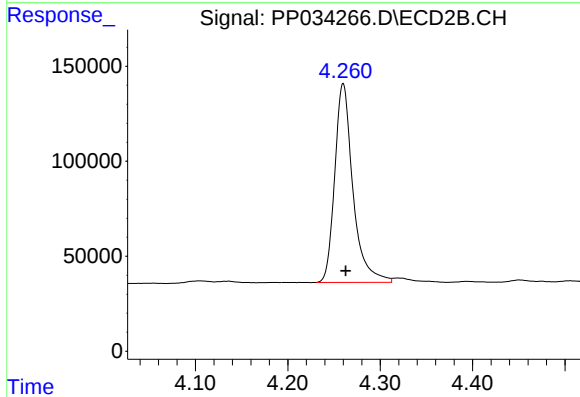


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.003 min
Response: 1432535
Conc: 32.37 ng/ml

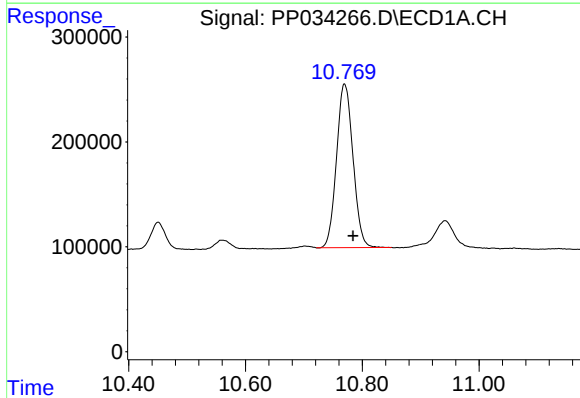


#2 Decachlorobiphenyl

R.T.: 10.770 min
Delta R.T.: -0.015 min
Response: 3054524
Conc: 38.92 ng/ml

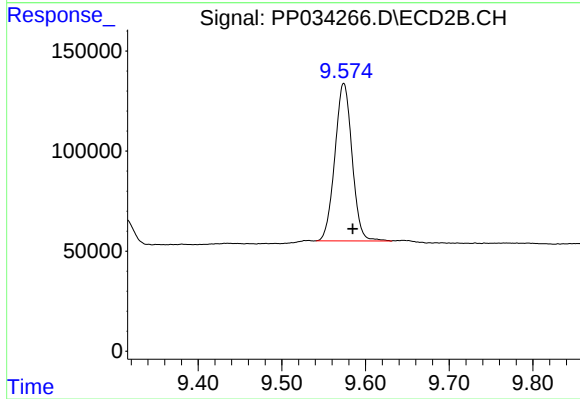

#2 Decachlorobiphenyl

R.T.: 9.574 min
Delta R.T.: -0.011 min
Response: 1123487
Conc: 42.57 ng/ml

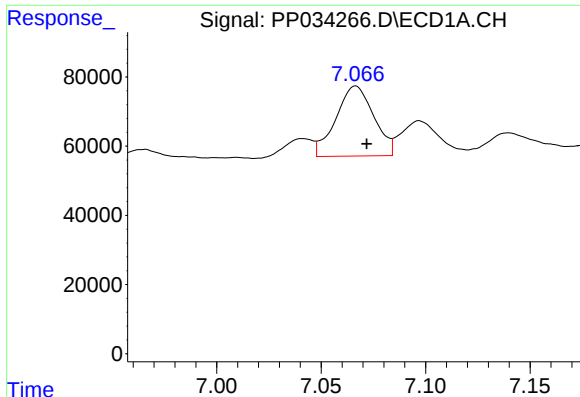


#26 AR-1254-1

R.T.: 7.067 min
Delta R.T.: -0.005 min
Response: 256009
Conc: 93.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6CRE


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:25 PM

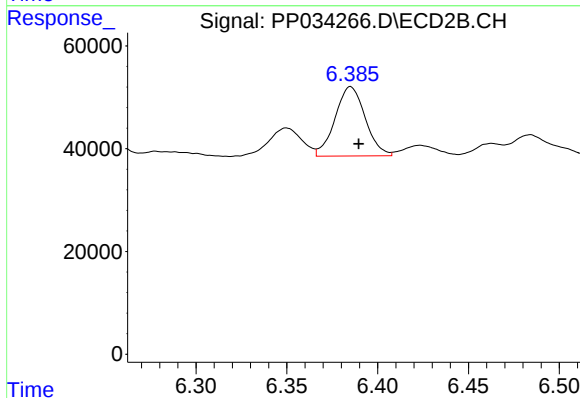


#26 AR-1254-1

R.T.: 6.385 min
Delta R.T.: -0.004 min
Response: 156137
Conc: 93.11 ng/ml

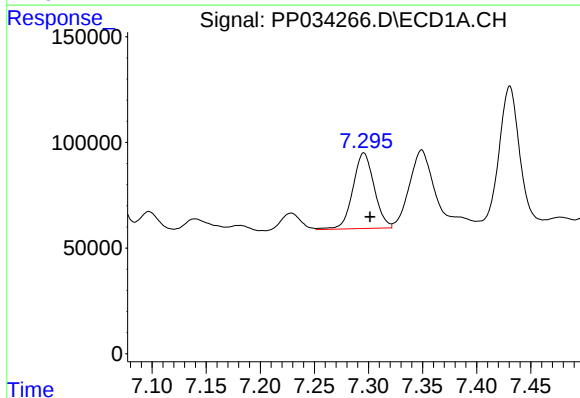


#27 AR-1254-2

R.T.: 7.296 min
Delta R.T.: -0.006 min
Response: 489043
Conc: 117.44 ng/ml

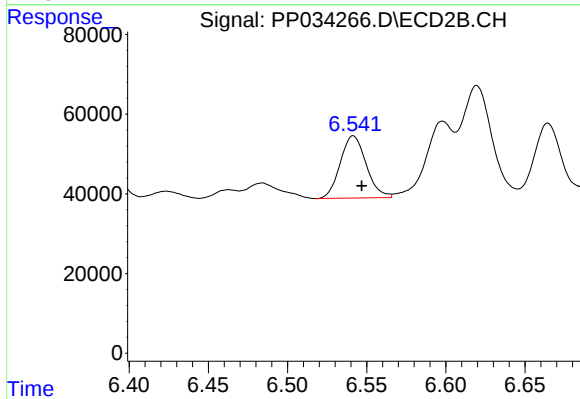

#27 AR-1254-2

R.T.: 6.542 min
Delta R.T.: -0.005 min
Response: 178567
Conc: 123.13 ng/ml

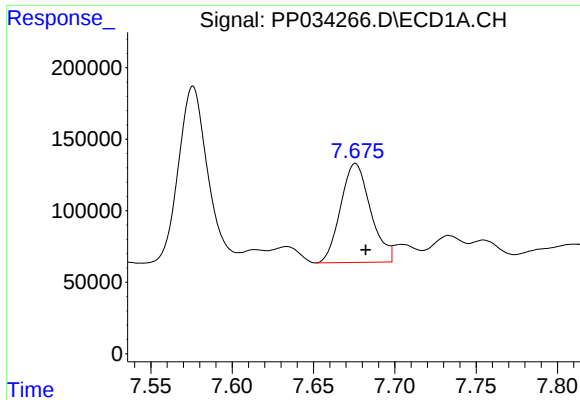


#28 AR-1254-3

R.T.: 7.676 min
Delta R.T.: -0.006 min
Response: 886718
Conc: 204.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6CRE


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:25 PM

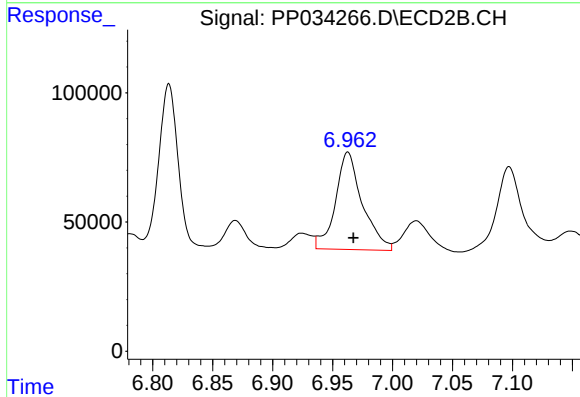


#28 AR-1254-3

R.T.: 6.963 min
Delta R.T.: -0.005 min
Response: 587952
Conc: 256.73 ng/ml

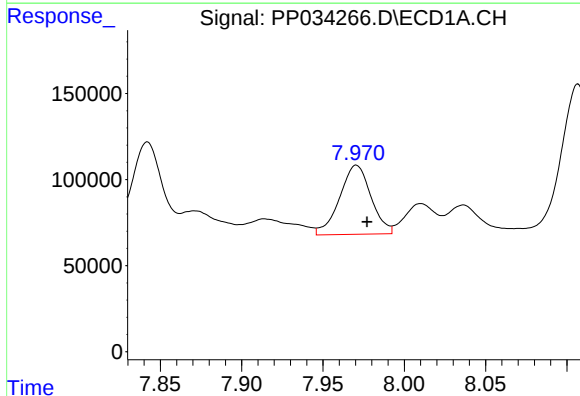


#29 AR-1254-4

R.T.: 7.971 min
Delta R.T.: -0.007 min
Response: 539669
Conc: 185.89 ng/ml

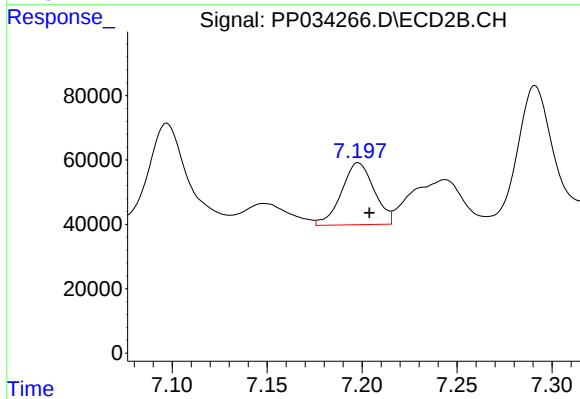

#29 AR-1254-4

R.T.: 7.198 min
Delta R.T.: -0.006 min
Response: 230663
Conc: 192.90 ng/ml

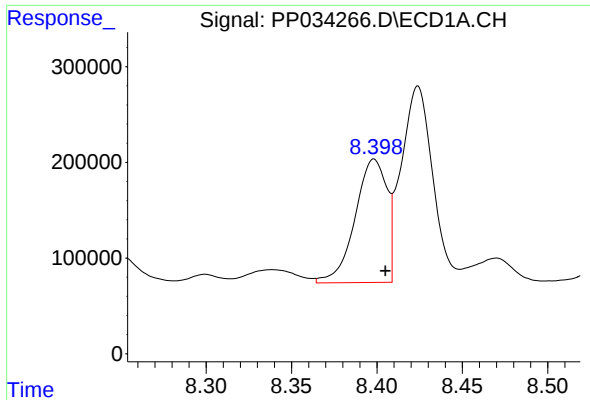


#30 AR-1254-5

R.T.: 8.398 min
Delta R.T.: -0.007 min
Response: 1669235
Conc: 500.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-6CRE

Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:25 PM

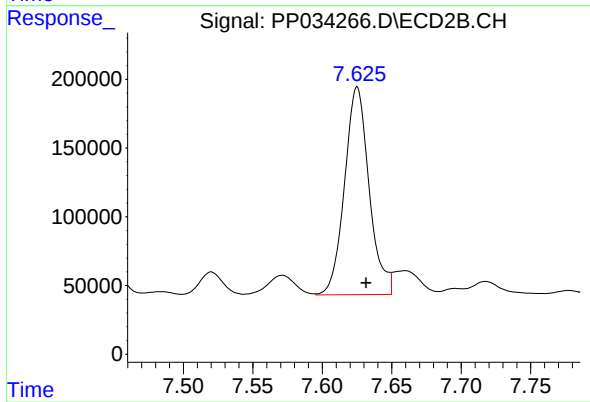

#30 AR-1254-5

R.T.: 7.625 min
Delta R.T.: -0.006 min
Response: 1861777
Conc: 1008.30 ng/ml