

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
 Data File : PP034267.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 10:58
 Operator : DD\AJ
 Sample : M1660-06DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 X127-2BDL

Manual Integrations
 APPROVED

Ankita
 3/24/2021 2:17:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 02:54:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.259	333910	186719	3.975	4.219
2) SA Decachlor...	10.770	9.574	253835	98960	3.235	3.750
Target Compounds						
26) L6 AR-1254-1	7.066	6.385	389356	287120	142.258m	171.222
27) L6 AR-1254-2	7.294	6.542	1223293	592284	293.775	408.421 #
28) L6 AR-1254-3	7.676	6.962	1781750	1082702	410.238	472.770
29) L6 AR-1254-4	7.971	7.198	1971997	860549	679.263	719.671
30) L6 AR-1254-5	8.399	7.625	3858334	2684139	1155.796	1453.670 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
Data File : PP034267.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 10:58
Operator : DD\AJ
Sample : M1660-06DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
X127-2BDL


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 02:54:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

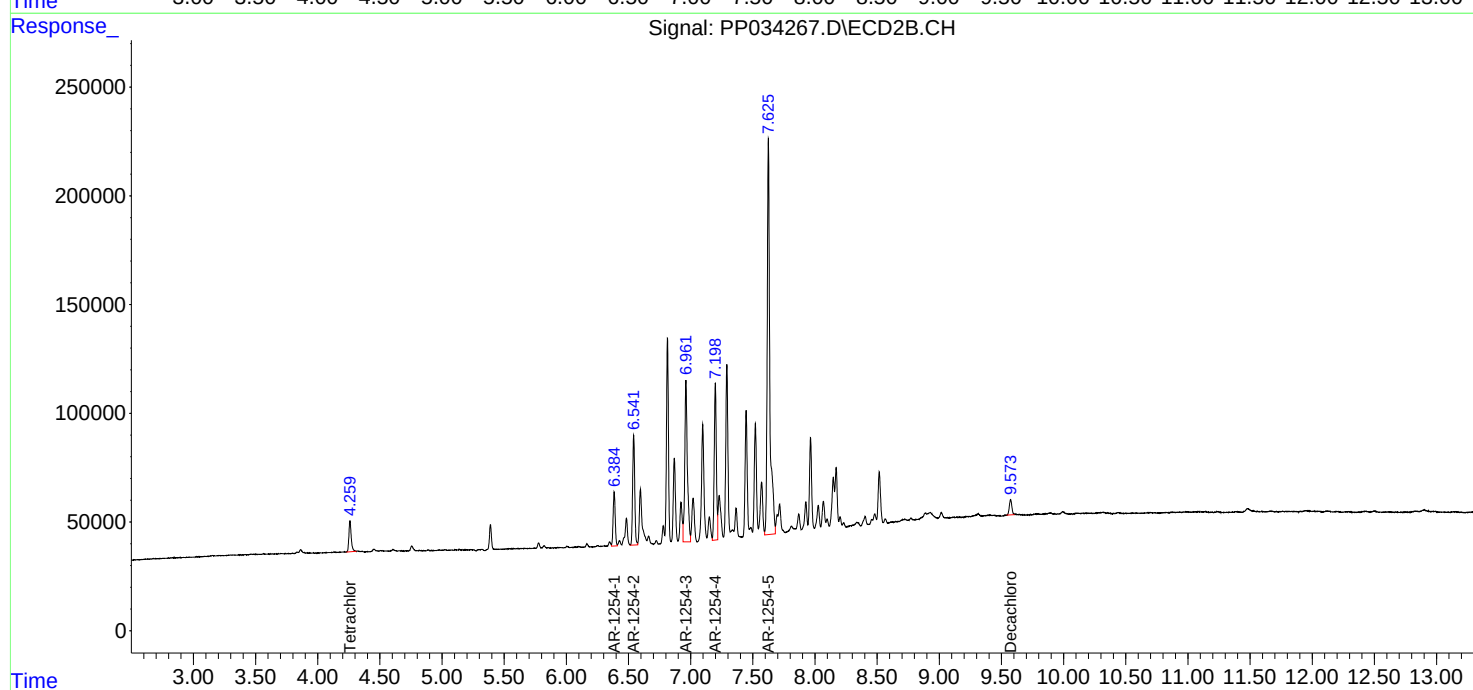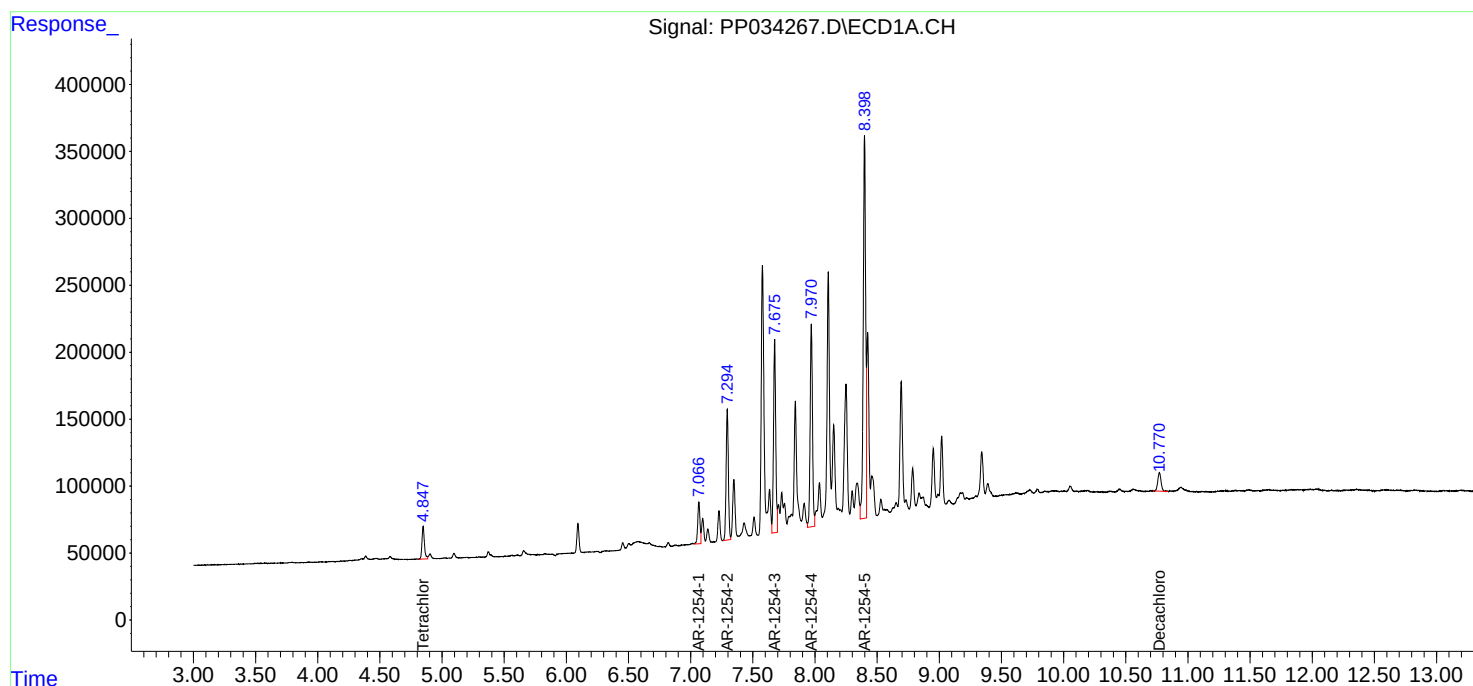

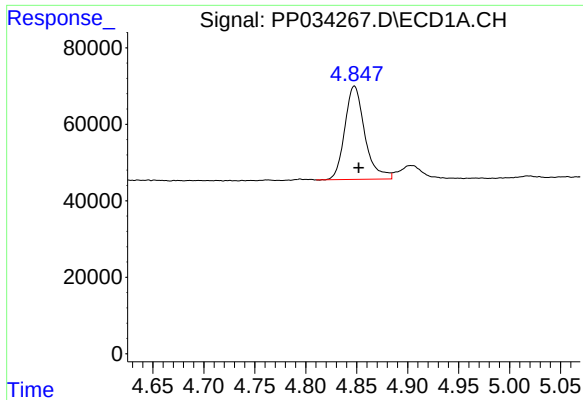


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 333910
Conc: 3.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-2BDL


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:27 PM

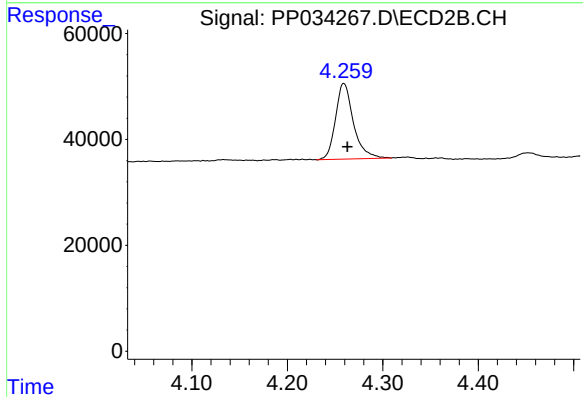


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: -0.004 min
Response: 186719
Conc: 4.22 ng/ml

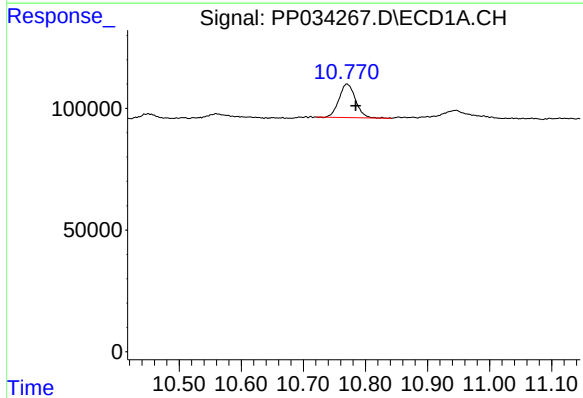


#2 Decachlorobiphenyl

R.T.: 10.770 min
Delta R.T.: -0.014 min
Response: 253835
Conc: 3.23 ng/ml

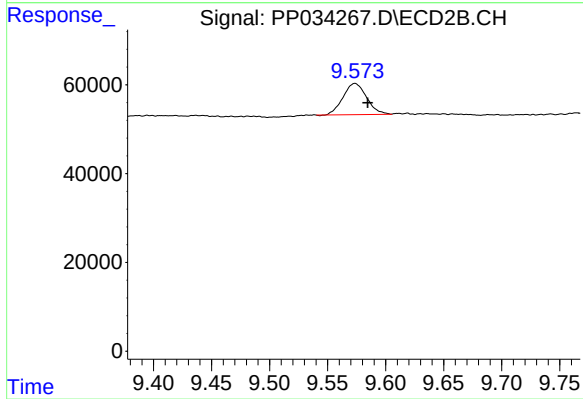

#2 Decachlorobiphenyl

R.T.: 9.574 min
Delta R.T.: -0.011 min
Response: 98960
Conc: 3.75 ng/ml

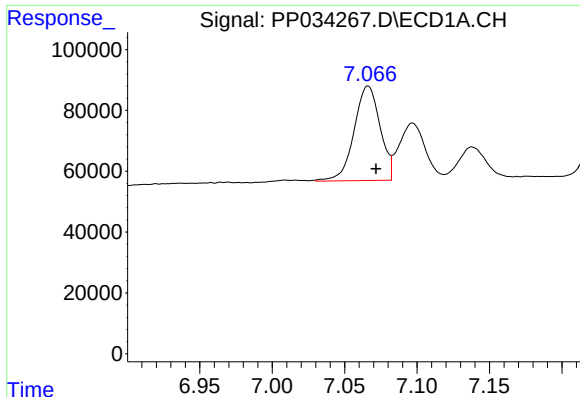


#26 AR-1254-1

R.T.: 7.066 min
Delta R.T.: -0.006 min
Response: 389356
Conc: 142.26 ng/ml m

Instrument :
ECD_P
ClientSampleId :
X127-2BDL


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:27 PM

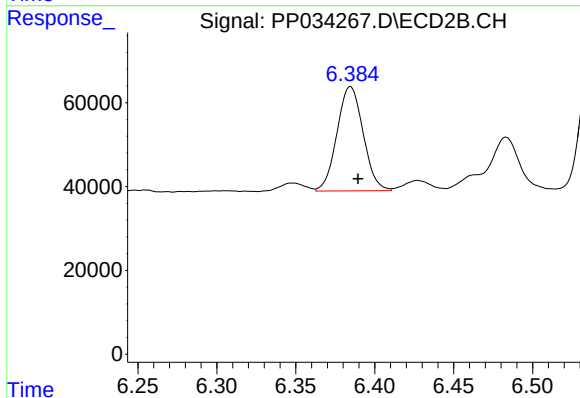


#26 AR-1254-1

R.T.: 6.385 min
Delta R.T.: -0.005 min
Response: 287120
Conc: 171.22 ng/ml

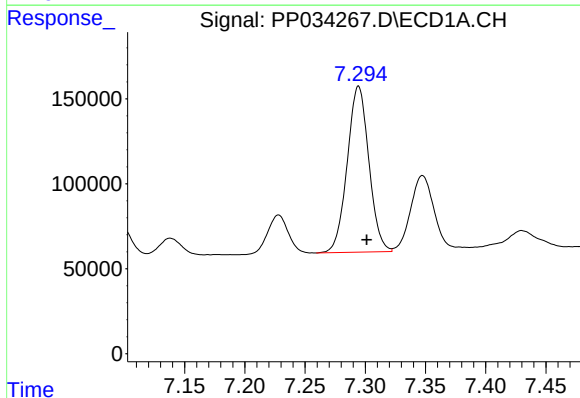


#27 AR-1254-2

R.T.: 7.294 min
Delta R.T.: -0.007 min
Response: 1223293
Conc: 293.78 ng/ml

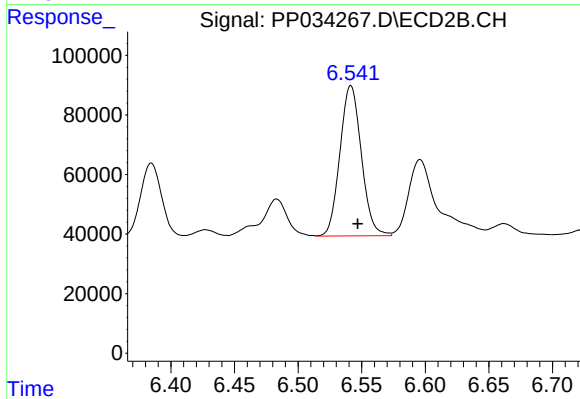

#27 AR-1254-2

R.T.: 6.542 min
Delta R.T.: -0.005 min
Response: 592284
Conc: 408.42 ng/ml

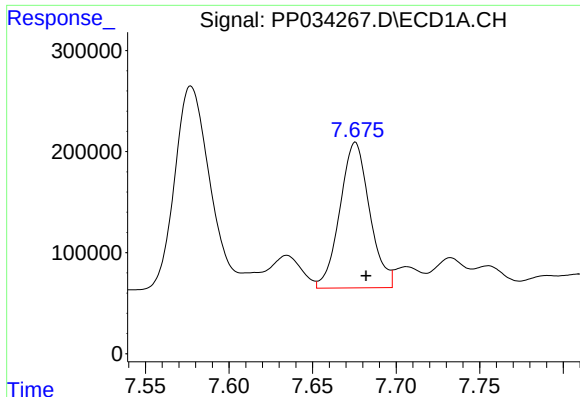


#28 AR-1254-3

R.T.: 7.676 min
Delta R.T.: -0.006 min
Response: 1781750
Conc: 410.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-2BDL


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:27 PM

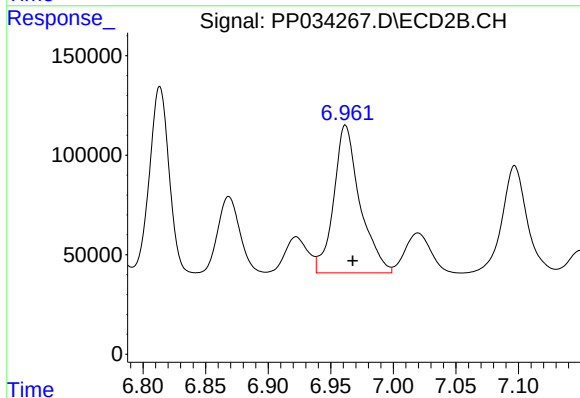


#28 AR-1254-3

R.T.: 6.962 min
Delta R.T.: -0.006 min
Response: 1082702
Conc: 472.77 ng/ml

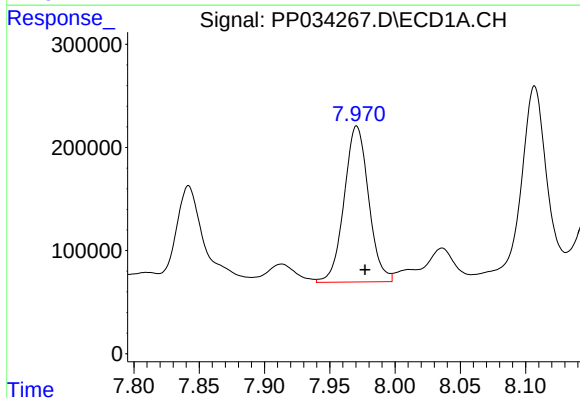


#29 AR-1254-4

R.T.: 7.971 min
Delta R.T.: -0.007 min
Response: 1971997
Conc: 679.26 ng/ml

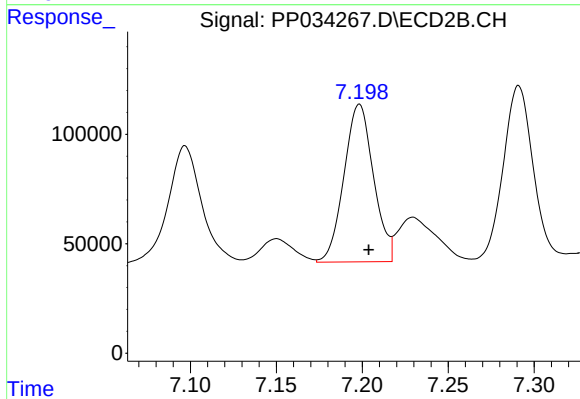

#29 AR-1254-4

R.T.: 7.198 min
Delta R.T.: -0.005 min
Response: 860549
Conc: 719.67 ng/ml

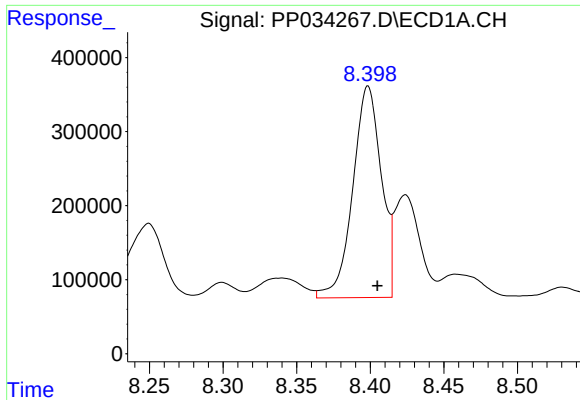


#30 AR-1254-5

R.T.: 8.399 min
Delta R.T.: -0.006 min
Response: 3858334
Conc: 1155.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
X127-2BDL

Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:27 PM

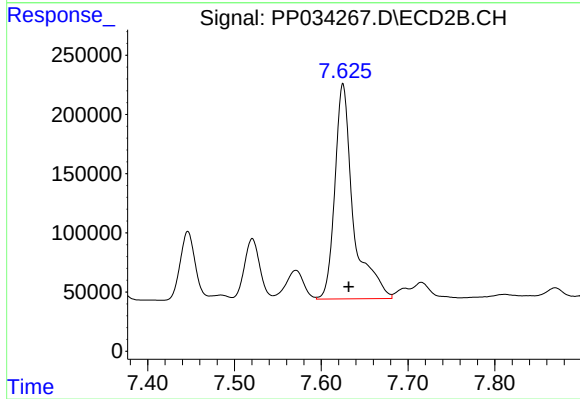

#30 AR-1254-5

R.T.: 7.625 min
Delta R.T.: -0.006 min
Response: 2684139
Conc: 1453.67 ng/ml