

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
 Data File : PP034273.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 12:39
 Operator : DD\AJ
 Sample : AR1242CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1242CCC500

Manual Integrations
 APPROVED

Ankita
 3/24/2021 2:17:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 02:57:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.261	4034399	2265474	48.025	51.194
2) SA Decachlor...	10.770	9.574	4124427	1452650	52.556	55.047
Target Compounds						
16) L4 AR-1242-1	6.161	5.515	971236	478586	487.403	525.430
17) L4 AR-1242-2	6.184	5.536	1451804	700575	488.281	533.725
18) L4 AR-1242-3	6.249	5.729	918063	391031	493.361	537.790
19) L4 AR-1242-4	6.356	5.822	743609	376274	493.268	519.415
20) L4 AR-1242-5	7.134	6.384	754970	431864	495.212m	550.251

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
Data File : PP034273.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 12:39
Operator : DD\AJ
Sample : AR1242CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 02:57:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

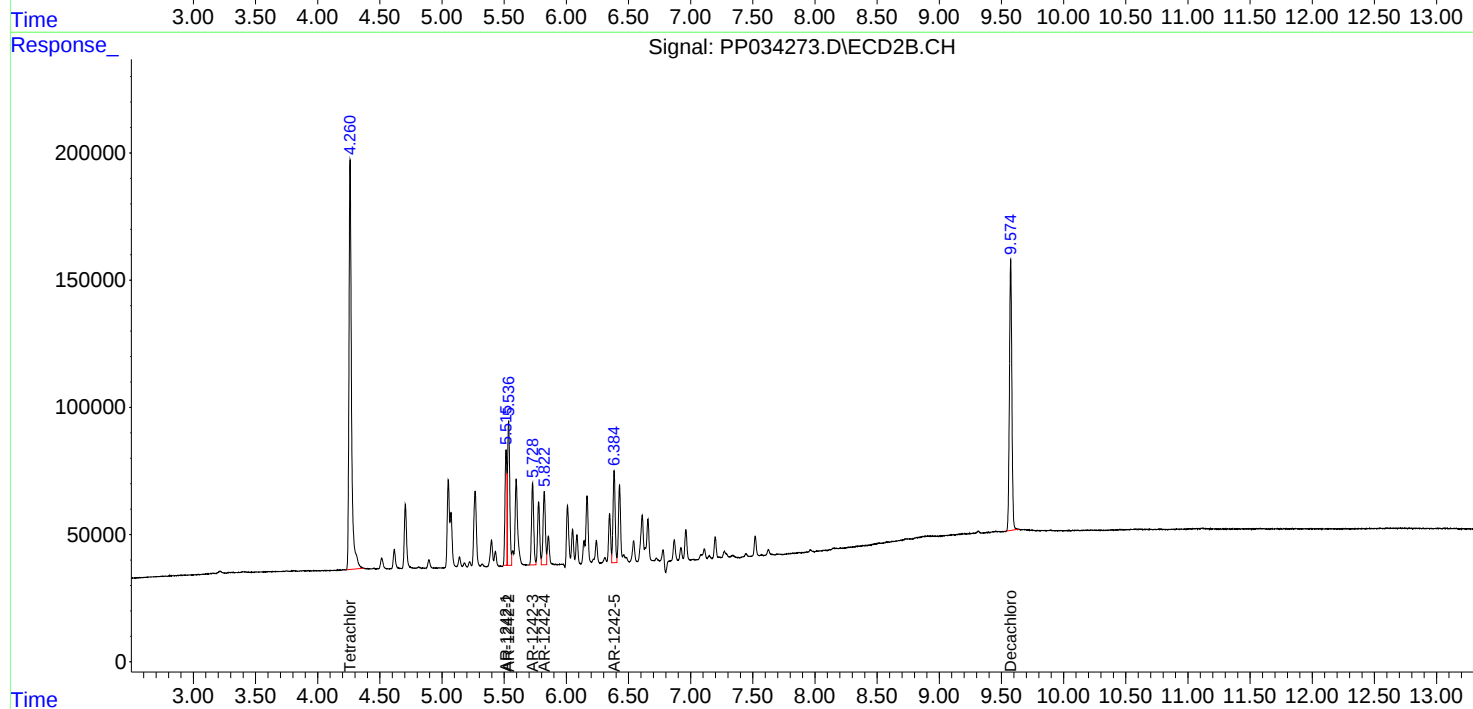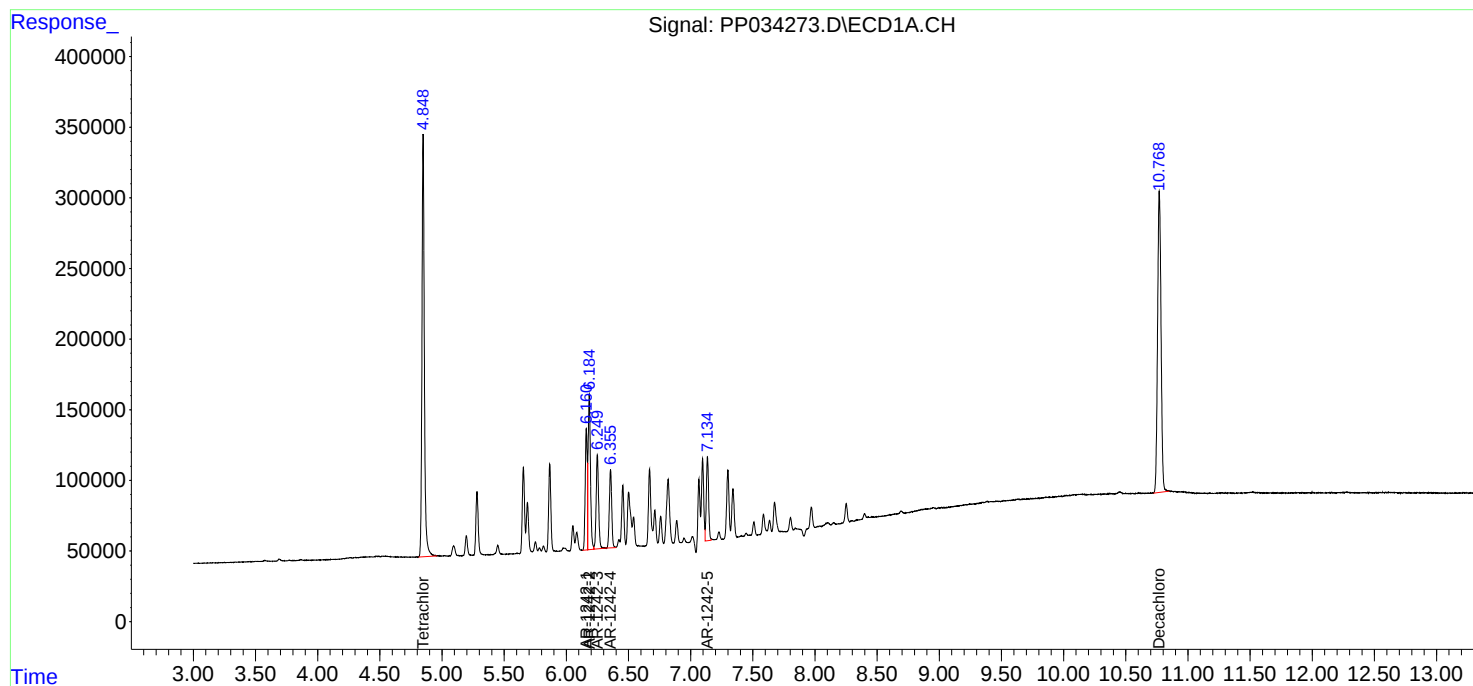

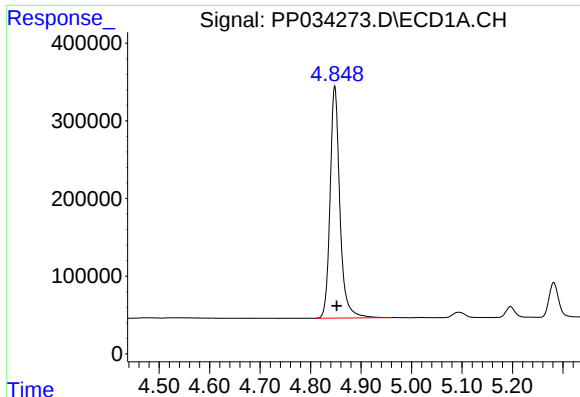


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 4034399
Conc: 48.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:30 PM

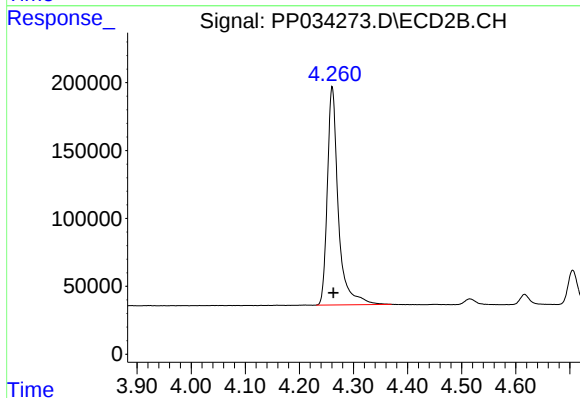


#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.002 min
Response: 2265474
Conc: 51.19 ng/ml

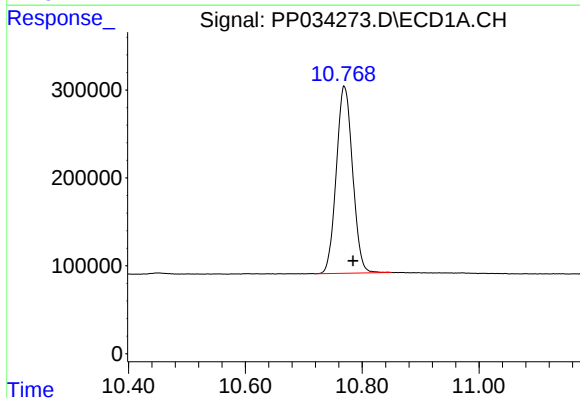


#2 Decachlorobiphenyl

R.T.: 10.770 min
Delta R.T.: -0.015 min
Response: 4124427
Conc: 52.56 ng/ml

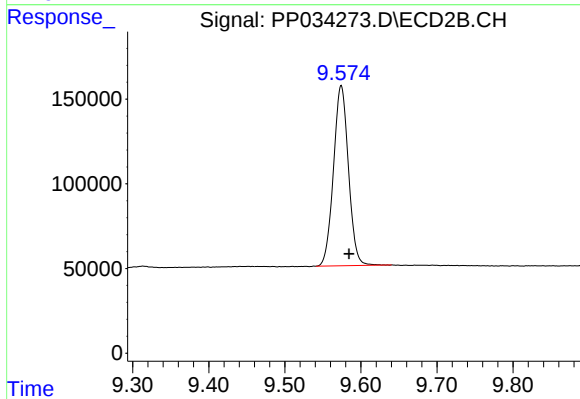

#2 Decachlorobiphenyl

R.T.: 9.574 min
Delta R.T.: -0.010 min
Response: 1452650
Conc: 55.05 ng/ml

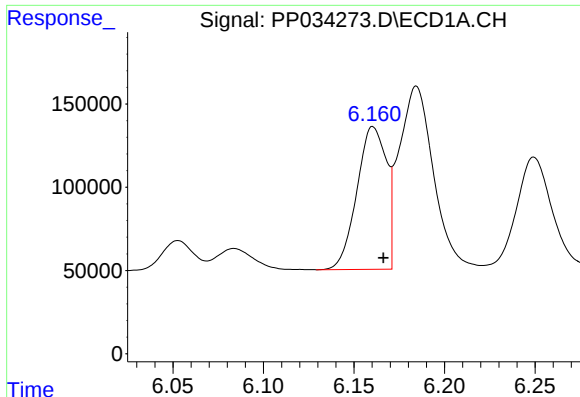


#16 AR-1242-1

R.T.: 6.161 min
Delta R.T.: -0.006 min
Response: 971236
Conc: 487.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:30 PM

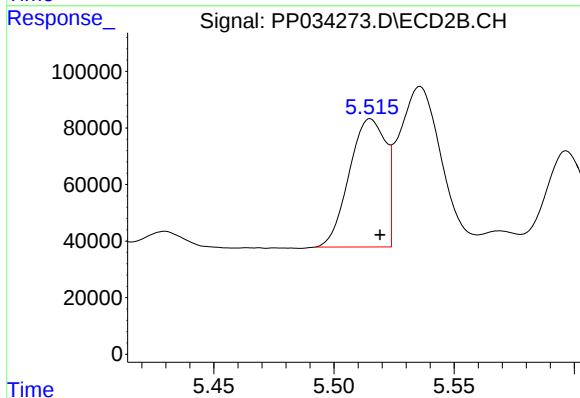


#16 AR-1242-1

R.T.: 5.515 min
Delta R.T.: -0.004 min
Response: 478586
Conc: 525.43 ng/ml

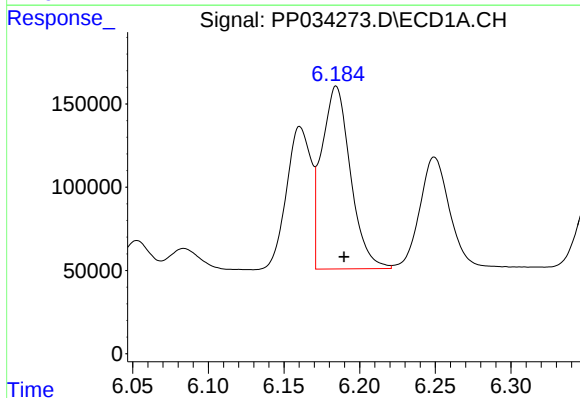


#17 AR-1242-2

R.T.: 6.184 min
Delta R.T.: -0.005 min
Response: 1451804
Conc: 488.28 ng/ml

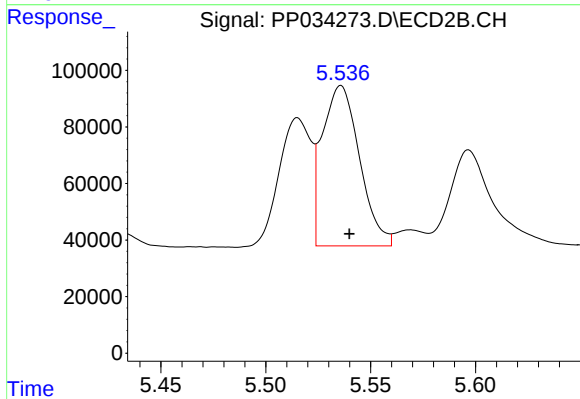

#17 AR-1242-2

R.T.: 5.536 min
Delta R.T.: -0.004 min
Response: 700575
Conc: 533.72 ng/ml

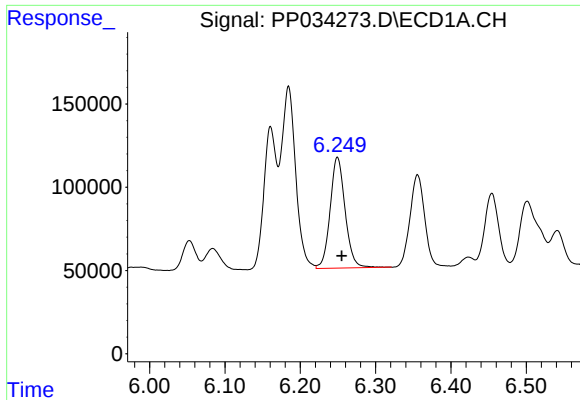


#18 AR-1242-3

R.T.: 6.249 min
Delta R.T.: -0.006 min
Response: 918063
Conc: 493.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:30 PM

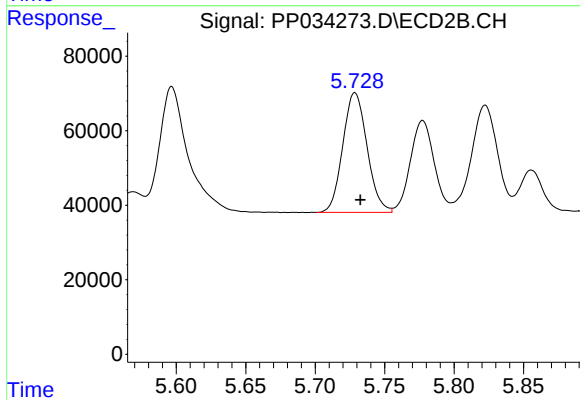


#18 AR-1242-3

R.T.: 5.729 min
Delta R.T.: -0.004 min
Response: 391031
Conc: 537.79 ng/ml

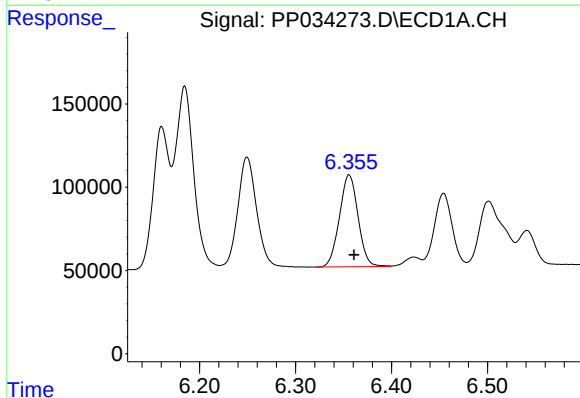


#19 AR-1242-4

R.T.: 6.356 min
Delta R.T.: -0.005 min
Response: 743609
Conc: 493.27 ng/ml

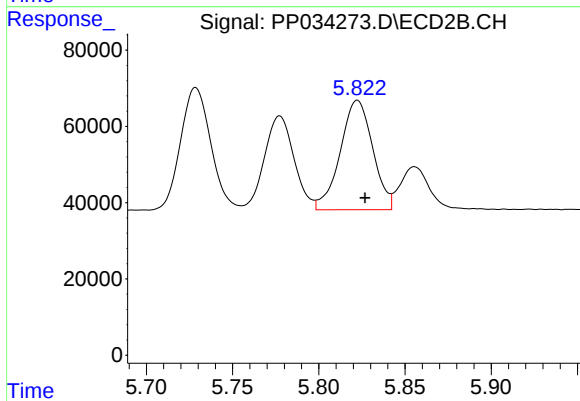

#19 AR-1242-4

R.T.: 5.822 min
Delta R.T.: -0.004 min
Response: 376274
Conc: 519.42 ng/ml

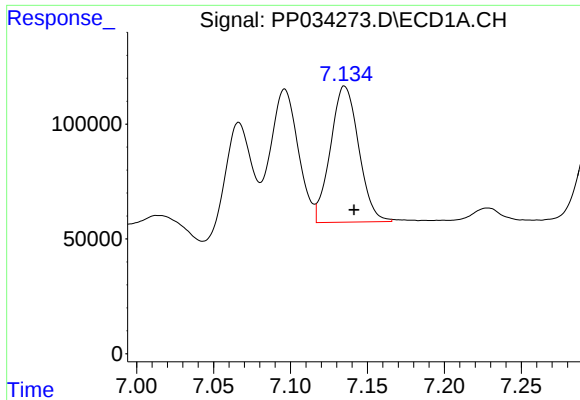


#20 AR-1242-5

R.T.: 7.134 min
Delta R.T.: -0.007 min
Response: 754970
Conc: 495.21 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500

Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:30 PM

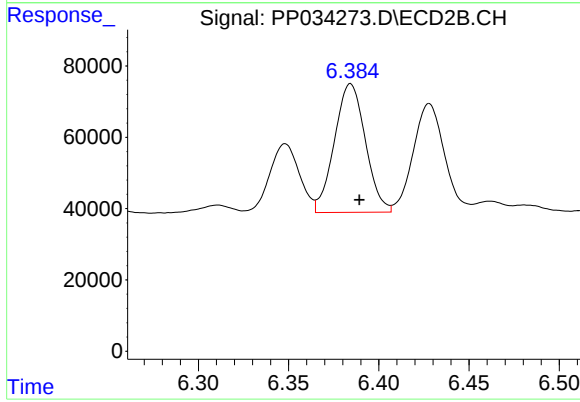

#20 AR-1242-5

R.T.: 6.384 min
Delta R.T.: -0.005 min
Response: 431864
Conc: 550.25 ng/ml