

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
 Data File : PP034296.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 19:07
 Operator : DD\AJ
 Sample : M1739-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HP-627

Manual Integrations
 APPROVED

Ankita
 3/24/2021 2:17:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 03:05:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.845	4.252	670716	704613	7.984m	15.923 #
2) SA Decachlor...	10.774	9.574	458916	216269	5.848	8.195 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
Data File : PP034296.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 19:07
Operator : DD\AJ
Sample : M1739-06
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HP-627


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 03:05:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

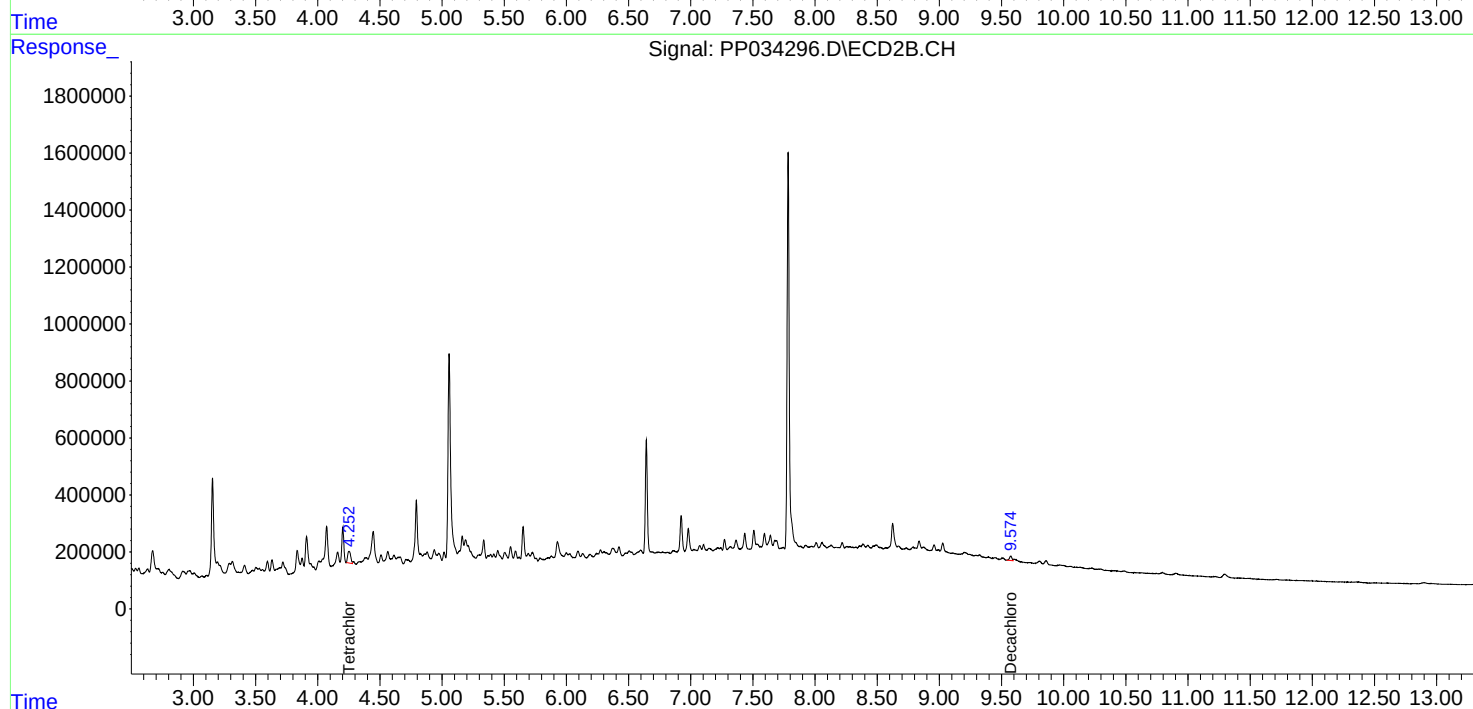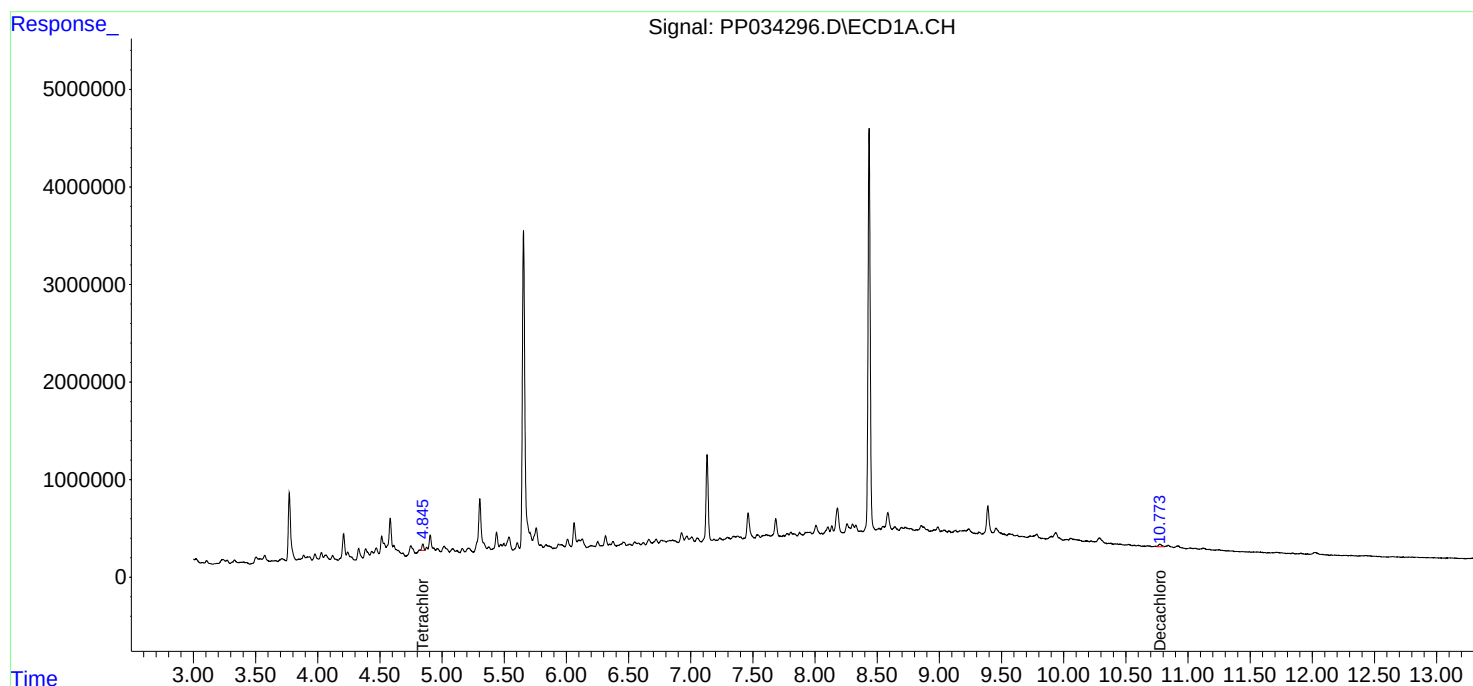

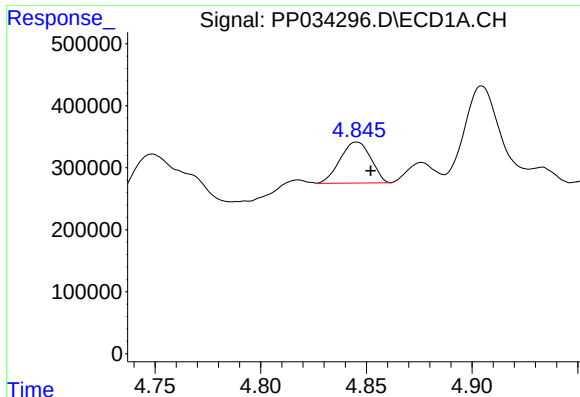


#1 Tetrachloro-m-xylene

R.T.: 4.845 min
Delta R.T.: -0.007 min
Response: 670716
Conc: 7.98 ng/ml m

Instrument :
ECD_P
ClientSampleId :
HP-627


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:37 PM

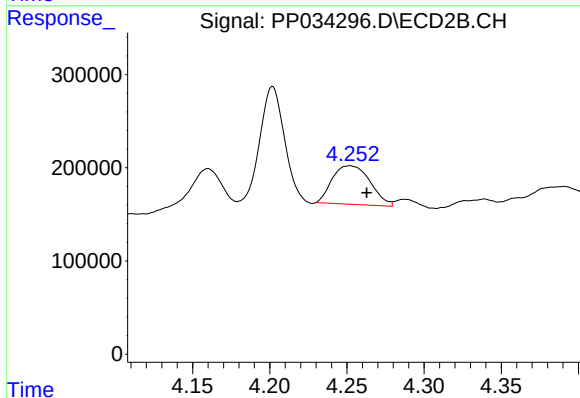


#1 Tetrachloro-m-xylene

R.T.: 4.252 min
Delta R.T.: -0.011 min
Response: 704613
Conc: 15.92 ng/ml

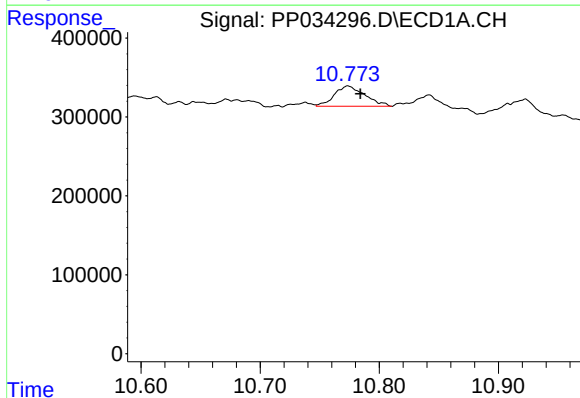

#2 Decachlorobiphenyl

R.T.: 10.774 min
Delta R.T.: -0.010 min
Response: 458916
Conc: 5.85 ng/ml

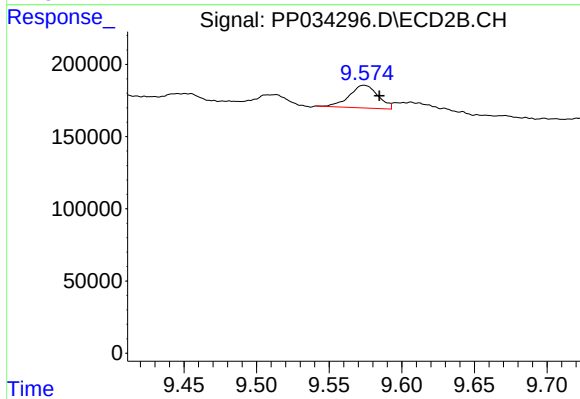

#2 Decachlorobiphenyl

R.T.: 9.574 min
Delta R.T.: -0.010 min
Response: 216269
Conc: 8.20 ng/ml