

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
 Data File : PP034298.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 19:40
 Operator : DD\AJ
 Sample : M1763-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 EL-509-WATER-SAMPLE

Manual Integrations
 APPROVED

Ankita
 3/24/2021 2:17:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 03:06:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.260	996059	488666	11.857m	11.043m
2) SA Decachlor...	10.772	9.574	762766	283653	9.720	10.749

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
Data File : PP034298.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 19:40
Operator : DD\AJ
Sample : M1763-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
EL-509-WATER-SAMPLE


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 03:06:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

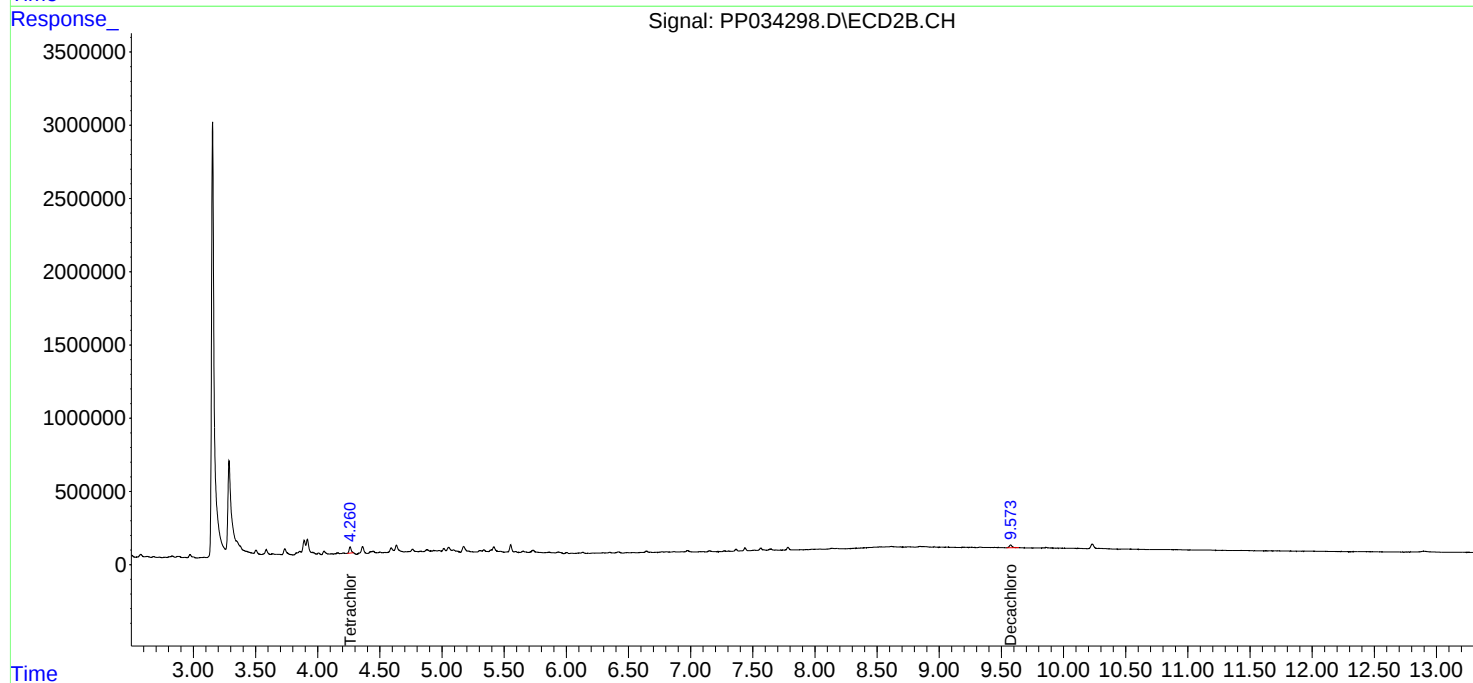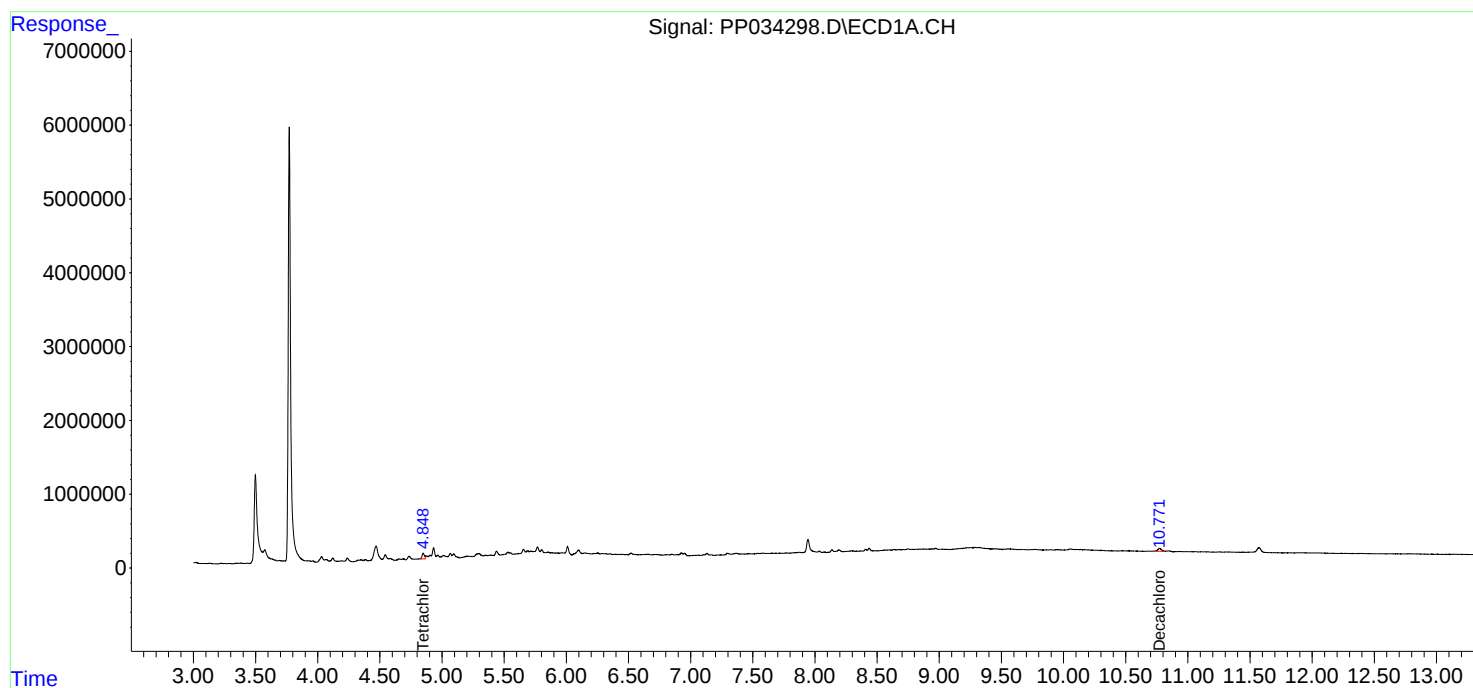

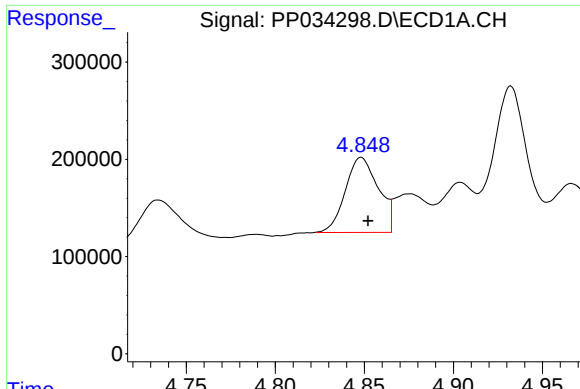


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
 Delta R.T.: -0.004 min
 Response: 996059
 Conc: 11.86 ng/ml m


Instrument :
 ECD_P
 ClientSampleId :
 EL-509-WATER-SAMPLE

Manual Integrations
 APPROVED
 Ankita
 3/24/2021 2:17:41 PM

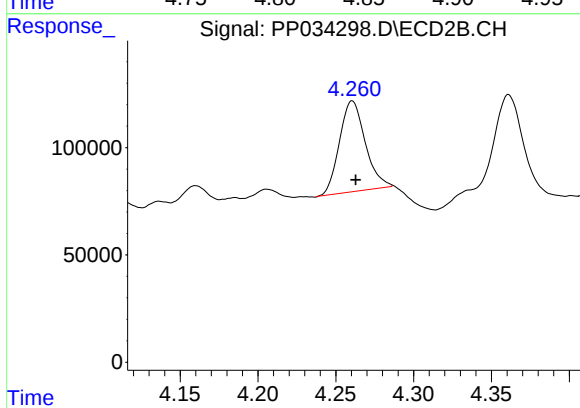


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
 Delta R.T.: -0.003 min
 Response: 488666
 Conc: 11.04 ng/ml m

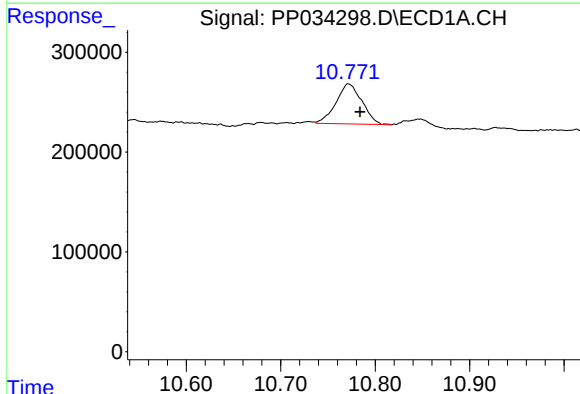

#2 Decachlorobiphenyl

R.T.: 10.772 min
 Delta R.T.: -0.012 min
 Response: 762766
 Conc: 9.72 ng/ml

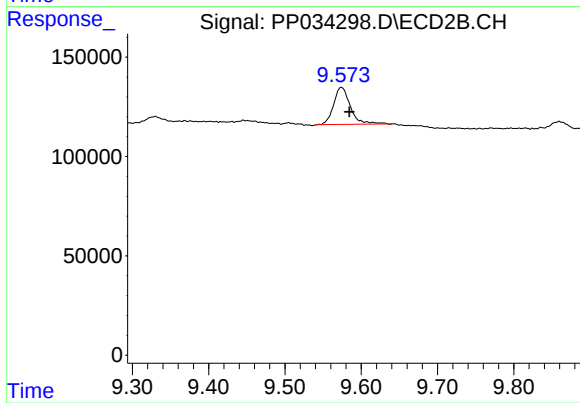

#2 Decachlorobiphenyl

R.T.: 9.574 min
 Delta R.T.: -0.011 min
 Response: 283653
 Conc: 10.75 ng/ml