

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
 Data File : PP034300.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 20:31
 Operator : DD\AJ
 Sample : AR1242CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1242CCC500

Manual Integrations
 APPROVED

Ankita
 3/24/2021 2:17:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 03:07:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.848	4.260	3926383	2309407	46.739	52.187
2)	SA Decachlor...	10.770	9.573	3887093	1438388	49.532	54.507
Target Compounds							
16)	L4 AR-1242-1	6.161	5.515	942879	498693	473.172	547.504
17)	L4 AR-1242-2	6.184	5.536	1426902	729993	479.906	556.136
18)	L4 AR-1242-3	6.250	5.728	884013	408880	475.063	562.338
19)	L4 AR-1242-4	6.356	5.822	718050	386776	476.313	533.913
20)	L4 AR-1242-5	7.135	6.384	728228	452093	477.671m	576.026

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
Data File : PP034300.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 20:31
Operator : DD\AJ
Sample : AR1242CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 03:07:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

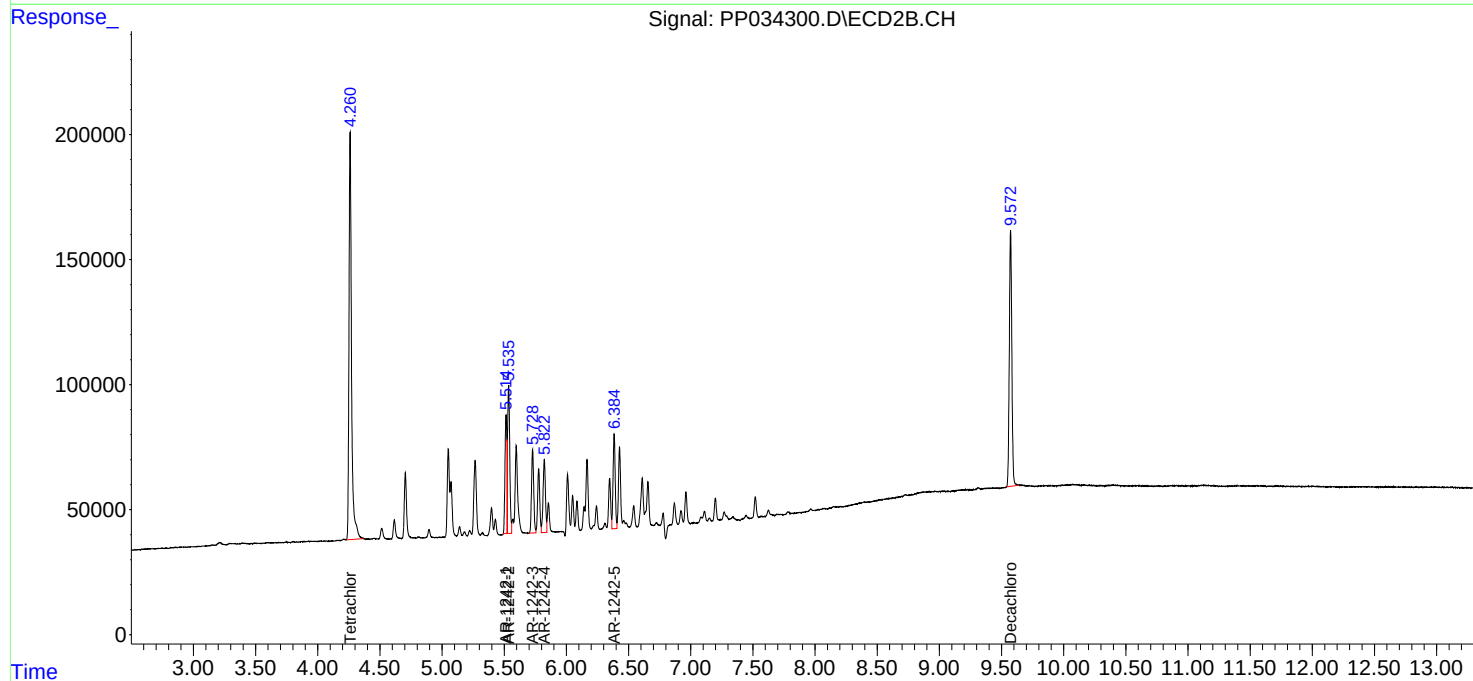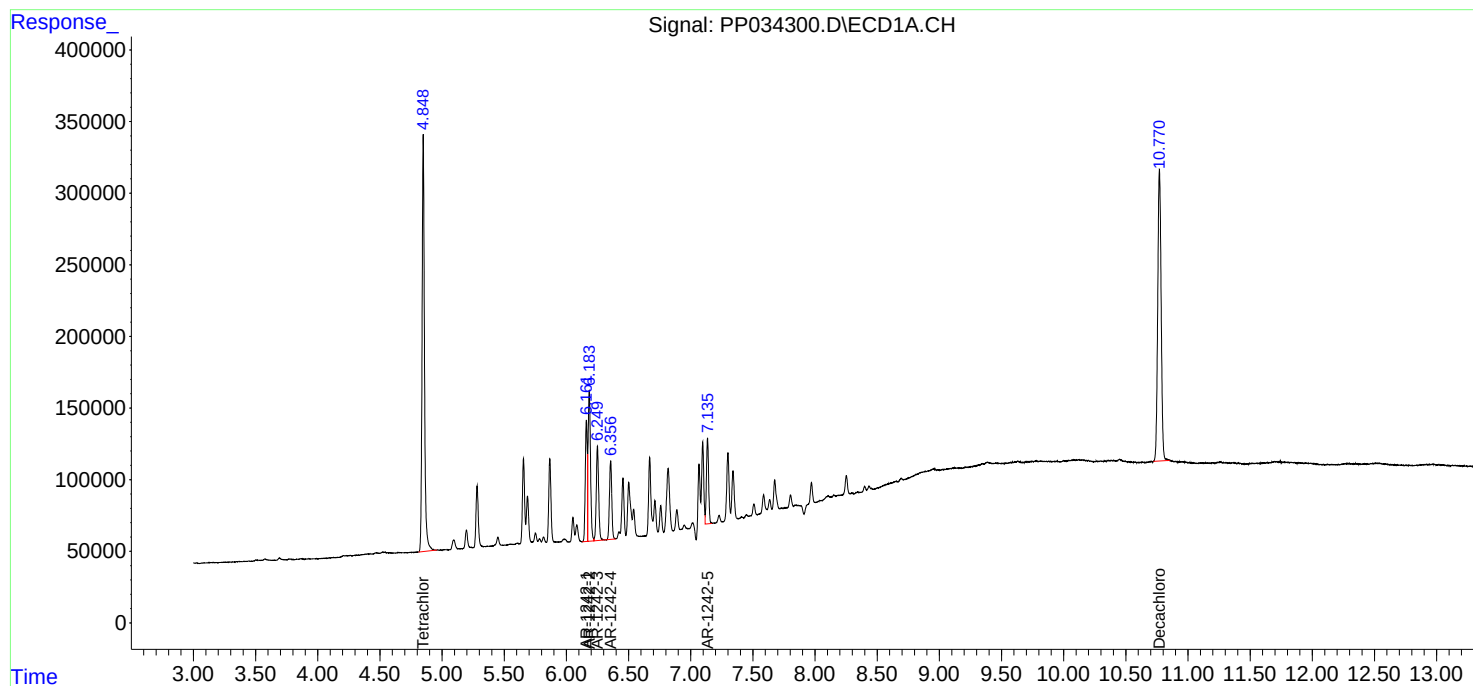

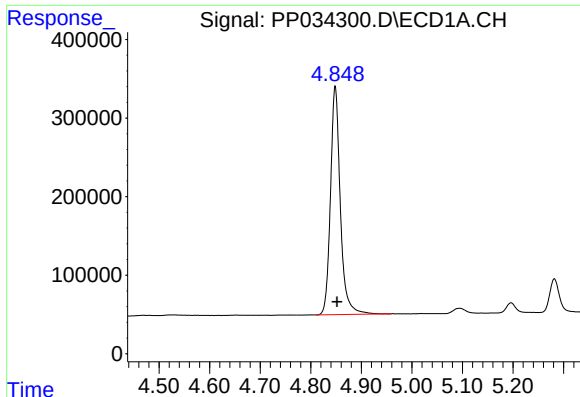


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 3926383
Conc: 46.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:42 PM

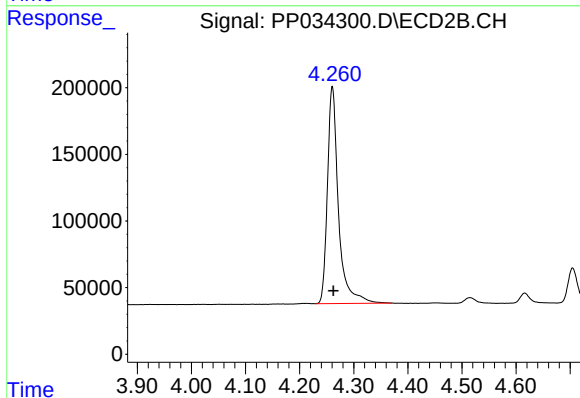


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.002 min
Response: 2309407
Conc: 52.19 ng/ml

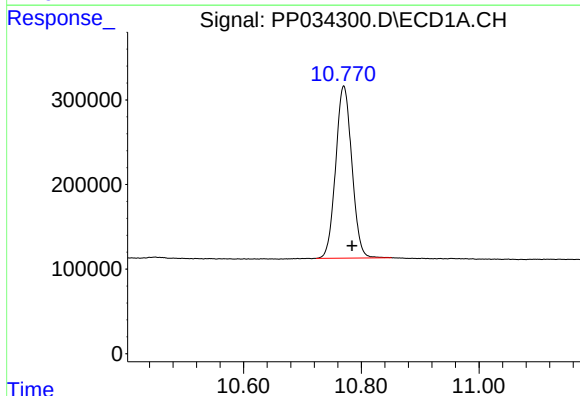


#2 Decachlorobiphenyl

R.T.: 10.770 min
Delta R.T.: -0.014 min
Response: 3887093
Conc: 49.53 ng/ml

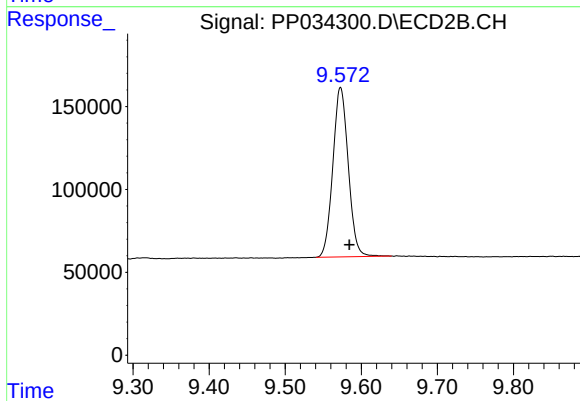

#2 Decachlorobiphenyl

R.T.: 9.573 min
Delta R.T.: -0.012 min
Response: 1438388
Conc: 54.51 ng/ml

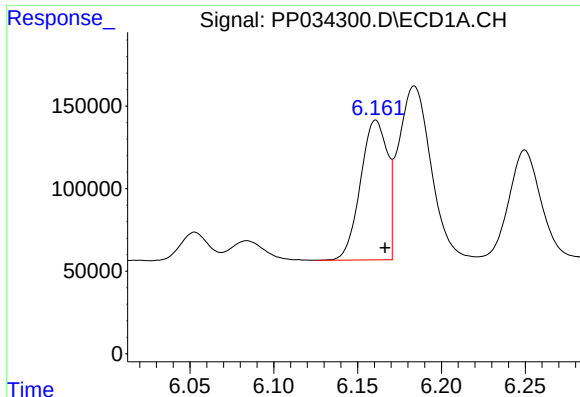


#16 AR-1242-1

R.T.: 6.161 min
Delta R.T.: -0.005 min
Response: 942879
Conc: 473.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:42 PM

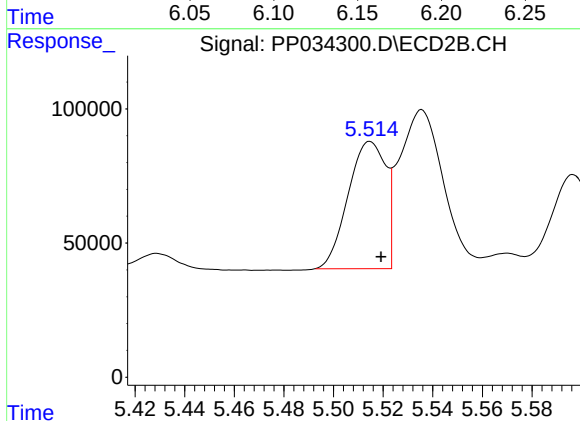


#16 AR-1242-1

R.T.: 5.515 min
Delta R.T.: -0.004 min
Response: 498693
Conc: 547.50 ng/ml

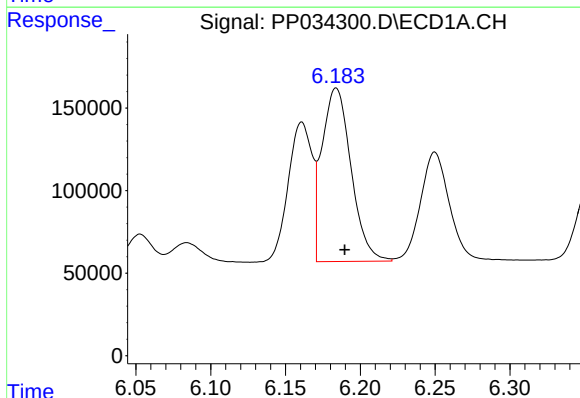


#17 AR-1242-2

R.T.: 6.184 min
Delta R.T.: -0.006 min
Response: 1426902
Conc: 479.91 ng/ml

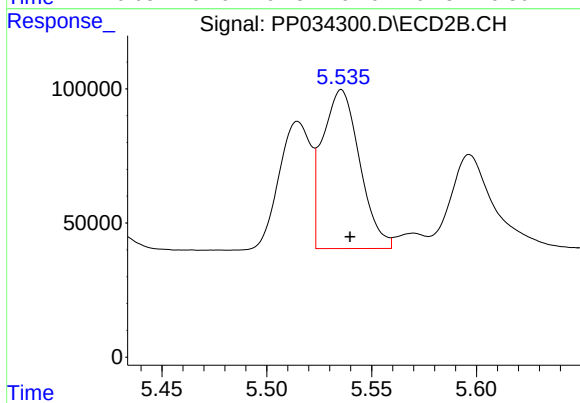

#17 AR-1242-2

R.T.: 5.536 min
Delta R.T.: -0.004 min
Response: 729993
Conc: 556.14 ng/ml

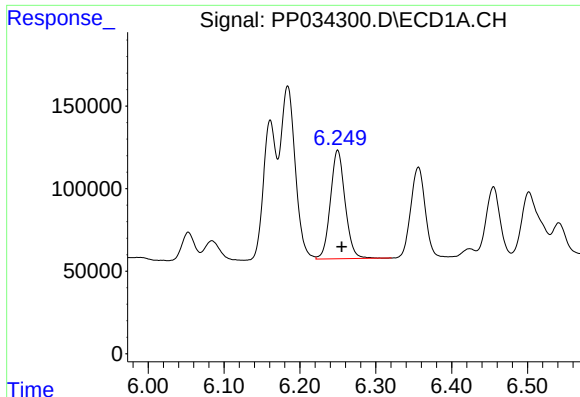


#18 AR-1242-3

R.T.: 6.250 min
Delta R.T.: -0.005 min
Response: 884013
Conc: 475.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:42 PM

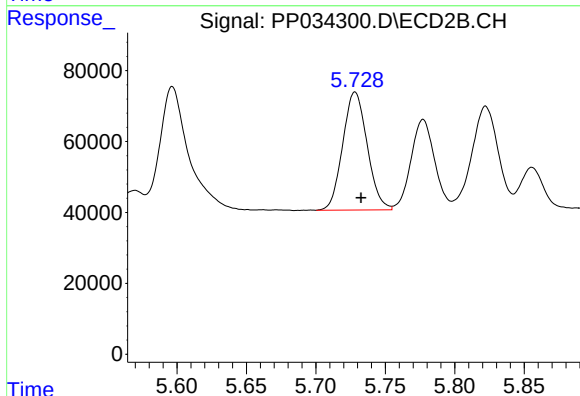


#18 AR-1242-3

R.T.: 5.728 min
Delta R.T.: -0.004 min
Response: 408880
Conc: 562.34 ng/ml

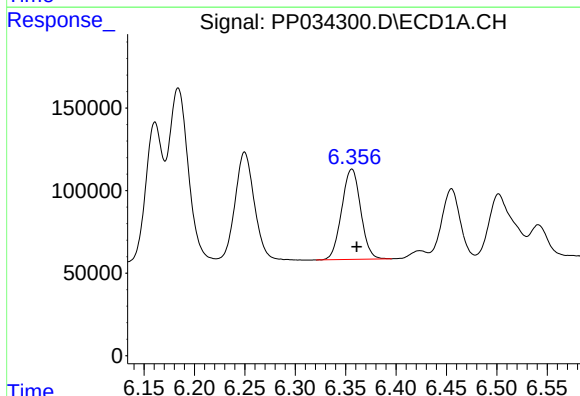


#19 AR-1242-4

R.T.: 6.356 min
Delta R.T.: -0.005 min
Response: 718050
Conc: 476.31 ng/ml

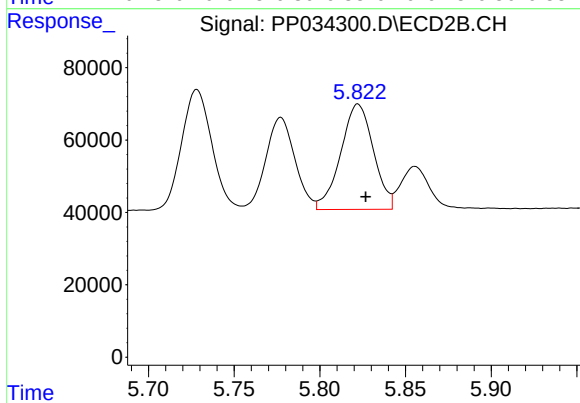

#19 AR-1242-4

R.T.: 5.822 min
Delta R.T.: -0.005 min
Response: 386776
Conc: 533.91 ng/ml

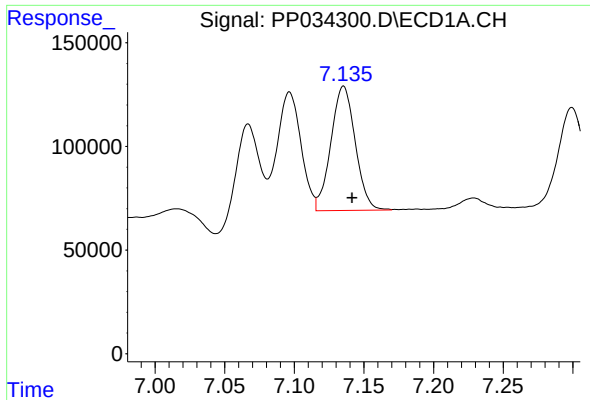


#20 AR-1242-5

R.T.: 7.135 min
Delta R.T.: -0.006 min
Response: 728228
Conc: 477.67 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500

Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:42 PM

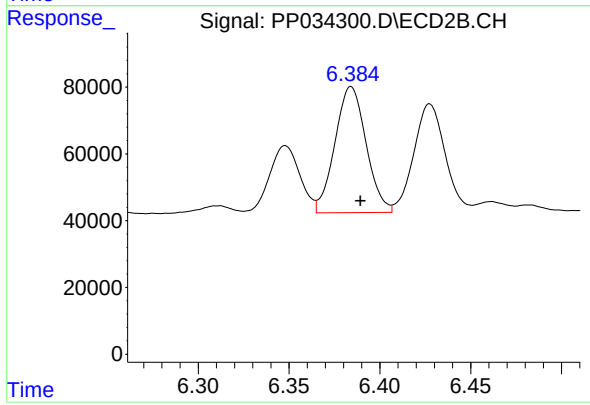

#20 AR-1242-5

R.T.: 6.384 min
Delta R.T.: -0.005 min
Response: 452093
Conc: 576.03 ng/ml