

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
 Data File : PP034301.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 20:48
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 3/24/2021 2:17:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 03:07:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.260	3940873	2297656	46.911	51.921
2) SA Decachlor...	10.772	9.574	3970820	1474302	50.599	55.868
Target Compounds						
21) L5 AR-1248-1	6.161	5.515	719067	389914	480.939	566.824
22) L5 AR-1248-2	6.454	5.777	971890	530297	463.149	531.045
23) L5 AR-1248-3	6.670	5.822	1194028	567483	468.860	538.118
24) L5 AR-1248-4	7.097	6.008	1387820	567279	537.142	462.262
25) L5 AR-1248-5	7.136	6.427	1436934	565365	553.716	559.960m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
Data File : PP034301.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 20:48
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 03:07:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

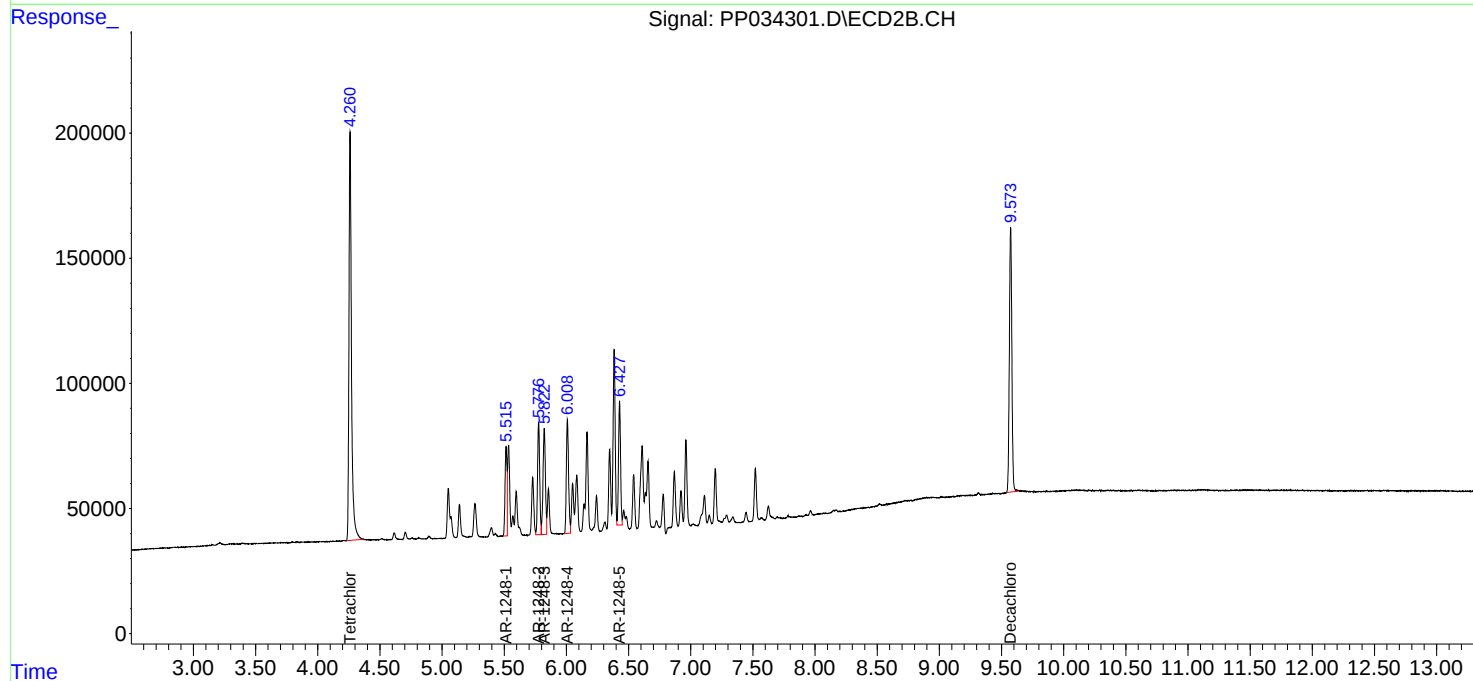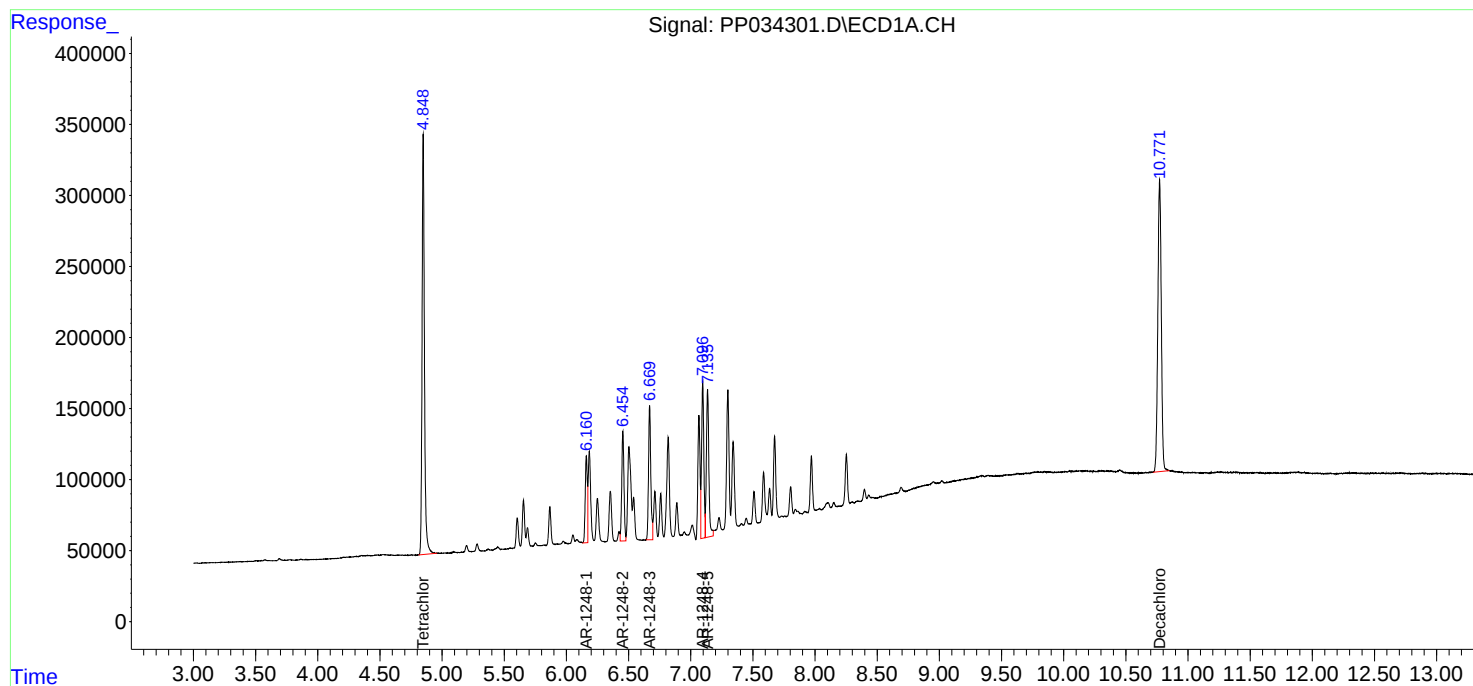

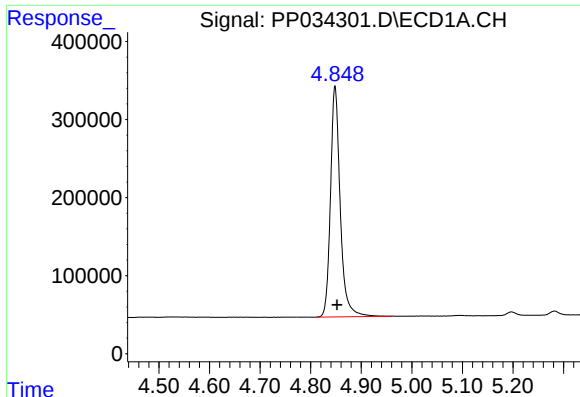


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 3940873
Conc: 46.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:44 PM

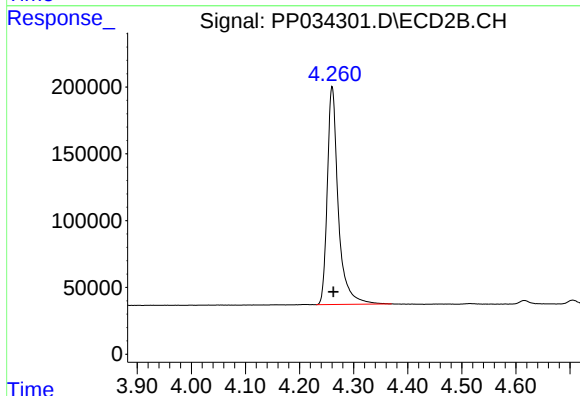


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.003 min
Response: 2297656
Conc: 51.92 ng/ml

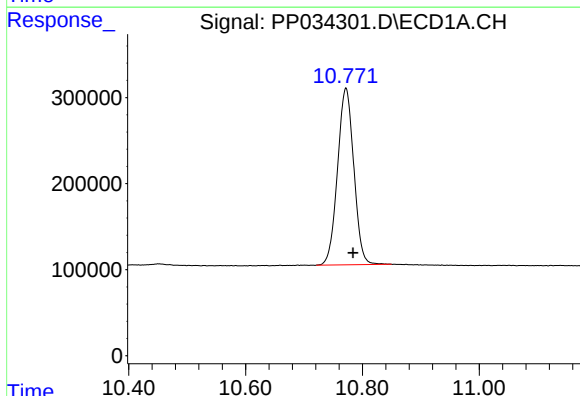


#2 Decachlorobiphenyl

R.T.: 10.772 min
Delta R.T.: -0.012 min
Response: 3970820
Conc: 50.60 ng/ml

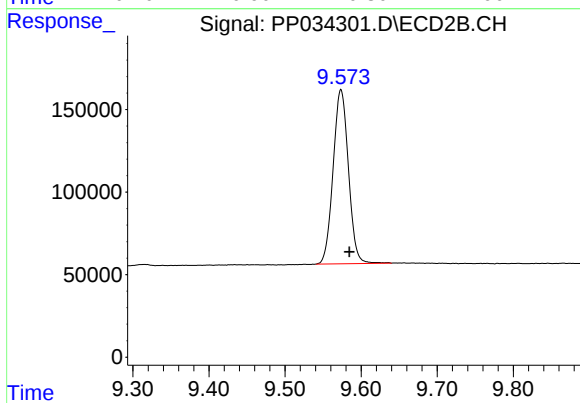

#2 Decachlorobiphenyl

R.T.: 9.574 min
Delta R.T.: -0.011 min
Response: 1474302
Conc: 55.87 ng/ml

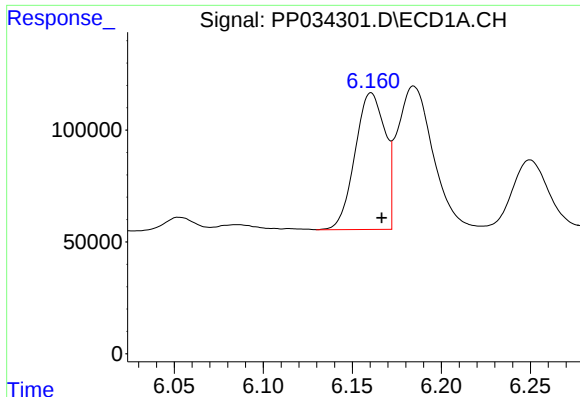


#21 AR-1248-1

R.T.: 6.161 min
Delta R.T.: -0.006 min
Response: 719067
Conc: 480.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:44 PM

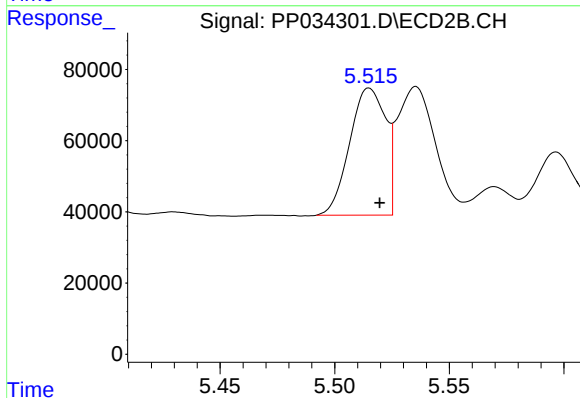


#21 AR-1248-1

R.T.: 5.515 min
Delta R.T.: -0.005 min
Response: 389914
Conc: 566.82 ng/ml

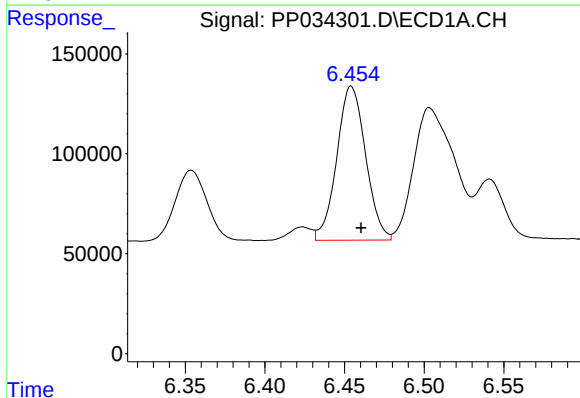


#22 AR-1248-2

R.T.: 6.454 min
Delta R.T.: -0.006 min
Response: 971890
Conc: 463.15 ng/ml

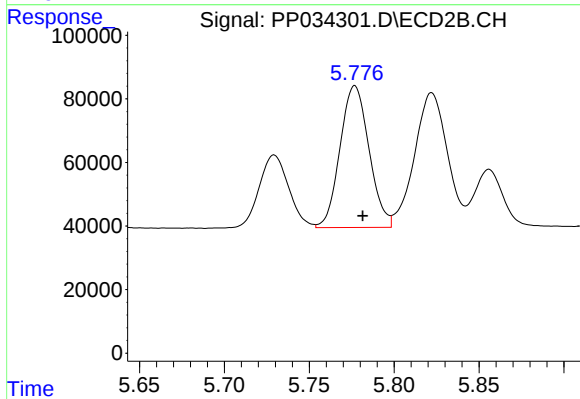

#22 AR-1248-2

R.T.: 5.777 min
Delta R.T.: -0.005 min
Response: 530297
Conc: 531.04 ng/ml

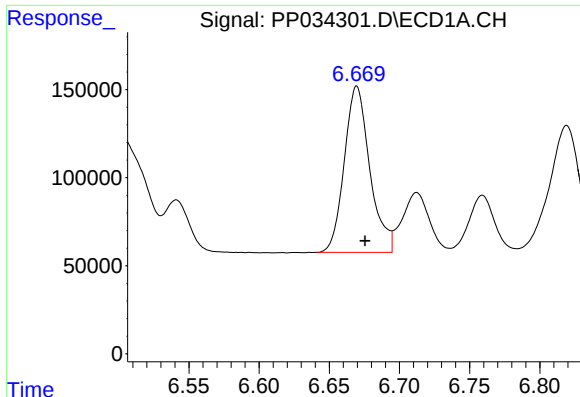


#23 AR-1248-3

R.T.: 6.670 min
Delta R.T.: -0.006 min
Response: 1194028
Conc: 468.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:44 PM

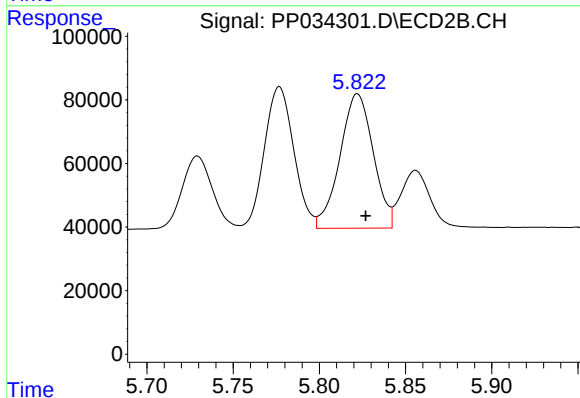


#23 AR-1248-3

R.T.: 5.822 min
Delta R.T.: -0.005 min
Response: 567483
Conc: 538.12 ng/ml

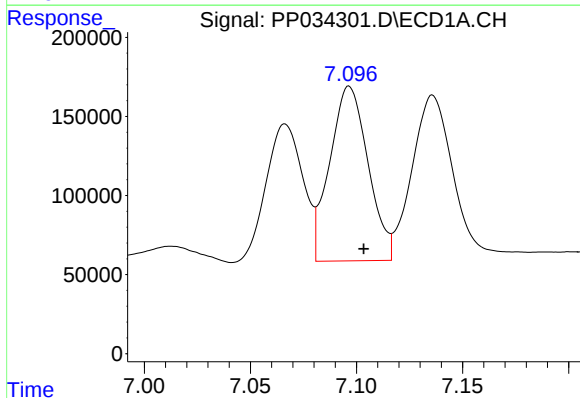


#24 AR-1248-4

R.T.: 7.097 min
Delta R.T.: -0.007 min
Response: 1387820
Conc: 537.14 ng/ml

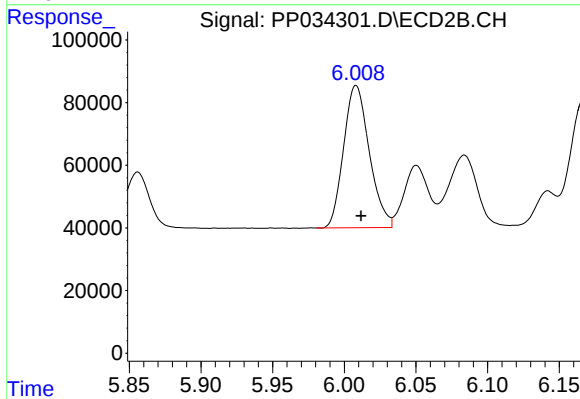

#24 AR-1248-4

R.T.: 6.008 min
Delta R.T.: -0.003 min
Response: 567279
Conc: 462.26 ng/ml

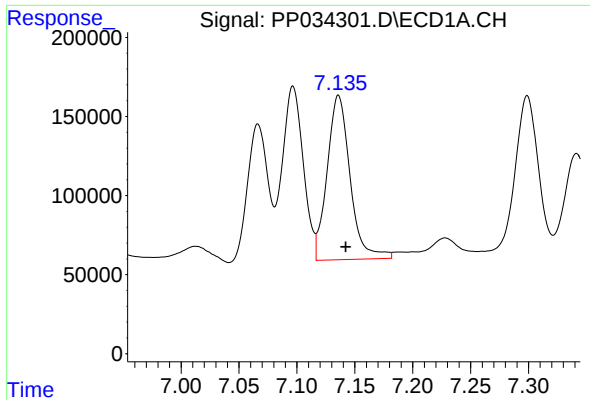


#25 AR-1248-5

R.T.: 7.136 min
Delta R.T.: -0.006 min
Response: 1436934
Conc: 553.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:44 PM

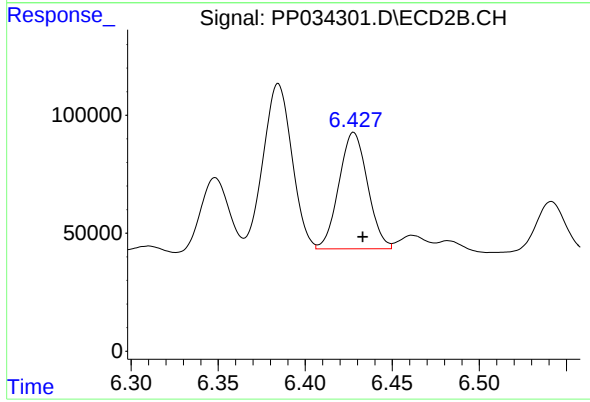

#25 AR-1248-5

R.T.: 6.427 min
Delta R.T.: -0.006 min
Response: 565365
Conc: 559.96 ng/ml m