

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
 Data File : PP034309.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 23:37
 Operator : DD\AJ
 Sample : AR1242CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1242CCC500

Manual Integrations
 APPROVED

Ankita
 3/24/2021 2:17:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 03:10:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.849	4.261	4047994	2349691	48.187	53.097
2)	SA Decachlor...	10.770	9.574	3849074	1474302	49.047	55.868
Target Compounds							
16)	L4 AR-1242-1	6.162	5.515	871069	508312	437.135	558.065 #
17)	L4 AR-1242-2	6.185	5.536	1285114	730869	432.219	556.804 #
18)	L4 AR-1242-3	6.250	5.729	804043	407013	432.088	559.771 #
19)	L4 AR-1242-4	6.357	5.823	652080	388794	432.552	536.699
20)	L4 AR-1242-5	7.136	6.385	744493	439235	488.340m	559.644

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
Data File : PP034309.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 23:37
Operator : DD\AJ
Sample : AR1242CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 03:10:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

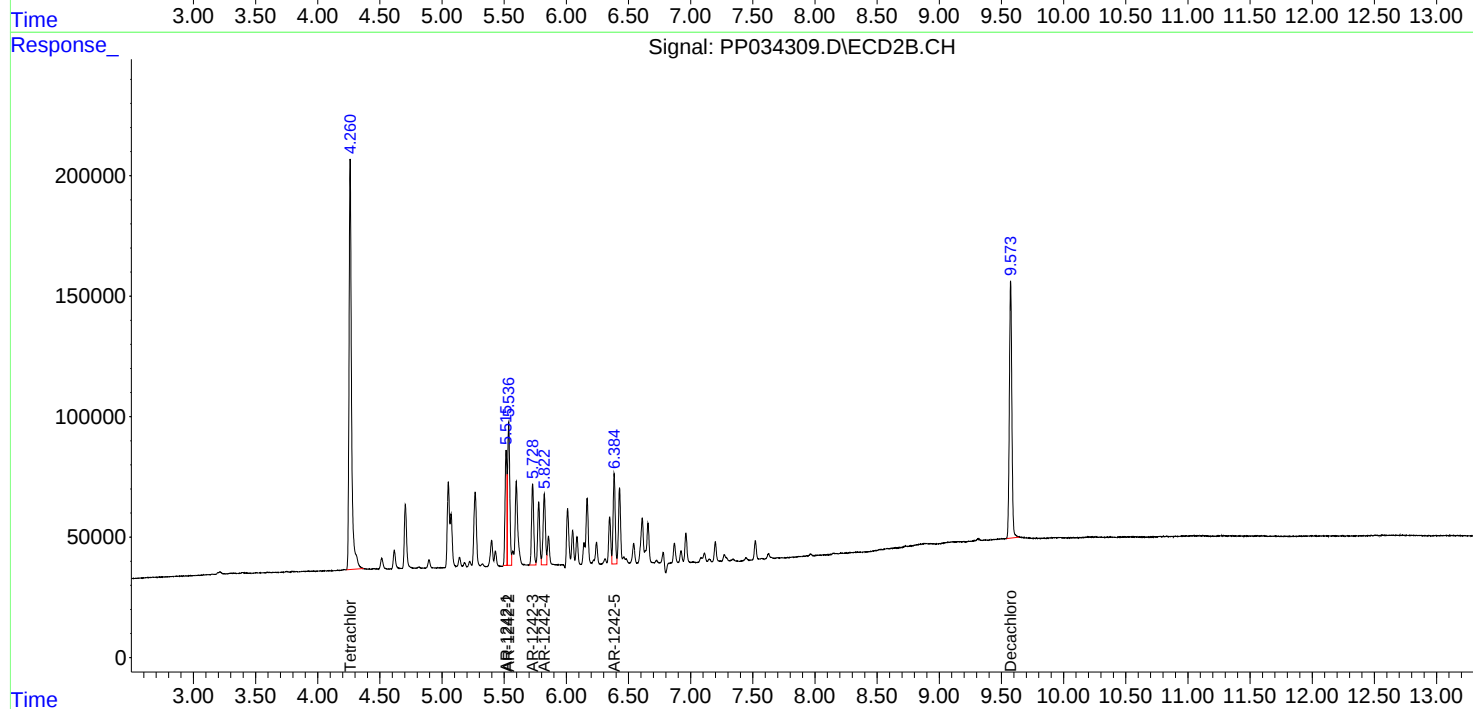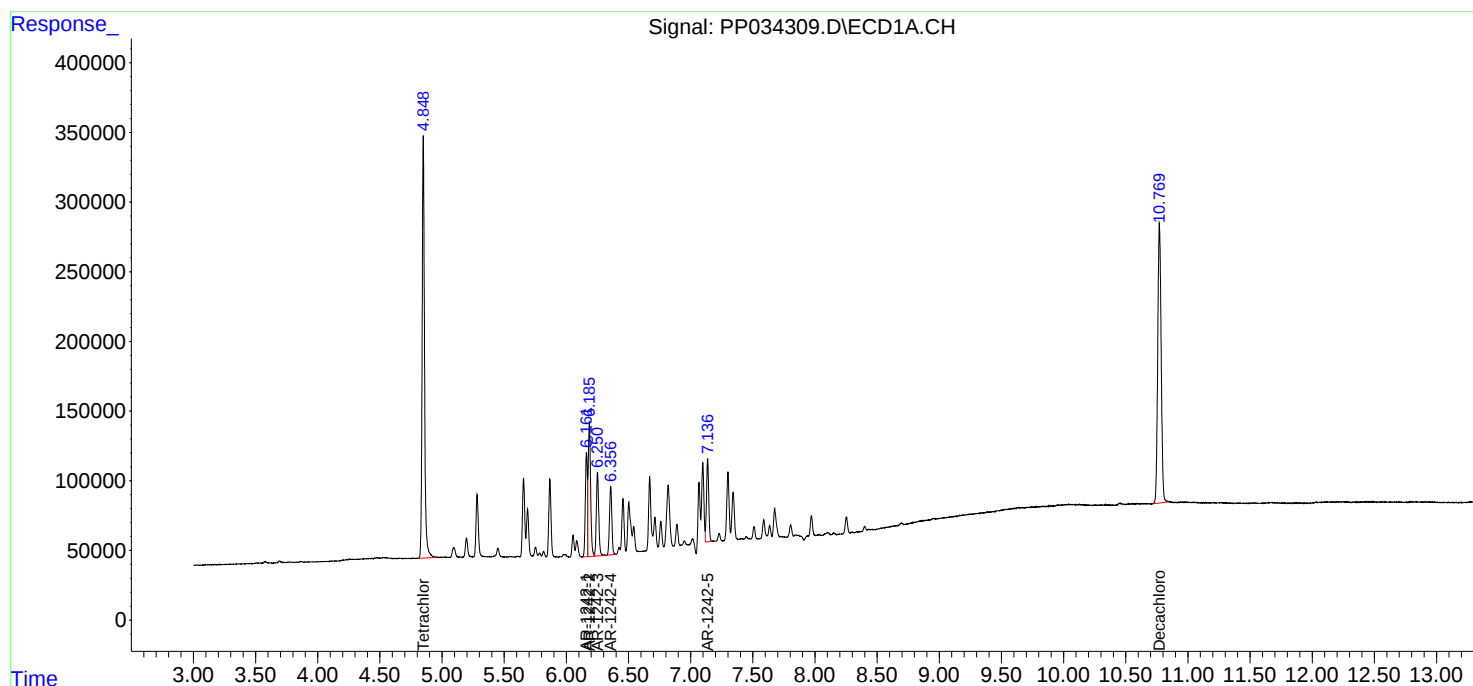

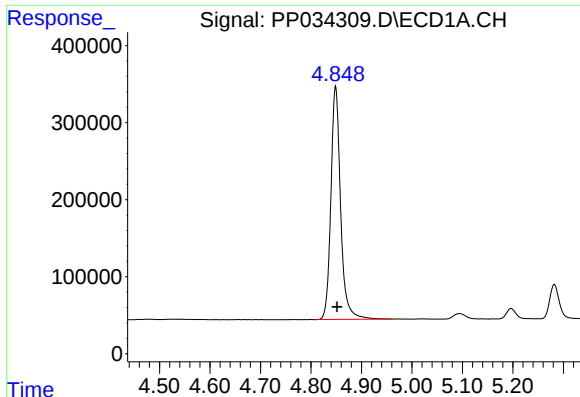


#1 Tetrachloro-m-xylene

R.T.: 4.849 min
Delta R.T.: -0.003 min
Response: 4047994
Conc: 48.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:47 PM

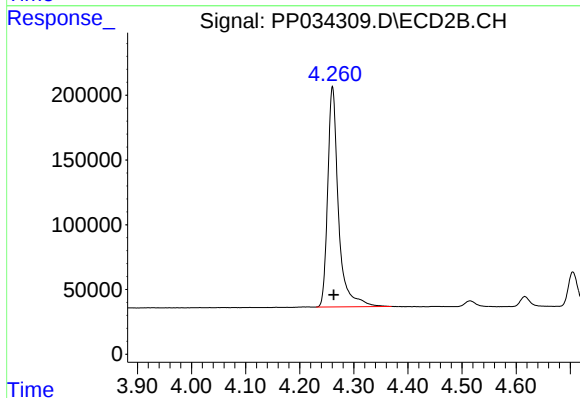


#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.002 min
Response: 2349691
Conc: 53.10 ng/ml

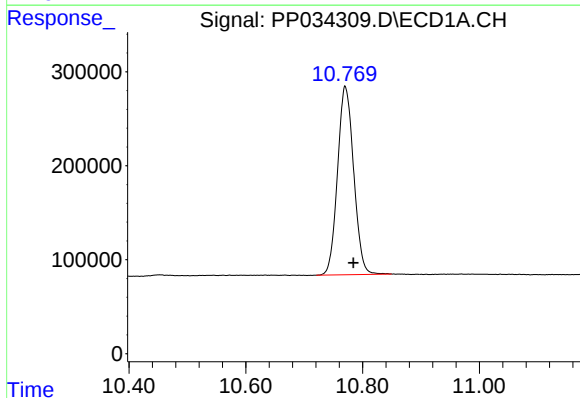


#2 Decachlorobiphenyl

R.T.: 10.770 min
Delta R.T.: -0.014 min
Response: 3849074
Conc: 49.05 ng/ml

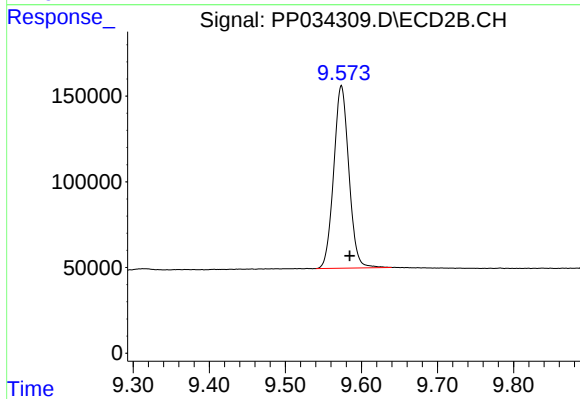

#2 Decachlorobiphenyl

R.T.: 9.574 min
Delta R.T.: -0.011 min
Response: 1474302
Conc: 55.87 ng/ml

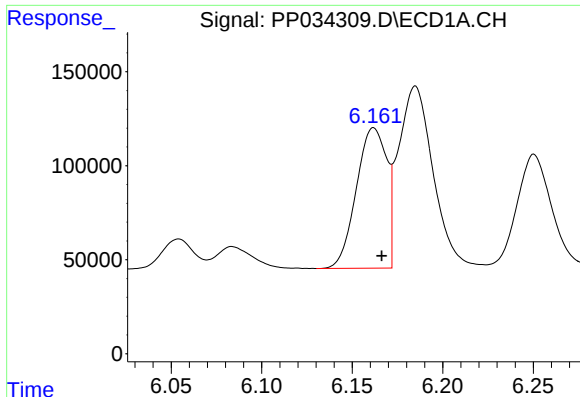


#16 AR-1242-1

R.T.: 6.162 min
Delta R.T.: -0.004 min
Response: 871069
Conc: 437.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:47 PM

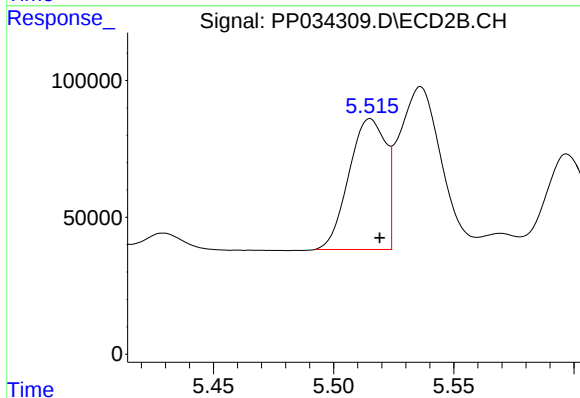


#16 AR-1242-1

R.T.: 5.515 min
Delta R.T.: -0.004 min
Response: 508312
Conc: 558.07 ng/ml

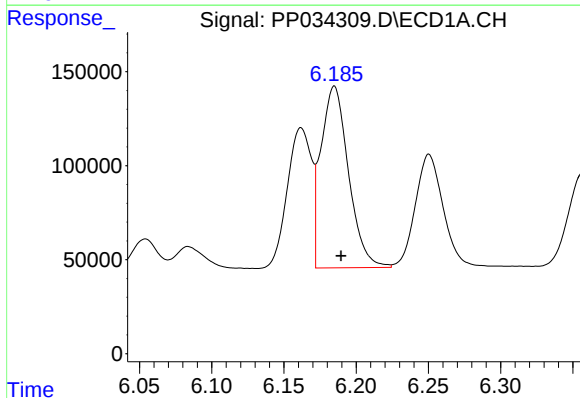


#17 AR-1242-2

R.T.: 6.185 min
Delta R.T.: -0.005 min
Response: 1285114
Conc: 432.22 ng/ml

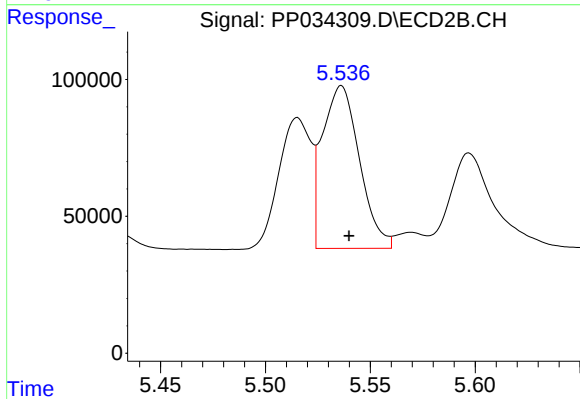

#17 AR-1242-2

R.T.: 5.536 min
Delta R.T.: -0.004 min
Response: 730869
Conc: 556.80 ng/ml

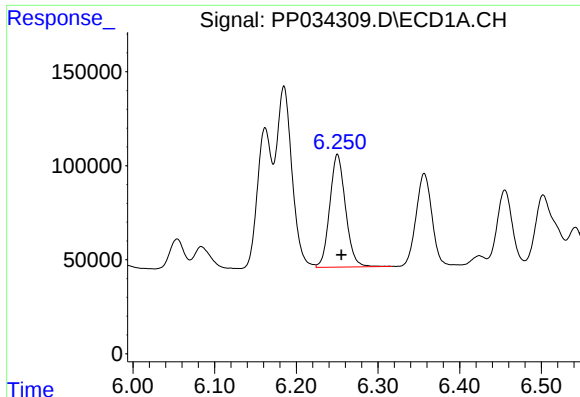


#18 AR-1242-3

R.T.: 6.250 min
Delta R.T.: -0.005 min
Response: 804043
Conc: 432.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:47 PM

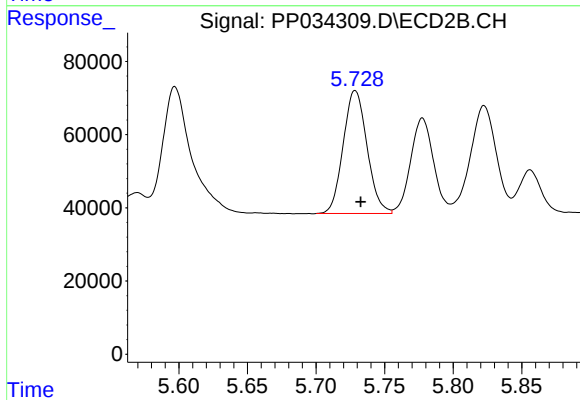


#18 AR-1242-3

R.T.: 5.729 min
Delta R.T.: -0.004 min
Response: 407013
Conc: 559.77 ng/ml

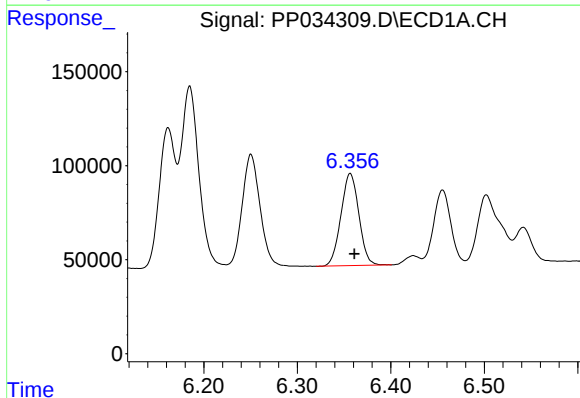


#19 AR-1242-4

R.T.: 6.357 min
Delta R.T.: -0.004 min
Response: 652080
Conc: 432.55 ng/ml

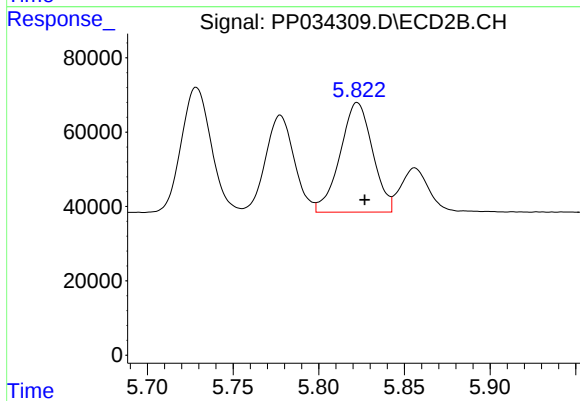

#19 AR-1242-4

R.T.: 5.823 min
Delta R.T.: -0.004 min
Response: 388794
Conc: 536.70 ng/ml

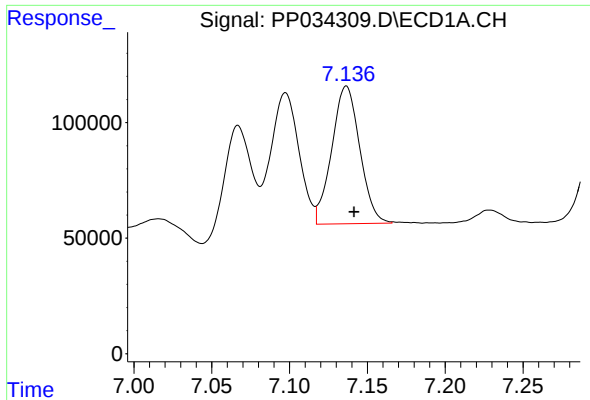


#20 AR-1242-5

R.T.: 7.136 min
Delta R.T.: -0.005 min
Response: 744493
Conc: 488.34 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500

Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:47 PM

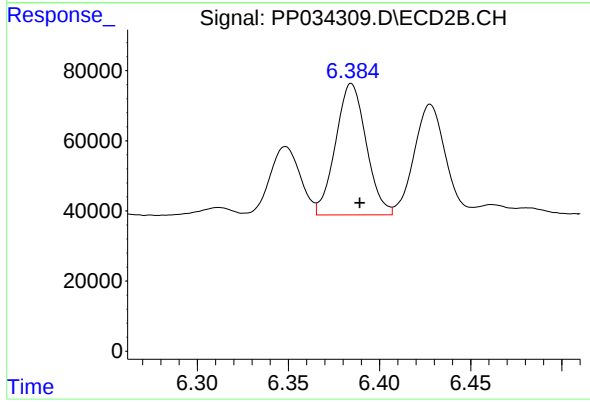

#20 AR-1242-5

R.T.: 6.385 min
Delta R.T.: -0.005 min
Response: 439235
Conc: 559.64 ng/ml