

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
 Data File : PP034310.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Mar 2021 23:54
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 3/24/2021 2:17:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 03:10:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.260	4032901	2350701	48.007	53.120
2) SA Decachlor...	10.769	9.573	3889232	1464449	49.559	55.495
Target Compounds						
21) L5 AR-1248-1	6.160	5.515	679321	389382	454.356	566.050
22) L5 AR-1248-2	6.454	5.777	896200	541274	427.079	542.038 #
23) L5 AR-1248-3	6.669	5.822	1094789	575036	429.891	545.281 #
24) L5 AR-1248-4	7.097	6.008	1355371	567040	524.583	462.067
25) L5 AR-1248-5	7.135	6.427	1450668	594952	559.008	589.264m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032321\
Data File : PP034310.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Mar 2021 23:54
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 03:10:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

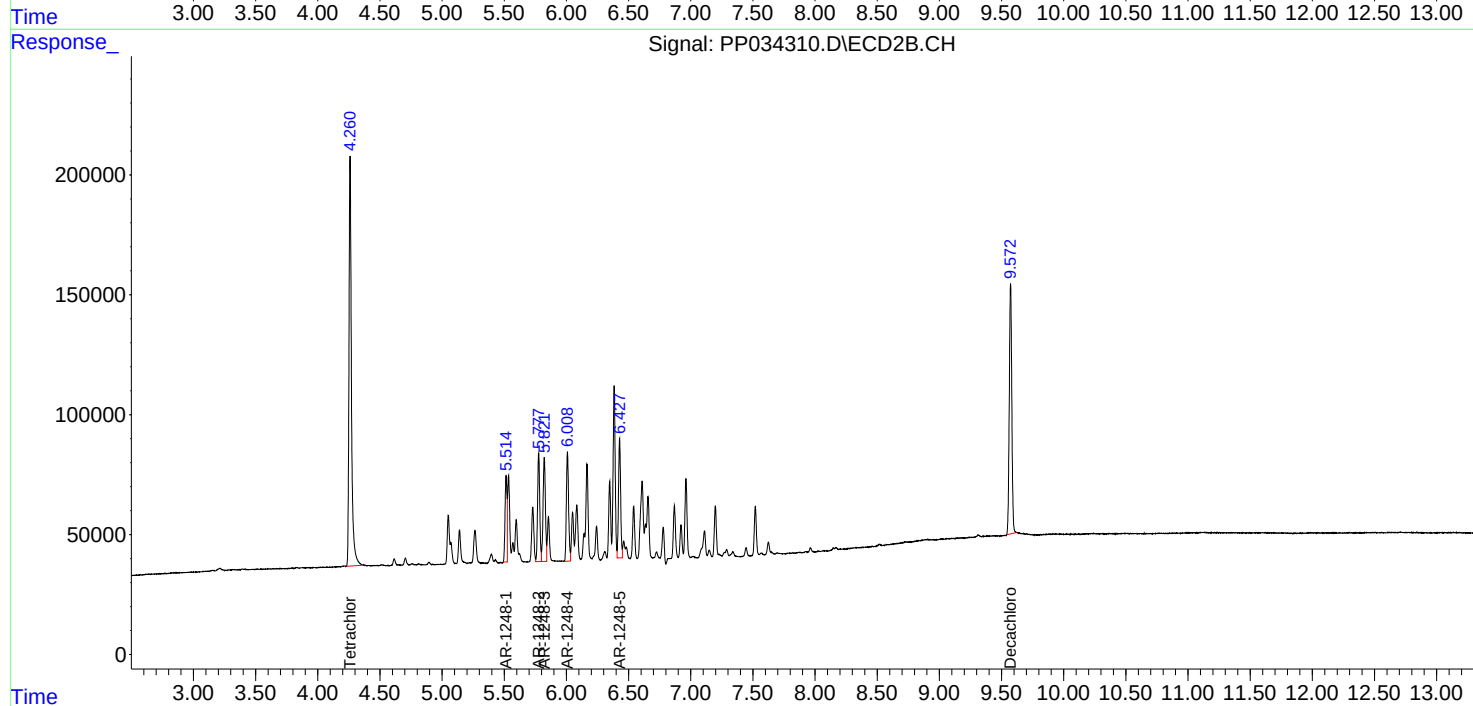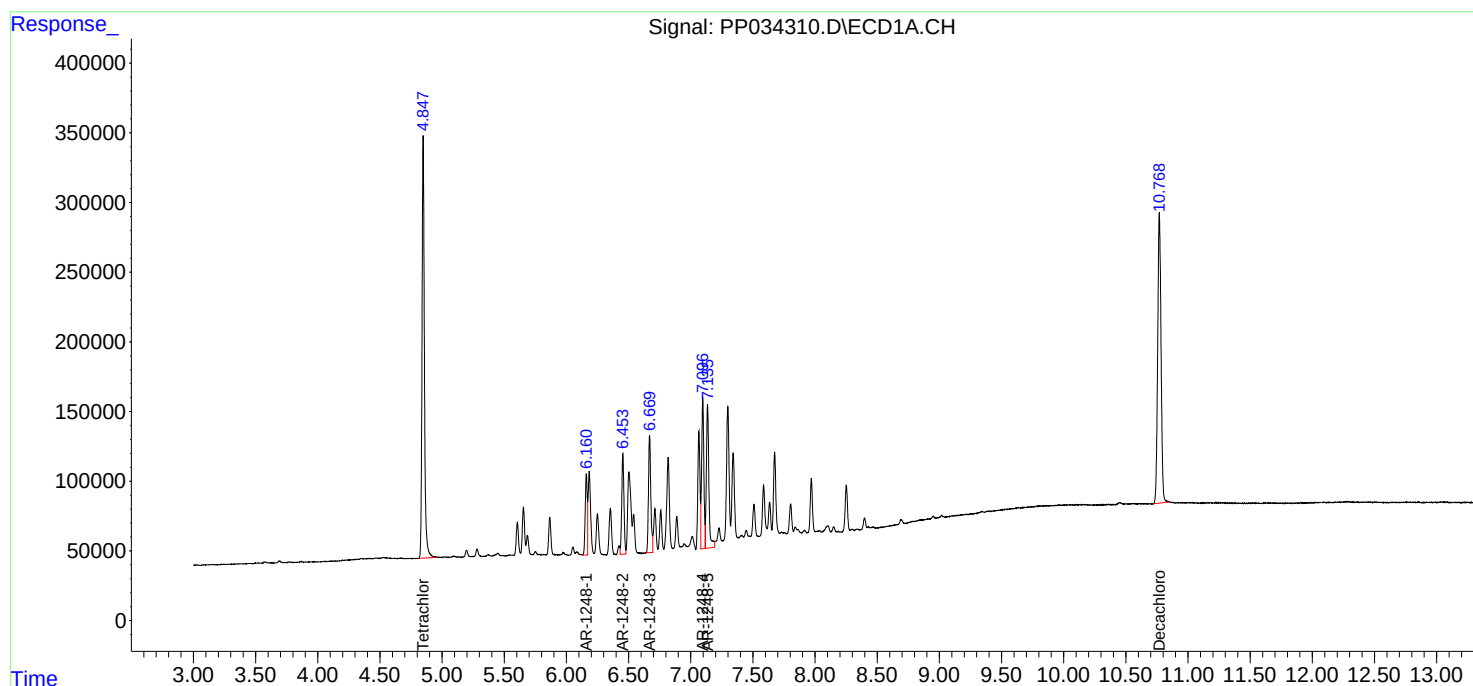

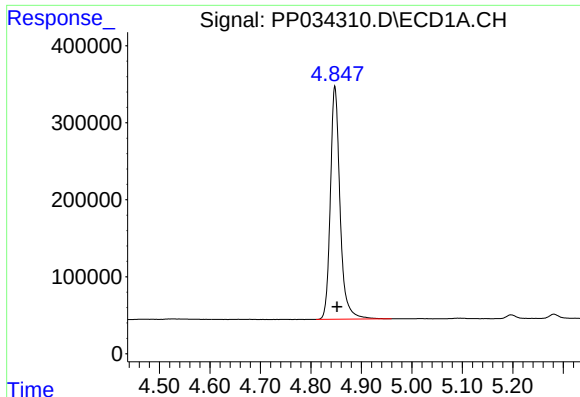


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 4032901
Conc: 48.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:50 PM

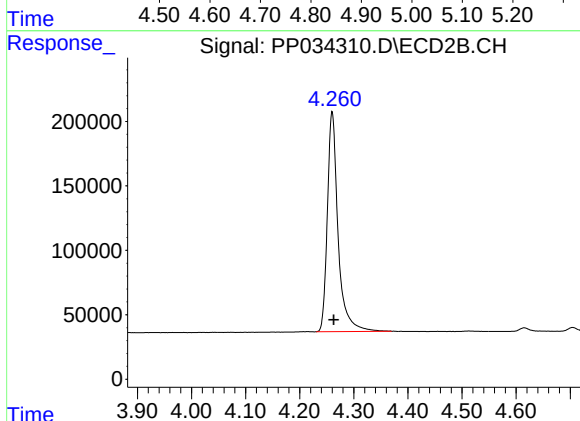


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.003 min
Response: 2350701
Conc: 53.12 ng/ml

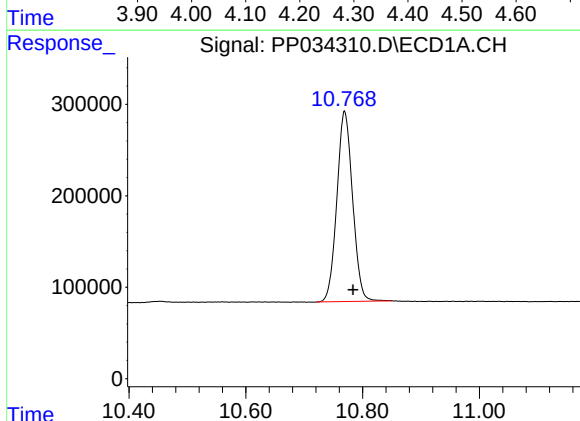


#2 Decachlorobiphenyl

R.T.: 10.769 min
Delta R.T.: -0.015 min
Response: 3889232
Conc: 49.56 ng/ml

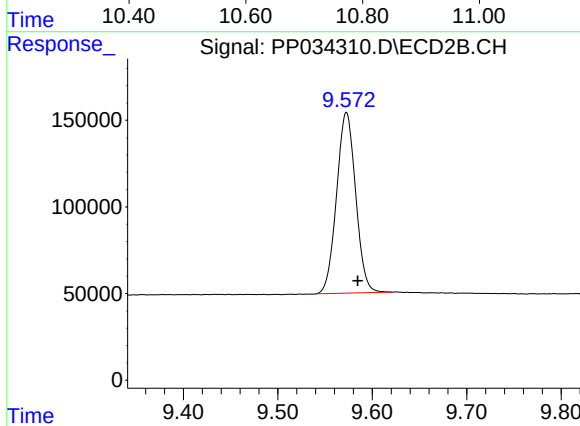

#2 Decachlorobiphenyl

R.T.: 9.573 min
Delta R.T.: -0.012 min
Response: 1464449
Conc: 55.49 ng/ml

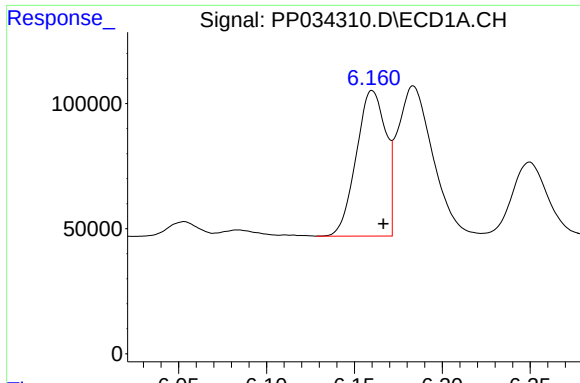


#21 AR-1248-1

R.T.: 6.160 min
Delta R.T.: -0.006 min
Response: 679321
Conc: 454.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:50 PM

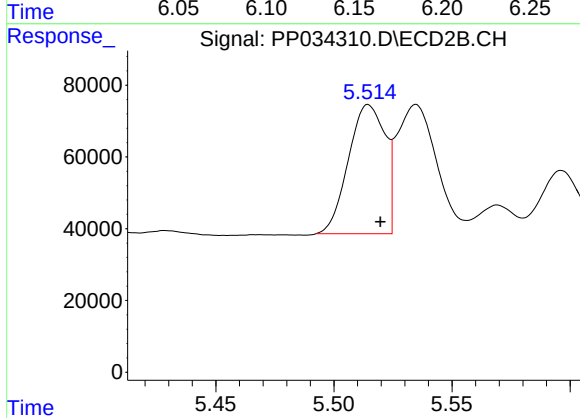


#21 AR-1248-1

R.T.: 5.515 min
Delta R.T.: -0.005 min
Response: 389382
Conc: 566.05 ng/ml

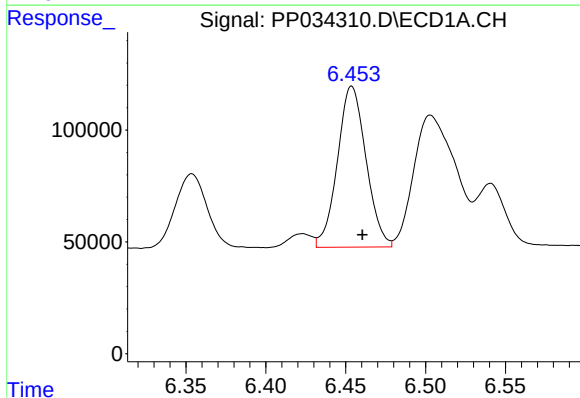


#22 AR-1248-2

R.T.: 6.454 min
Delta R.T.: -0.007 min
Response: 896200
Conc: 427.08 ng/ml

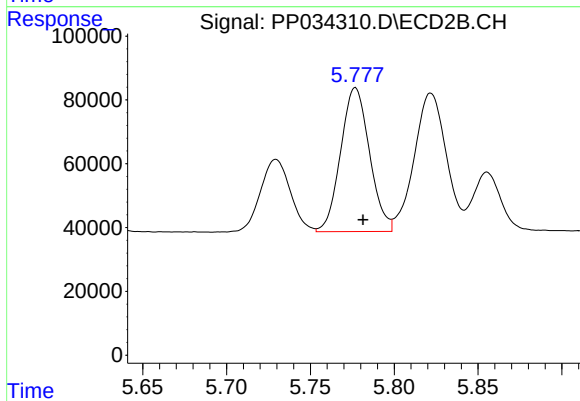

#22 AR-1248-2

R.T.: 5.777 min
Delta R.T.: -0.005 min
Response: 541274
Conc: 542.04 ng/ml

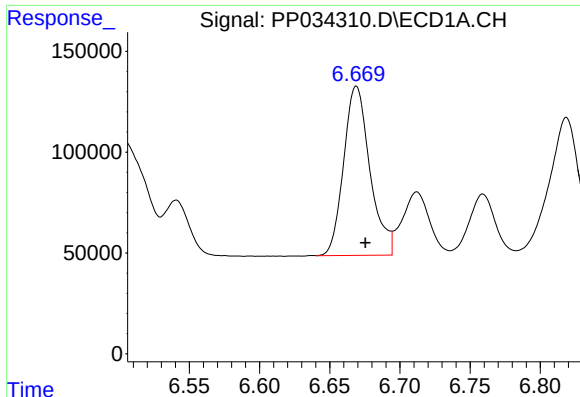


#23 AR-1248-3

R.T.: 6.669 min
Delta R.T.: -0.006 min
Response: 1094789
Conc: 429.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:50 PM

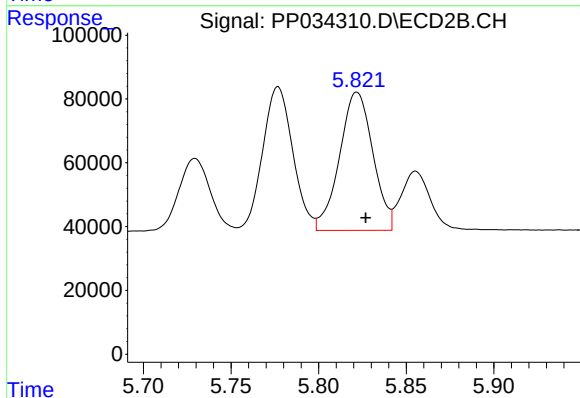


#23 AR-1248-3

R.T.: 5.822 min
Delta R.T.: -0.005 min
Response: 575036
Conc: 545.28 ng/ml

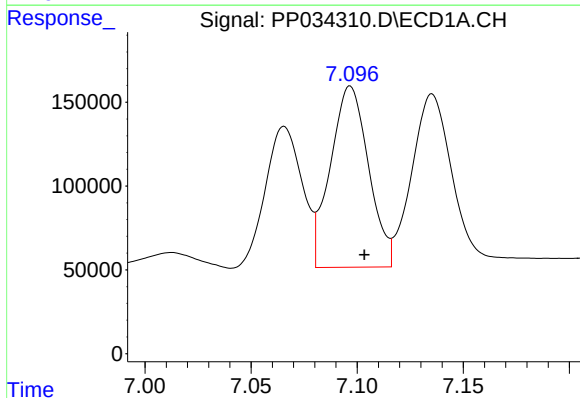


#24 AR-1248-4

R.T.: 7.097 min
Delta R.T.: -0.007 min
Response: 1355371
Conc: 524.58 ng/ml

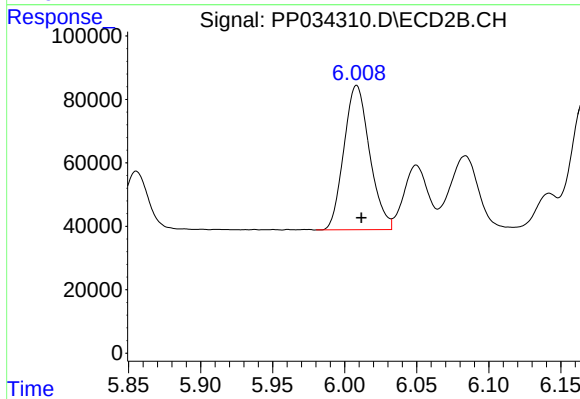

#24 AR-1248-4

R.T.: 6.008 min
Delta R.T.: -0.003 min
Response: 567040
Conc: 462.07 ng/ml

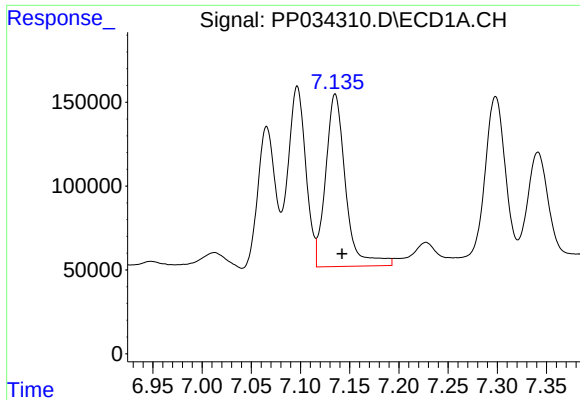


#25 AR-1248-5

R.T.: 7.135 min
Delta R.T.: -0.007 min
Response: 1450668
Conc: 559.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
3/24/2021 2:17:50 PM

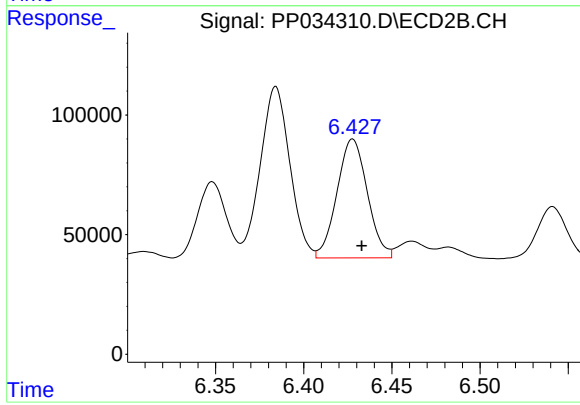

#25 AR-1248-5

R.T.: 6.427 min
Delta R.T.: -0.006 min
Response: 594952
Conc: 589.26 ng/ml m