

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032322\
 Data File : PP045024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 13:40
 Operator : YP\AJ
 Sample : N2055-04 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-31B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/24/2022
 Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 06:13:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.895	3.153	3565291	3257858	1.957m	2.472m#
2) SA Decachlor...	10.025	8.509	4739822	3778308	3.682	2.908m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032322\
Data File : PP045024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 13:40
Operator : YP\AJ
Sample : N2055-04 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CLI-2022-31B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 06:13:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

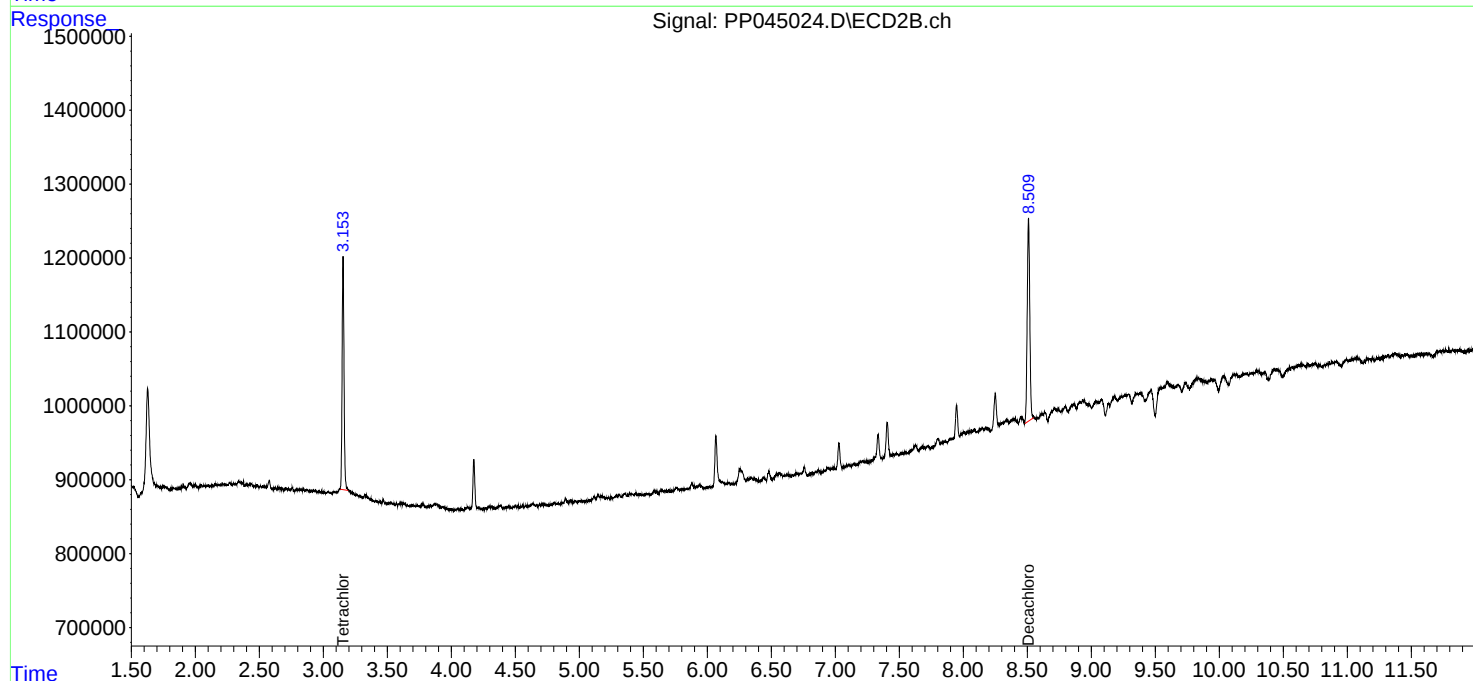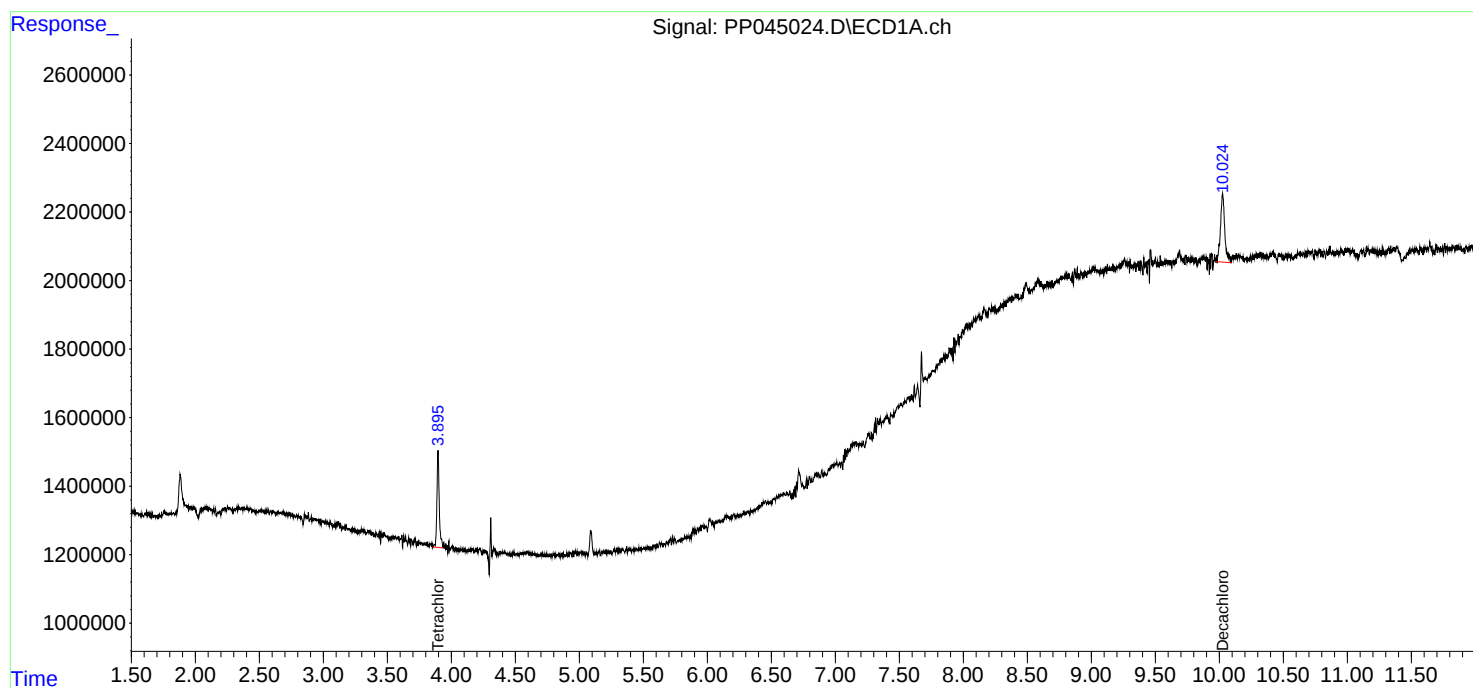

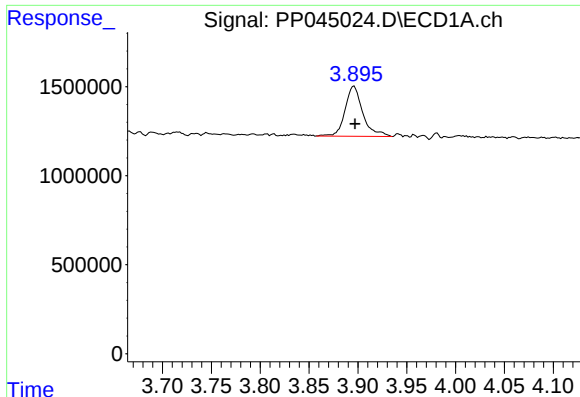


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: -0.002 min
Response: 3565291
Conc: 1.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-31B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

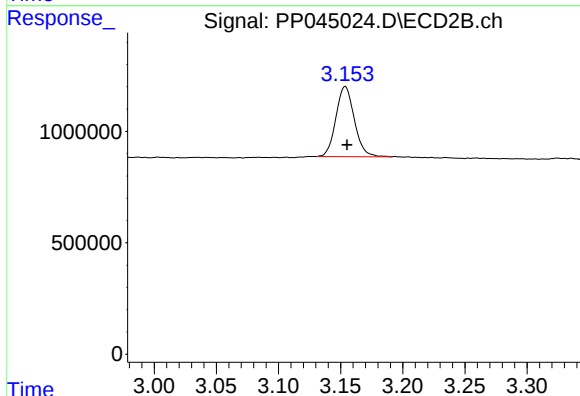


#1 Tetrachloro-m-xylene

R.T.: 3.153 min
Delta R.T.: -0.002 min
Response: 3257858
Conc: 2.47 ng/ml m

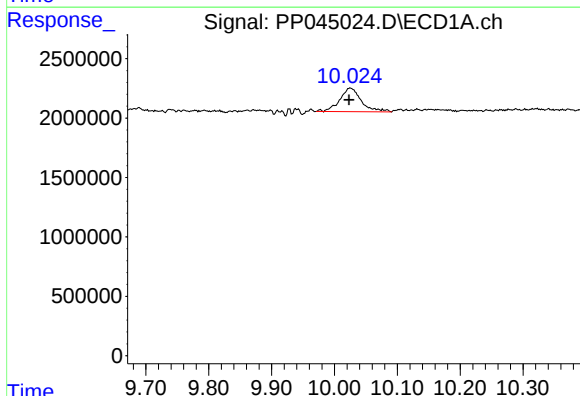

#2 Decachlorobiphenyl

R.T.: 10.025 min
Delta R.T.: 0.002 min
Response: 4739822
Conc: 3.68 ng/ml

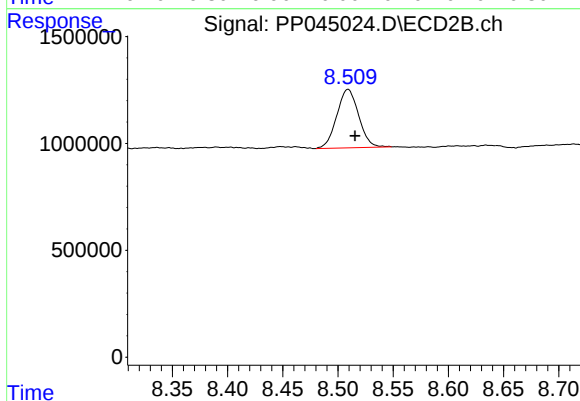

#2 Decachlorobiphenyl

R.T.: 8.509 min
Delta R.T.: -0.007 min
Response: 3778308
Conc: 2.91 ng/ml m