

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032322\
 Data File : PP045038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 18:16
 Operator : YP\AJ
 Sample : N2064-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20220281-FIELD-BLANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 06:20:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.895	3.155	35069273	27806762	19.247	21.100
2) SA Decachlor...	10.016	8.508	9458317	11572935	7.348	8.907

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032322\
Data File : PP045038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 18:16
Operator : YP\AJ
Sample : N2064-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20220281-FIELD-BLANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 06:20:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

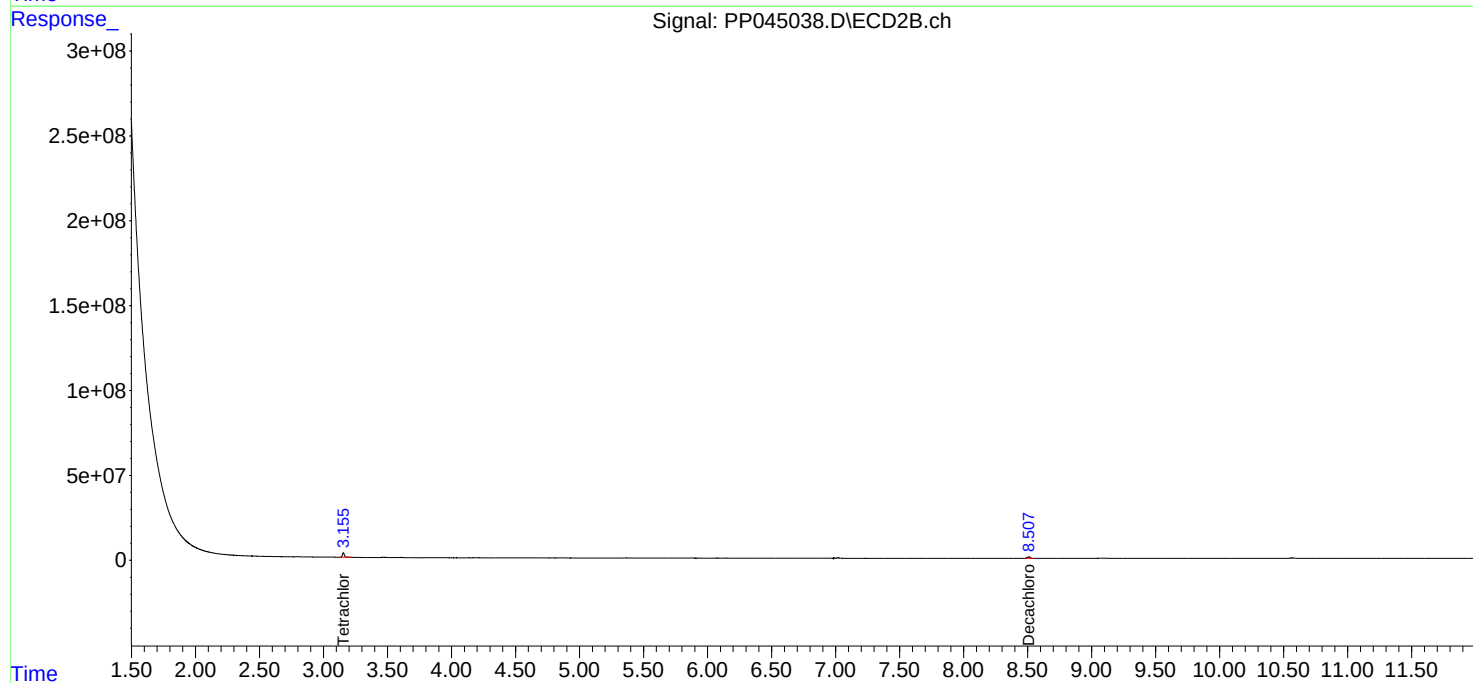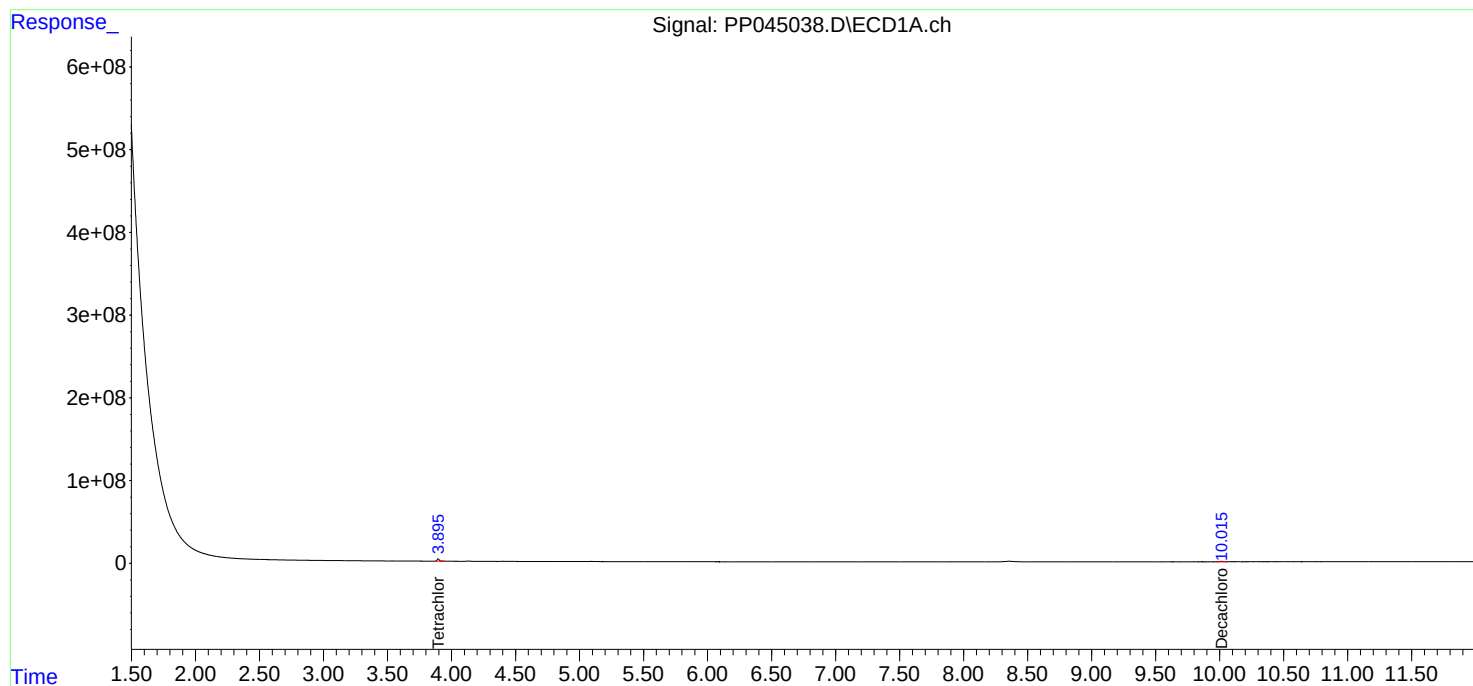


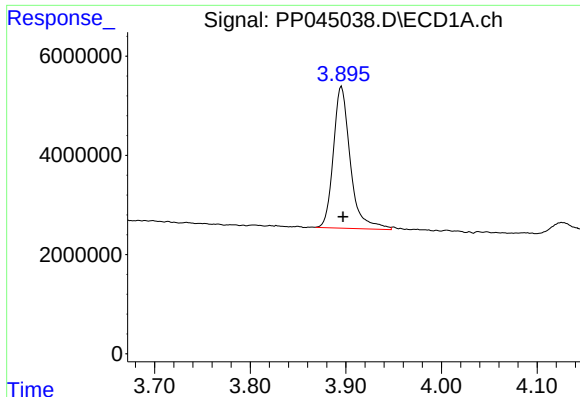

#1 Tetrachloro-m-xylene


R.T.: 3.895 min
Delta R.T.: -0.002 min
Response: 35069273
Conc: 19.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
20220281-FIELD-BLANK

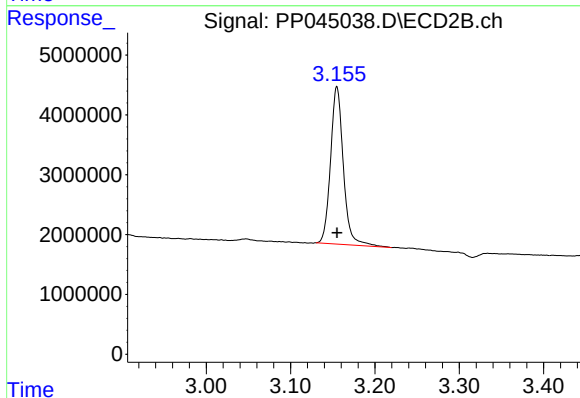


#1 Tetrachloro-m-xylene

R.T.: 3.155 min
Delta R.T.: 0.000 min
Response: 27806762
Conc: 21.10 ng/ml

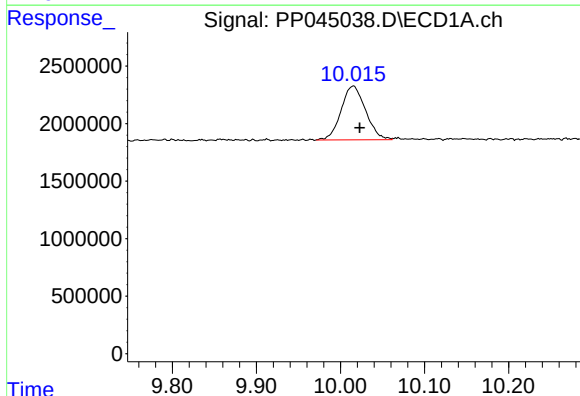

#2 Decachlorobiphenyl

R.T.: 10.016 min
Delta R.T.: -0.007 min
Response: 9458317
Conc: 7.35 ng/ml

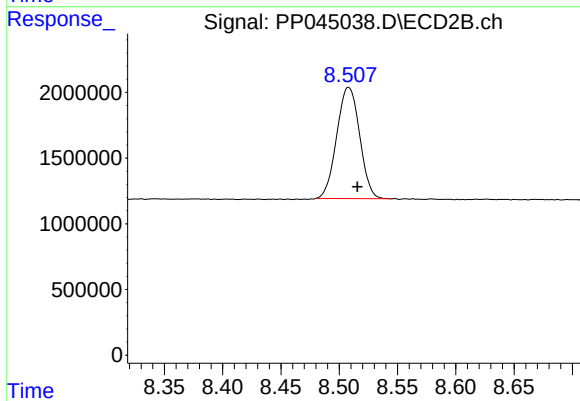

#2 Decachlorobiphenyl

R.T.: 8.508 min
Delta R.T.: -0.007 min
Response: 11572935
Conc: 8.91 ng/ml