

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032322\
 Data File : PP045070.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 04:19
 Operator : YP\AJ
 Sample : N2056-01 10X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC157517LOK-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/24/2022
 Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 09:04:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.894	3.154	2803564	2499899	1.539m	1.897
2) SA Decachlor...	10.015	8.507	3127775	3196125	2.430m	2.460

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032322\
Data File : PP045070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 04:19
Operator : YP\AJ
Sample : N2056-01 10X
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC157517LOK-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 09:04:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

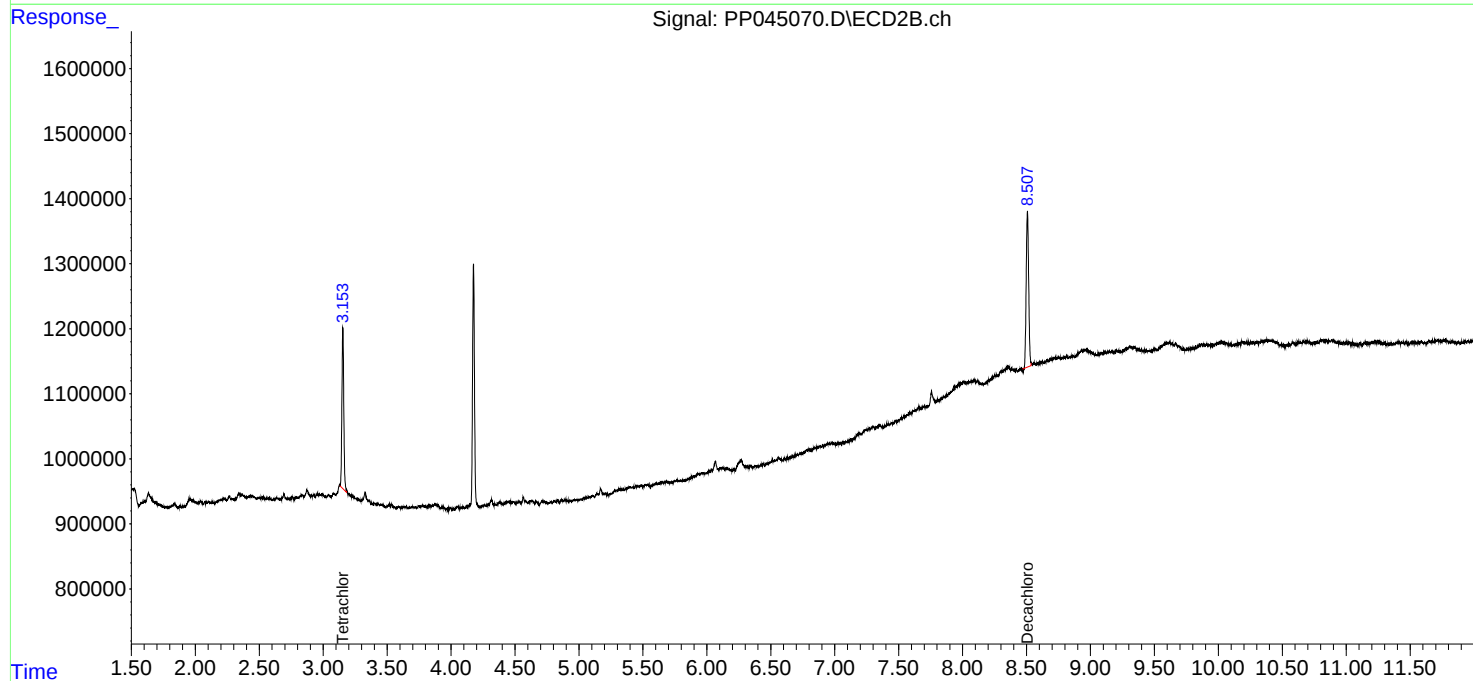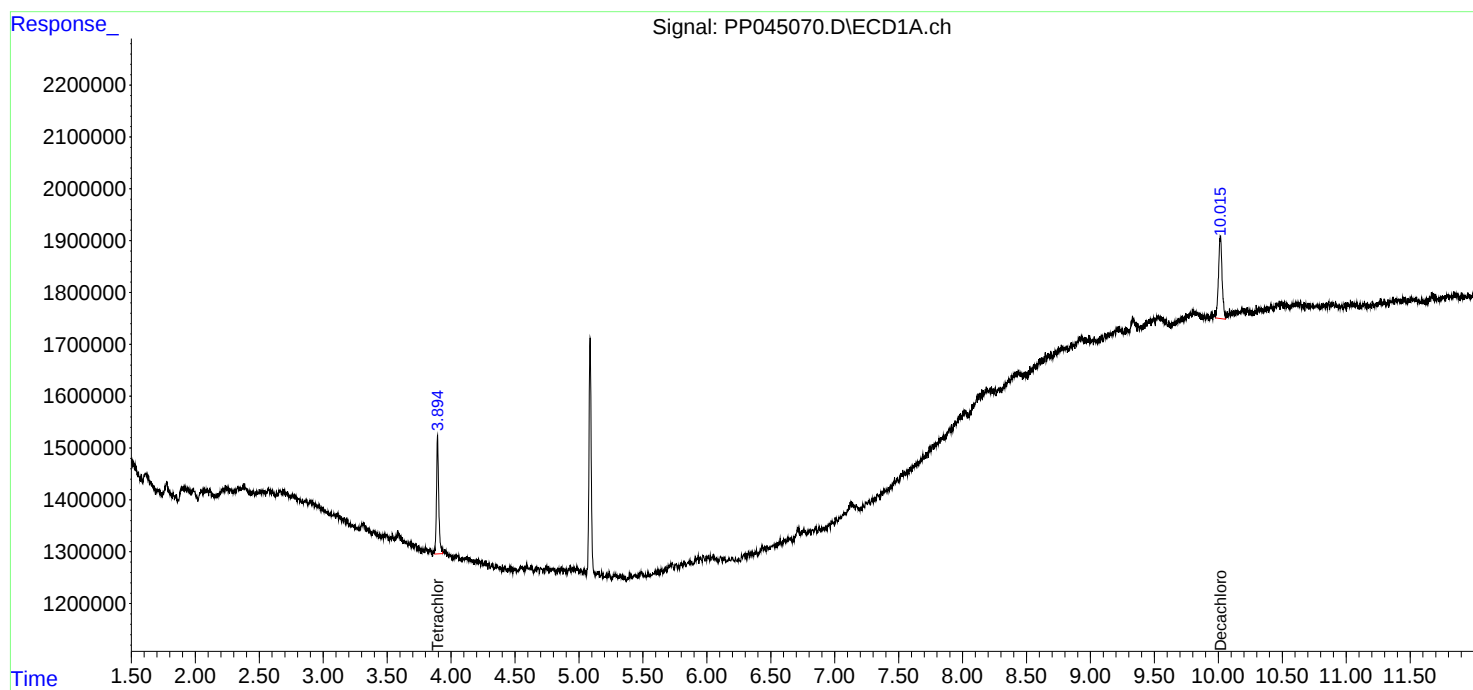

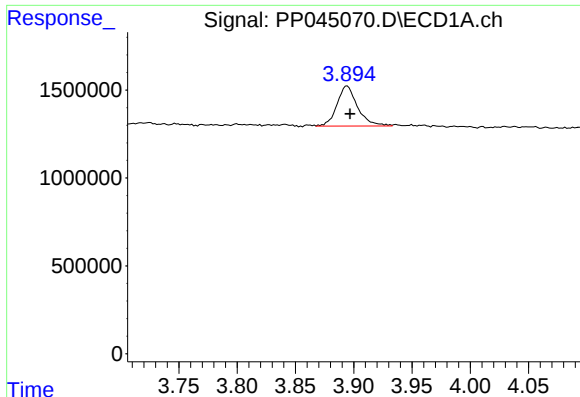


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: -0.003 min
Response: 2803564
Conc: 1.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC157517LOK-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

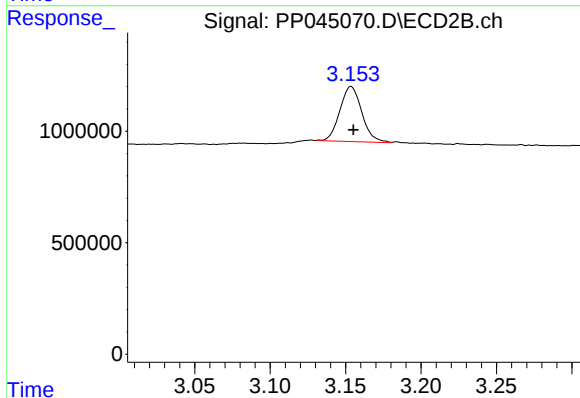


#1 Tetrachloro-m-xylene

R.T.: 3.154 min
Delta R.T.: -0.001 min
Response: 2499899
Conc: 1.90 ng/ml

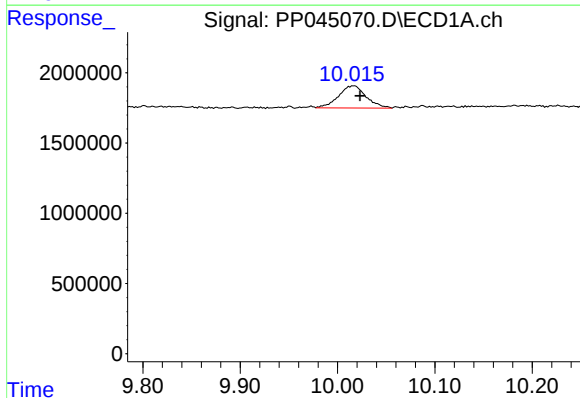

#2 Decachlorobiphenyl

R.T.: 10.015 min
Delta R.T.: -0.008 min
Response: 3127775
Conc: 2.43 ng/ml m

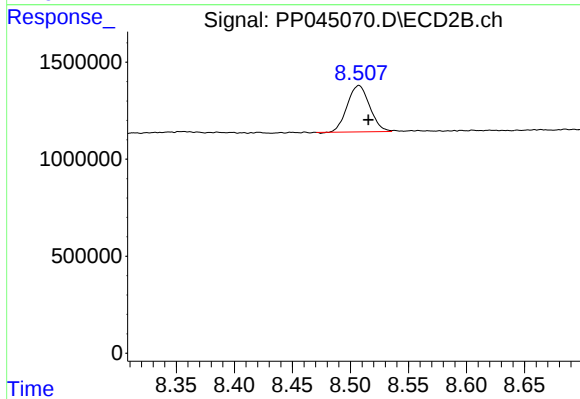

#2 Decachlorobiphenyl

R.T.: 8.507 min
Delta R.T.: -0.008 min
Response: 3196125
Conc: 2.46 ng/ml