

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032322\
 Data File : PP045072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 04:49
 Operator : YP\AJ
 Sample : N2055-15 10X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-37A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/24/2022
 Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 09:08:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.893	3.154	2834119	2581029	1.555m	1.959 #
2) SA Decachlor...	10.014	8.507	3014244	3590748	2.342m	2.763
Target Compounds						
26) L6 AR-1254-1	6.071	5.146	587098	746980	8.842m	8.638
27) L6 AR-1254-2	6.310	5.308	828686	927491	8.294	12.464 #
28) L6 AR-1254-3	6.708	5.737	782707	948306	7.653	8.253
29) L6 AR-1254-4	7.022	5.988	555529	706619	7.638	9.478
30) L6 AR-1254-5	7.481	6.437	1106894	1180502	14.311	11.464

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032322\
Data File : PP045072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 04:49
Operator : YP\AJ
Sample : N2055-15 10X
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CLI-2022-37A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 09:08:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

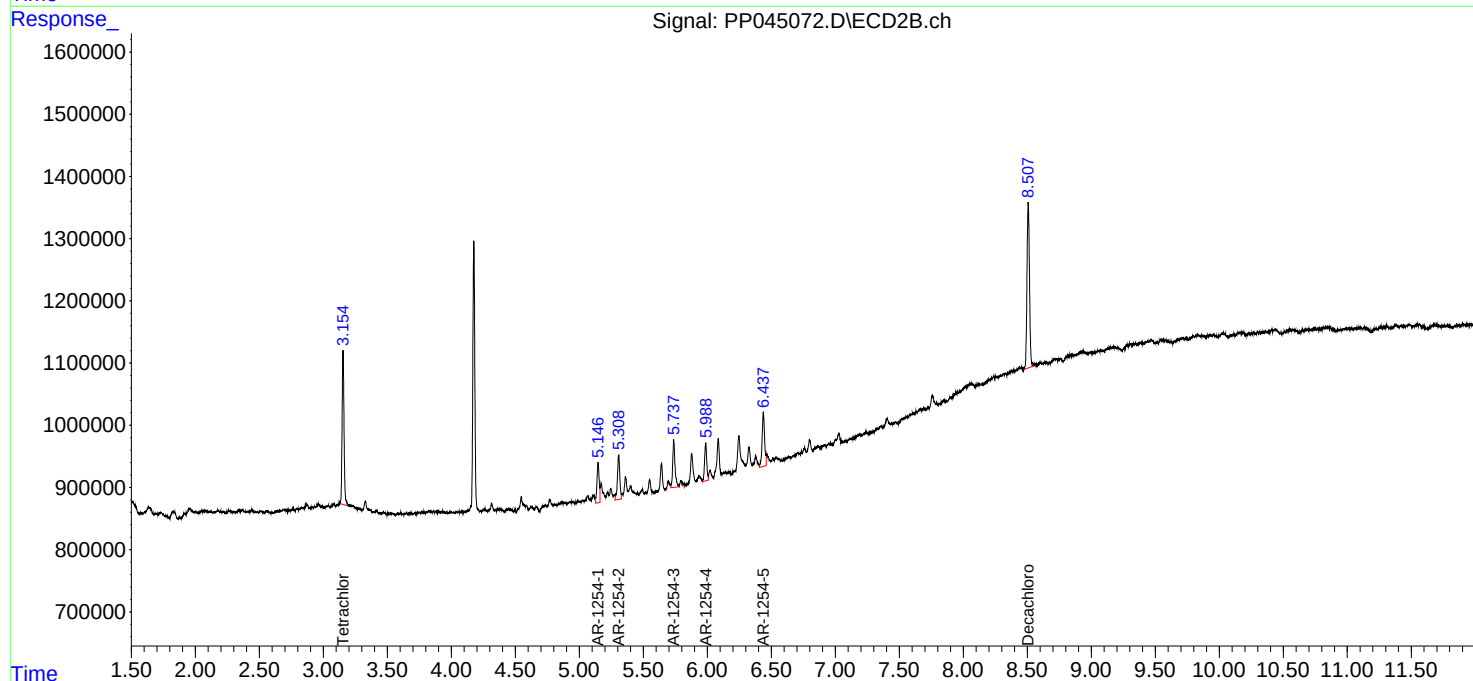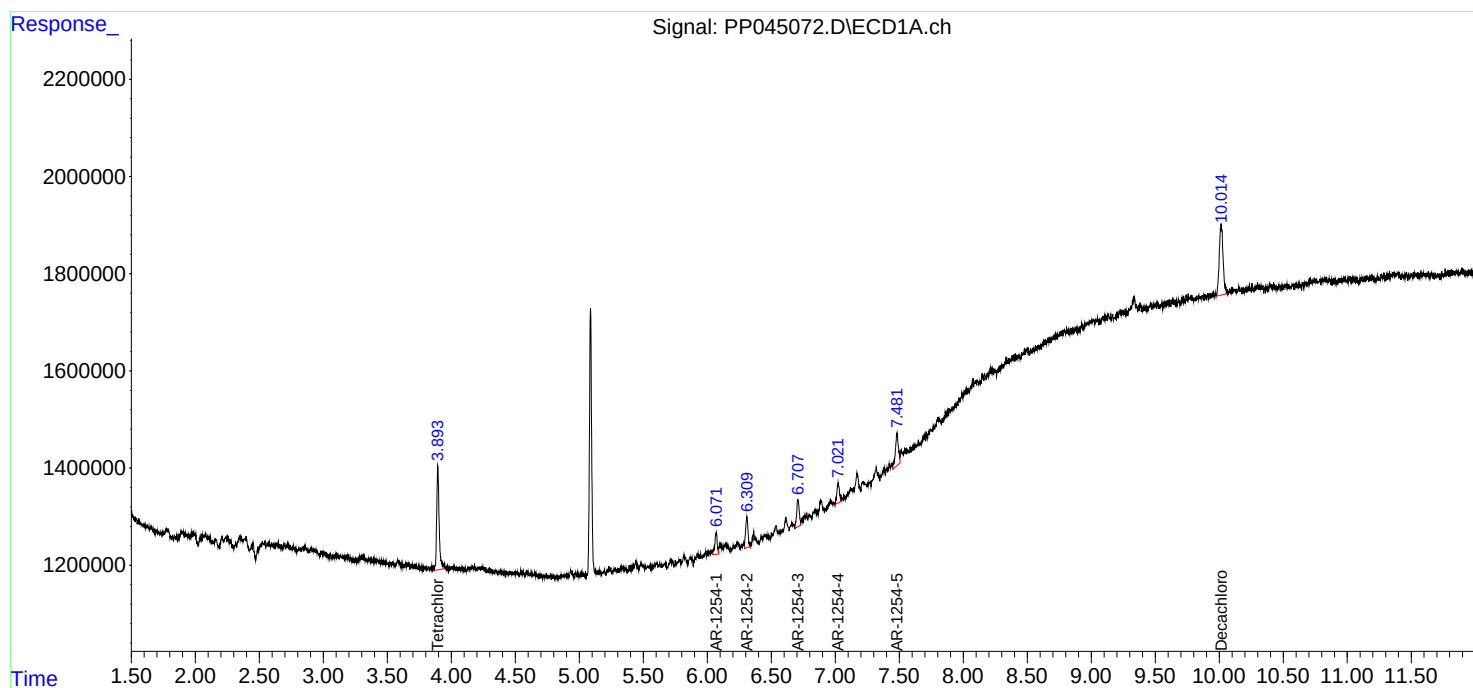

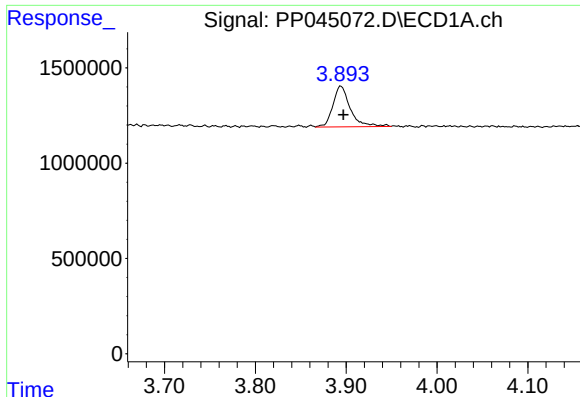


#1 Tetrachloro-m-xylene

R.T.: 3.893 min
Delta R.T.: -0.004 min
Response: 2834119
Conc: 1.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-37A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

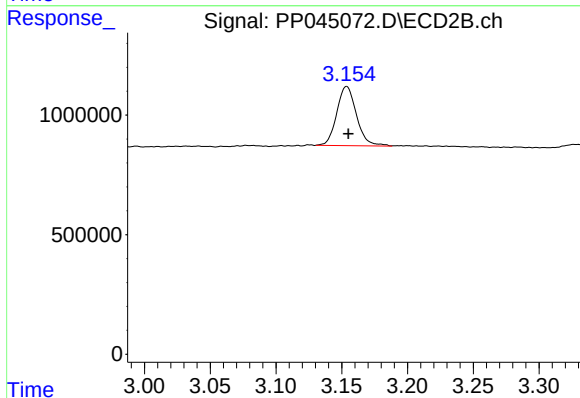


#1 Tetrachloro-m-xylene

R.T.: 3.154 min
Delta R.T.: -0.001 min
Response: 2581029
Conc: 1.96 ng/ml

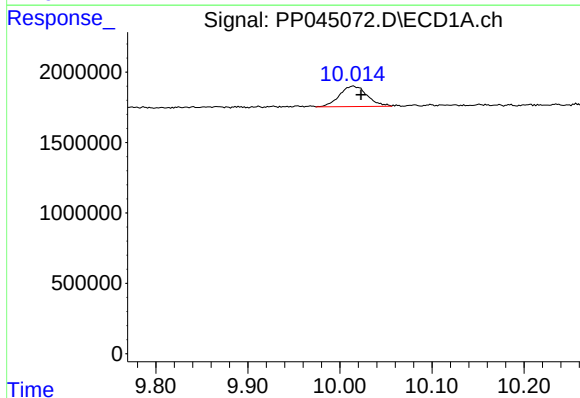


#2 Decachlorobiphenyl

R.T.: 10.014 min
Delta R.T.: -0.009 min
Response: 3014244
Conc: 2.34 ng/ml m

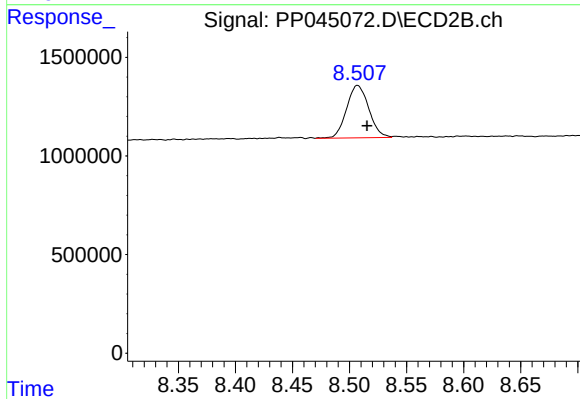

#2 Decachlorobiphenyl

R.T.: 8.507 min
Delta R.T.: -0.008 min
Response: 3590748
Conc: 2.76 ng/ml

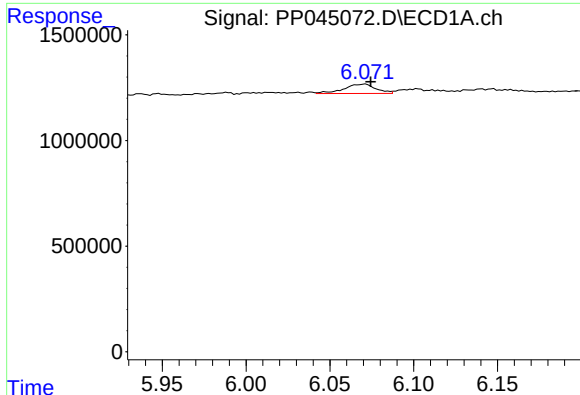


#26 AR-1254-1

R.T.: 6.071 min
Delta R.T.: -0.004 min
Response: 587098
Conc: 8.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-37A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

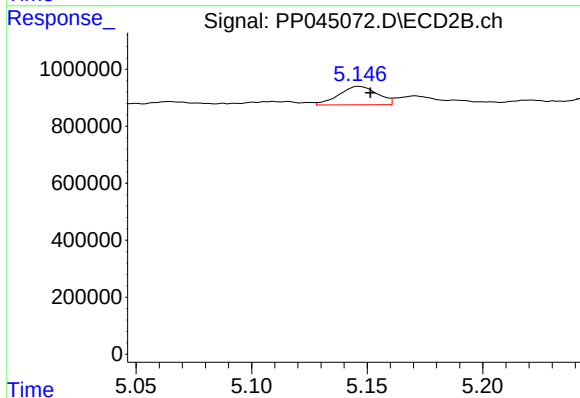


#26 AR-1254-1

R.T.: 5.146 min
Delta R.T.: -0.005 min
Response: 746980
Conc: 8.64 ng/ml

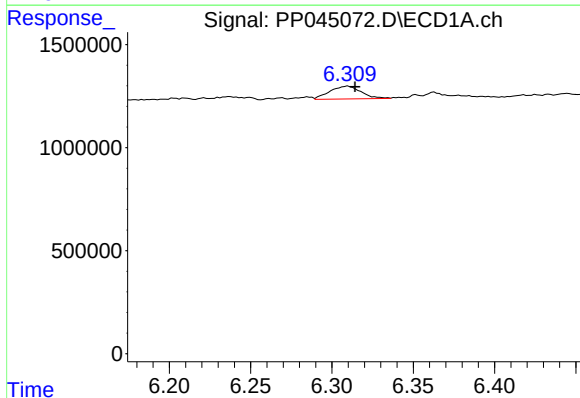


#27 AR-1254-2

R.T.: 6.310 min
Delta R.T.: -0.004 min
Response: 828686
Conc: 8.29 ng/ml

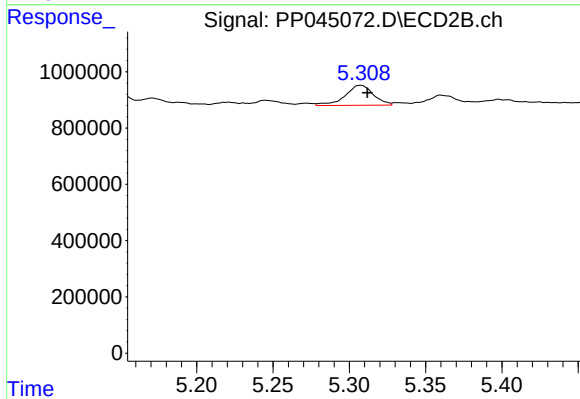

#27 AR-1254-2

R.T.: 5.308 min
Delta R.T.: -0.004 min
Response: 927491
Conc: 12.46 ng/ml

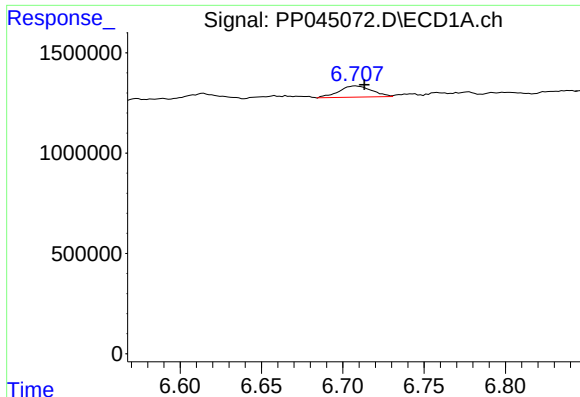


#28 AR-1254-3

R.T.: 6.708 min
Delta R.T.: -0.005 min
Response: 782707
Conc: 7.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-37A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

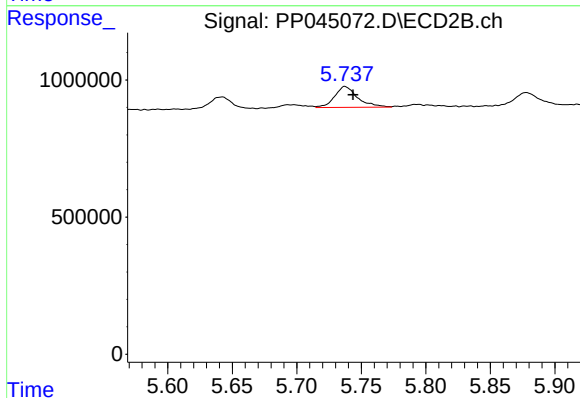


#28 AR-1254-3

R.T.: 5.737 min
Delta R.T.: -0.006 min
Response: 948306
Conc: 8.25 ng/ml

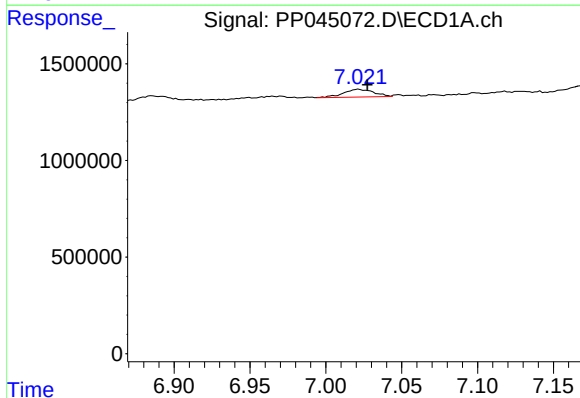


#29 AR-1254-4

R.T.: 7.022 min
Delta R.T.: -0.006 min
Response: 555529
Conc: 7.64 ng/ml

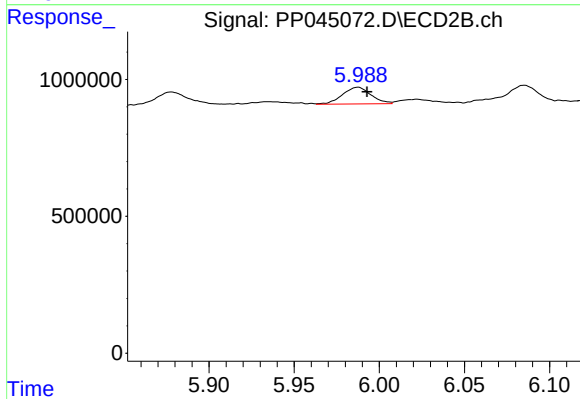

#29 AR-1254-4

R.T.: 5.988 min
Delta R.T.: -0.005 min
Response: 706619
Conc: 9.48 ng/ml

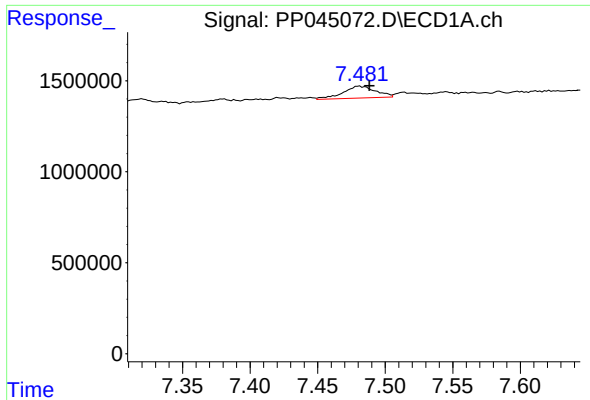


#30 AR-1254-5

R.T.: 7.481 min
Delta R.T.: -0.008 min
Response: 1106894
Conc: 14.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-37A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

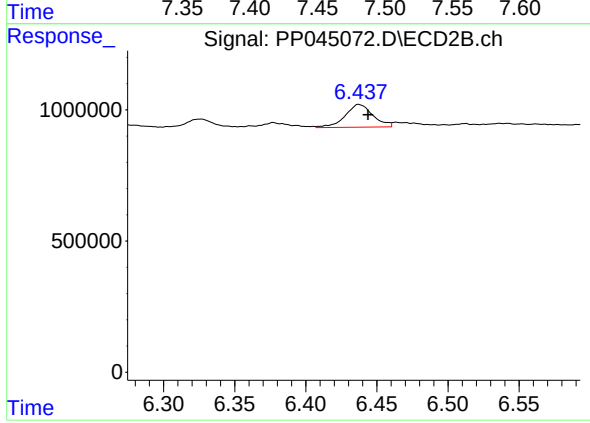

#30 AR-1254-5

R.T.: 6.437 min
Delta R.T.: -0.007 min
Response: 1180502
Conc: 11.46 ng/ml