

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032322\
 Data File : PP045073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 05:04
 Operator : YP\AJ
 Sample : N2055-14 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-36B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/24/2022
 Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 09:11:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.894	3.155	2838509	2812951	1.558m	2.135 #
2) SA Decachlor...	10.019	8.507	3349341	3782905	2.602	2.911
Target Compounds						
26) L6 AR-1254-1	6.068	5.147	769929	931551	11.595	10.772
27) L6 AR-1254-2	6.308	5.307	1081388	1052255	10.823	14.141 #
28) L6 AR-1254-3	6.708	5.738	1035464	1383321	10.124	12.039
29) L6 AR-1254-4	7.022	5.988	693427	905573	9.534	12.146 #
30) L6 AR-1254-5	7.483	6.438	1229095	1524457	15.891	14.805

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032322\
Data File : PP045073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 05:04
Operator : YP\AJ
Sample : N2055-14 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CLI-2022-36B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 09:11:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

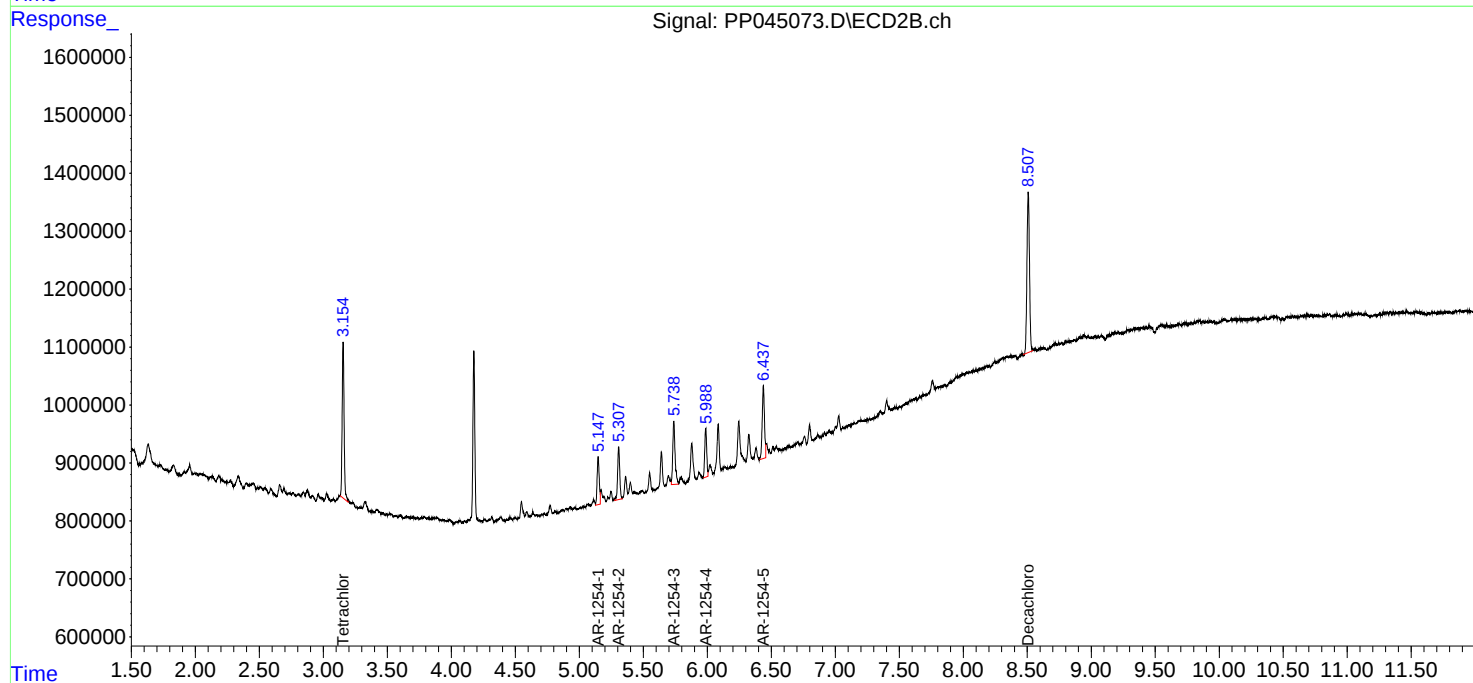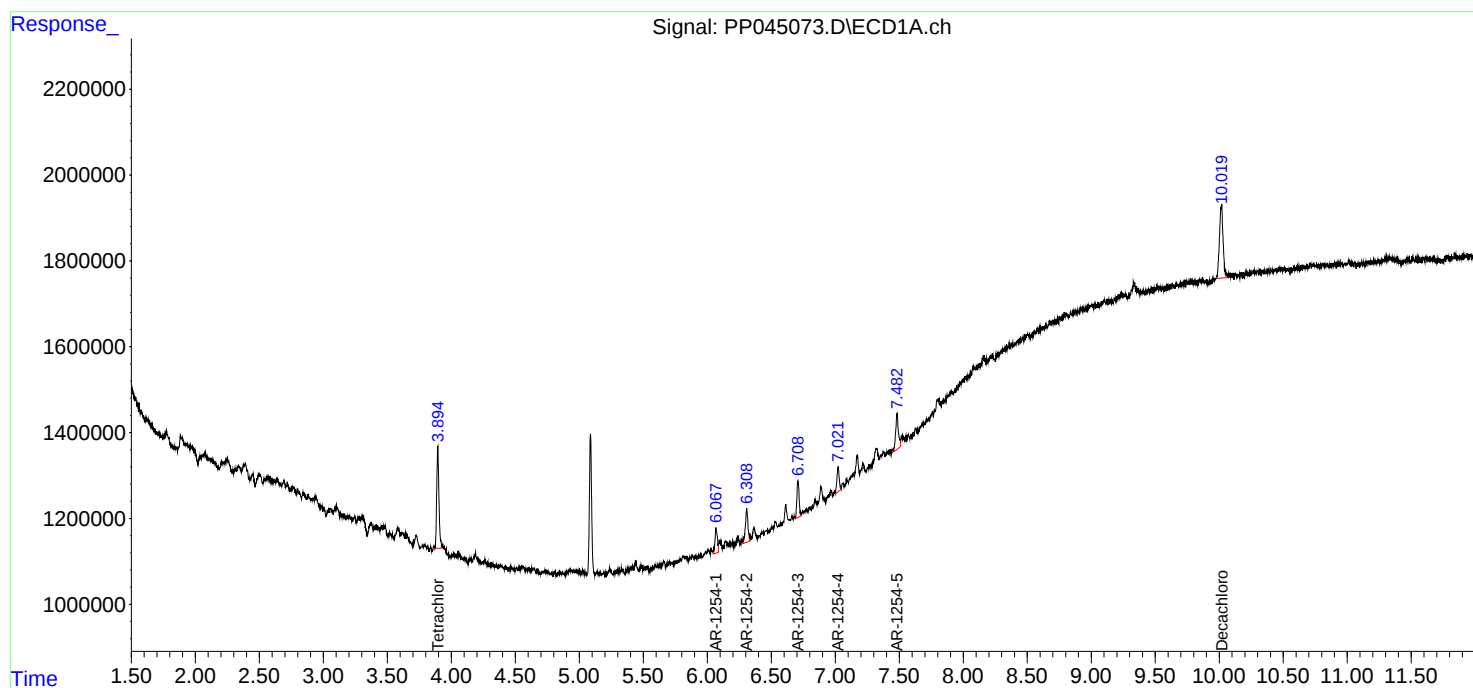

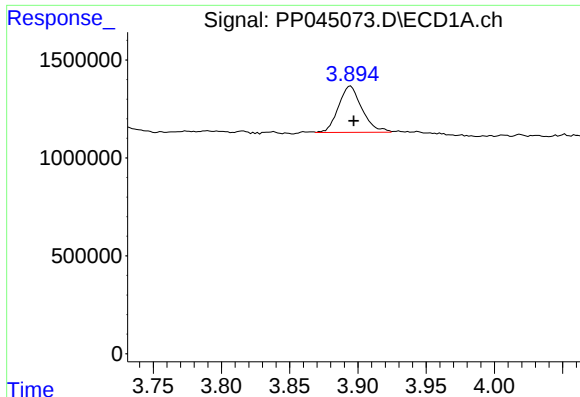


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: -0.003 min
Response: 2838509
Conc: 1.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-36B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

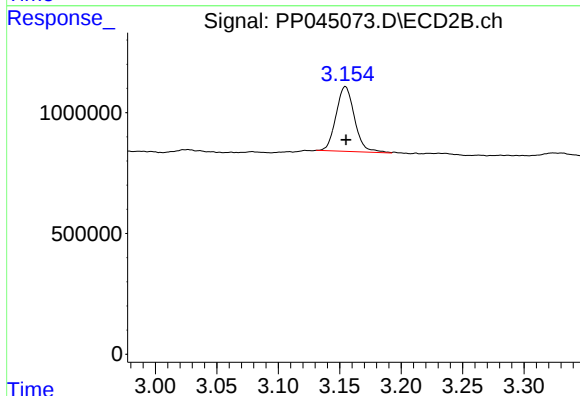


#1 Tetrachloro-m-xylene

R.T.: 3.155 min
Delta R.T.: 0.000 min
Response: 2812951
Conc: 2.13 ng/ml

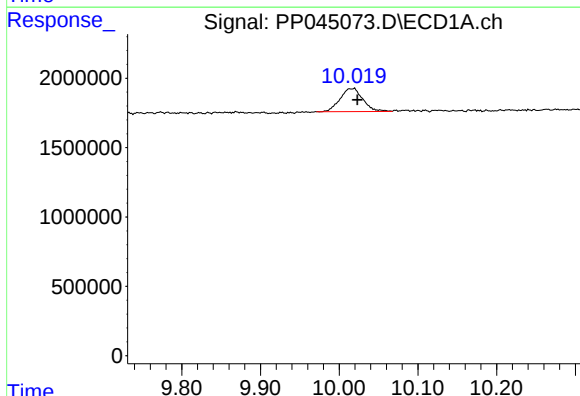


#2 Decachlorobiphenyl

R.T.: 10.019 min
Delta R.T.: -0.004 min
Response: 3349341
Conc: 2.60 ng/ml

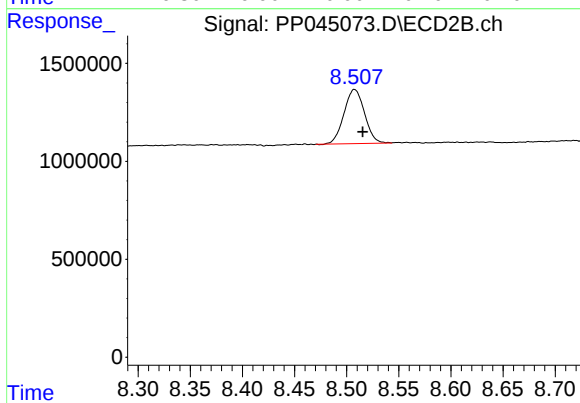

#2 Decachlorobiphenyl

R.T.: 8.507 min
Delta R.T.: -0.008 min
Response: 3782905
Conc: 2.91 ng/ml

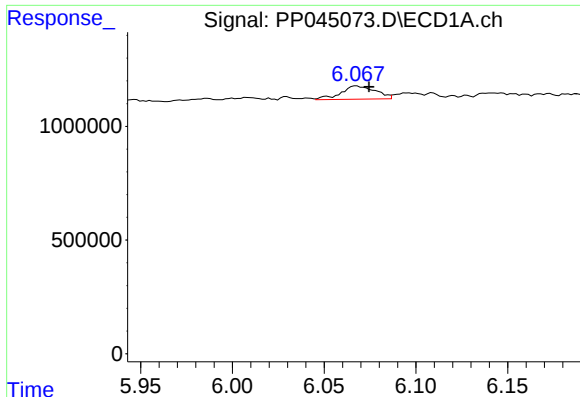


#26 AR-1254-1

R.T.: 6.068 min
Delta R.T.: -0.007 min
Response: 769929
Conc: 11.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-36B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

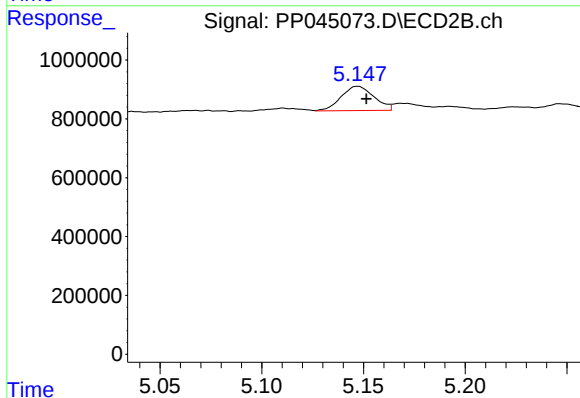


#26 AR-1254-1

R.T.: 5.147 min
Delta R.T.: -0.004 min
Response: 931551
Conc: 10.77 ng/ml

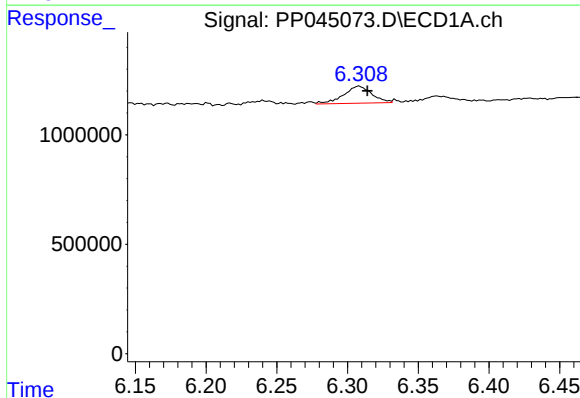


#27 AR-1254-2

R.T.: 6.308 min
Delta R.T.: -0.006 min
Response: 1081388
Conc: 10.82 ng/ml

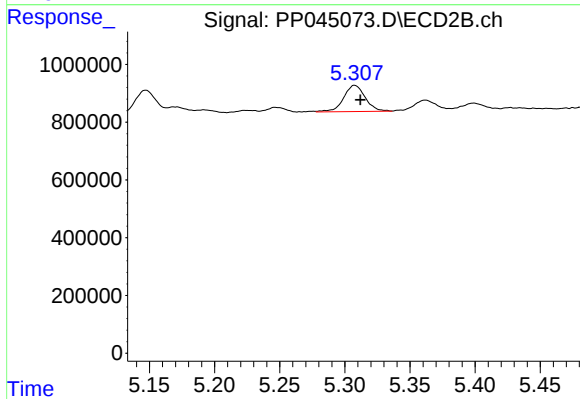

#27 AR-1254-2

R.T.: 5.307 min
Delta R.T.: -0.004 min
Response: 1052255
Conc: 14.14 ng/ml

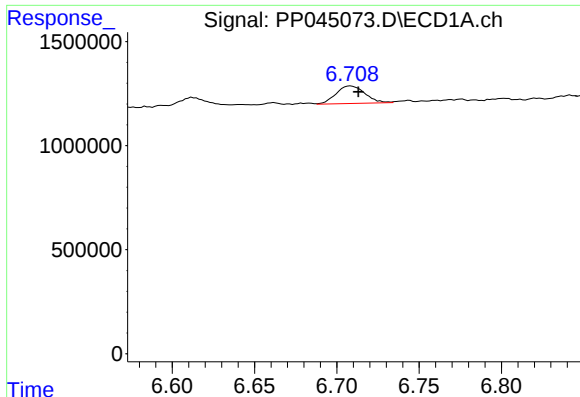


#28 AR-1254-3

R.T.: 6.708 min
Delta R.T.: -0.005 min
Response: 1035464
Conc: 10.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-36B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

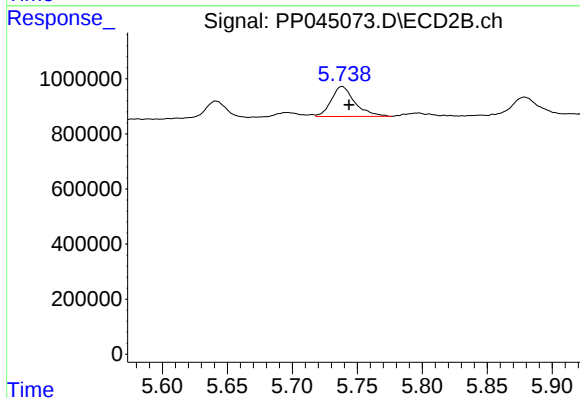


#28 AR-1254-3

R.T.: 5.738 min
Delta R.T.: -0.005 min
Response: 1383321
Conc: 12.04 ng/ml

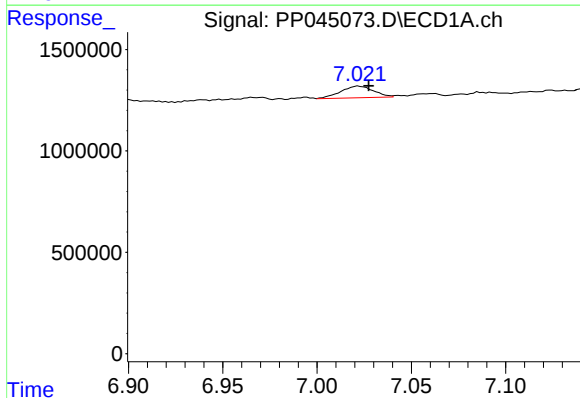


#29 AR-1254-4

R.T.: 7.022 min
Delta R.T.: -0.005 min
Response: 693427
Conc: 9.53 ng/ml

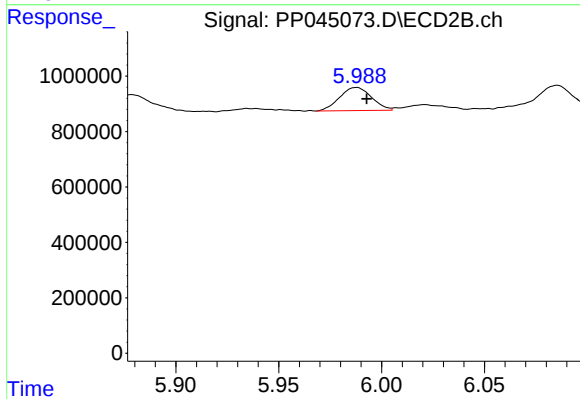

#29 AR-1254-4

R.T.: 5.988 min
Delta R.T.: -0.005 min
Response: 905573
Conc: 12.15 ng/ml

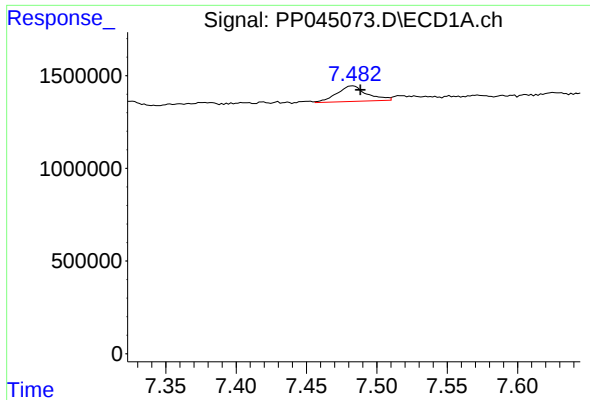


#30 AR-1254-5

R.T.: 7.483 min
Delta R.T.: -0.006 min
Response: 1229095
Conc: 15.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-36B

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

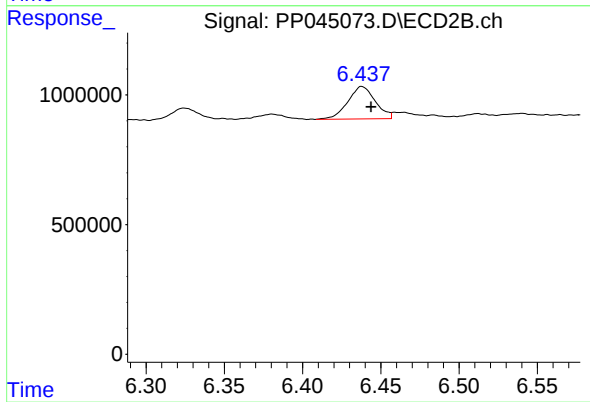

#30 AR-1254-5

R.T.: 6.438 min
Delta R.T.: -0.006 min
Response: 1524457
Conc: 14.80 ng/ml