

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032421\
 Data File : PP034325.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 13:40
 Operator : DD\AJ
 Sample : M1769-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SVE-03

Manual Integrations
 APPROVED

Ankita
 3/25/2021 9:08:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 13:55:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.849	4.263	1427615	827572	16.994m	18.701
2) SA Decachlor...	10.769	9.572	1838137	667438	23.423	25.292m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032421\
Data File : PP034325.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 13:40
Operator : DD\AJ
Sample : M1769-02
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
SVE-03


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 13:55:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

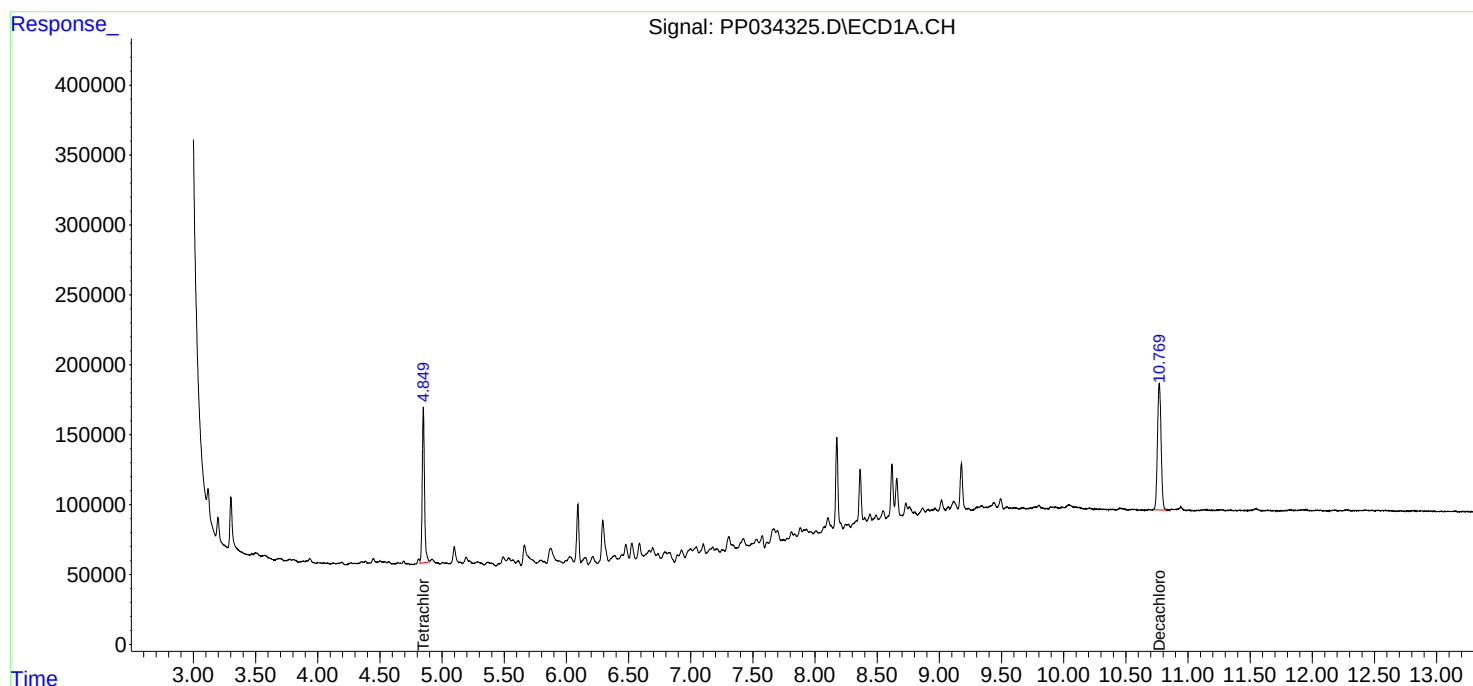

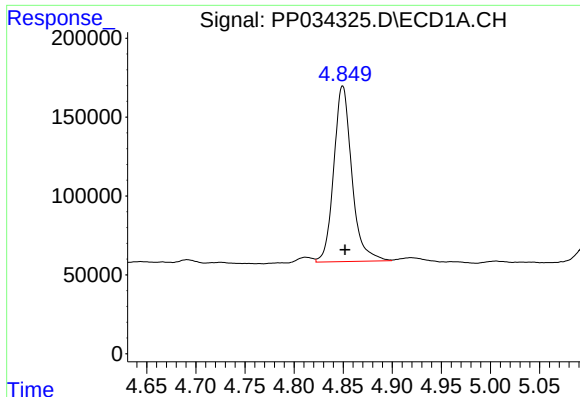


#1 Tetrachloro-m-xylene

R.T.: 4.849 min
Delta R.T.: -0.003 min
Response: 1427615
Conc: 16.99 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SVE-03


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:10 AM

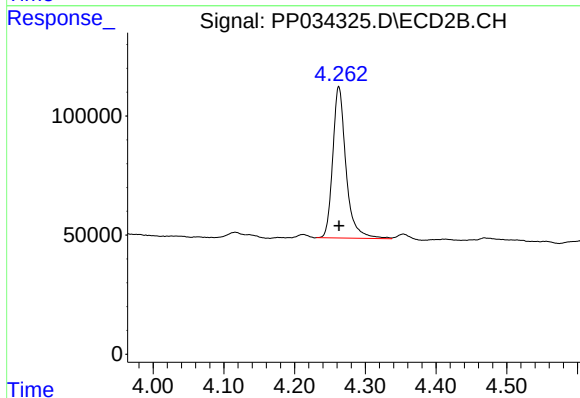


#1 Tetrachloro-m-xylene

R.T.: 4.263 min
Delta R.T.: 0.000 min
Response: 827572
Conc: 18.70 ng/ml

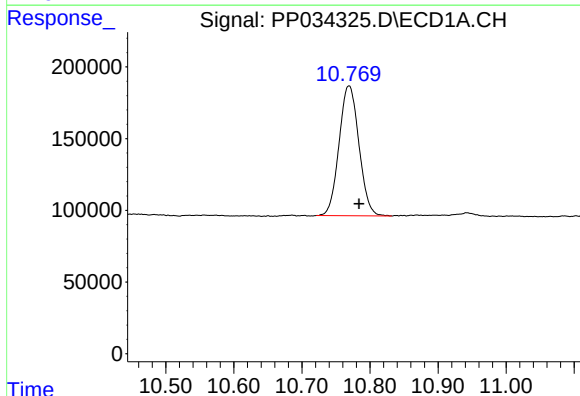

#2 Decachlorobiphenyl

R.T.: 10.769 min
Delta R.T.: -0.015 min
Response: 1838137
Conc: 23.42 ng/ml

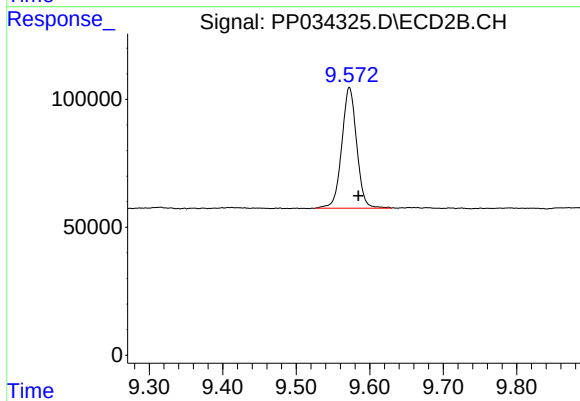

#2 Decachlorobiphenyl

R.T.: 9.572 min
Delta R.T.: -0.013 min
Response: 667438
Conc: 25.29 ng/ml m