

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032421\
 Data File : PP034327.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 14:14
 Operator : DD\AJ
 Sample : M1774-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 30808

Manual Integrations
 APPROVED

Ankita
 3/25/2021 9:08:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 16:24:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.850	4.263	1353962	731052	16.117	16.520
2) SA Decachlor...	10.769	9.573	1350634	462026	17.211m	17.508

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032421\
Data File : PP034327.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 14:14
Operator : DD\AJ
Sample : M1774-04
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
30808


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 16:24:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

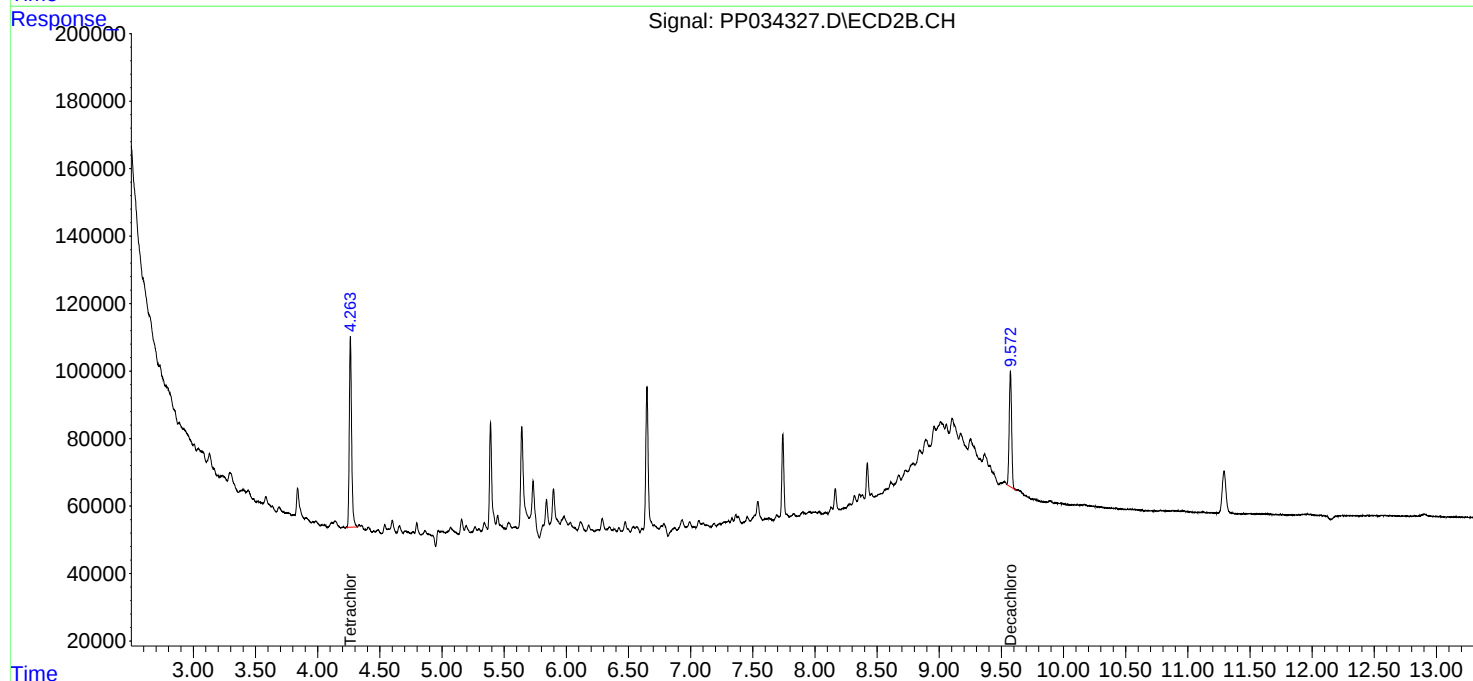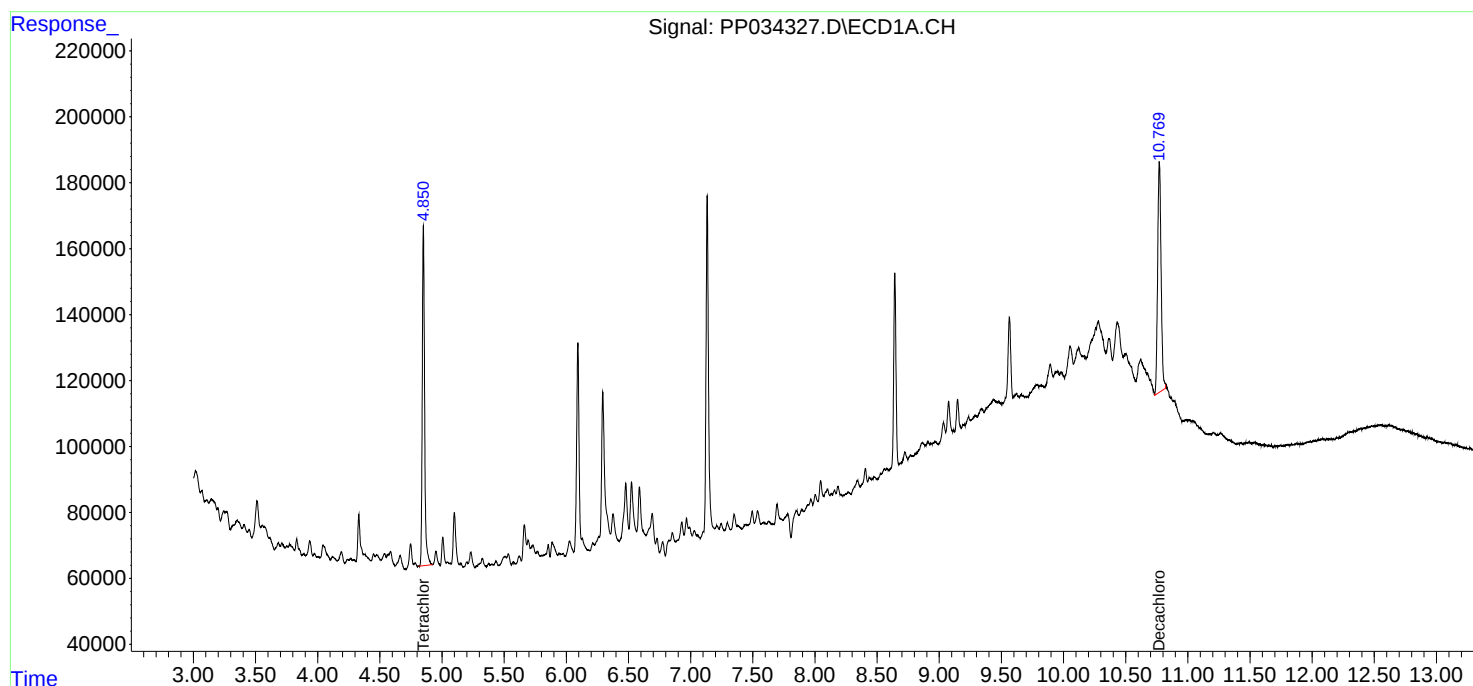

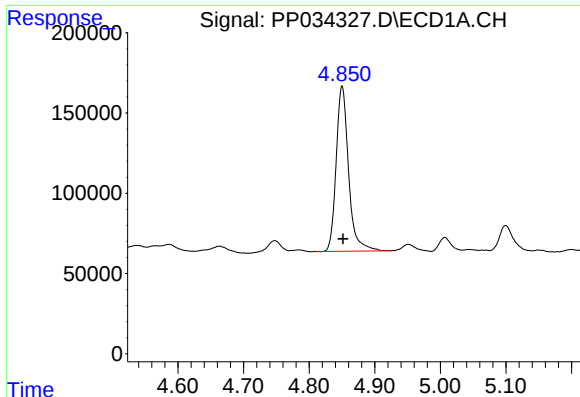


#1 Tetrachloro-m-xylene

R.T.: 4.850 min
Delta R.T.: -0.002 min
Response: 1353962
Conc: 16.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
30808


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:12 AM

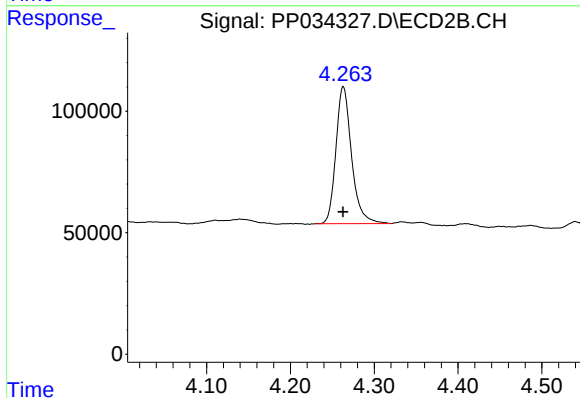


#1 Tetrachloro-m-xylene

R.T.: 4.263 min
Delta R.T.: 0.000 min
Response: 731052
Conc: 16.52 ng/ml

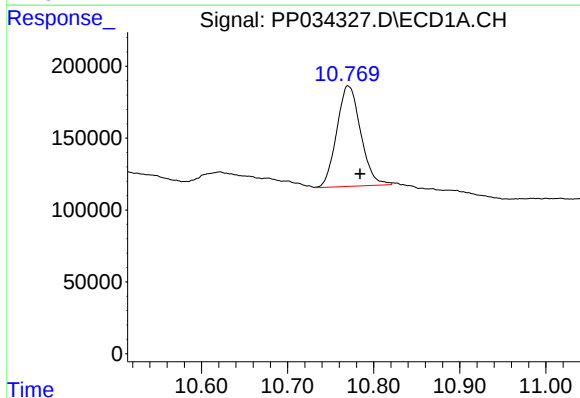

#2 Decachlorobiphenyl

R.T.: 10.769 min
Delta R.T.: -0.015 min
Response: 1350634
Conc: 17.21 ng/ml m

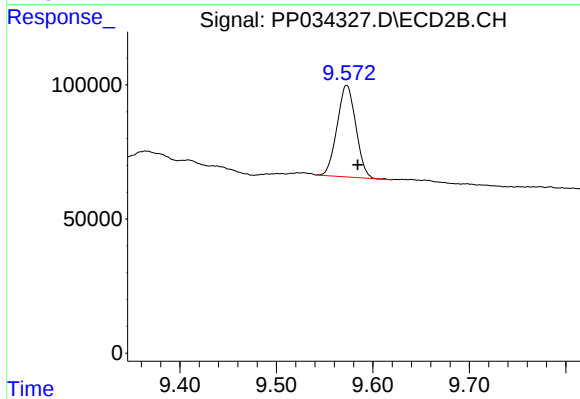

#2 Decachlorobiphenyl

R.T.: 9.573 min
Delta R.T.: -0.012 min
Response: 462026
Conc: 17.51 ng/ml