

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032421\
 Data File : PP034334.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 16:12
 Operator : DD\AJ
 Sample : M1786-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SP-1

Manual Integrations
 APPROVED

Ankita
 3/25/2021 9:08:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 16:28:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.260	1901235	1095341	22.632	24.752
2) SA Decachlor...	10.770	9.572	1864161	681673	23.754	25.832
Target Compounds						
31) L7 AR-1260-1	7.842	7.097	116190	63782	36.453	40.913
32) L7 AR-1260-2	8.106	7.290	208038	67604	55.359	37.782 #
33) L7 AR-1260-3	8.469	7.446	50941	54959	16.692	32.480 #
34) L7 AR-1260-4	8.693f	7.925	145513	30865	41.795m	21.678 #
35) L7 AR-1260-5	9.020	8.169	107643	52401	15.724	16.875m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032421\
Data File : PP034334.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 16:12
Operator : DD\AJ
Sample : M1786-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SP-1


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 16:28:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

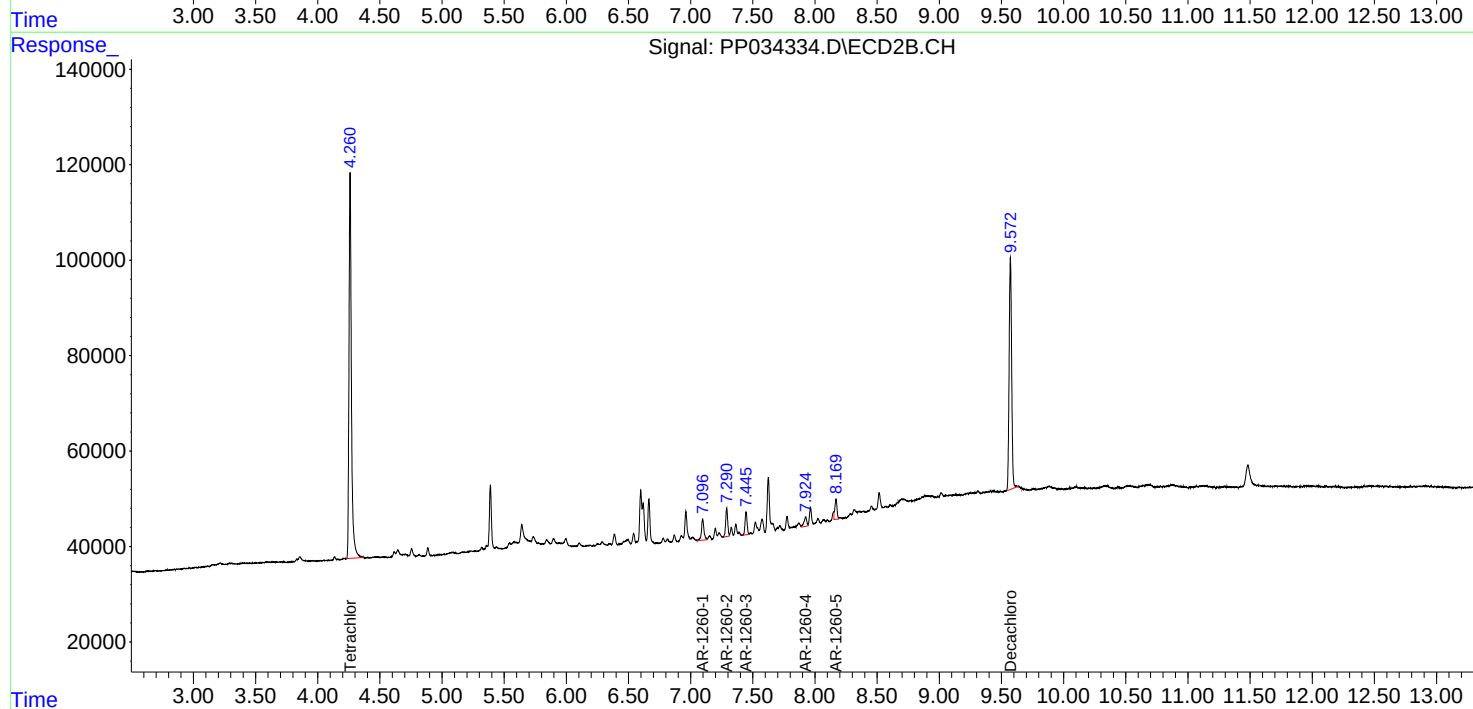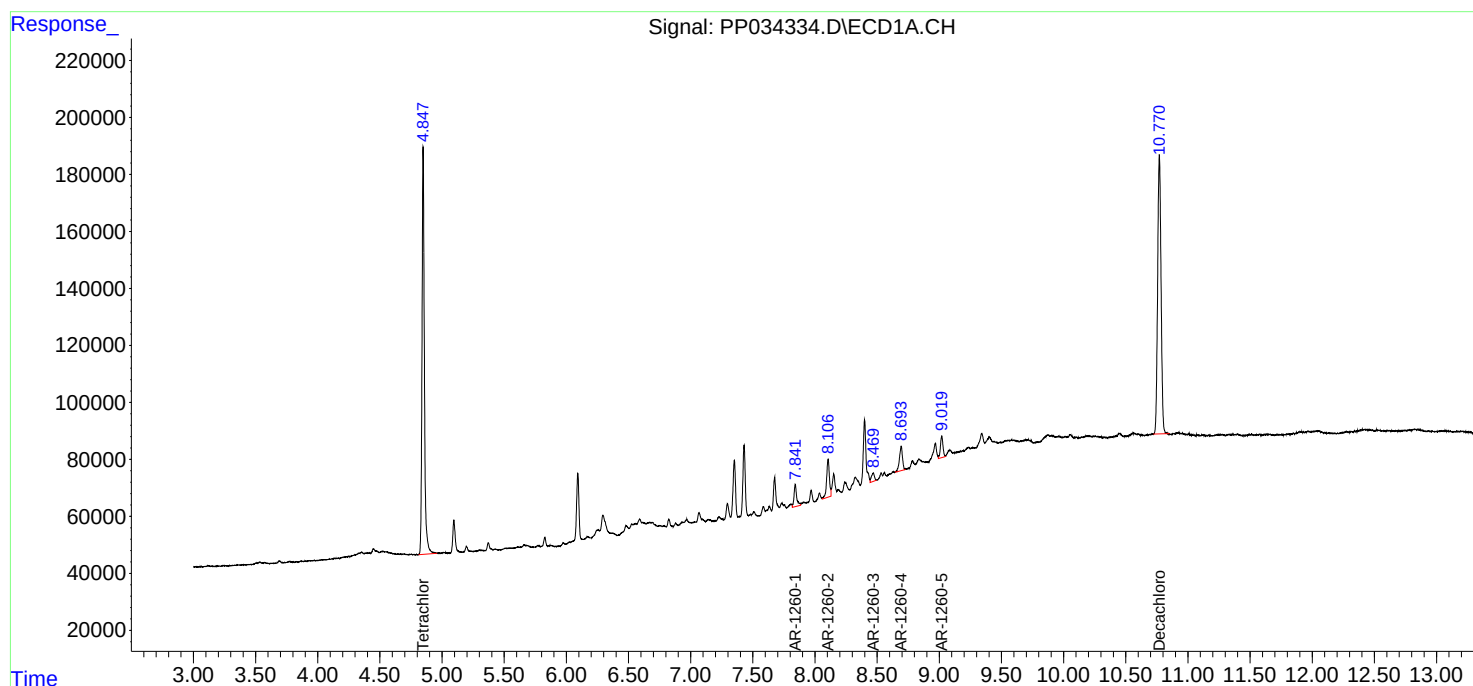

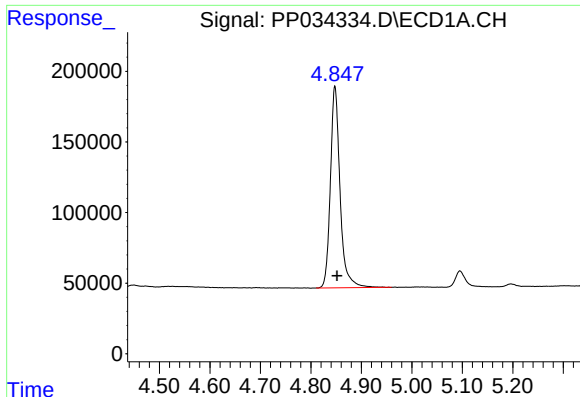


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 1901235
Conc: 22.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
SP-1


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:14 AM

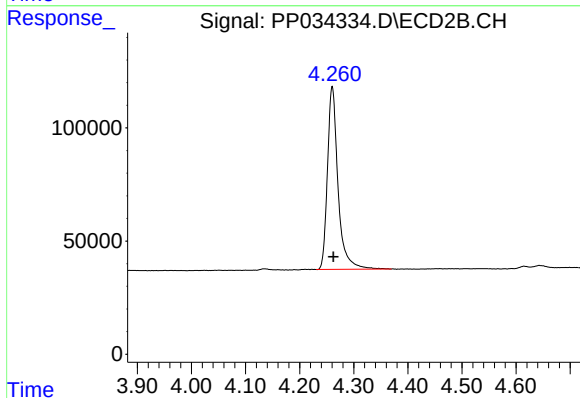


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.003 min
Response: 1095341
Conc: 24.75 ng/ml

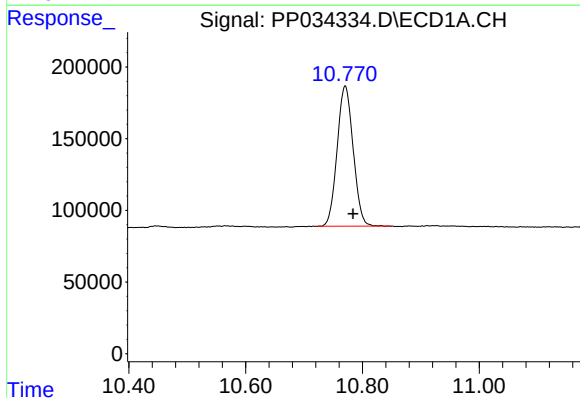


#2 Decachlorobiphenyl

R.T.: 10.770 min
Delta R.T.: -0.014 min
Response: 1864161
Conc: 23.75 ng/ml

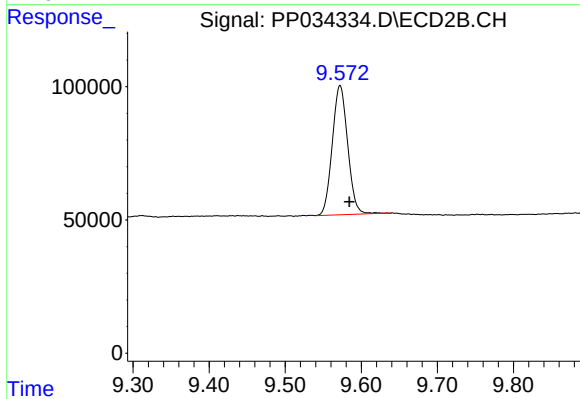

#2 Decachlorobiphenyl

R.T.: 9.572 min
Delta R.T.: -0.012 min
Response: 681673
Conc: 25.83 ng/ml

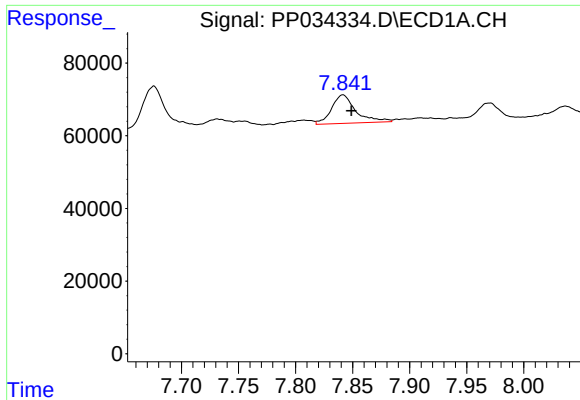


#31 AR-1260-1

R.T.: 7.842 min
Delta R.T.: -0.007 min
Response: 116190
Conc: 36.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
SP-1


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:14 AM

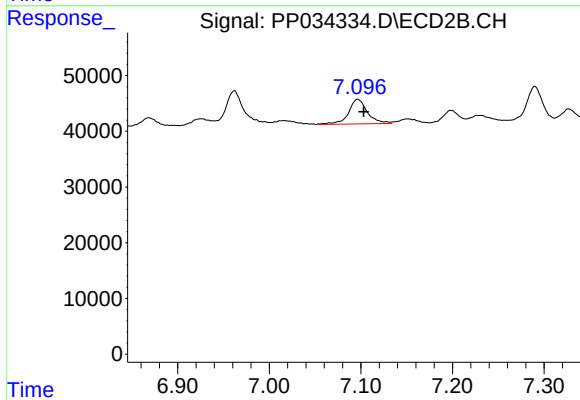


#31 AR-1260-1

R.T.: 7.097 min
Delta R.T.: -0.007 min
Response: 63782
Conc: 40.91 ng/ml

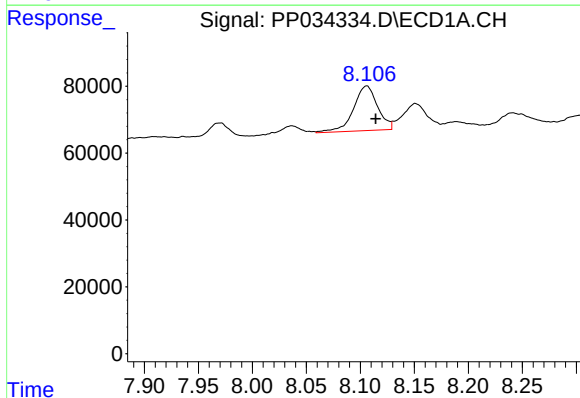


#32 AR-1260-2

R.T.: 8.106 min
Delta R.T.: -0.008 min
Response: 208038
Conc: 55.36 ng/ml

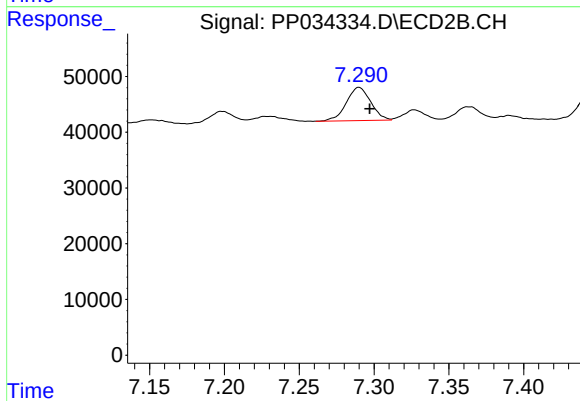

#32 AR-1260-2

R.T.: 7.290 min
Delta R.T.: -0.007 min
Response: 67604
Conc: 37.78 ng/ml

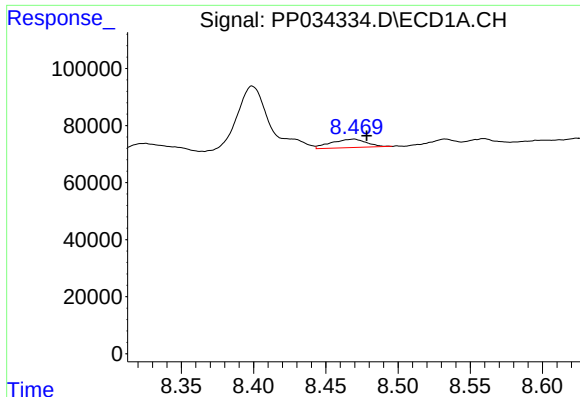


#33 AR-1260-3

R.T.: 8.469 min
Delta R.T.: -0.009 min
Response: 50941
Conc: 16.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
SP-1


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:14 AM

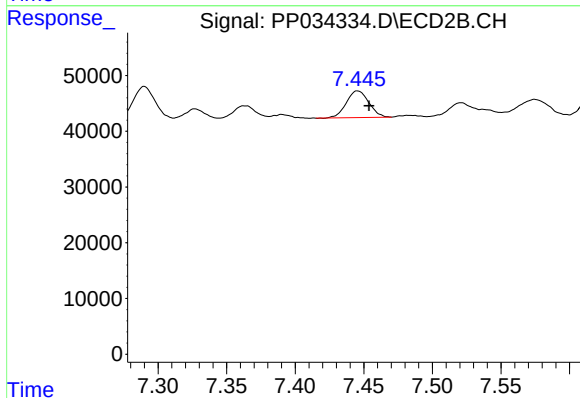


#33 AR-1260-3

R.T.: 7.446 min
Delta R.T.: -0.008 min
Response: 54959
Conc: 32.48 ng/ml

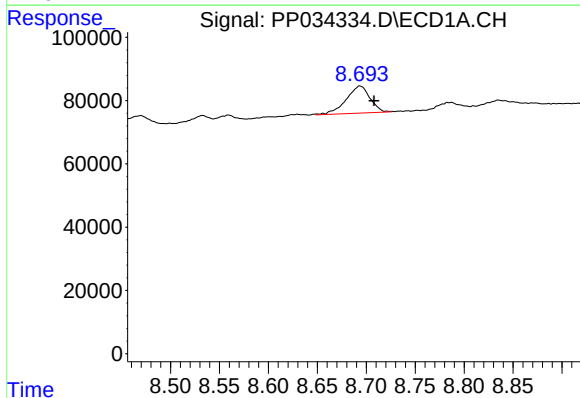


#34 AR-1260-4

R.T.: 8.693 min
Delta R.T.: -0.015 min
Response: 145513
Conc: 41.80 ng/ml m

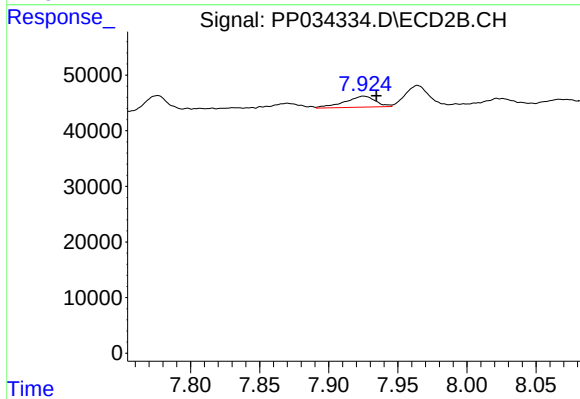

#34 AR-1260-4

R.T.: 7.925 min
Delta R.T.: -0.009 min
Response: 30865
Conc: 21.68 ng/ml

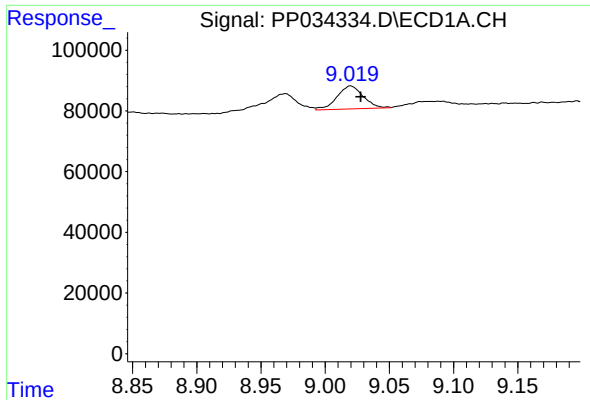


#35 AR-1260-5

R.T.: 9.020 min
Delta R.T.: -0.008 min
Response: 107643
Conc: 15.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
SP-1

Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:14 AM

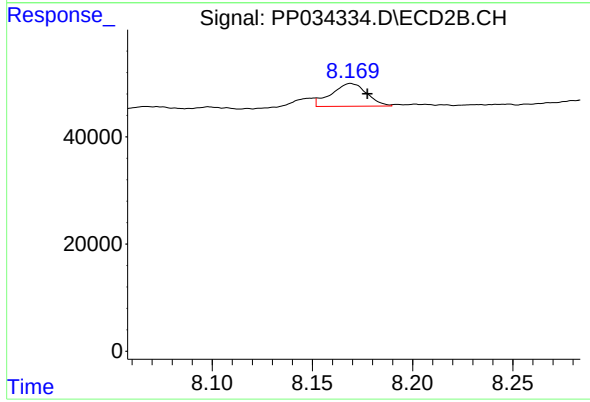

#35 AR-1260-5

R.T.: 8.169 min
Delta R.T.: -0.009 min
Response: 52401
Conc: 16.88 ng/ml m