

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032421\
 Data File : PP034337.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 17:03
 Operator : DD\AJ
 Sample : M1730-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-8A

Manual Integrations
 APPROVED

Ankita
 3/25/2021 9:08:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 01:38:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.260	1656782	940266	19.722	21.248
2) SA Decachlor...	10.771	9.572	1818975	674295	23.178	25.552
Target Compounds						
26) L6 AR-1254-1	7.068	6.387	127377	78360	46.539	46.729
27) L6 AR-1254-2	7.298	6.541	304952	52865	73.235	36.454 #
28) L6 AR-1254-3	7.687	6.962	475758	57374	109.541	25.053m#
29) L6 AR-1254-4	7.970	7.197	133976	49049	46.148	41.019
30) L6 AR-1254-5	8.397	7.624	260615	317371	78.069	171.881 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032421\
Data File : PP034337.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 17:03
Operator : DD\AJ
Sample : M1730-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TP-8A


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 01:38:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

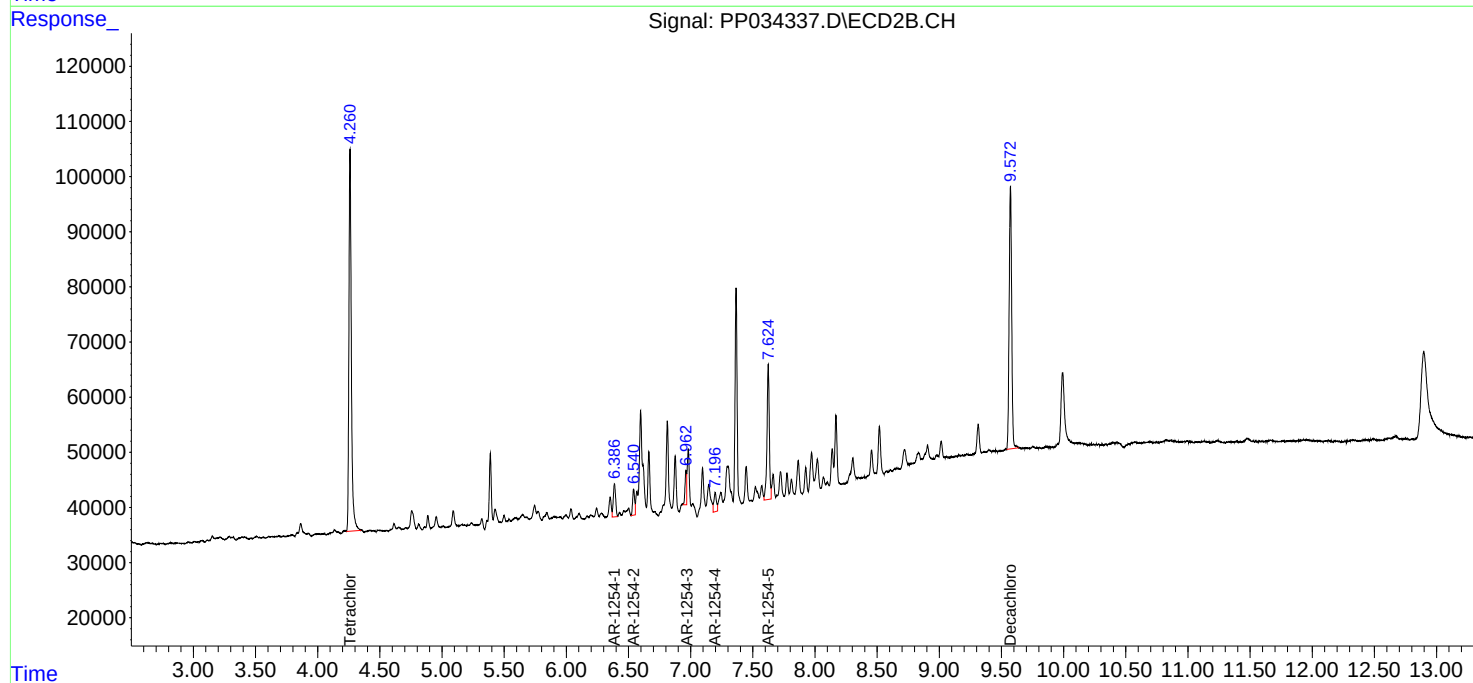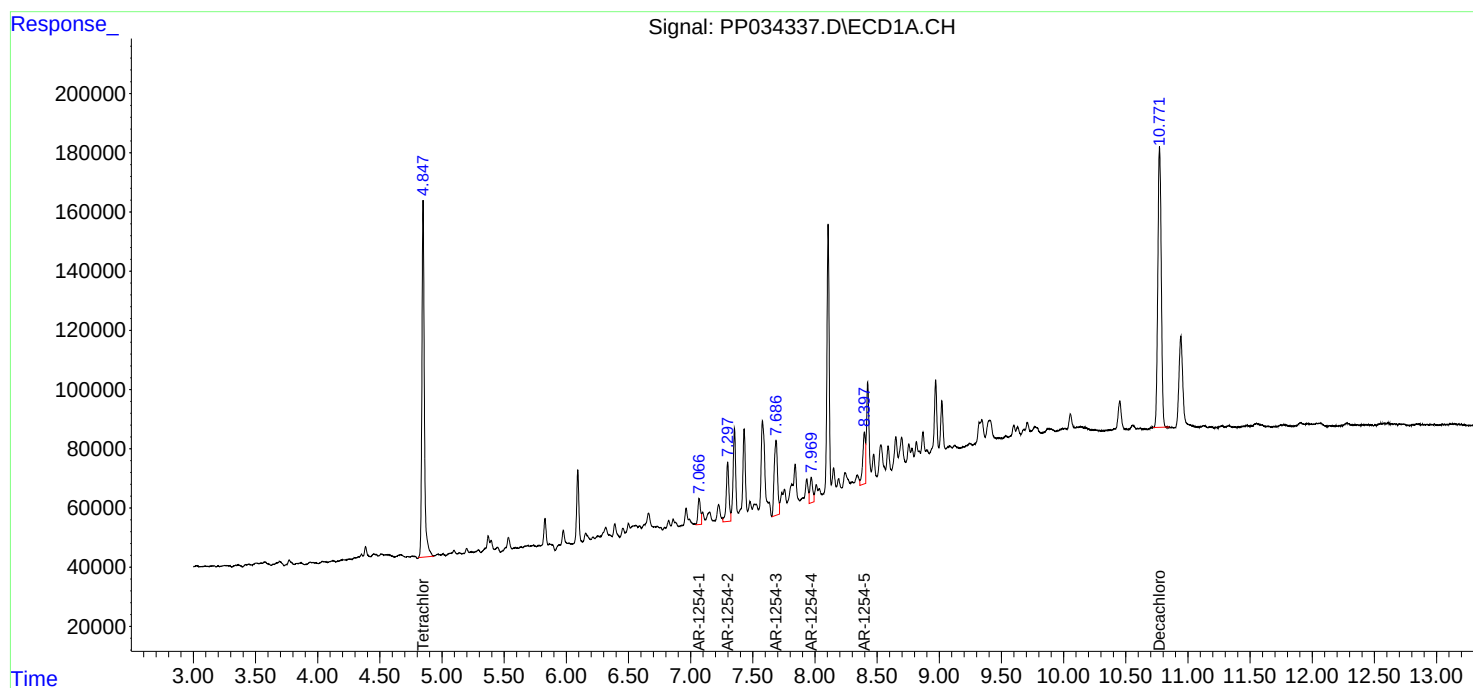

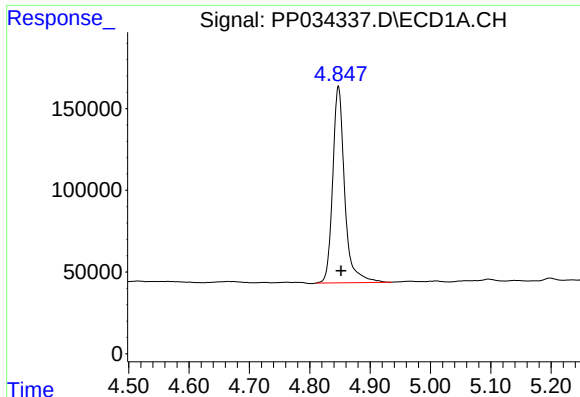


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.005 min
Response: 1656782
Conc: 19.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-8A


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:17 AM

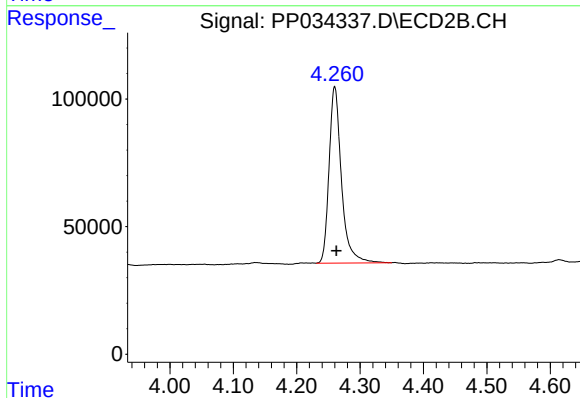


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.003 min
Response: 940266
Conc: 21.25 ng/ml

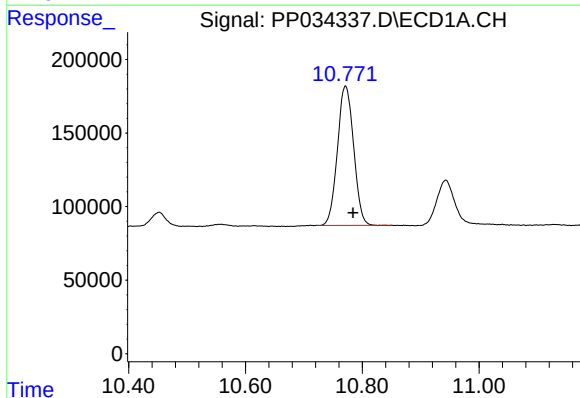


#2 Decachlorobiphenyl

R.T.: 10.771 min
Delta R.T.: -0.013 min
Response: 1818975
Conc: 23.18 ng/ml

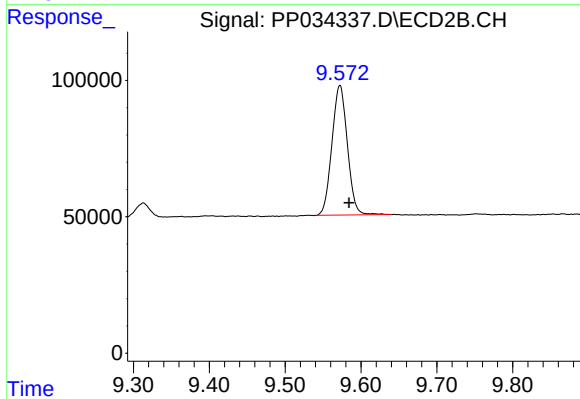

#2 Decachlorobiphenyl

R.T.: 9.572 min
Delta R.T.: -0.012 min
Response: 674295
Conc: 25.55 ng/ml

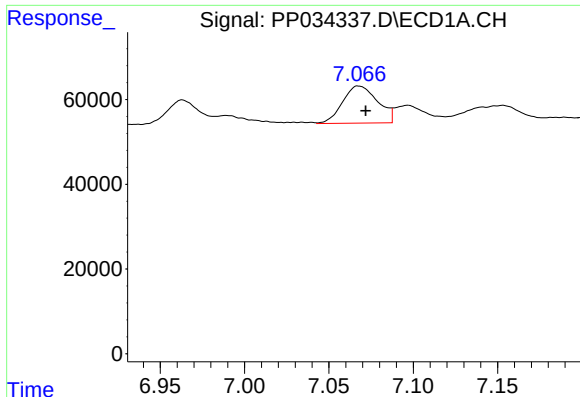


#26 AR-1254-1

R.T.: 7.068 min
Delta R.T.: -0.004 min
Response: 127377
Conc: 46.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-8A


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:17 AM

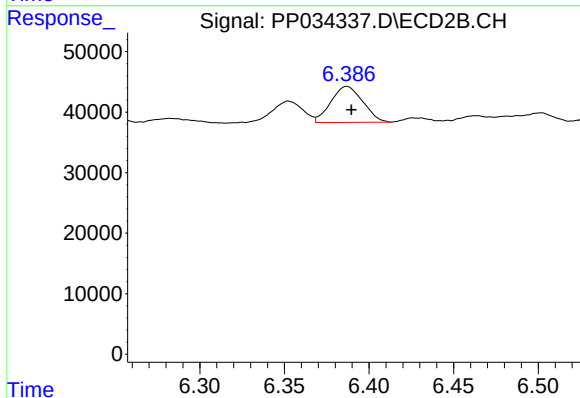


#26 AR-1254-1

R.T.: 6.387 min
Delta R.T.: -0.003 min
Response: 78360
Conc: 46.73 ng/ml

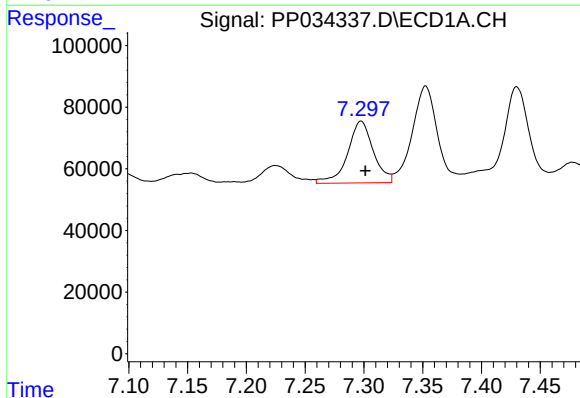


#27 AR-1254-2

R.T.: 7.298 min
Delta R.T.: -0.004 min
Response: 304952
Conc: 73.23 ng/ml

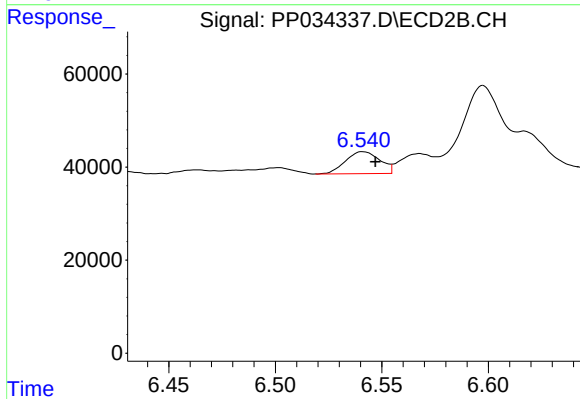

#27 AR-1254-2

R.T.: 6.541 min
Delta R.T.: -0.006 min
Response: 52865
Conc: 36.45 ng/ml

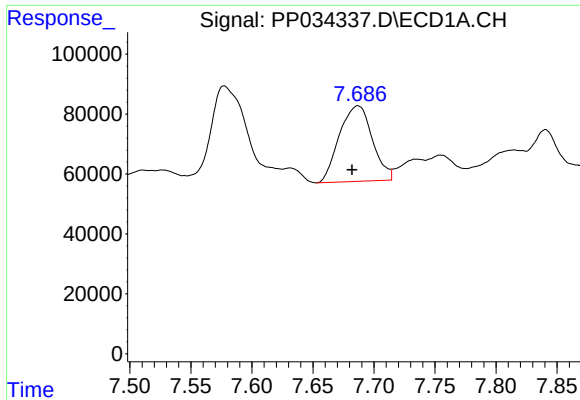


#28 AR-1254-3

R.T.: 7.687 min
Delta R.T.: 0.005 min
Response: 475758
Conc: 109.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-8A


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:17 AM

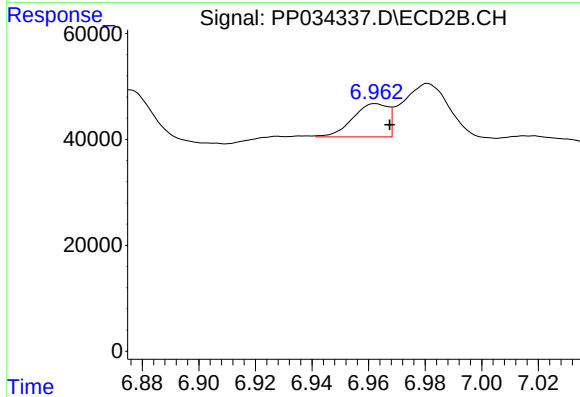


#28 AR-1254-3

R.T.: 6.962 min
Delta R.T.: -0.006 min
Response: 57374
Conc: 25.05 ng/ml m

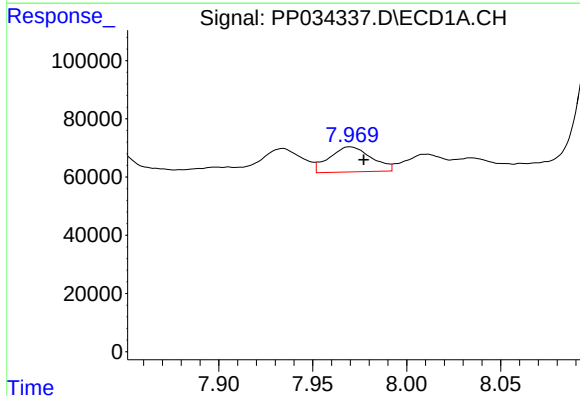


#29 AR-1254-4

R.T.: 7.970 min
Delta R.T.: -0.007 min
Response: 133976
Conc: 46.15 ng/ml

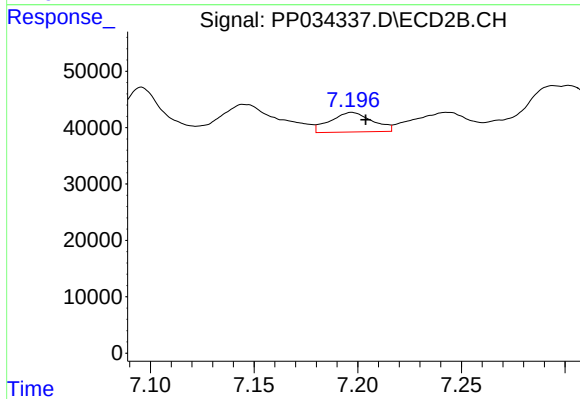

#29 AR-1254-4

R.T.: 7.197 min
Delta R.T.: -0.007 min
Response: 49049
Conc: 41.02 ng/ml

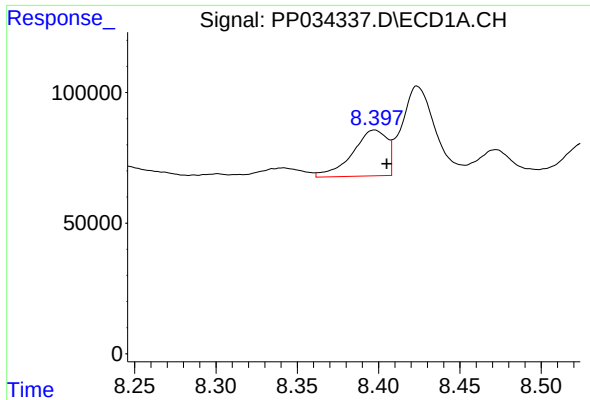


#30 AR-1254-5

R.T.: 8.397 min
Delta R.T.: -0.008 min
Response: 260615
Conc: 78.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-8A

Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:17 AM

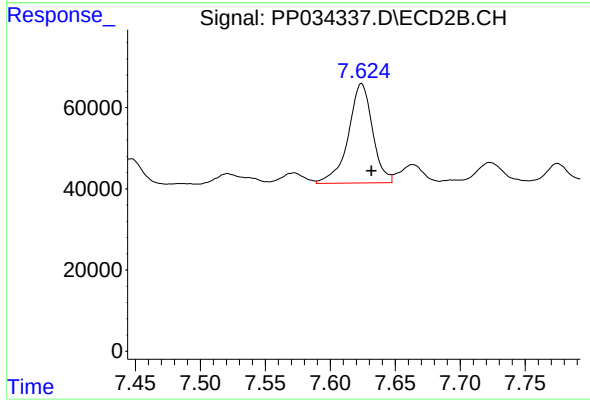

#30 AR-1254-5

R.T.: 7.624 min
Delta R.T.: -0.008 min
Response: 317371
Conc: 171.88 ng/ml