

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032421\
 Data File : PP034343.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Mar 2021 19:02
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 3/25/2021 9:08:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 01:40:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.849	4.260	3752280	2125109	44.667	48.022
2) SA Decachlor...	10.771	9.572	3828295	1404674	48.782	53.229
Target Compounds						
21) L5 AR-1248-1	6.161	5.515	689992	351142	461.493	510.461
22) L5 AR-1248-2	6.455	5.777	955847	484820	455.504	485.504
23) L5 AR-1248-3	6.670	5.822	1142053	518183	448.451	491.369
24) L5 AR-1248-4	7.097	6.008	1200335	519380	464.578m	423.230
25) L5 AR-1248-5	7.136	6.428	1172885	550656	451.966m	545.391

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032421\
Data File : PP034343.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Mar 2021 19:02
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 01:40:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

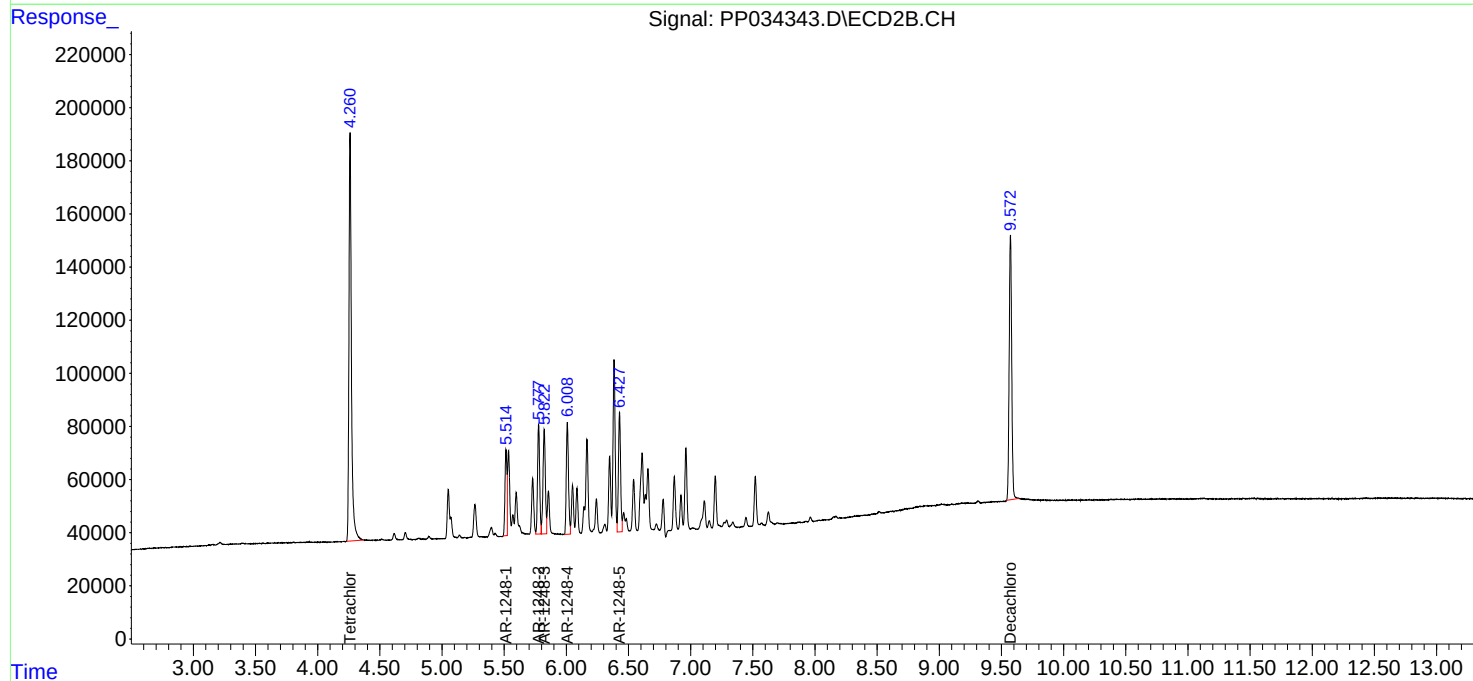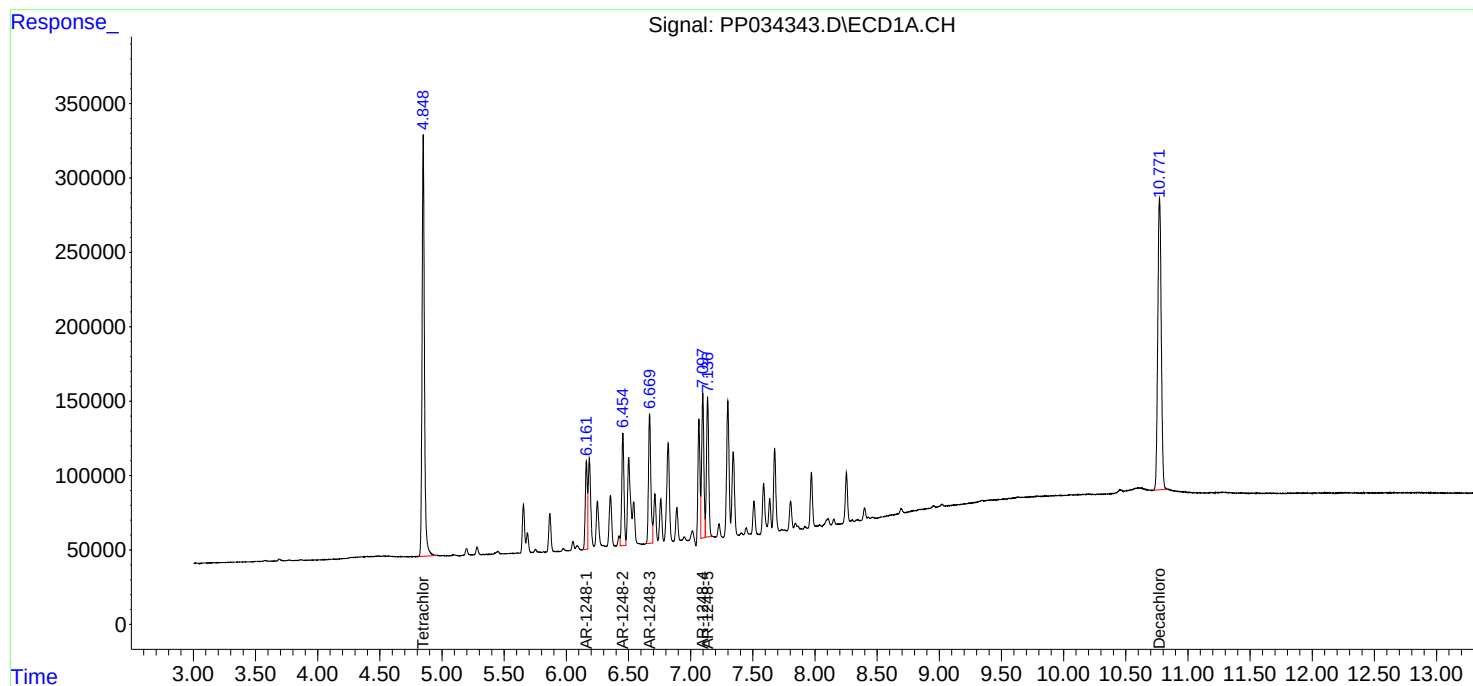

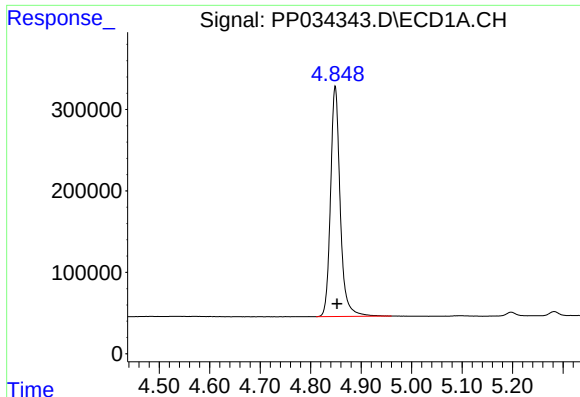


#1 Tetrachloro-m-xylene

R.T.: 4.849 min
Delta R.T.: -0.003 min
Response: 3752280
Conc: 44.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:19 AM

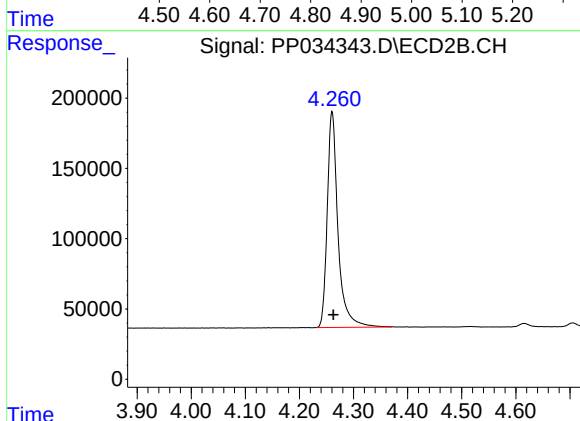


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.002 min
Response: 2125109
Conc: 48.02 ng/ml

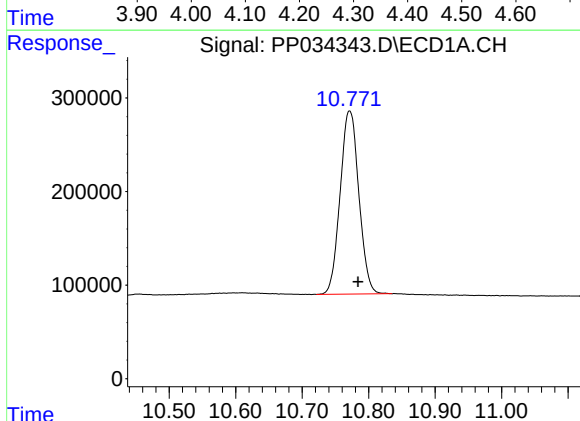


#2 Decachlorobiphenyl

R.T.: 10.771 min
Delta R.T.: -0.013 min
Response: 3828295
Conc: 48.78 ng/ml

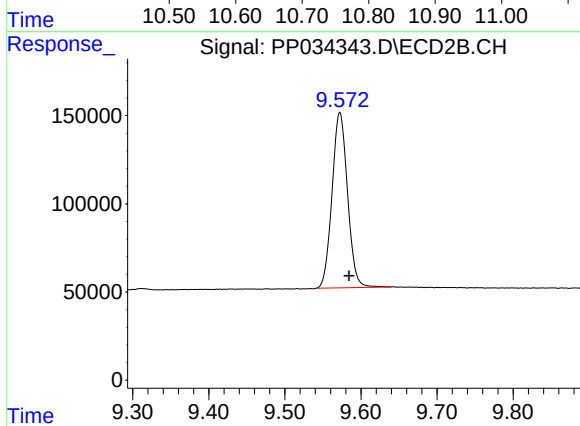

#2 Decachlorobiphenyl

R.T.: 9.572 min
Delta R.T.: -0.012 min
Response: 1404674
Conc: 53.23 ng/ml

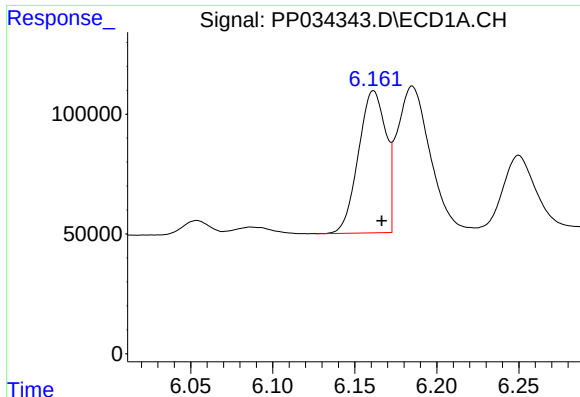


#21 AR-1248-1

R.T.: 6.161 min
Delta R.T.: -0.005 min
Response: 689992
Conc: 461.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:19 AM

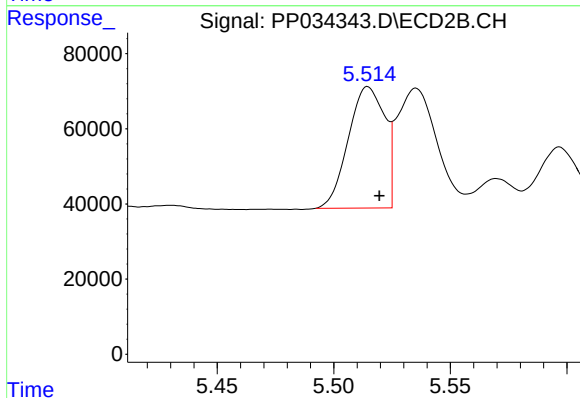


#21 AR-1248-1

R.T.: 5.515 min
Delta R.T.: -0.005 min
Response: 351142
Conc: 510.46 ng/ml

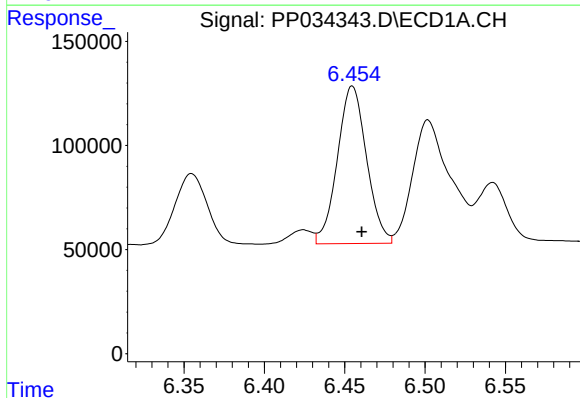


#22 AR-1248-2

R.T.: 6.455 min
Delta R.T.: -0.006 min
Response: 955847
Conc: 455.50 ng/ml

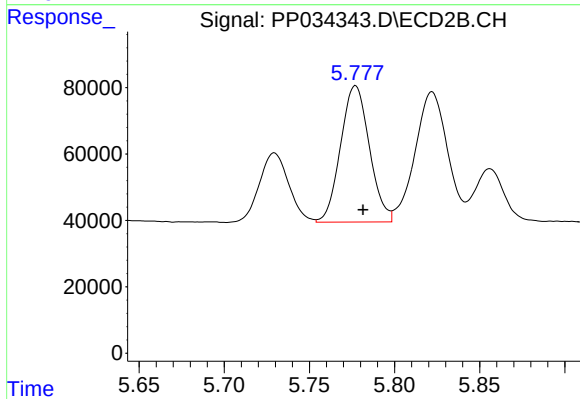

#22 AR-1248-2

R.T.: 5.777 min
Delta R.T.: -0.004 min
Response: 484820
Conc: 485.50 ng/ml

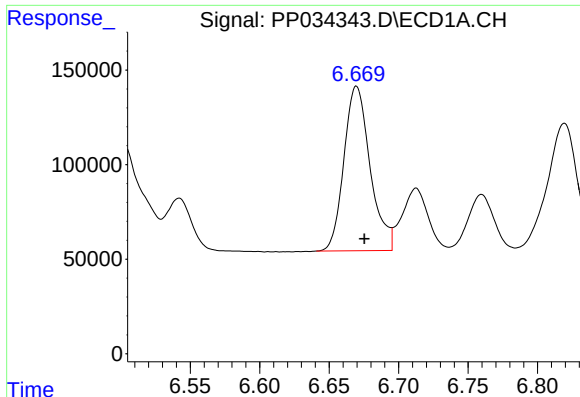


#23 AR-1248-3

R.T.: 6.670 min
Delta R.T.: -0.006 min
Response: 1142053
Conc: 448.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:19 AM

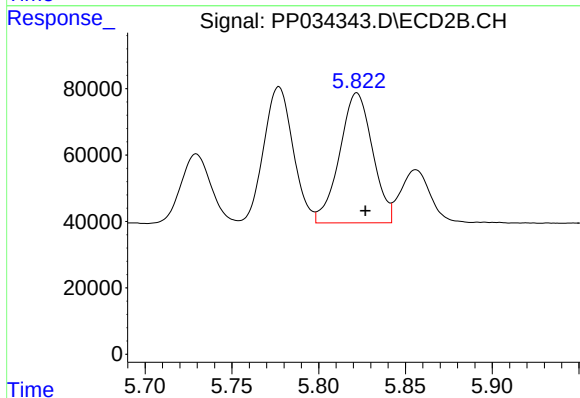


#23 AR-1248-3

R.T.: 5.822 min
Delta R.T.: -0.005 min
Response: 518183
Conc: 491.37 ng/ml

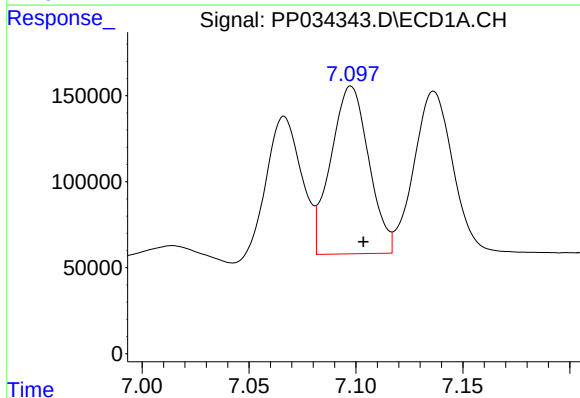


#24 AR-1248-4

R.T.: 7.097 min
Delta R.T.: -0.006 min
Response: 1200335
Conc: 464.58 ng/ml m

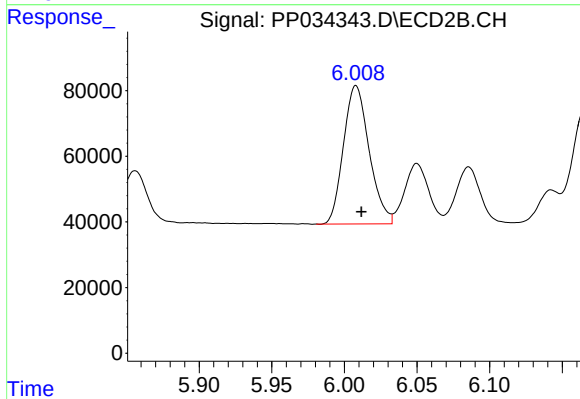

#24 AR-1248-4

R.T.: 6.008 min
Delta R.T.: -0.004 min
Response: 519380
Conc: 423.23 ng/ml

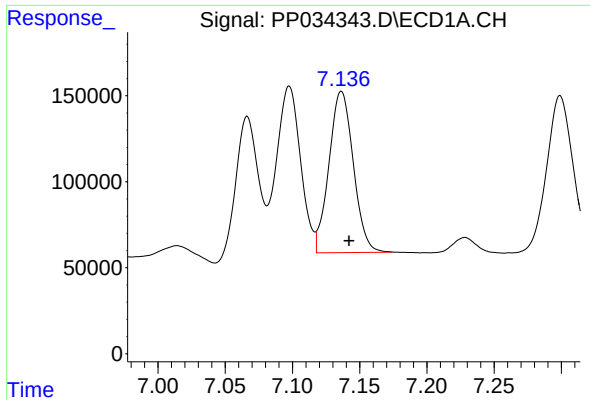


#25 AR-1248-5

R.T.: 7.136 min
Delta R.T.: -0.006 min
Response: 1172885
Conc: 451.97 ng/ml m

Instrument :
ECD_P
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
3/25/2021 9:08:19 AM

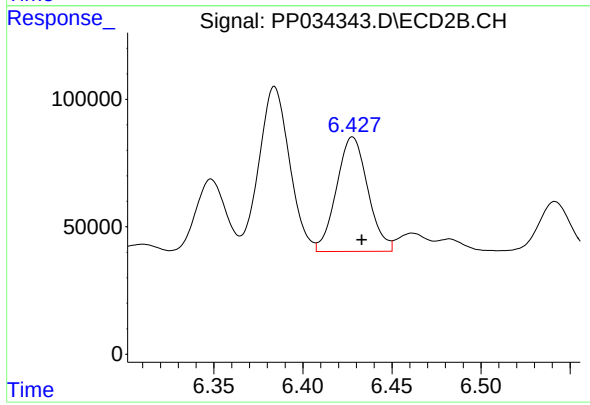

#25 AR-1248-5

R.T.: 6.428 min
Delta R.T.: -0.005 min
Response: 550656
Conc: 545.39 ng/ml