

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032422\
 Data File : PP045085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 13:49
 Operator : YP\AJ
 Sample : N2063-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-2-(10-10.5)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/25/2022
 Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 03:01:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.905	3.155	61317738	45221689	33.653	34.315
2) SA Decachlor...	10.033	8.513	39359012	45179719	30.576m	34.770

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032422\
Data File : PP045085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 13:49
Operator : YP\AJ
Sample : N2063-02
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-2-(10-10.5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 03:01:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

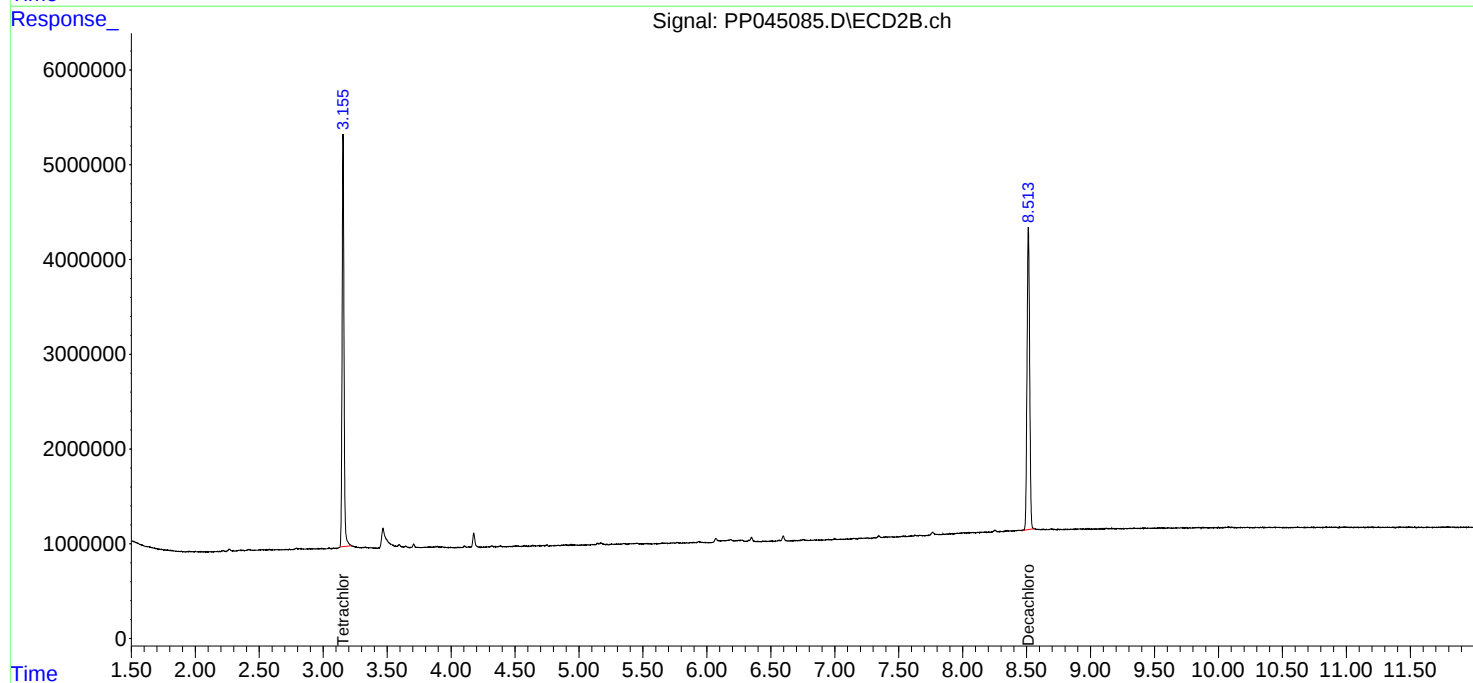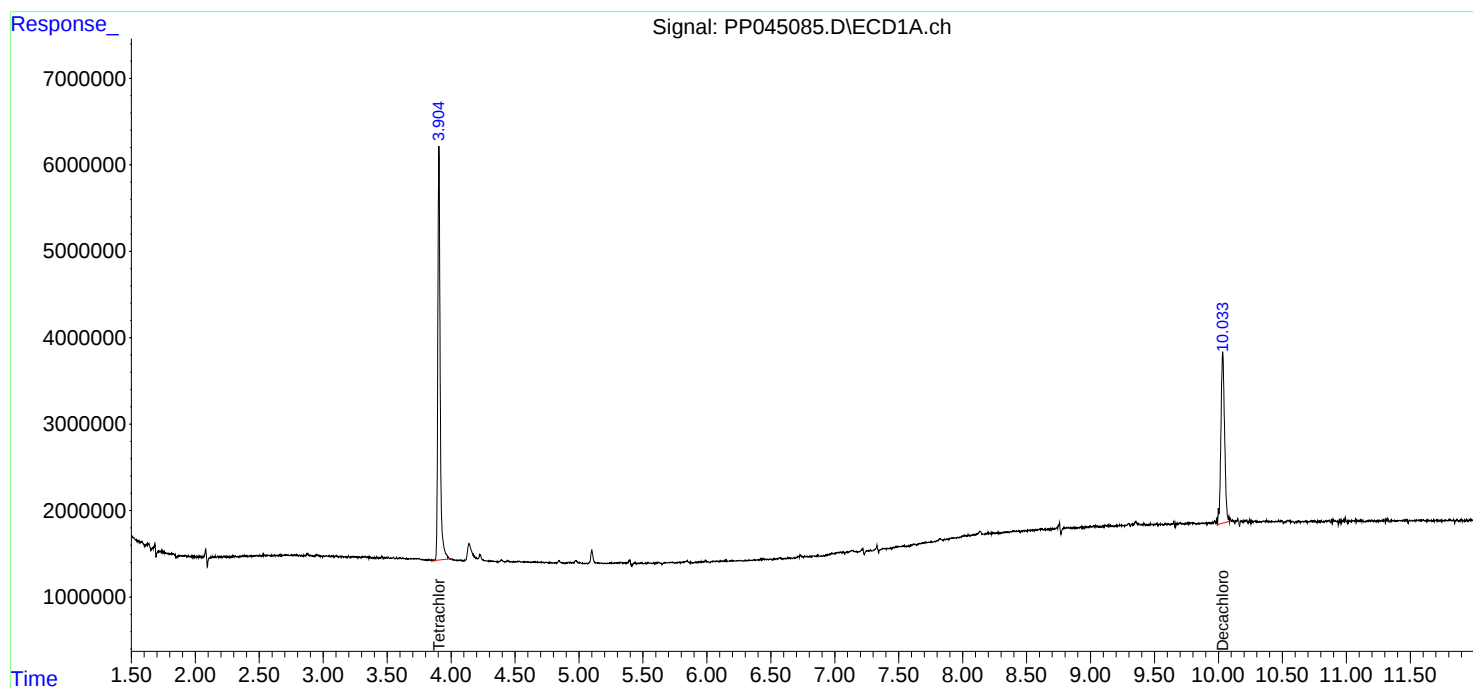

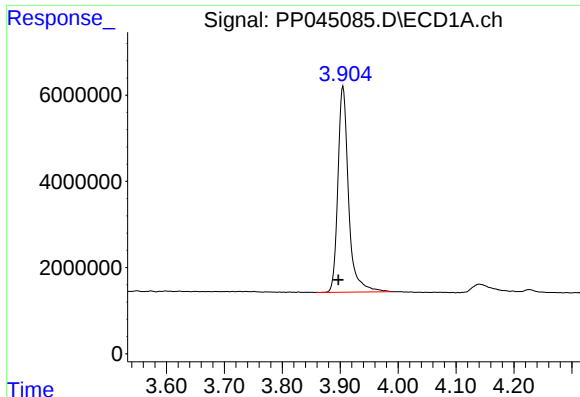

#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: 0.008 min
Response: 61317738
Conc: 33.65 ng/ml

Instrument :

ECD_P

ClientSampleId :


WC-2-(10-10.5)

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 03/25/2022

Supervised By :mohammad ahmed 03/25/2022

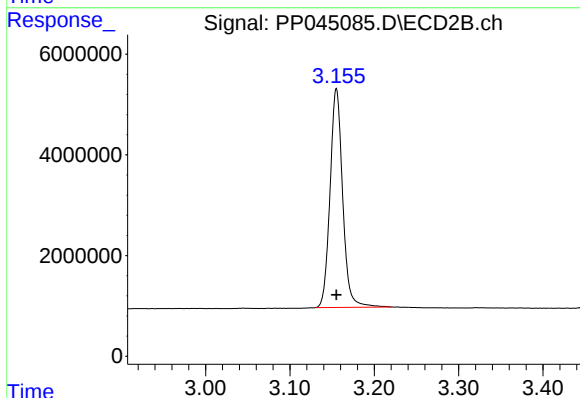


#1 Tetrachloro-m-xylene

R.T.: 3.155 min
Delta R.T.: 0.000 min
Response: 45221689
Conc: 34.32 ng/ml

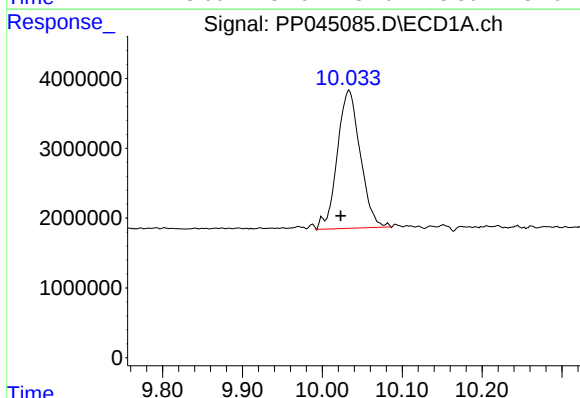

#2 Decachlorobiphenyl

R.T.: 10.033 min
Delta R.T.: 0.010 min
Response: 39359012
Conc: 30.58 ng/ml m

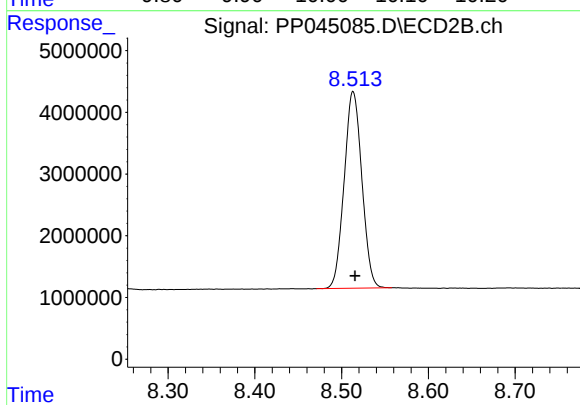

#2 Decachlorobiphenyl

R.T.: 8.513 min
Delta R.T.: -0.002 min
Response: 45179719
Conc: 34.77 ng/ml