

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032422\
 Data File : PP045092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 15:36
 Operator : YP\AJ
 Sample : N2055-14 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-36B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/25/2022
 Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 03:04:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.893	3.154	3018770	2341717	1.657m	1.777
2) SA Decachlor...	10.010	8.507	2829922	2552878	2.198m	1.965
Target Compounds						
26) L6 AR-1254-1	6.066	5.146	564935	672648	8.508	7.778
27) L6 AR-1254-2	6.308	5.307	791766	770054	7.925	10.348 #
28) L6 AR-1254-3	6.710	5.737	1094540	1078387	10.701	9.385
29) L6 AR-1254-4	7.021	5.986	1341679	632795	18.446	8.488 #
30) L6 AR-1254-5	7.483	6.437	1240659	1143252	16.041m	11.103 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032422\
Data File : PP045092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 15:36
Operator : YP\AJ
Sample : N2055-14 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CLI-2022-36B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 03:04:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

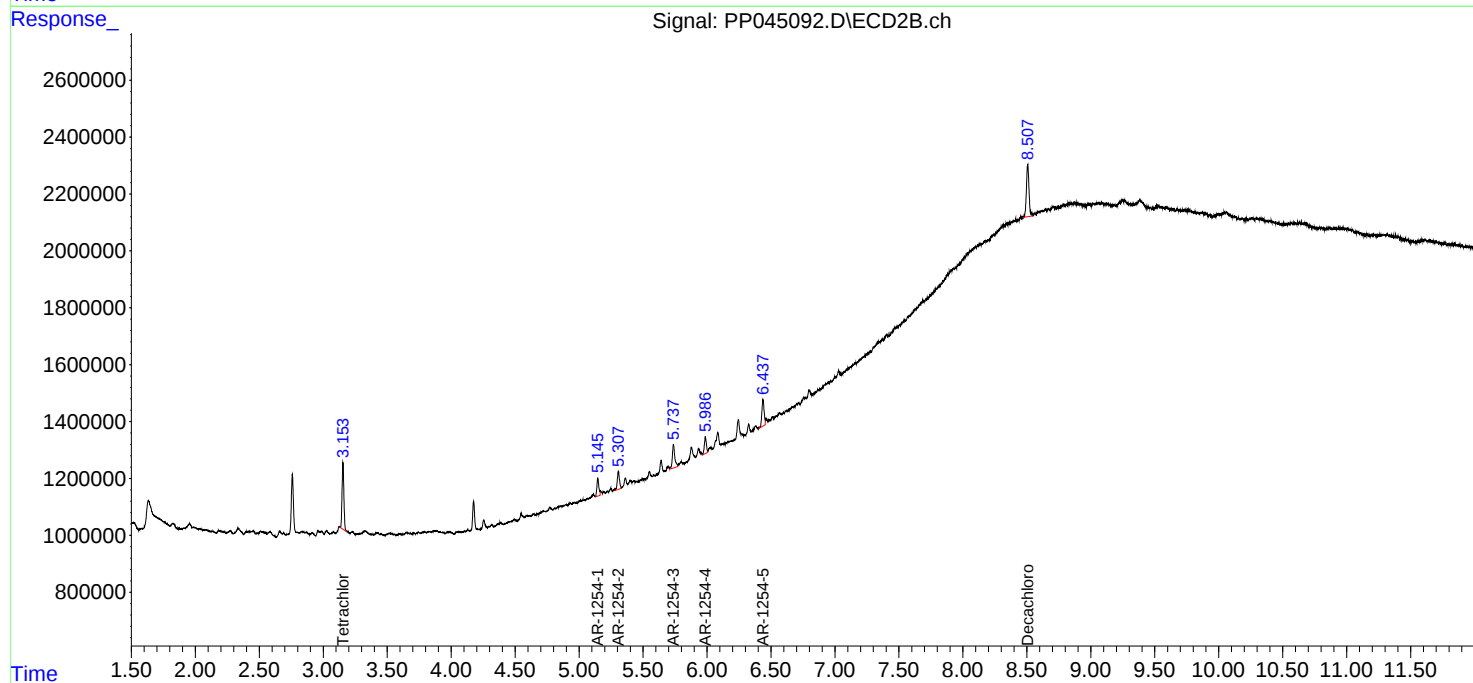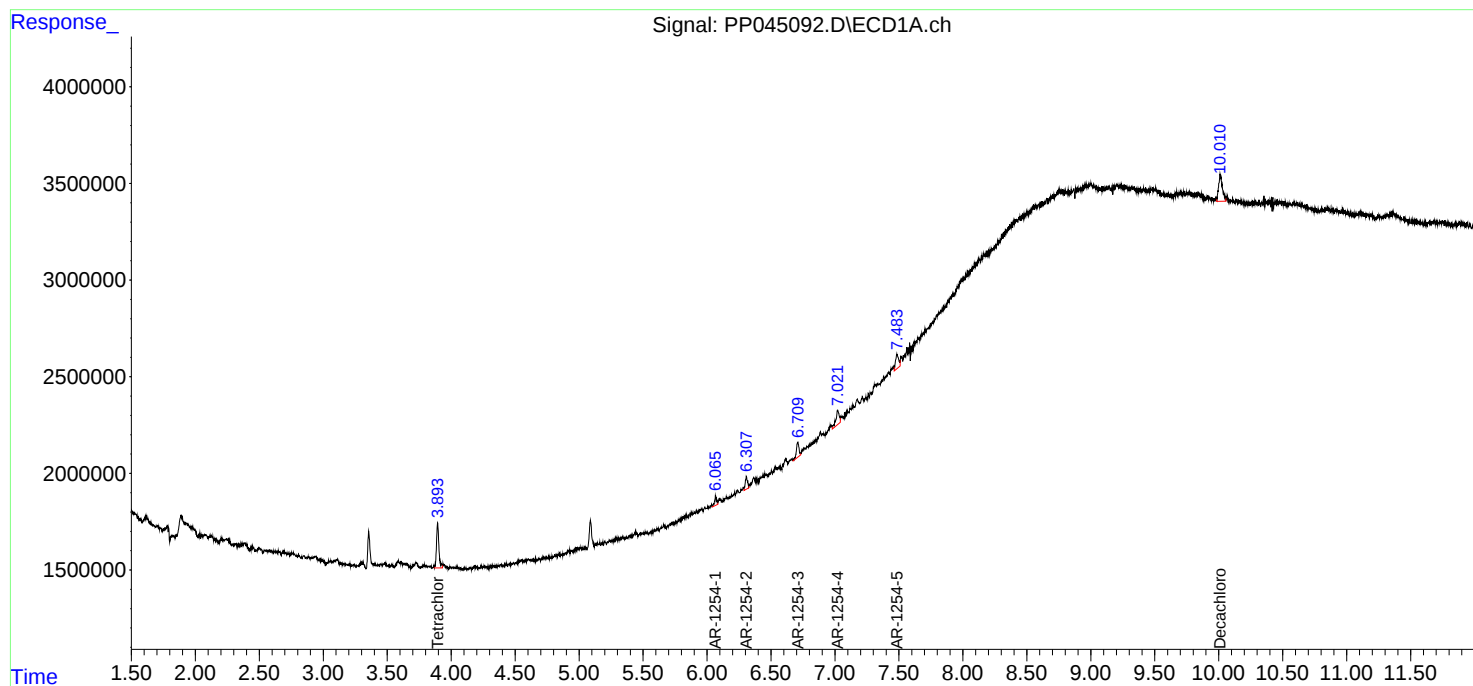

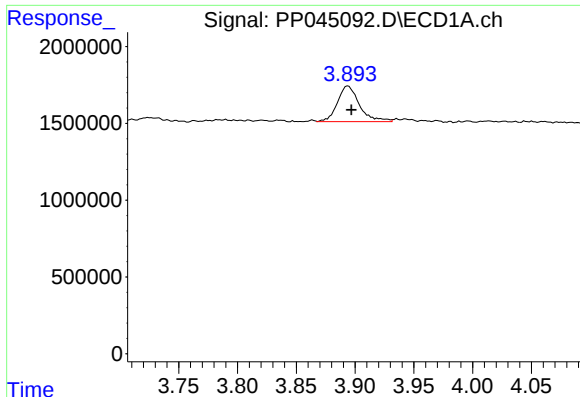


#1 Tetrachloro-m-xylene

R.T.: 3.893 min
Delta R.T.: -0.004 min
Response: 3018770
Conc: 1.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-36B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

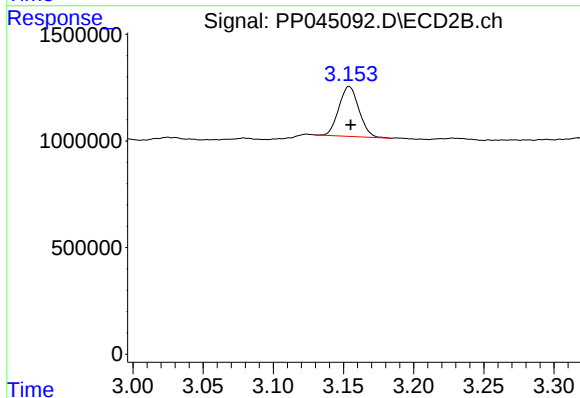


#1 Tetrachloro-m-xylene

R.T.: 3.154 min
Delta R.T.: -0.001 min
Response: 2341717
Conc: 1.78 ng/ml

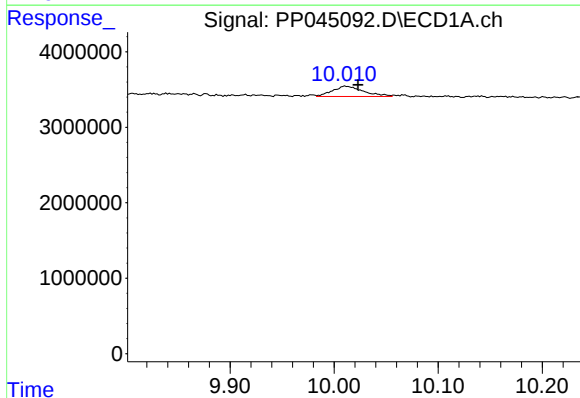


#2 Decachlorobiphenyl

R.T.: 10.010 min
Delta R.T.: -0.013 min
Response: 2829922
Conc: 2.20 ng/ml m

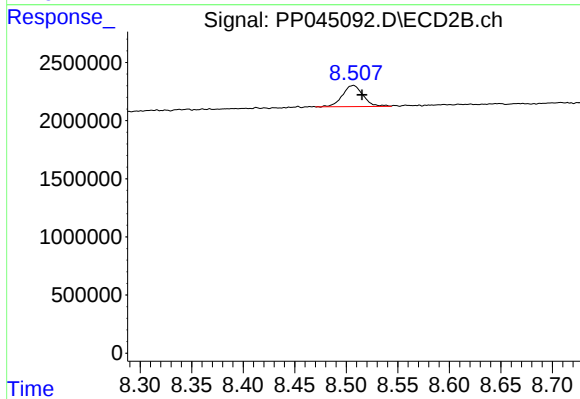

#2 Decachlorobiphenyl

R.T.: 8.507 min
Delta R.T.: -0.009 min
Response: 2552878
Conc: 1.96 ng/ml

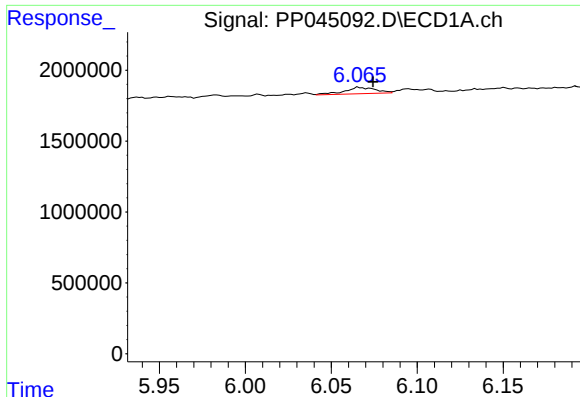


#26 AR-1254-1

R.T.: 6.066 min
Delta R.T.: -0.008 min
Response: 564935
Conc: 8.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-36B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

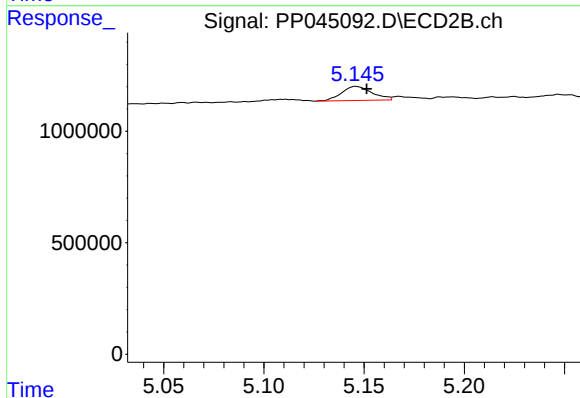


#26 AR-1254-1

R.T.: 5.146 min
Delta R.T.: -0.005 min
Response: 672648
Conc: 7.78 ng/ml

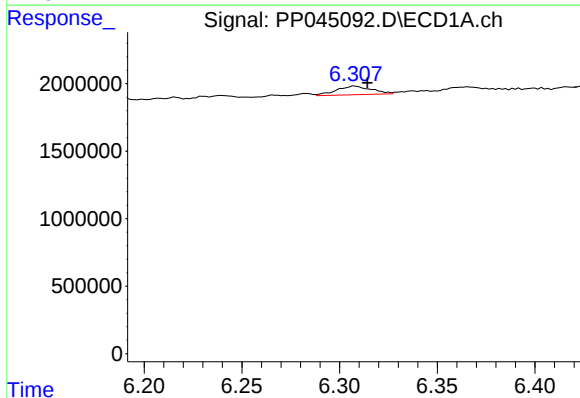


#27 AR-1254-2

R.T.: 6.308 min
Delta R.T.: -0.006 min
Response: 791766
Conc: 7.92 ng/ml

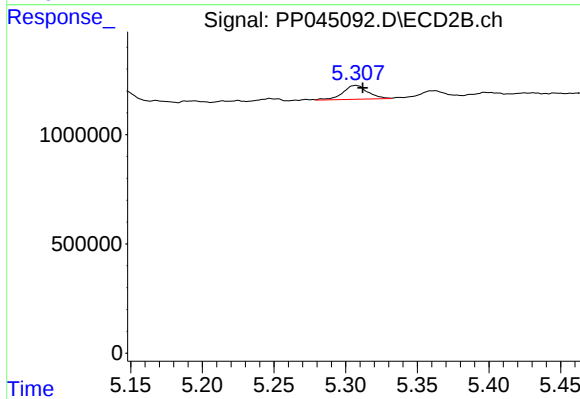

#27 AR-1254-2

R.T.: 5.307 min
Delta R.T.: -0.005 min
Response: 770054
Conc: 10.35 ng/ml

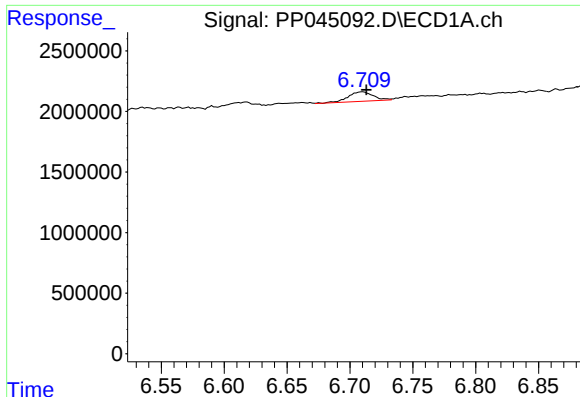


#28 AR-1254-3

R.T.: 6.710 min
Delta R.T.: -0.003 min
Response: 1094540
Conc: 10.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-36B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

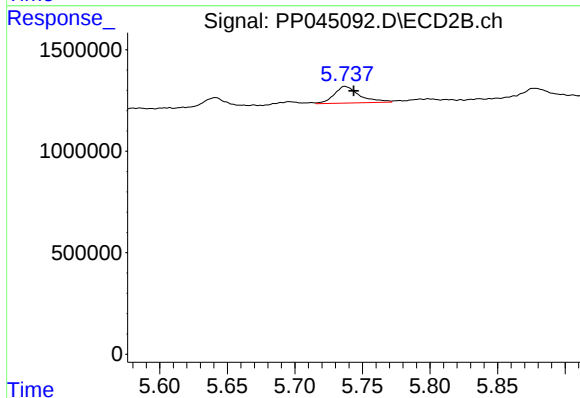


#28 AR-1254-3

R.T.: 5.737 min
Delta R.T.: -0.007 min
Response: 1078387
Conc: 9.39 ng/ml

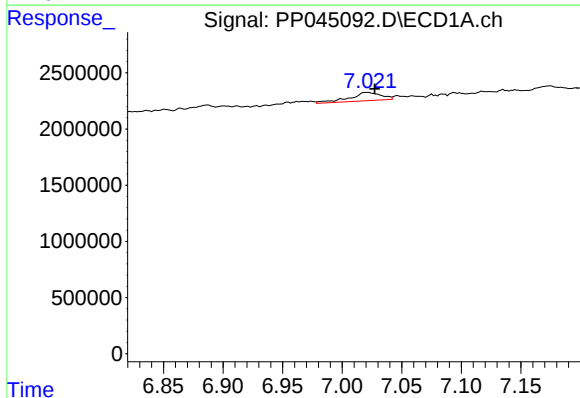


#29 AR-1254-4

R.T.: 7.021 min
Delta R.T.: -0.006 min
Response: 1341679
Conc: 18.45 ng/ml

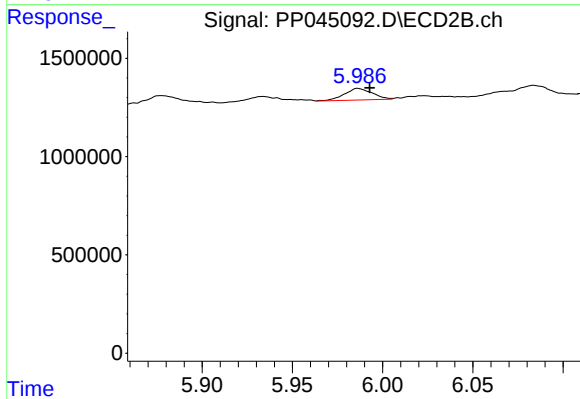

#29 AR-1254-4

R.T.: 5.986 min
Delta R.T.: -0.007 min
Response: 632795
Conc: 8.49 ng/ml

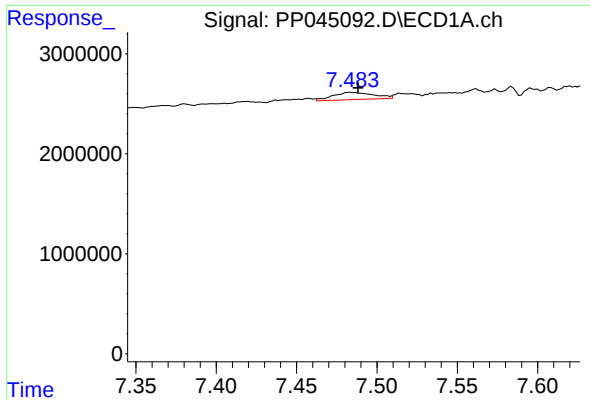


#30 AR-1254-5

R.T.: 7.483 min
Delta R.T.: -0.005 min
Response: 1240659
Conc: 16.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-36B

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

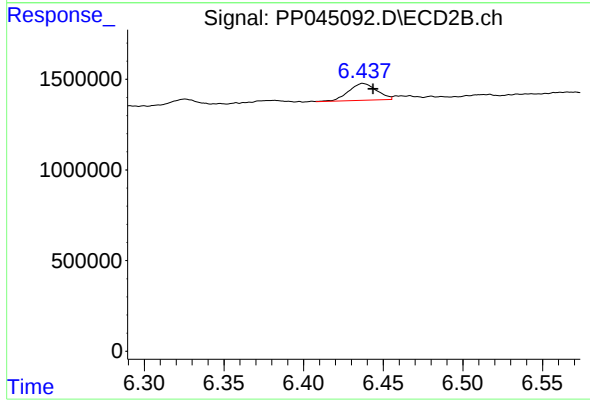

#30 AR-1254-5

R.T.: 6.437 min
Delta R.T.: -0.006 min
Response: 1143252
Conc: 11.10 ng/ml