

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032422\
 Data File : PP045094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 16:06
 Operator : YP\AJ
 Sample : N2055-16 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-37B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/25/2022
 Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 03:05:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.894	3.153	2770469	2274832	1.521	1.726
2) SA Decachlor...	10.013	8.506	2370582	2620054	1.842m	2.016
Target Compounds						
26) L6 AR-1254-1	6.070	5.146	588878	542478	8.869	6.273 #
27) L6 AR-1254-2	6.308	5.307	869956	626991	8.707	8.426
28) L6 AR-1254-3	6.708	5.737	788074	783606	7.705	6.820
29) L6 AR-1254-4	7.021	5.985	634661	521145	8.726	6.990
30) L6 AR-1254-5	7.478	6.438	786780	842070	10.173m	8.178

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032422\
Data File : PP045094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 16:06
Operator : YP\AJ
Sample : N2055-16 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CLI-2022-37B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 03:05:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

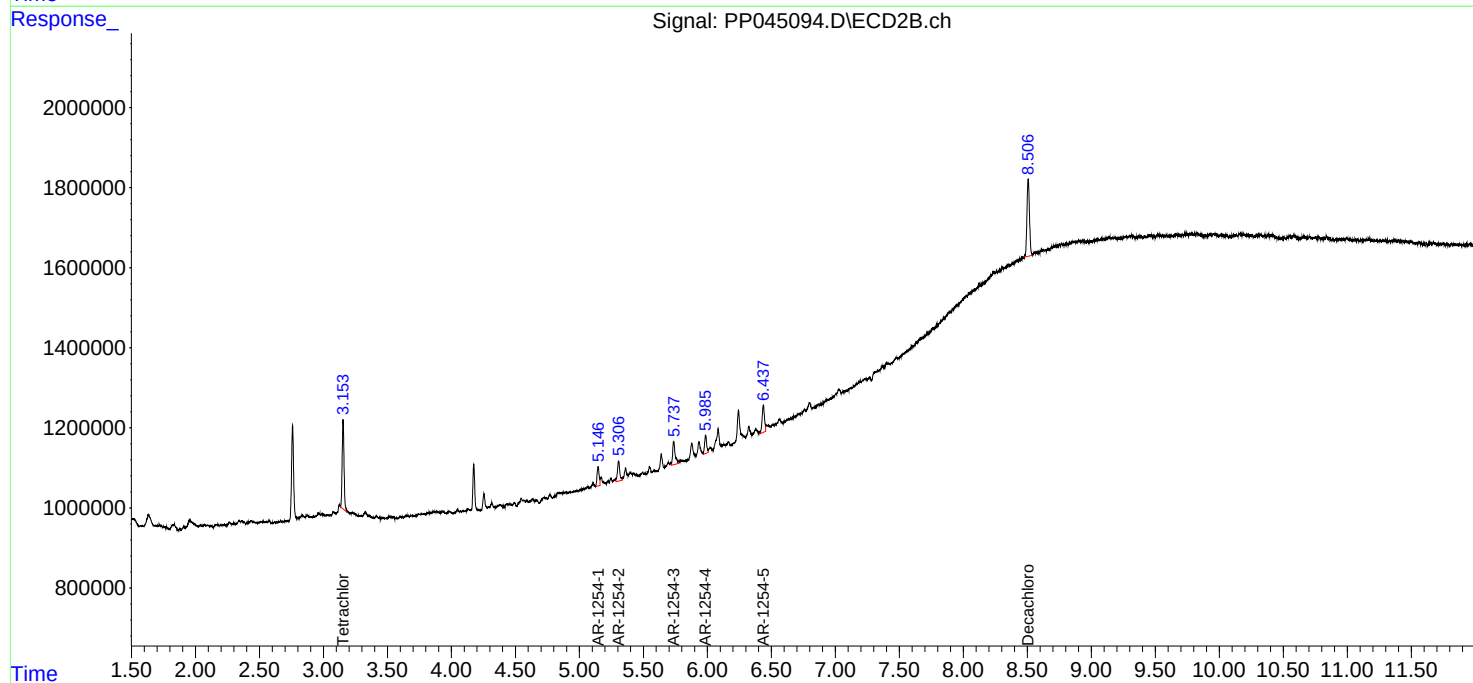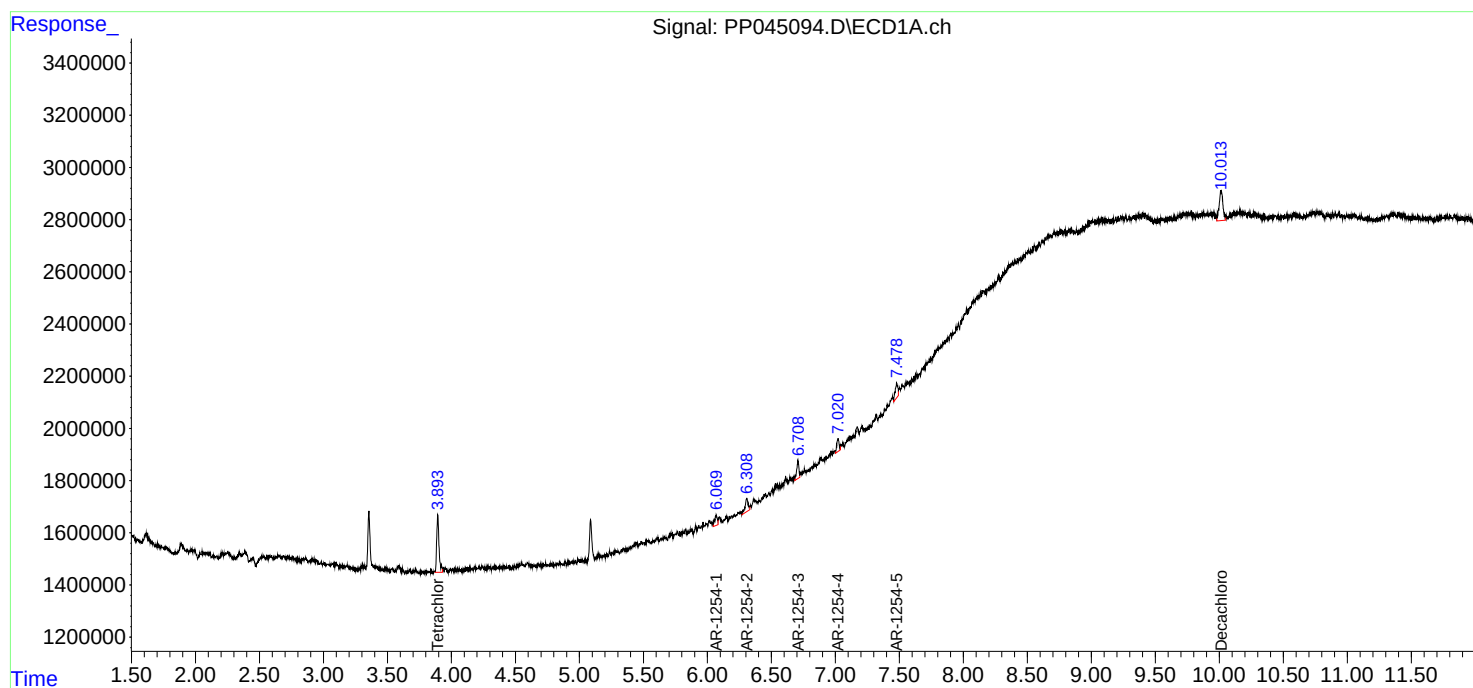

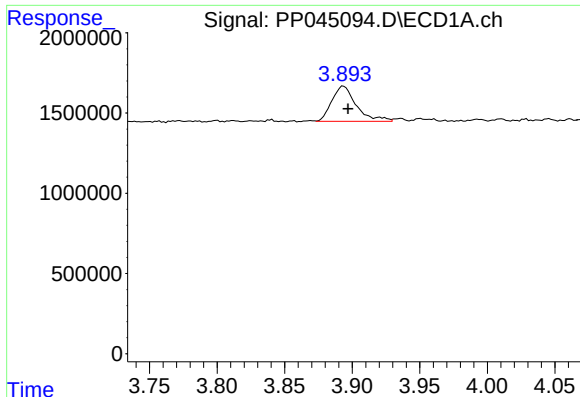


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: -0.003 min
Response: 2770469
Conc: 1.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-37B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

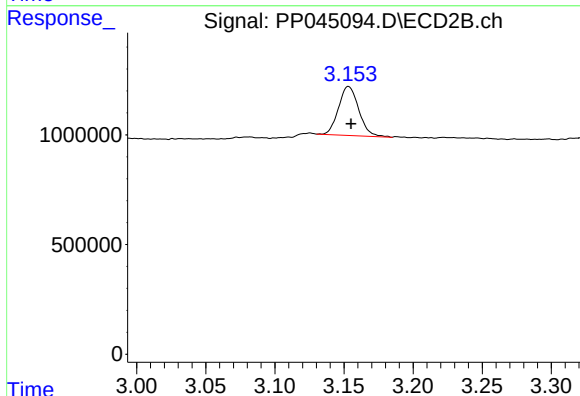


#1 Tetrachloro-m-xylene

R.T.: 3.153 min
Delta R.T.: -0.002 min
Response: 2274832
Conc: 1.73 ng/ml

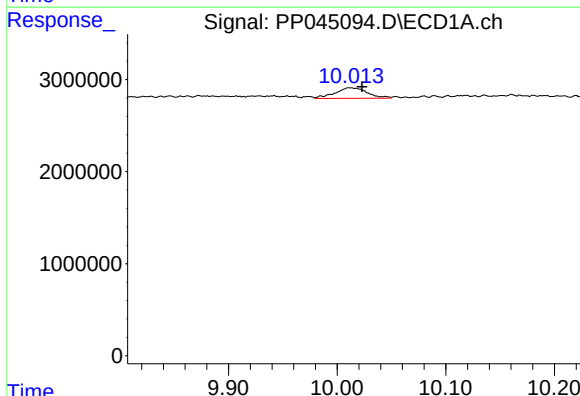


#2 Decachlorobiphenyl

R.T.: 10.013 min
Delta R.T.: -0.010 min
Response: 2370582
Conc: 1.84 ng/ml m

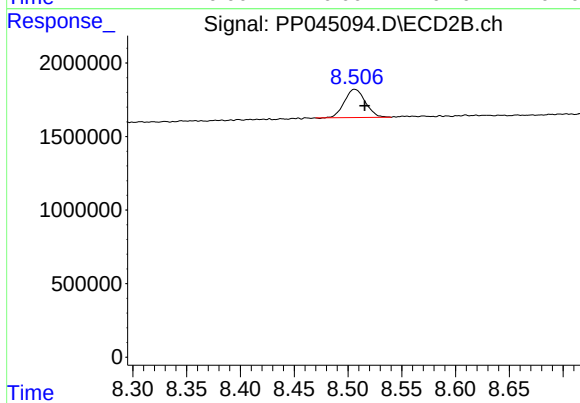

#2 Decachlorobiphenyl

R.T.: 8.506 min
Delta R.T.: -0.009 min
Response: 2620054
Conc: 2.02 ng/ml

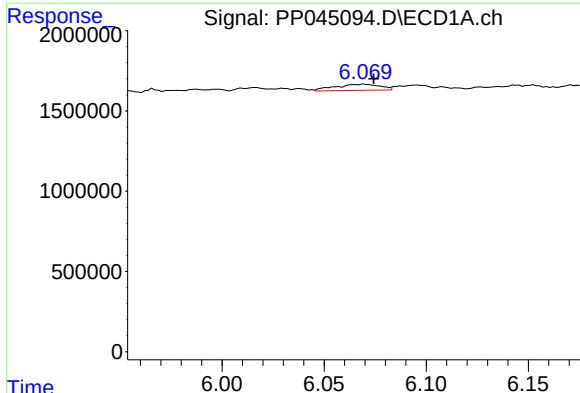


#26 AR-1254-1

R.T.: 6.070 min
Delta R.T.: -0.005 min
Response: 588878
Conc: 8.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-37B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

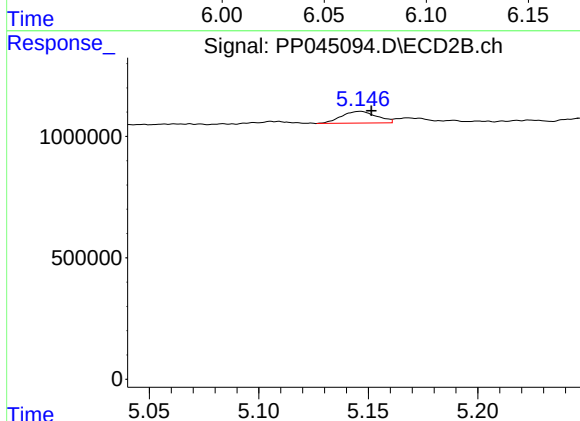


#26 AR-1254-1

R.T.: 5.146 min
Delta R.T.: -0.005 min
Response: 542478
Conc: 6.27 ng/ml

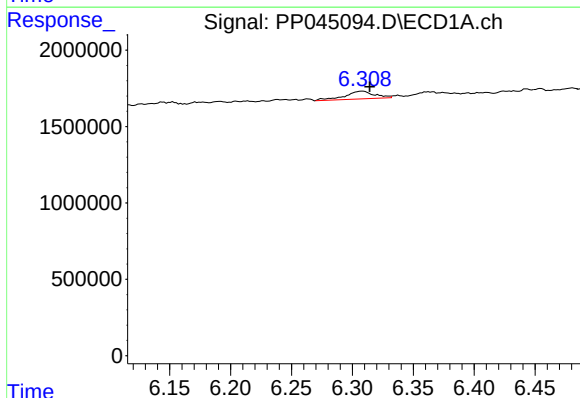


#27 AR-1254-2

R.T.: 6.308 min
Delta R.T.: -0.006 min
Response: 869956
Conc: 8.71 ng/ml

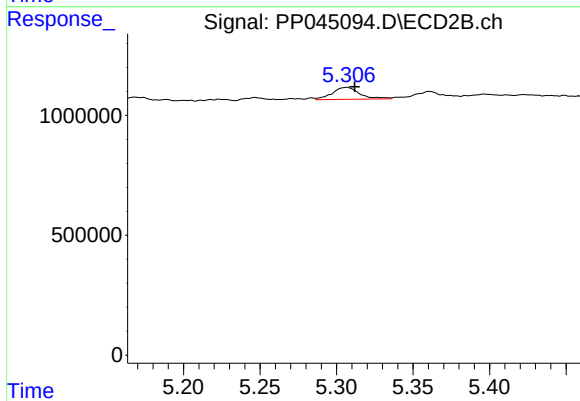

#27 AR-1254-2

R.T.: 5.307 min
Delta R.T.: -0.005 min
Response: 626991
Conc: 8.43 ng/ml

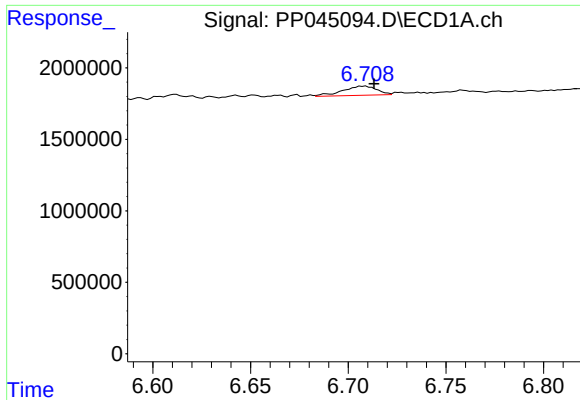


#28 AR-1254-3

R.T.: 6.708 min
Delta R.T.: -0.005 min
Response: 788074
Conc: 7.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-37B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

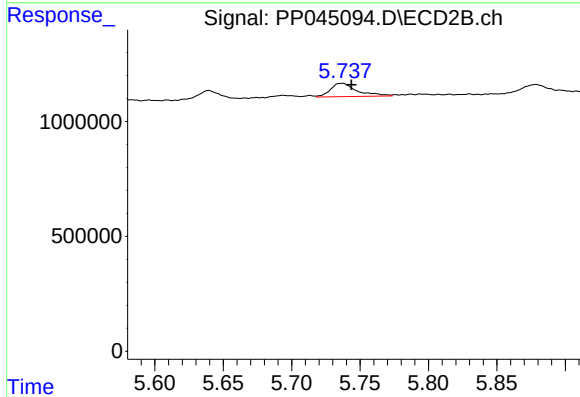


#28 AR-1254-3

R.T.: 5.737 min
Delta R.T.: -0.006 min
Response: 783606
Conc: 6.82 ng/ml

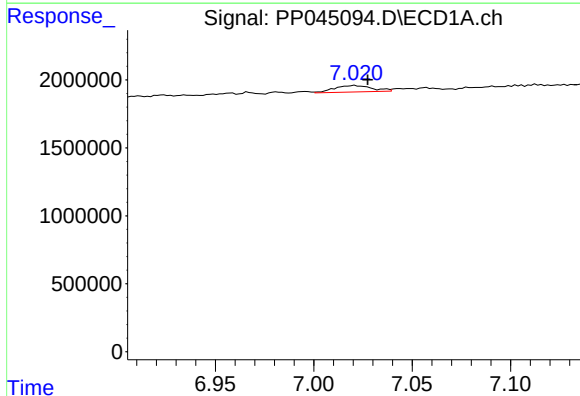


#29 AR-1254-4

R.T.: 7.021 min
Delta R.T.: -0.007 min
Response: 634661
Conc: 8.73 ng/ml

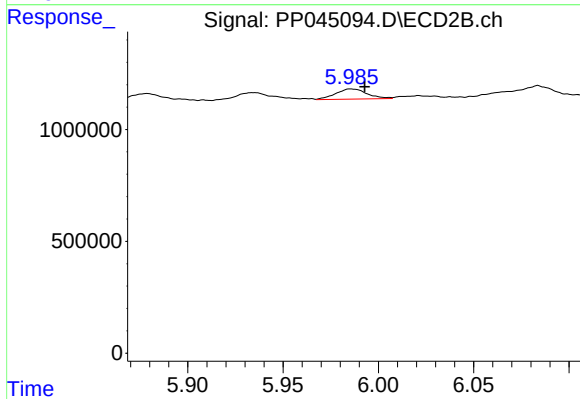

#29 AR-1254-4

R.T.: 5.985 min
Delta R.T.: -0.008 min
Response: 521145
Conc: 6.99 ng/ml

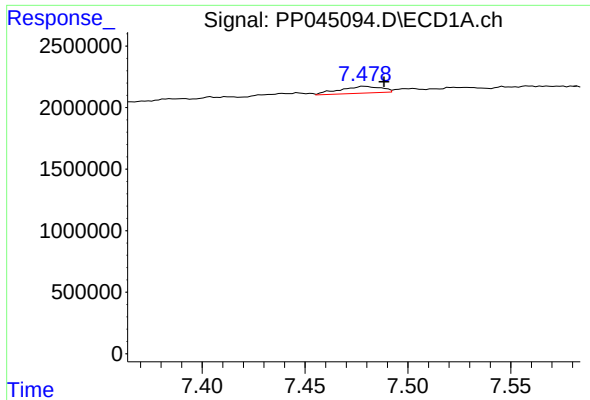


#30 AR-1254-5

R.T.: 7.478 min
Delta R.T.: -0.011 min
Response: 786780
Conc: 10.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-37B

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

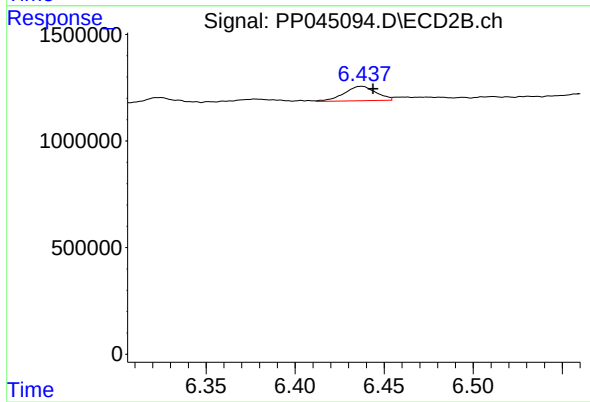

#30 AR-1254-5

R.T.: 6.438 min
Delta R.T.: -0.006 min
Response: 842070
Conc: 8.18 ng/ml