

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032422\
 Data File : PP045101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 20:07
 Operator : YP\AJ
 Sample : N2056-02 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC157517LOK-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/25/2022
 Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 03:08:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.894	3.153	2594186	2453693	1.424	1.862 #
2) SA Decachlor...	10.014	8.506	2718549	2841233	2.112m	2.187

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032422\
Data File : PP045101.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 20:07
Operator : YP\AJ
Sample : N2056-02 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC157517LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 03:08:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

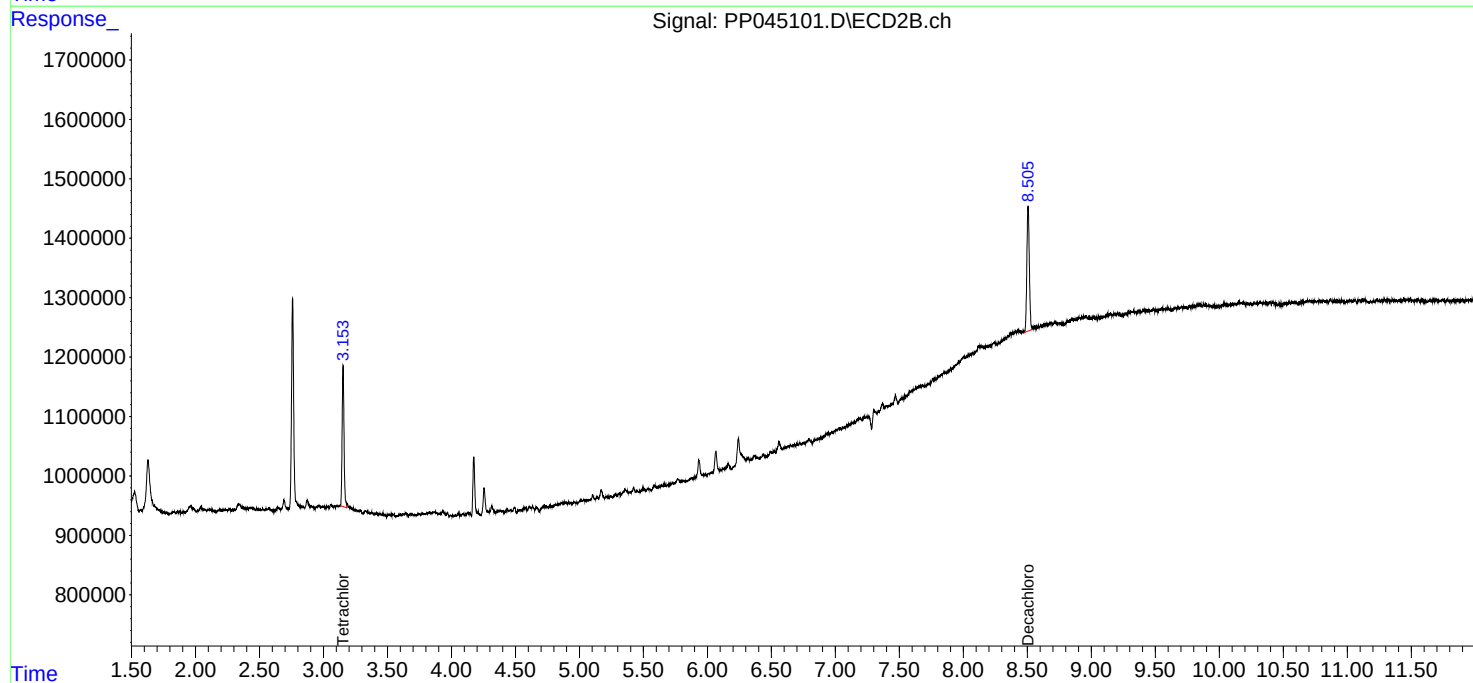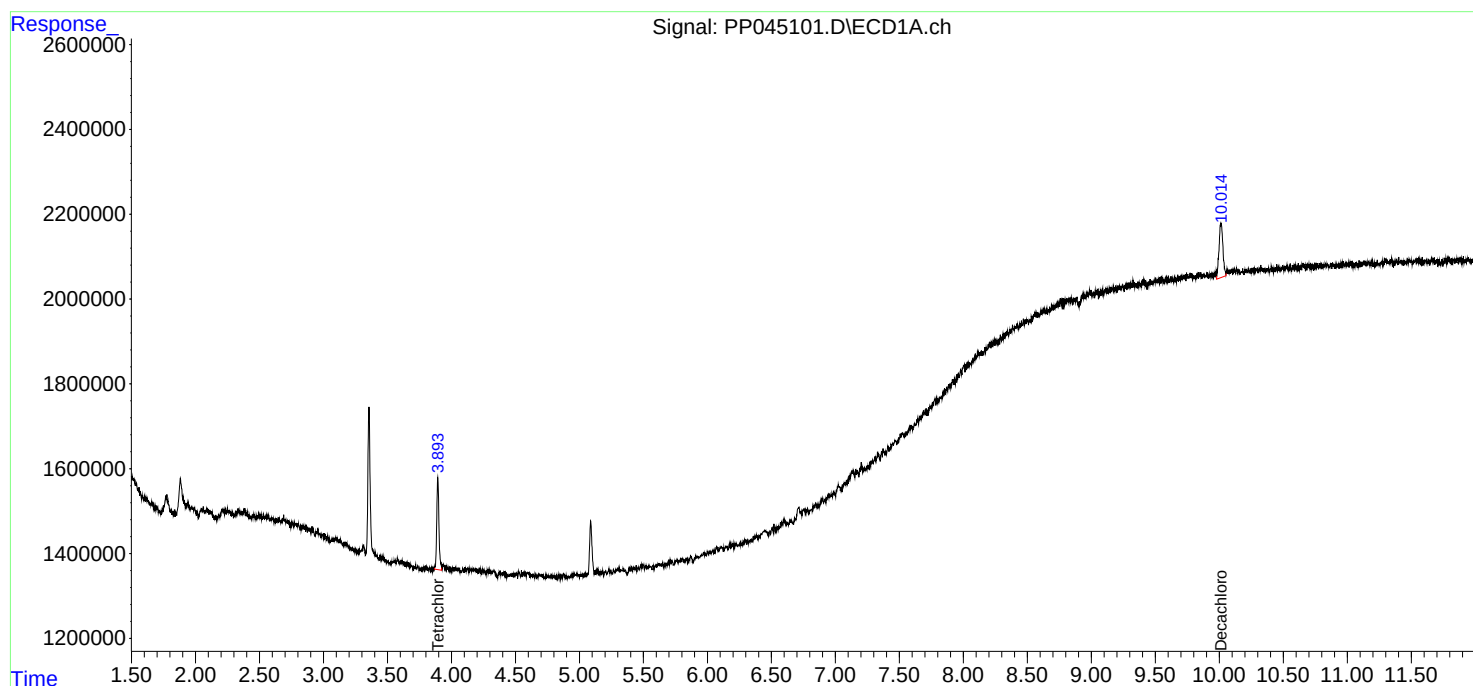

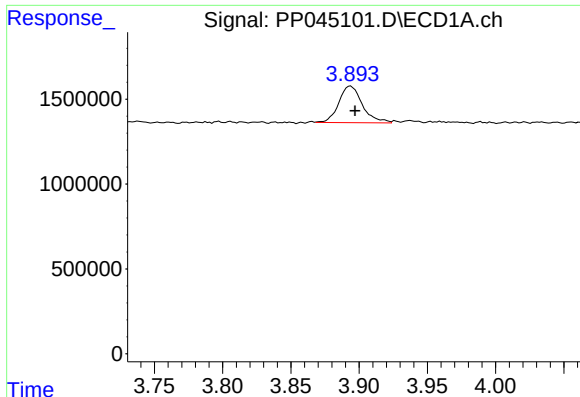


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: -0.003 min
Response: 2594186
Conc: 1.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC157517LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/25/2022
Supervised By :mohammad ahmed 03/25/2022

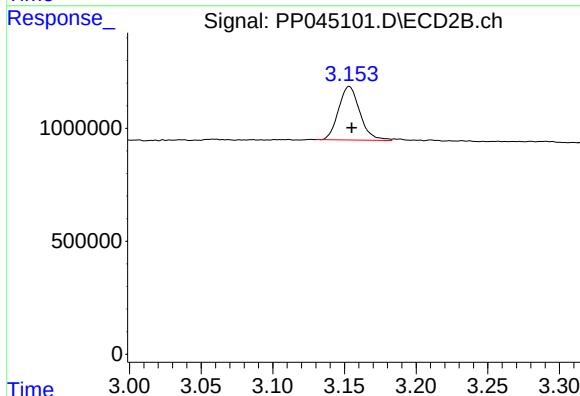


#1 Tetrachloro-m-xylene

R.T.: 3.153 min
Delta R.T.: -0.002 min
Response: 2453693
Conc: 1.86 ng/ml

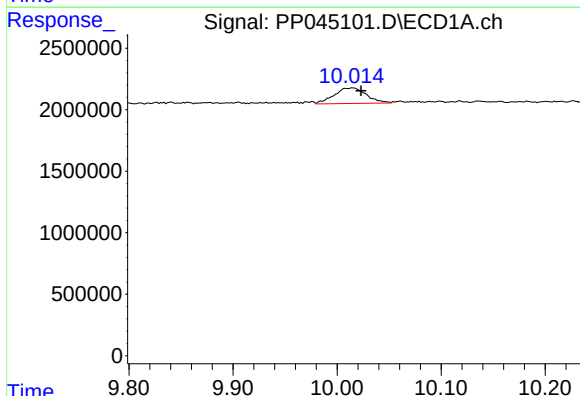

#2 Decachlorobiphenyl

R.T.: 10.014 min
Delta R.T.: -0.009 min
Response: 2718549
Conc: 2.11 ng/ml m

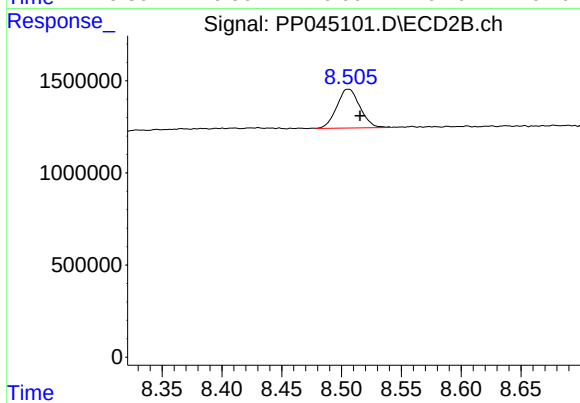

#2 Decachlorobiphenyl

R.T.: 8.506 min
Delta R.T.: -0.010 min
Response: 2841233
Conc: 2.19 ng/ml