

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032521\
 Data File : PP034356.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Mar 2021 12:21
 Operator : DD\AJ
 Sample : PB135341BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 03:03:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.851	4.260	1656921	918681	19.724	20.760
2)	SA Decachlor...	10.775	9.573	1827326	671429	23.285	25.443
Target Compounds							
8)	L2 AR-1221-1	5.100	0.000	65504	0	72.141	N.D. #
9)	L2 AR-1221-2	5.200	4.612	23934	19077	34.776	53.793 #
32)	L7 AR-1260-2	0.000	7.270f	0	15046	N.D.	8.409 #
35)	L7 AR-1260-5	0.000	8.178	0	3680	N.D.	1.185 #
37)	L8 AR-1262-2	0.000	8.178	0	3680	N.D.	1.140 #
40)	L8 AR-1262-5	0.000	9.024	0	4178	N.D.	3.974 #
44)	L9 AR-1268-4	0.000	9.024	0	4178	N.D.	3.472 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032521\
Data File : PP034356.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Mar 2021 12:21
Operator : DD\AJ
Sample : PB135341BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 03:03:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

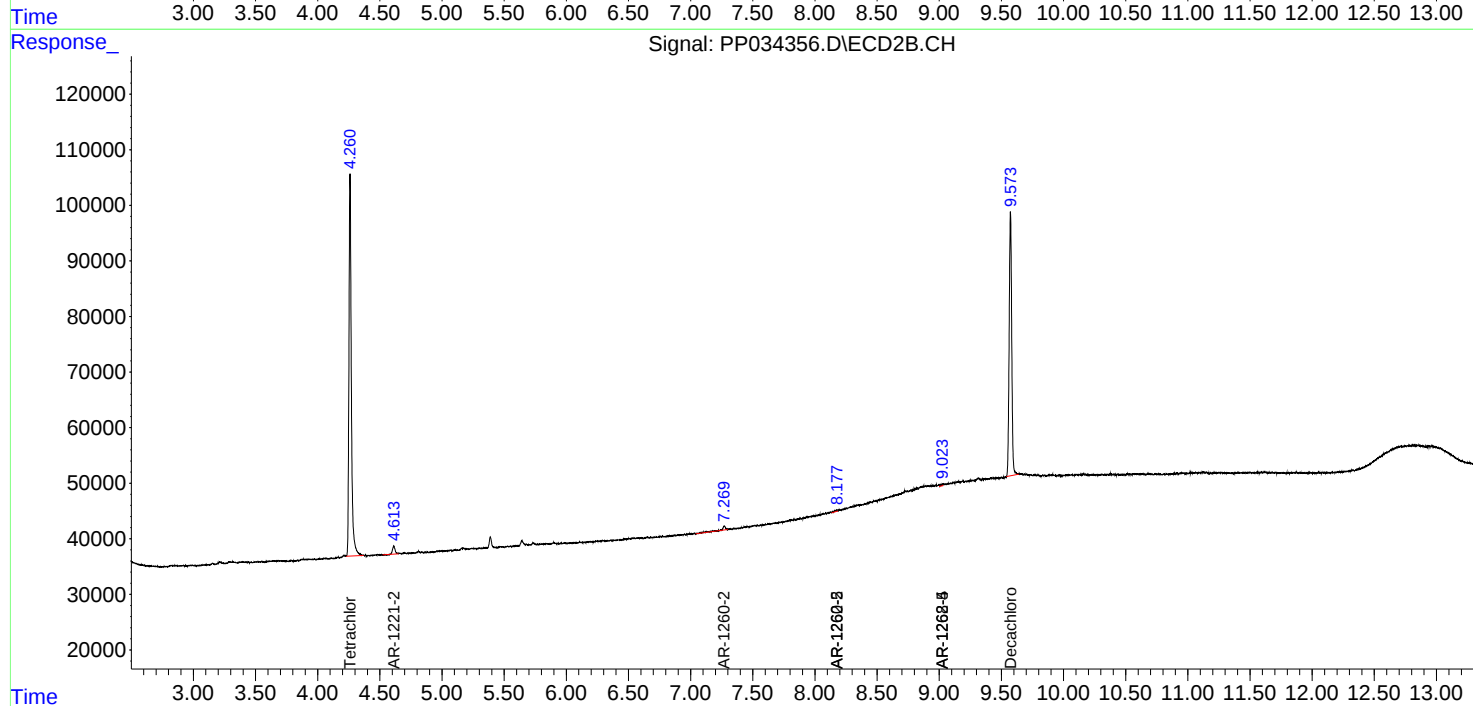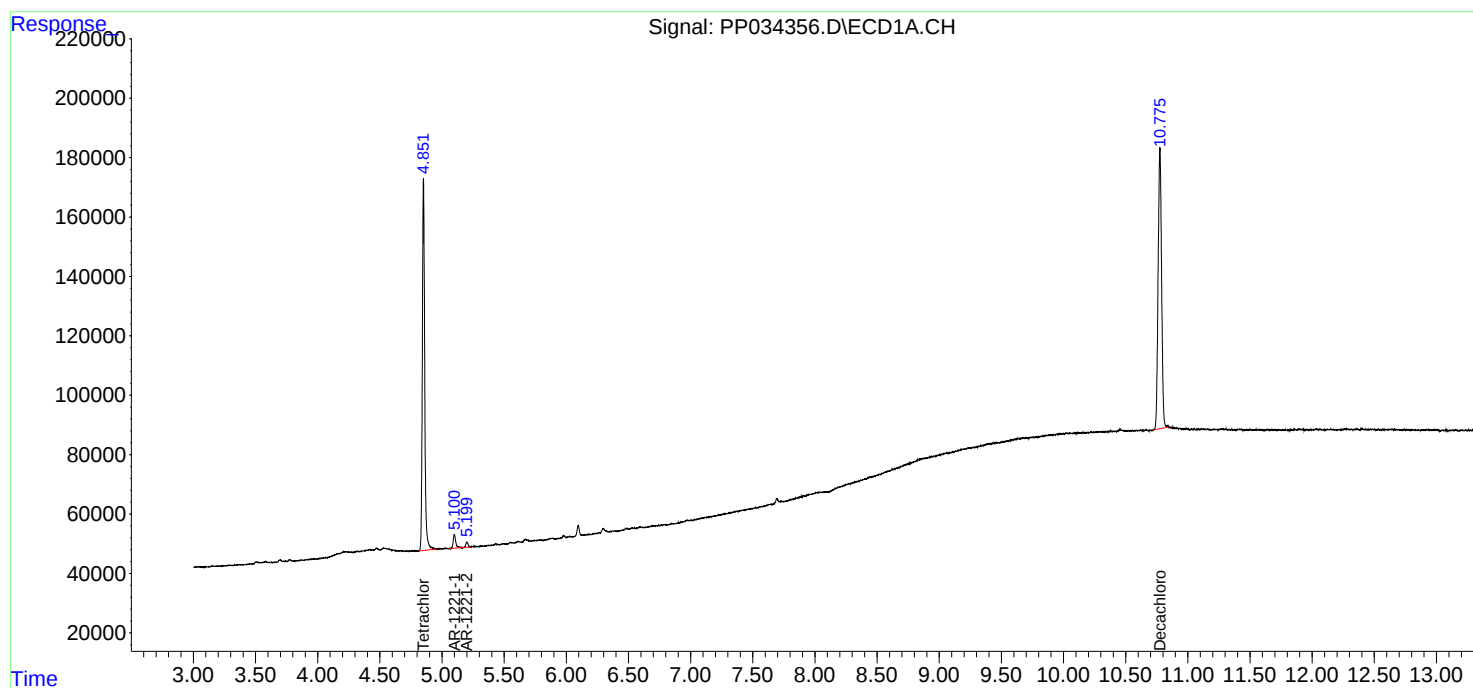


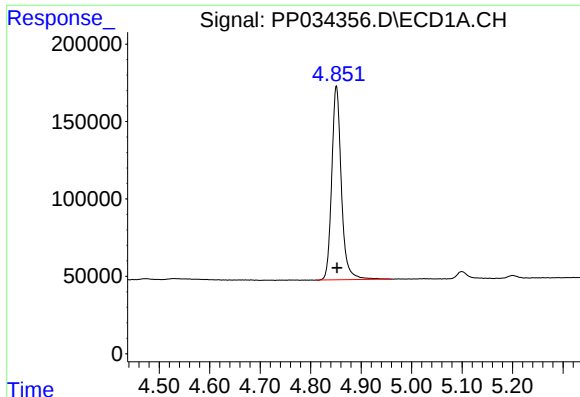

#1 Tetrachloro-m-xylene


R.T.: 4.851 min
Delta R.T.: 0.000 min
Response: 1656921
Conc: 19.72 ng/ml

Instrument :
ECD_P
ClientSampleId :

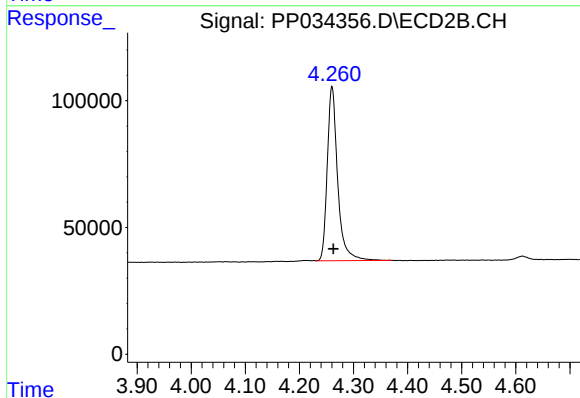


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.002 min
Response: 918681
Conc: 20.76 ng/ml

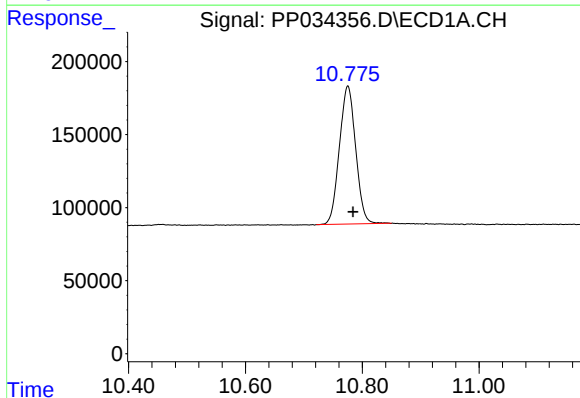


#2 Decachlorobiphenyl

R.T.: 10.775 min
Delta R.T.: -0.009 min
Response: 1827326
Conc: 23.28 ng/ml

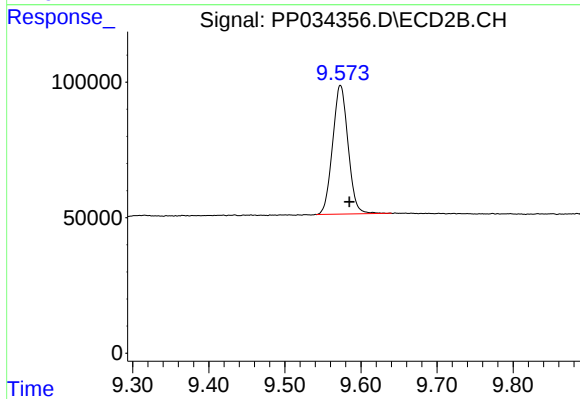

#2 Decachlorobiphenyl


R.T.: 9.573 min
Delta R.T.: -0.011 min
Response: 671429
Conc: 25.44 ng/ml

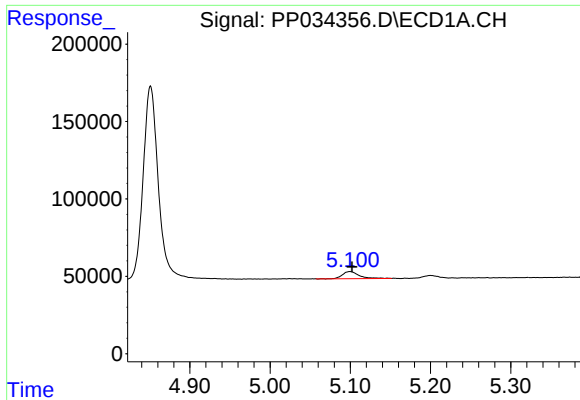

#8 AR-1221-1


R.T.: 5.100 min
Delta R.T.: -0.002 min
Response: 65504
Conc: 72.14 ng/ml

Instrument :
ECD_P
ClientSampleId :

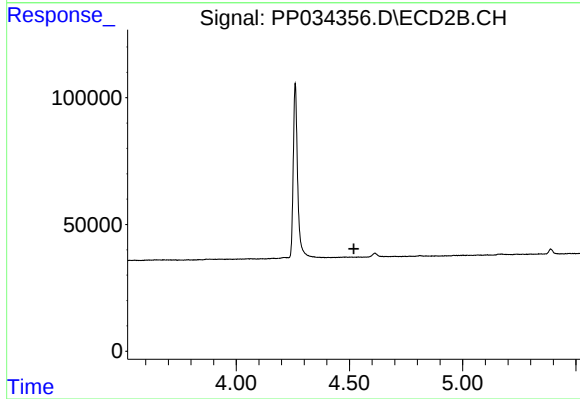


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.519 min
Response: 0
Conc: N.D.

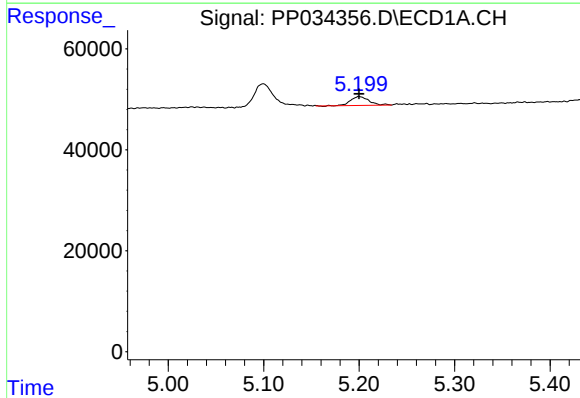


#9 AR-1221-2

R.T.: 5.200 min
Delta R.T.: 0.000 min
Response: 23934
Conc: 34.78 ng/ml

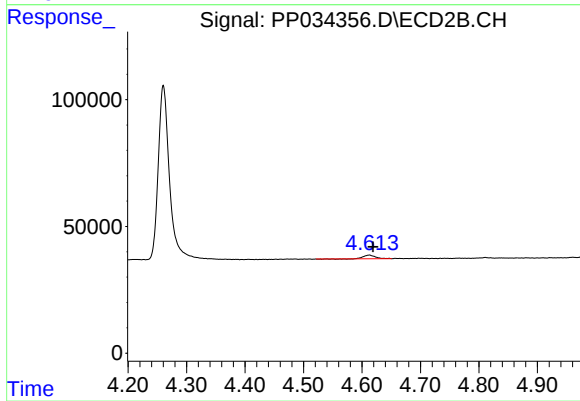

#9 AR-1221-2


R.T.: 4.612 min
Delta R.T.: -0.007 min
Response: 19077
Conc: 53.79 ng/ml

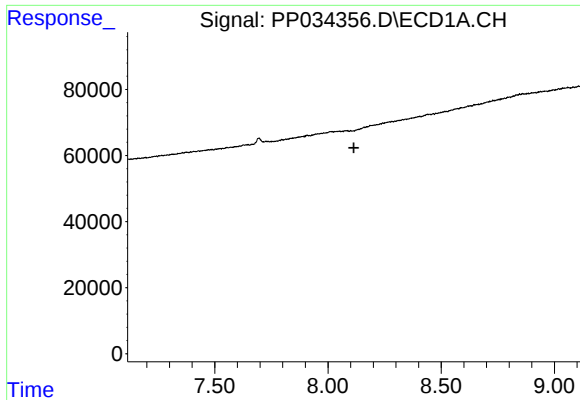

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

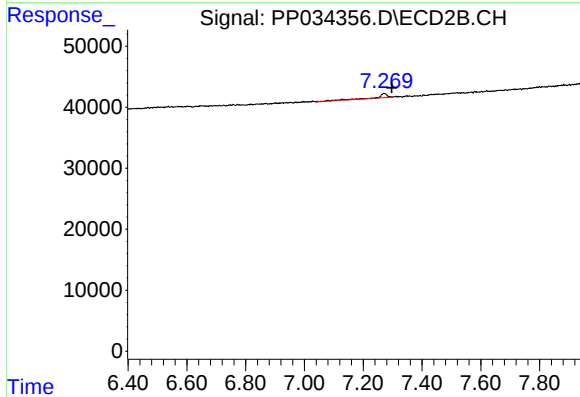


#32 AR-1260-2

R.T.: 7.270 min
Delta R.T.: -0.027 min
Response: 15046
Conc: 8.41 ng/ml

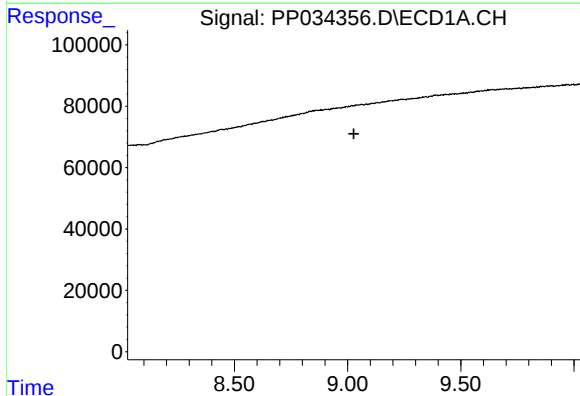


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 9.028 min
Response: 0
Conc: N.D.

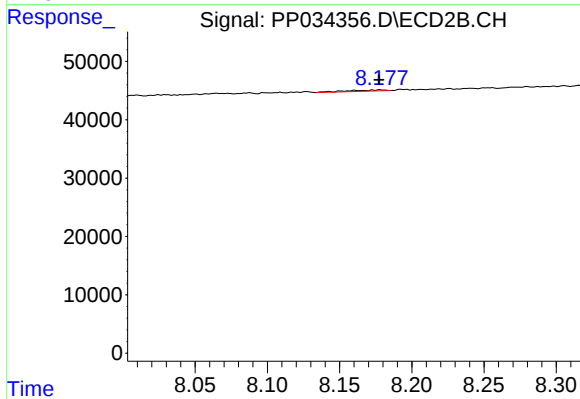

#35 AR-1260-5


R.T.: 8.178 min
Delta R.T.: 0.000 min
Response: 3680
Conc: 1.18 ng/ml

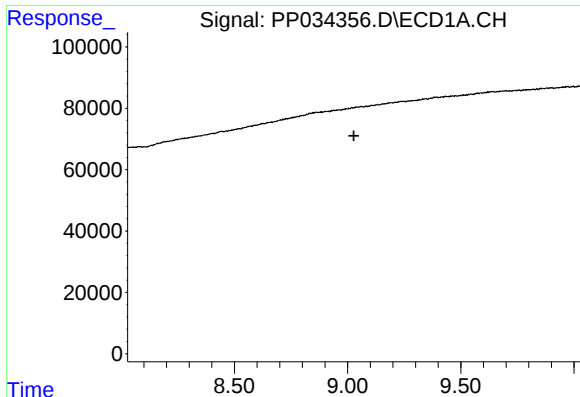

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 9.028 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

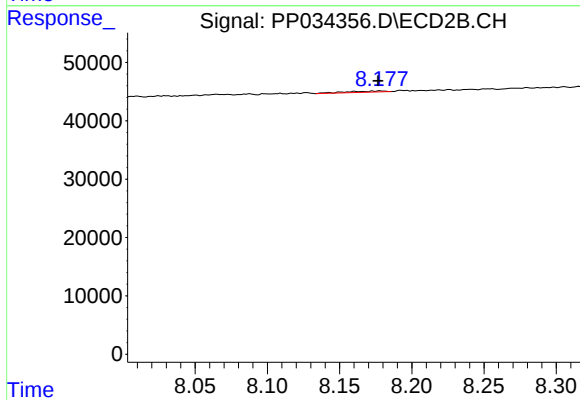


#37 AR-1262-2

R.T.: 8.178 min
Delta R.T.: 0.001 min
Response: 3680
Conc: 1.14 ng/ml

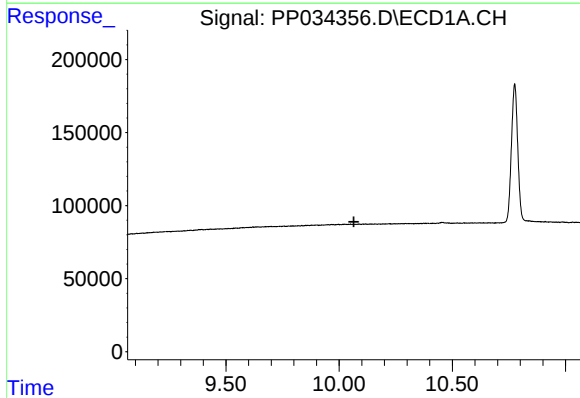


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 10.065 min
Response: 0
Conc: N.D.

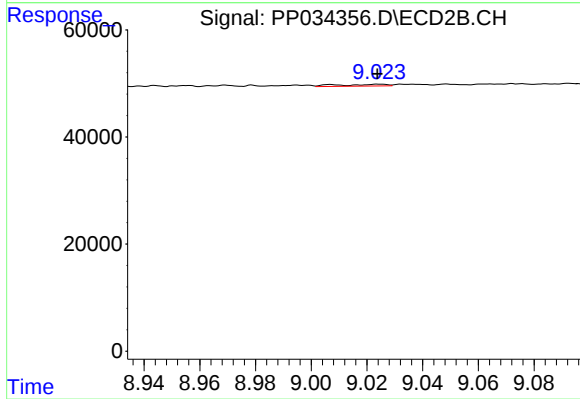

#40 AR-1262-5


R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 4178
Conc: 3.97 ng/ml

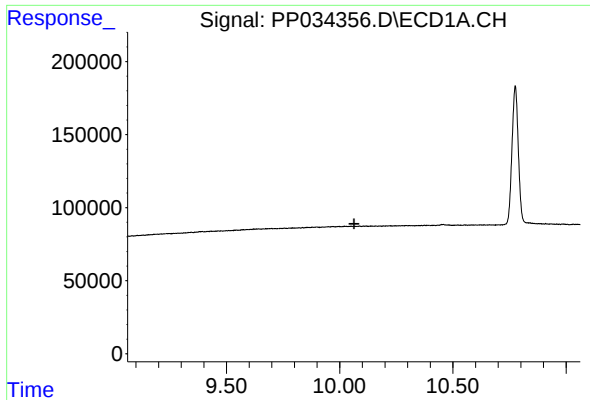

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 10.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

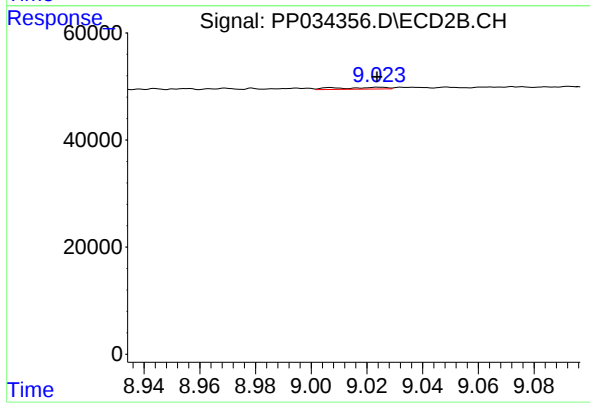

#44 AR-1268-4

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 4178
Conc: 3.47 ng/ml