

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032521\
 Data File : PP034362.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Mar 2021 14:02
 Operator : DD\AJ
 Sample : M1791-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GRAY-INTERIOR-BLOCK-1

Manual Integrations
 APPROVED

Ankita
 3/26/2021 1:13:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 03:06:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.260	1738109	837615	20.690	18.928
2) SA Decachlor...	10.772	9.573	1910872	674704	24.349	25.568
Target Compounds						
26) L6 AR-1254-1	7.068	6.385	3482594	1644923	1272.425m	980.939
27) L6 AR-1254-2	7.296	6.541	3220309	791870	773.361m	546.049 #
28) L6 AR-1254-3	7.676	6.962	2023688	981549	465.943m	428.601
29) L6 AR-1254-4	7.969	7.199	750820	259342	258.623m	216.886
30) L6 AR-1254-5	8.400	7.624	2116880	694184	634.129m	375.955 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032521\
Data File : PP034362.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Mar 2021 14:02
Operator : DD\AJ
Sample : M1791-09
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
GRAY-INTERIOR-BLOCK-1


Manual Integrations
APPROVED

Ankita
3/26/2021 1:13:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 03:06:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

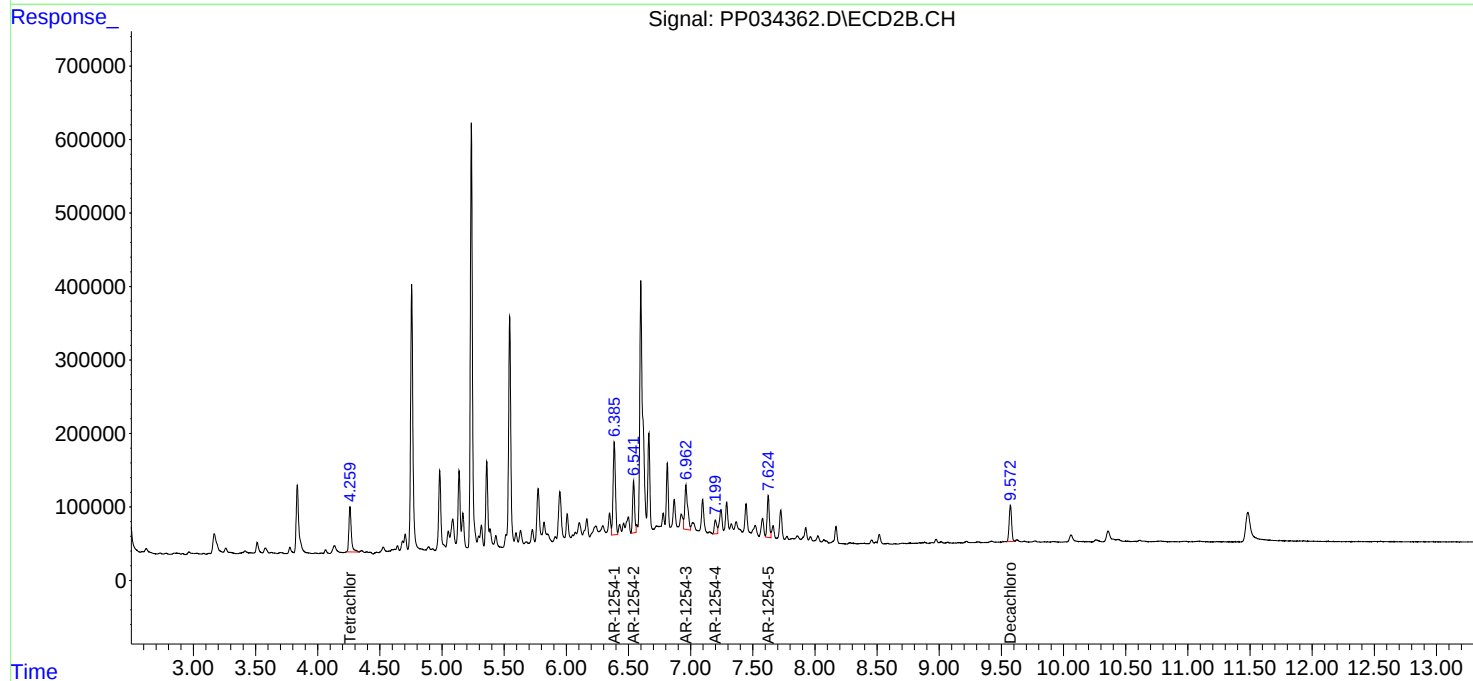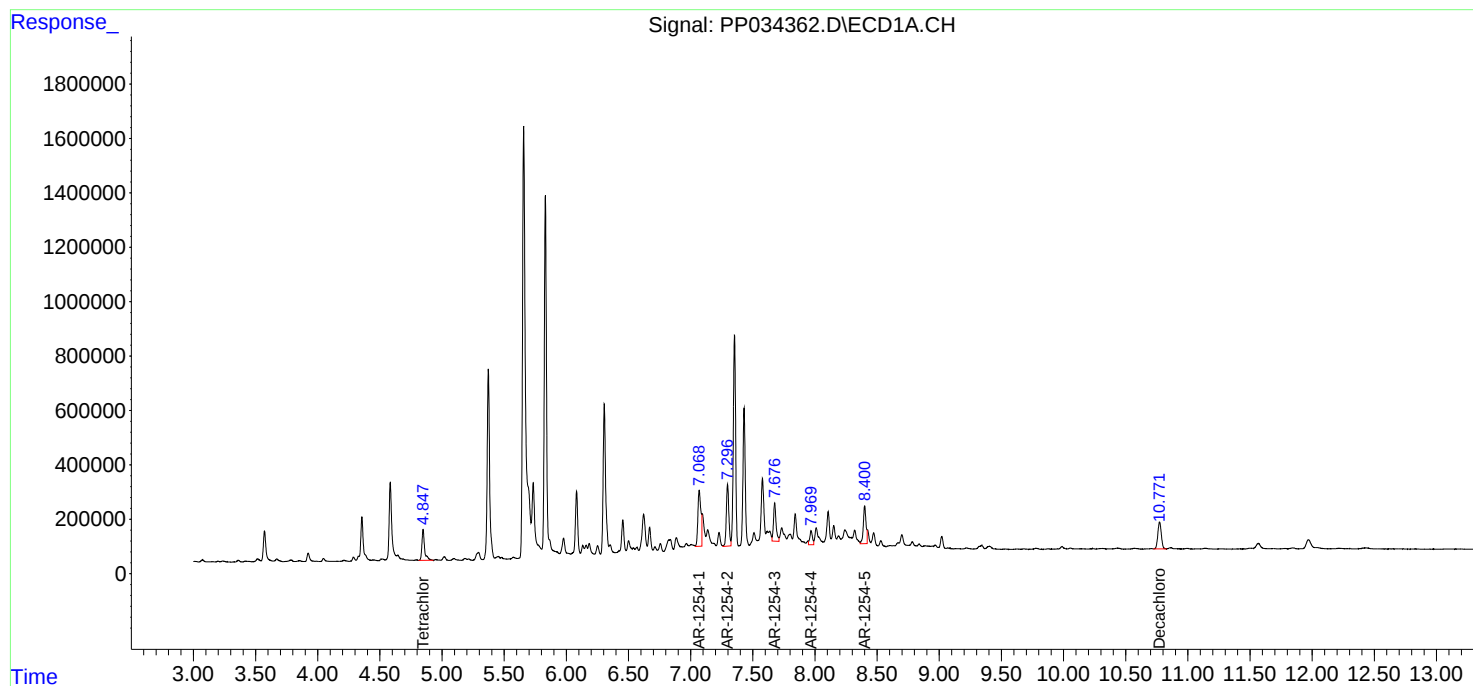

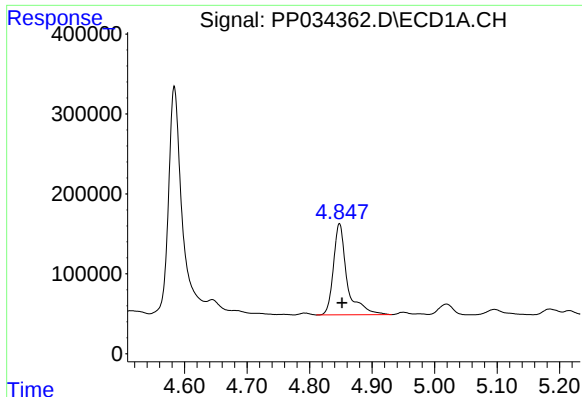


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 1738109
Conc: 20.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-INTERIOR-BLOCK-1


Manual Integrations
APPROVED

Ankita
3/26/2021 1:13:15 PM

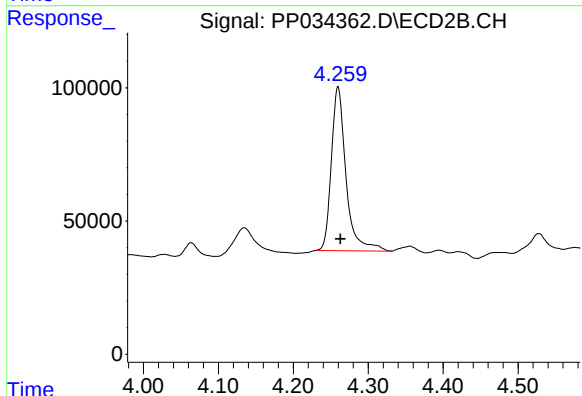


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.003 min
Response: 837615
Conc: 18.93 ng/ml

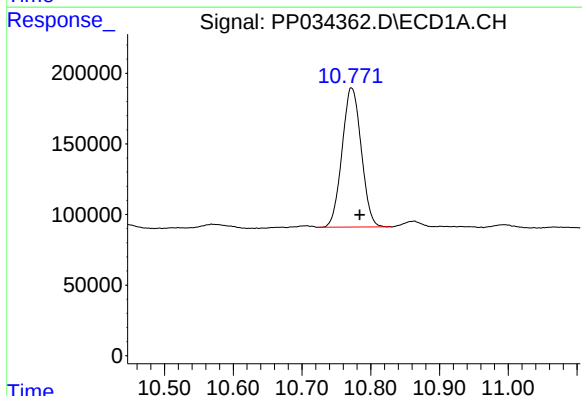


#2 Decachlorobiphenyl

R.T.: 10.772 min
Delta R.T.: -0.012 min
Response: 1910872
Conc: 24.35 ng/ml

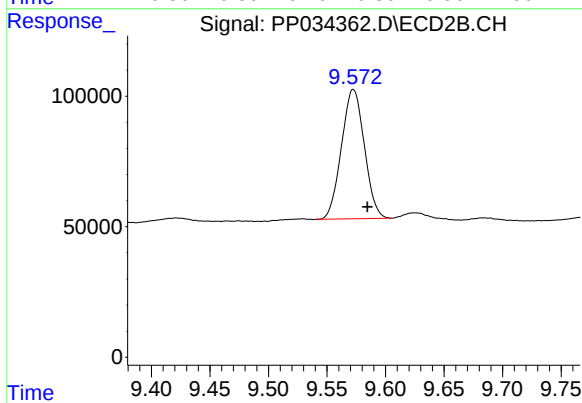

#2 Decachlorobiphenyl

R.T.: 9.573 min
Delta R.T.: -0.012 min
Response: 674704
Conc: 25.57 ng/ml

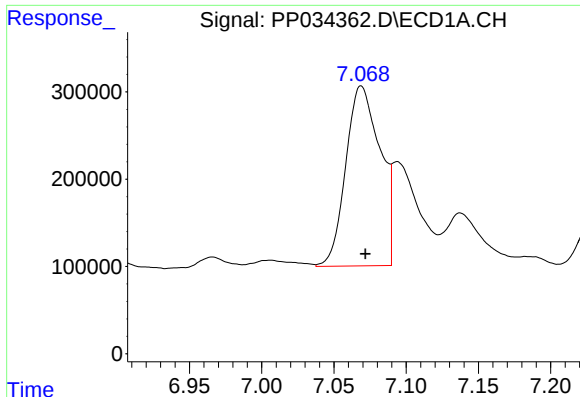


#26 AR-1254-1

R.T.: 7.068 min
Delta R.T.: -0.003 min
Response: 3482594
Conc: 1272.42 ng/ml m

Instrument :
ECD_P
ClientSampleId :
GRAY-INTERIOR-BLOCK-1


Manual Integrations
APPROVED

Ankita
3/26/2021 1:13:15 PM

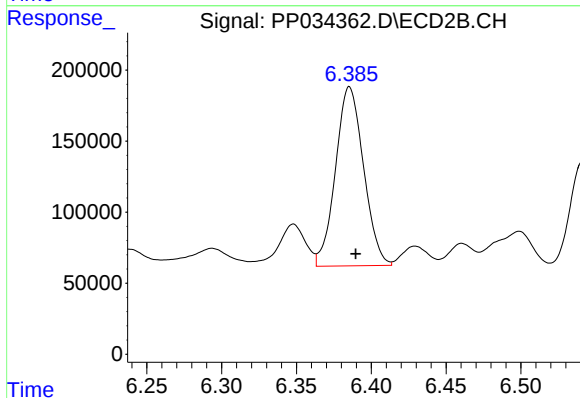


#26 AR-1254-1

R.T.: 6.385 min
Delta R.T.: -0.004 min
Response: 1644923
Conc: 980.94 ng/ml

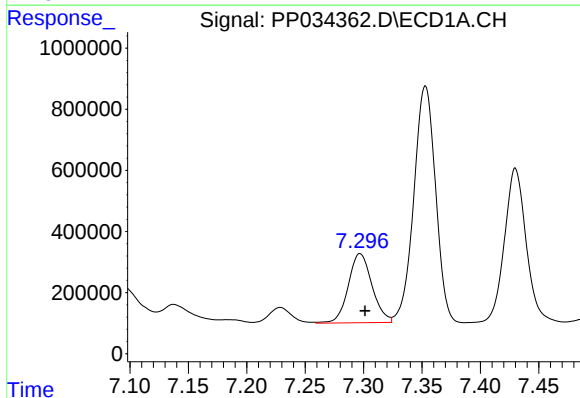


#27 AR-1254-2

R.T.: 7.296 min
Delta R.T.: -0.005 min
Response: 3220309
Conc: 773.36 ng/ml m

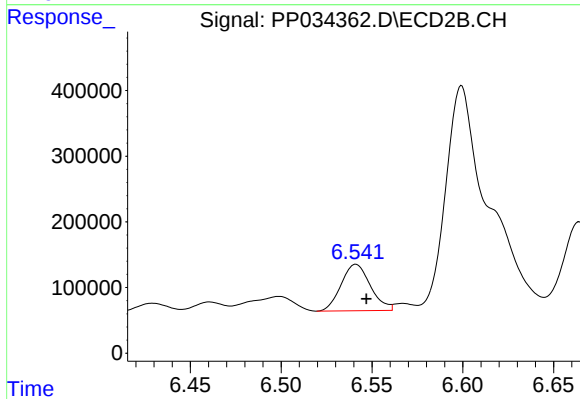

#27 AR-1254-2

R.T.: 6.541 min
Delta R.T.: -0.006 min
Response: 791870
Conc: 546.05 ng/ml

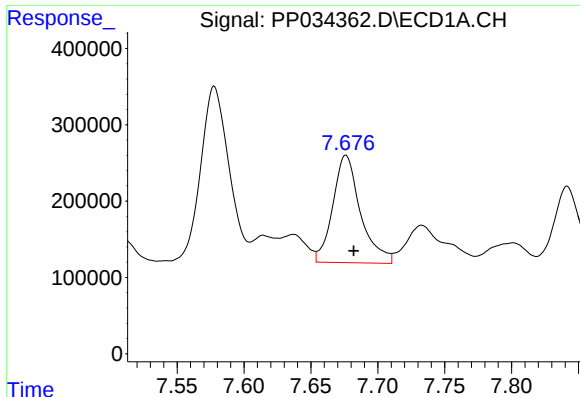


#28 AR-1254-3

R.T.: 7.676 min
Delta R.T.: -0.006 min
Response: 2023688
Conc: 465.94 ng/ml m

Instrument :
ECD_P
ClientSampleId :
GRAY-INTERIOR-BLOCK-1


Manual Integrations
APPROVED

Ankita
3/26/2021 1:13:15 PM

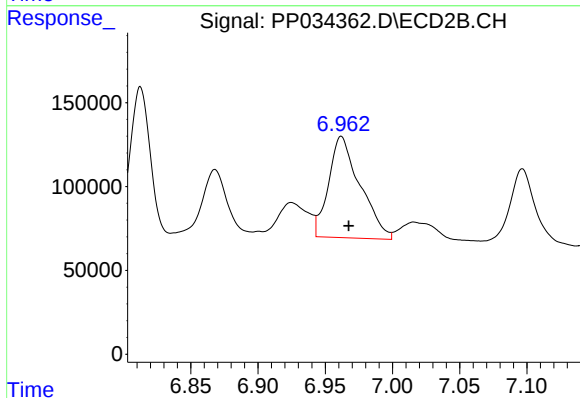


#28 AR-1254-3

R.T.: 6.962 min
Delta R.T.: -0.006 min
Response: 981549
Conc: 428.60 ng/ml

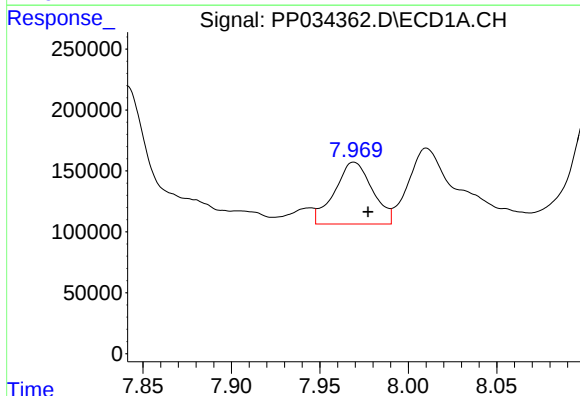


#29 AR-1254-4

R.T.: 7.969 min
Delta R.T.: -0.008 min
Response: 750820
Conc: 258.62 ng/ml m

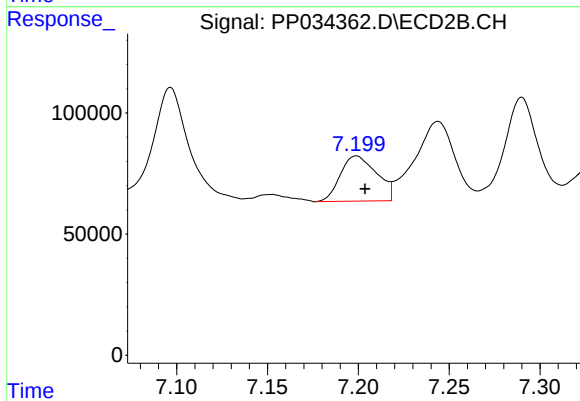

#29 AR-1254-4

R.T.: 7.199 min
Delta R.T.: -0.005 min
Response: 259342
Conc: 216.89 ng/ml

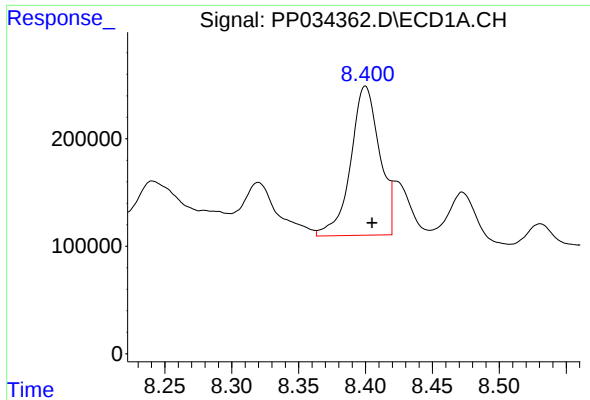


#30 AR-1254-5

R.T.: 8.400 min
Delta R.T.: -0.005 min
Response: 2116880
Conc: 634.13 ng/ml m

Instrument :
ECD_P
ClientSampleId :
GRAY-INTERIOR-BLOCK-1

Manual Integrations
APPROVED

Ankita
3/26/2021 1:13:15 PM

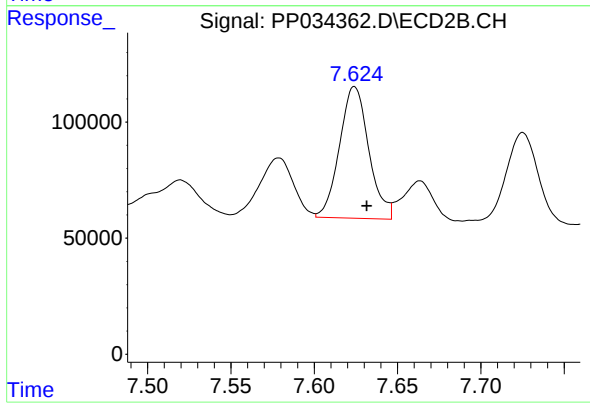

#30 AR-1254-5

R.T.: 7.624 min
Delta R.T.: -0.007 min
Response: 694184
Conc: 375.95 ng/ml