

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032521\
 Data File : PP034363.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Mar 2021 14:19
 Operator : DD\AJ
 Sample : M1791-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GRAY-INTERIOR-BLOCK-2

Manual Integrations
 APPROVED

Ankita
 3/26/2021 1:13:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 03:06:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.846	4.259	2053562	889094	24.445	20.091
2) SA Decachlor...	10.771	9.571	2031113	754839	25.882m	28.604m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032521\
Data File : PP034363.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Mar 2021 14:19
Operator : DD\AJ
Sample : M1791-11
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
GRAY-INTERIOR-BLOCK-2


Manual Integrations
APPROVED

Ankita
3/26/2021 1:13:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 03:06:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

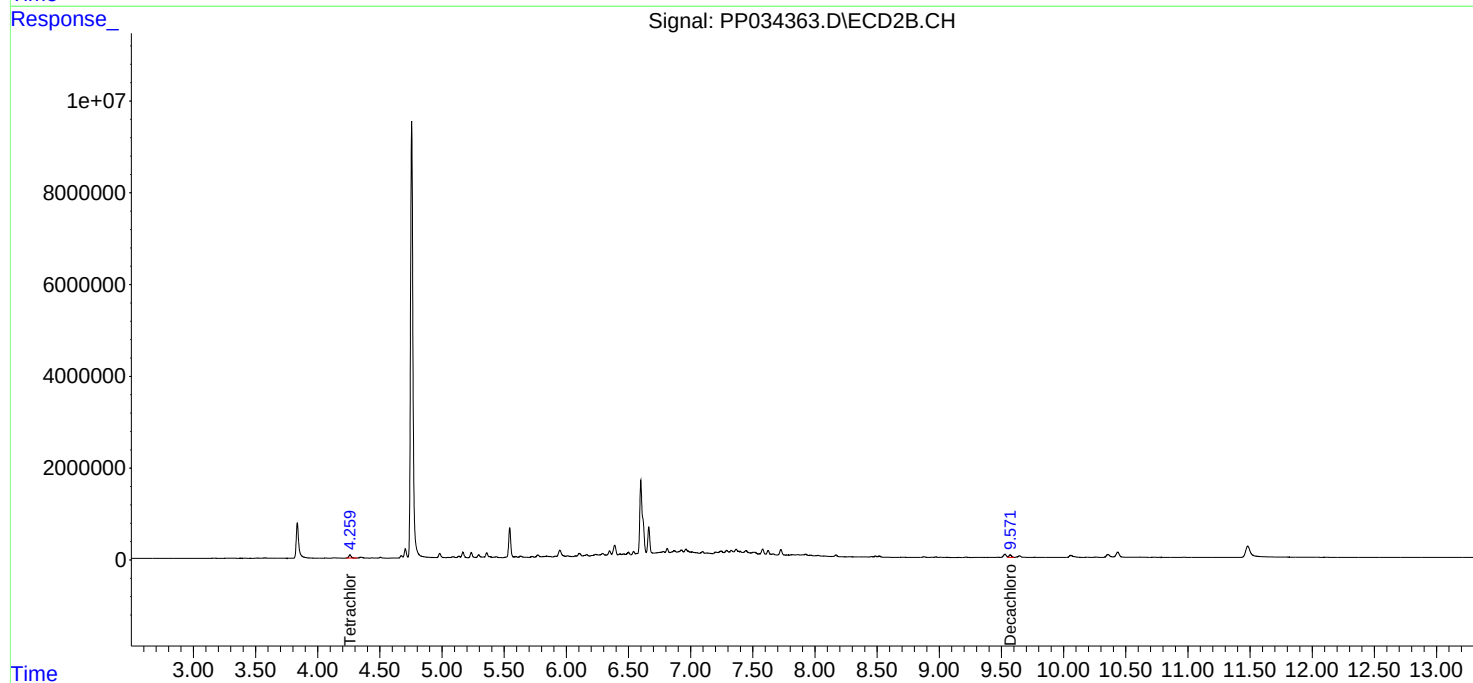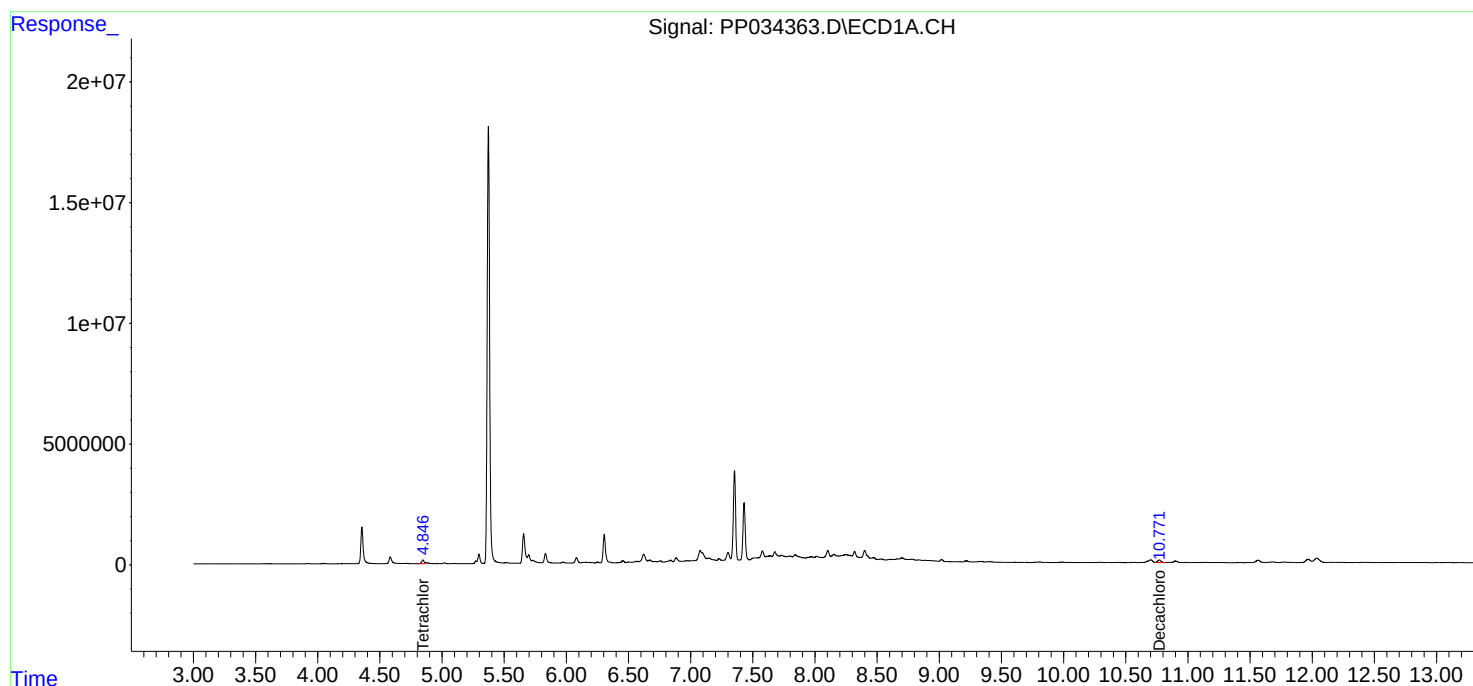

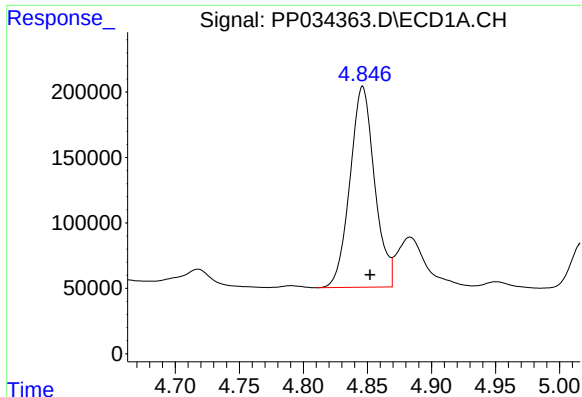


#1 Tetrachloro-m-xylene

R.T.: 4.846 min
Delta R.T.: -0.006 min
Response: 2053562
Conc: 24.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-INTERIOR-BLOCK-2


Manual Integrations
APPROVED

Ankita
3/26/2021 1:13:17 PM

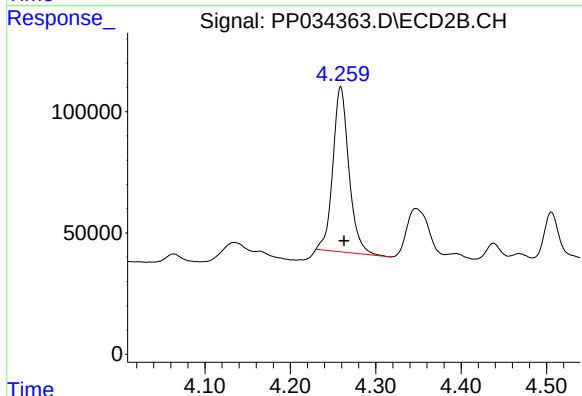


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: -0.004 min
Response: 889094
Conc: 20.09 ng/ml

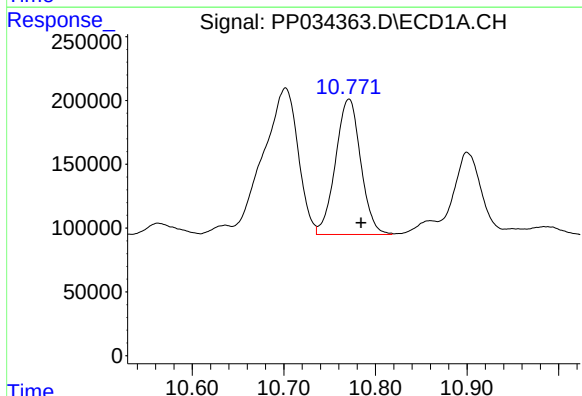

#2 Decachlorobiphenyl

R.T.: 10.771 min
Delta R.T.: -0.013 min
Response: 2031113
Conc: 25.88 ng/ml m

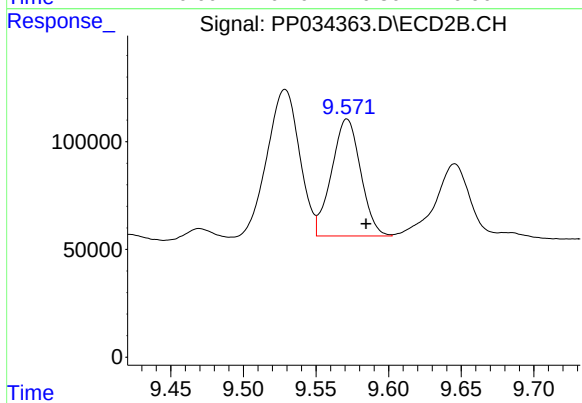

#2 Decachlorobiphenyl

R.T.: 9.571 min
Delta R.T.: -0.014 min
Response: 754839
Conc: 28.60 ng/ml m