

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032522\
 Data File : PP045196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2022 18:30
 Operator : YP\AJ
 Sample : N2143-07 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEH428B-END-2-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 21:09:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.891	3.151	4209457	3843124	2.310m	2.916m#
2) SA Decachlor...	10.015	8.508	3927257	3708637	3.051m	2.854

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032522\
Data File : PP045196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2022 18:30
Operator : YP\AJ
Sample : N2143-07 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HEH428B-END-2-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 21:09:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

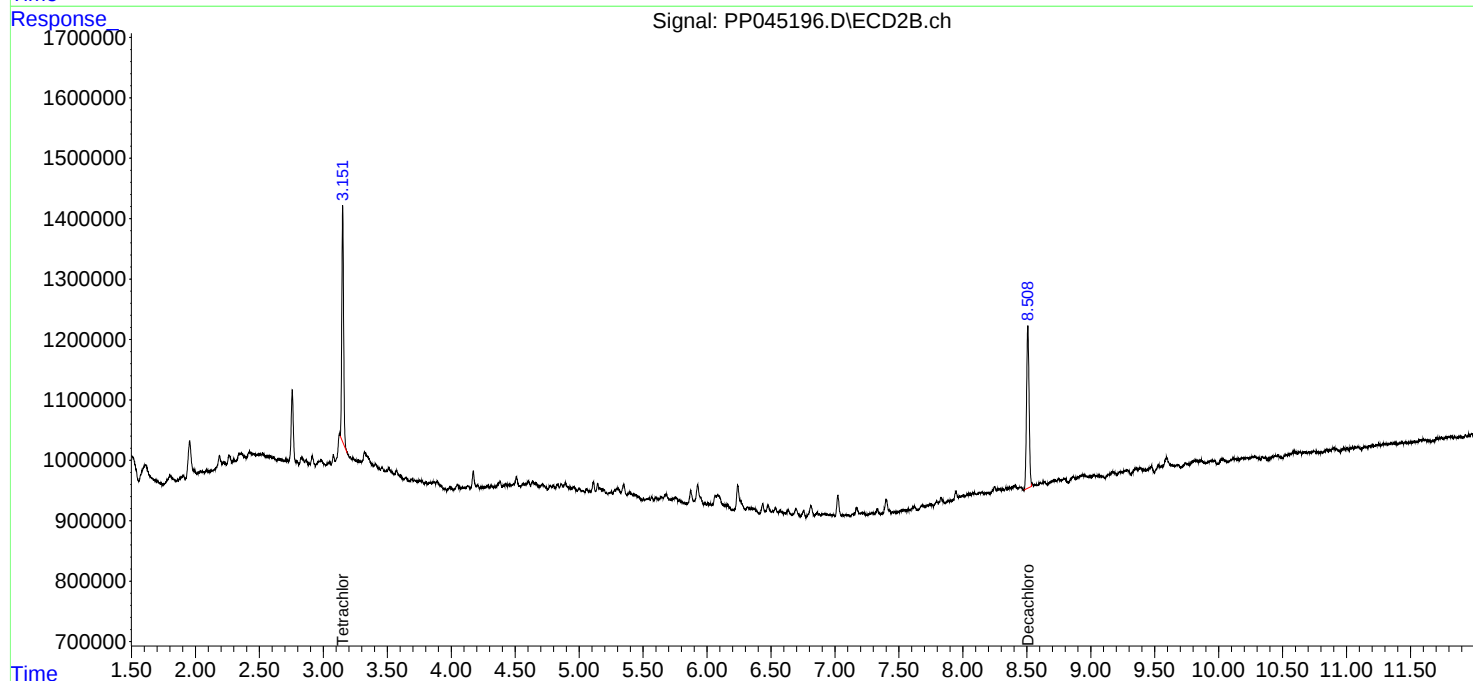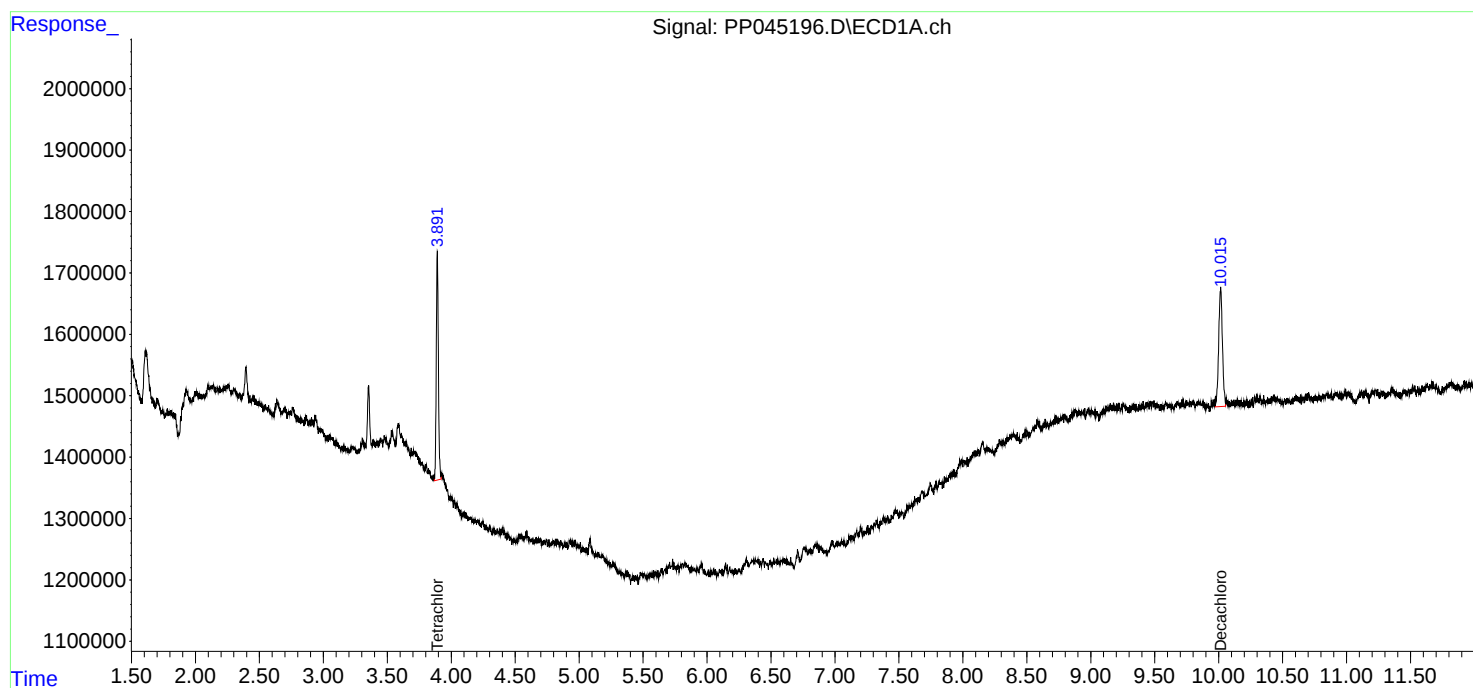

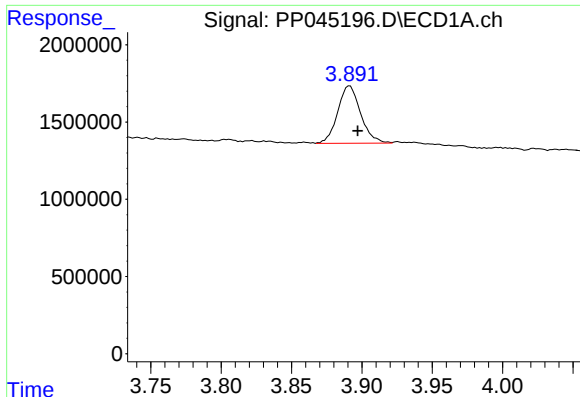


#1 Tetrachloro-m-xylene

R.T.: 3.891 min
Delta R.T.: -0.006 min
Response: 4209457
Conc: 2.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEH428B-END-2-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

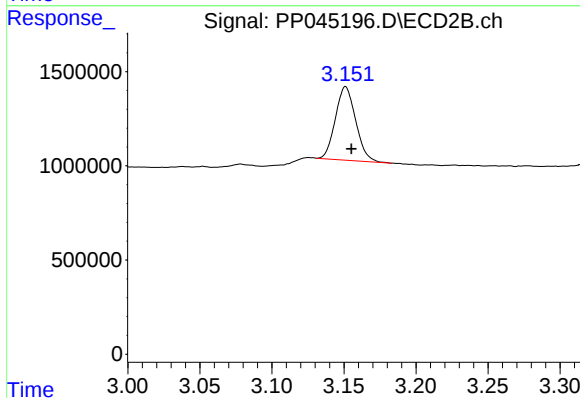


#1 Tetrachloro-m-xylene

R.T.: 3.151 min
Delta R.T.: -0.004 min
Response: 3843124
Conc: 2.92 ng/ml m

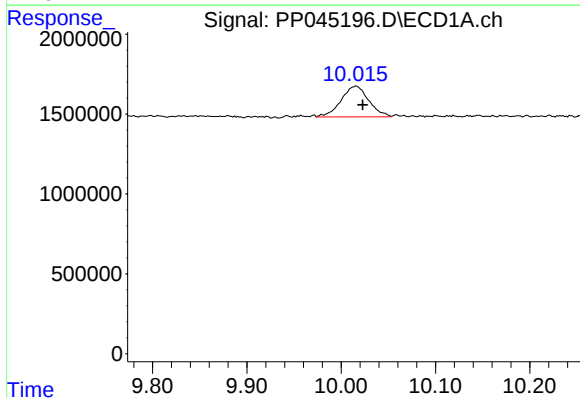

#2 Decachlorobiphenyl

R.T.: 10.015 min
Delta R.T.: -0.008 min
Response: 3927257
Conc: 3.05 ng/ml m

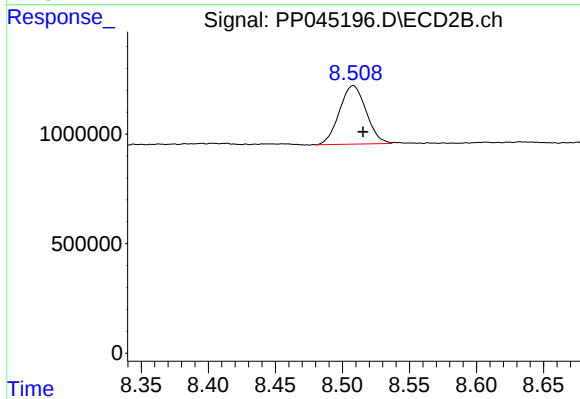

#2 Decachlorobiphenyl

R.T.: 8.508 min
Delta R.T.: -0.007 min
Response: 3708637
Conc: 2.85 ng/ml