

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032522\
 Data File : PP045200.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2022 19:31
 Operator : YP\AJ
 Sample : N2141-03 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-39A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 21:11:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.890	3.151	3272424	3180681	1.796m	2.414 #
2) SA Decachlor...	10.016	8.507	3162569	3018745	2.457m	2.323
Target Compounds						
31) L7 AR-1260-1	6.887	5.873	598344	703895	8.691	9.997
32) L7 AR-1260-2	7.169	6.082	502821	1218021	6.476	13.620 #
33) L7 AR-1260-3	7.564	6.244	255292	694303	4.057	8.152 #
34) L7 AR-1260-4	7.811	6.754	409278	335422	5.579	4.991
35) L7 AR-1260-5	8.153	7.023	722848	1027992	5.162m	6.579 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032522\
Data File : PP045200.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2022 19:31
Operator : YP\AJ
Sample : N2141-03 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CLI-2022-39A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 21:11:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

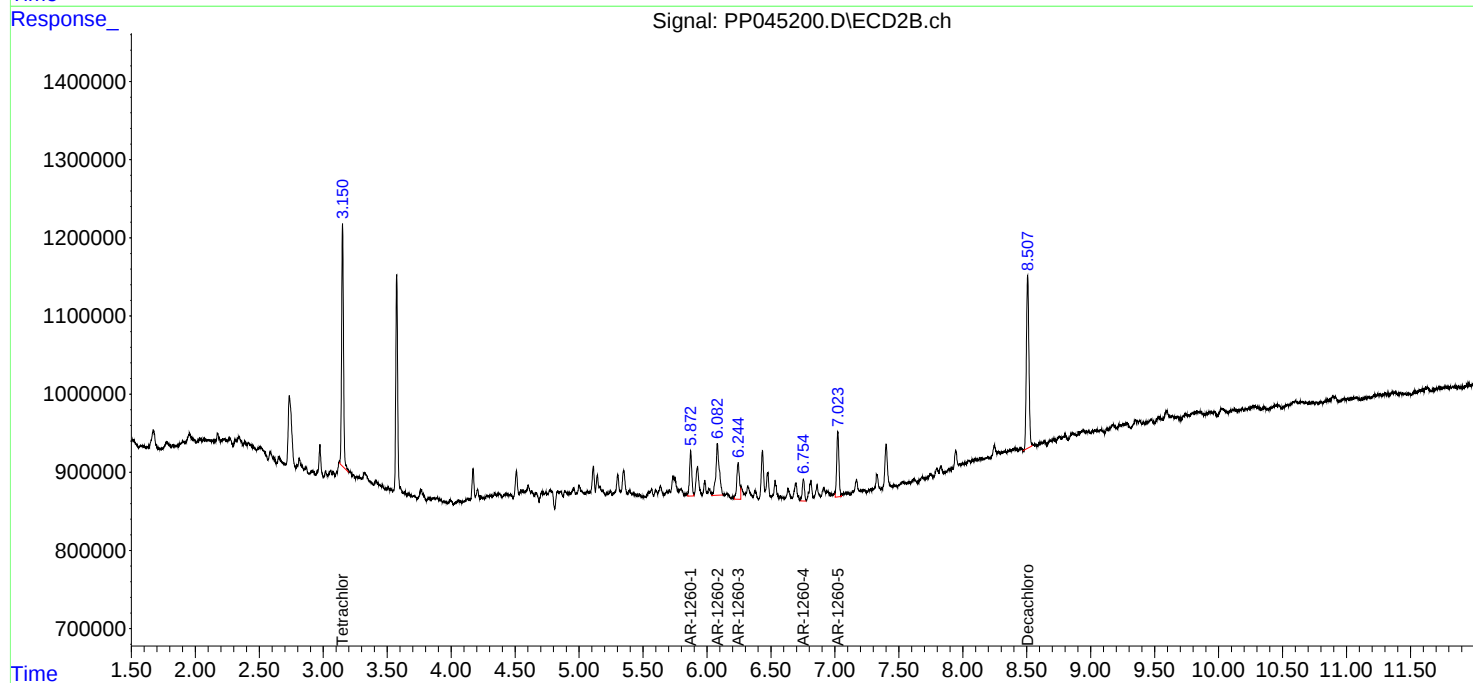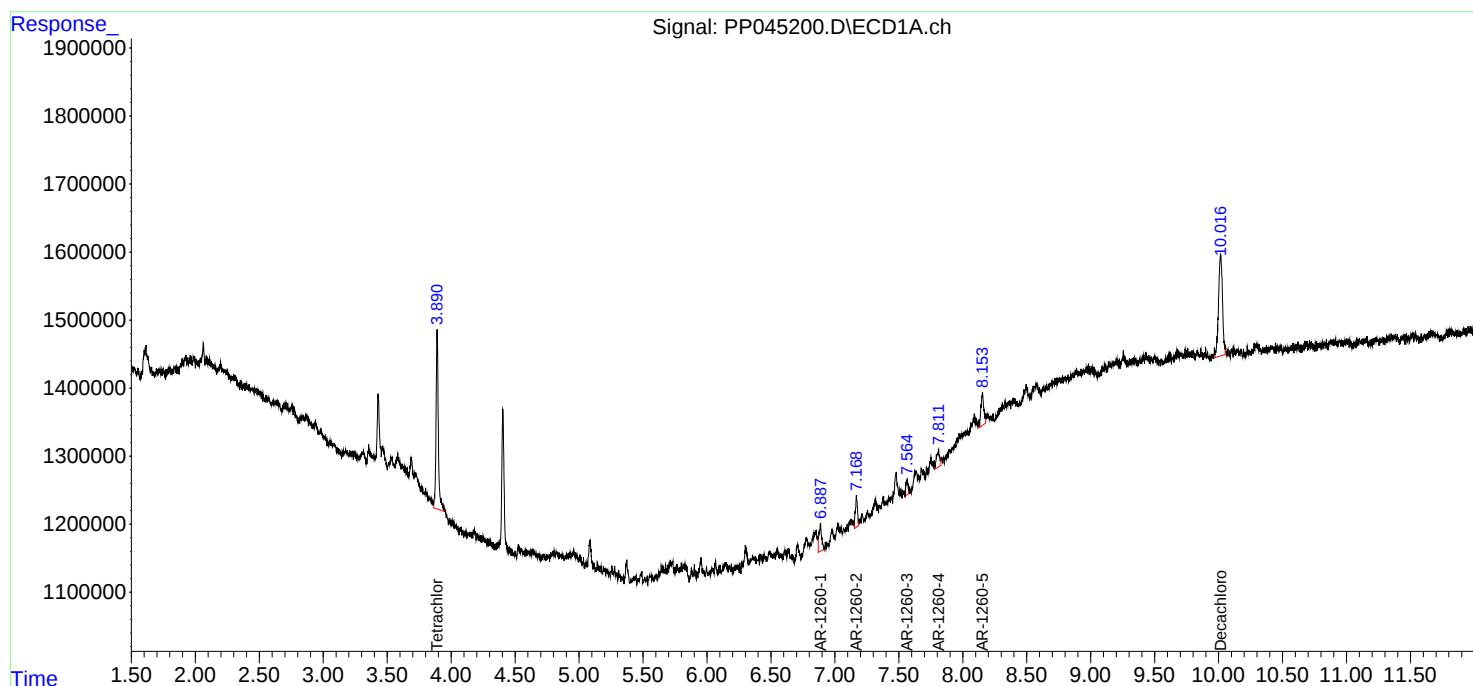

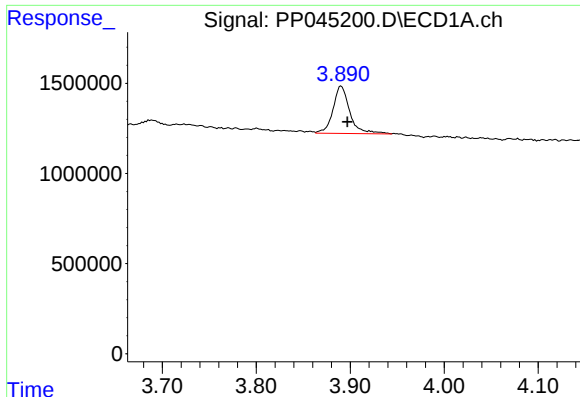


#1 Tetrachloro-m-xylene

R.T.: 3.890 min
Delta R.T.: -0.007 min
Response: 3272424
Conc: 1.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-39A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

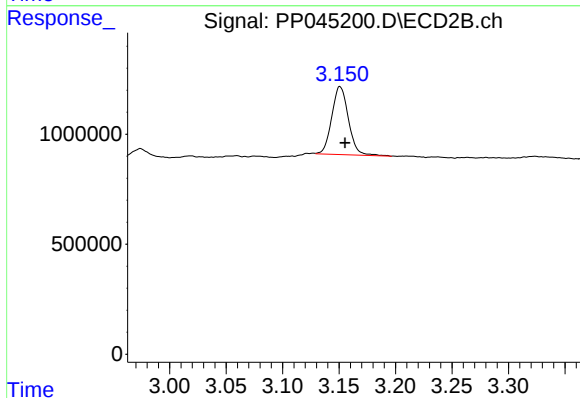


#1 Tetrachloro-m-xylene

R.T.: 3.151 min
Delta R.T.: -0.004 min
Response: 3180681
Conc: 2.41 ng/ml

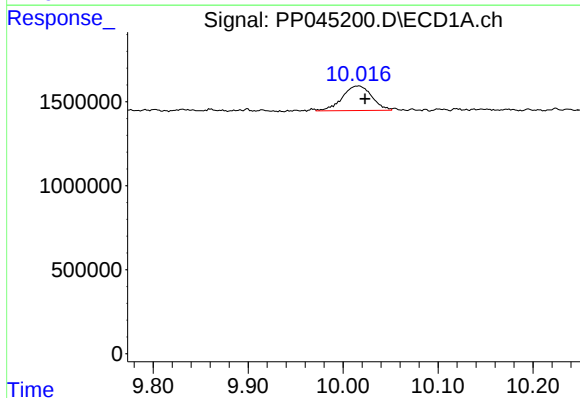


#2 Decachlorobiphenyl

R.T.: 10.016 min
Delta R.T.: -0.007 min
Response: 3162569
Conc: 2.46 ng/ml m

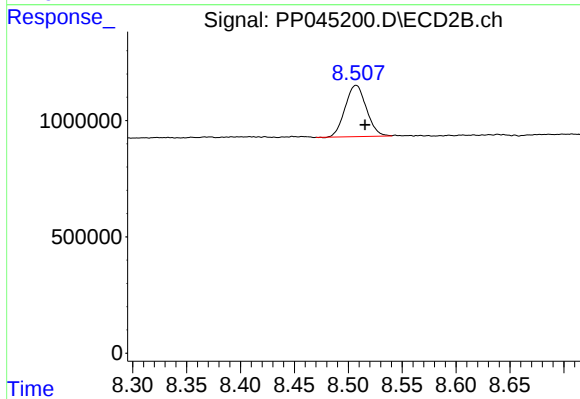

#2 Decachlorobiphenyl

R.T.: 8.507 min
Delta R.T.: -0.008 min
Response: 3018745
Conc: 2.32 ng/ml

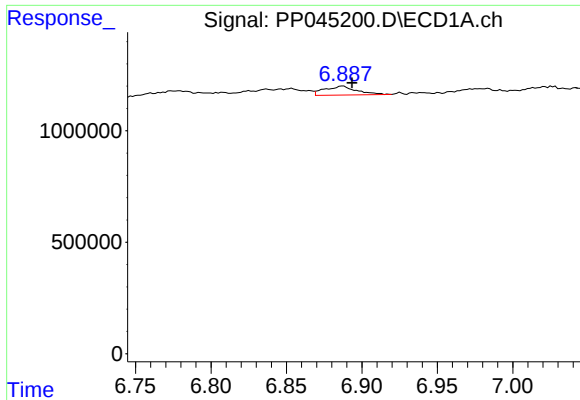


#31 AR-1260-1

R.T.: 6.887 min
Delta R.T.: -0.006 min
Response: 598344
Conc: 8.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-39A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

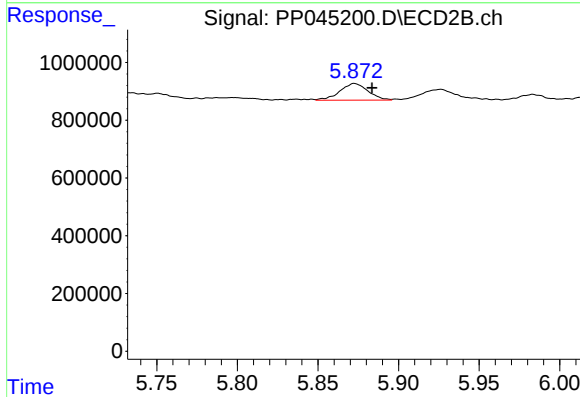


#31 AR-1260-1

R.T.: 5.873 min
Delta R.T.: -0.011 min
Response: 703895
Conc: 10.00 ng/ml

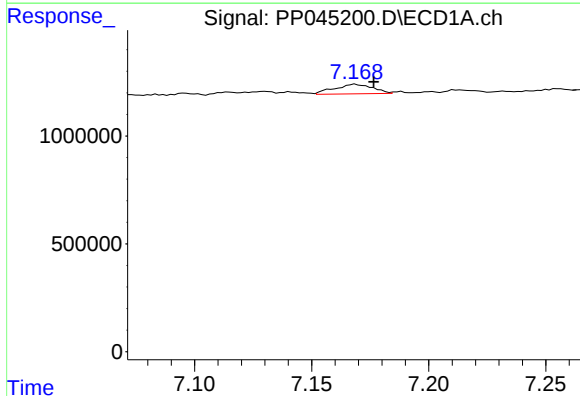


#32 AR-1260-2

R.T.: 7.169 min
Delta R.T.: -0.008 min
Response: 502821
Conc: 6.48 ng/ml

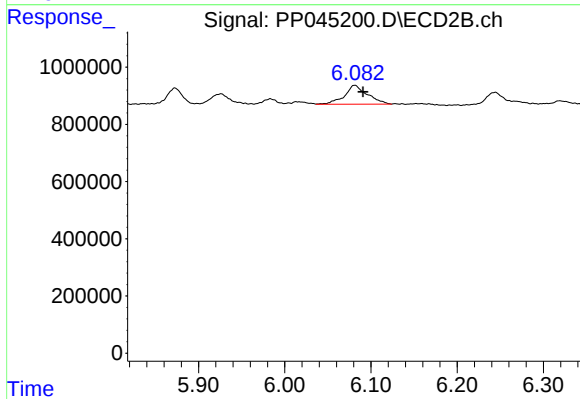

#32 AR-1260-2

R.T.: 6.082 min
Delta R.T.: -0.009 min
Response: 1218021
Conc: 13.62 ng/ml

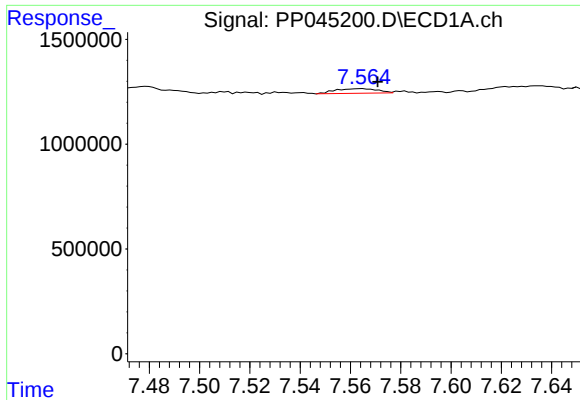


#33 AR-1260-3

R.T.: 7.564 min
Delta R.T.: -0.006 min
Response: 255292
Conc: 4.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-39A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

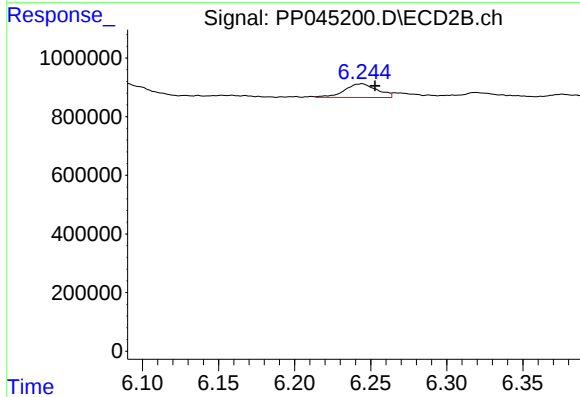


#33 AR-1260-3

R.T.: 6.244 min
Delta R.T.: -0.008 min
Response: 694303
Conc: 8.15 ng/ml

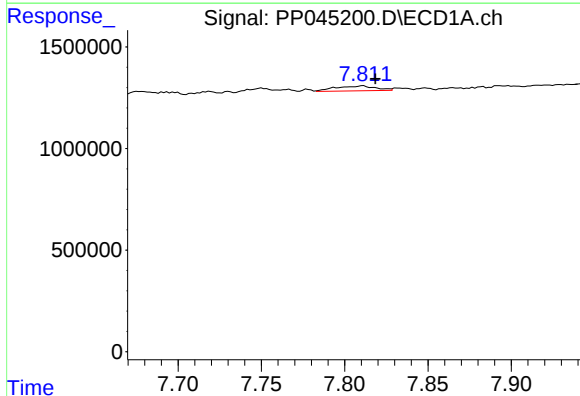


#34 AR-1260-4

R.T.: 7.811 min
Delta R.T.: -0.007 min
Response: 409278
Conc: 5.58 ng/ml

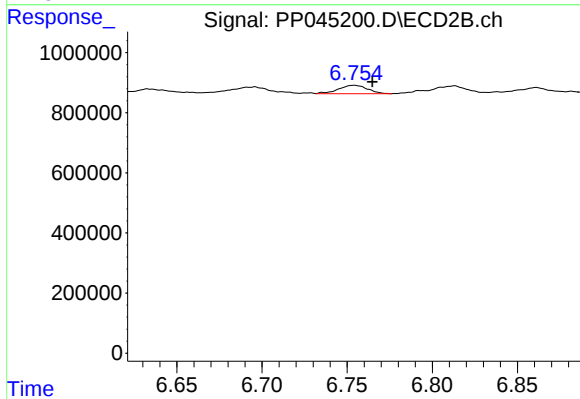

#34 AR-1260-4

R.T.: 6.754 min
Delta R.T.: -0.011 min
Response: 335422
Conc: 4.99 ng/ml

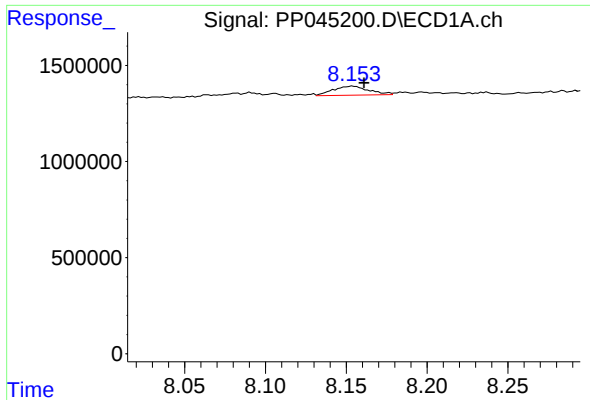


#35 AR-1260-5

R.T.: 8.153 min
Delta R.T.: -0.008 min
Response: 722848
Conc: 5.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-39A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

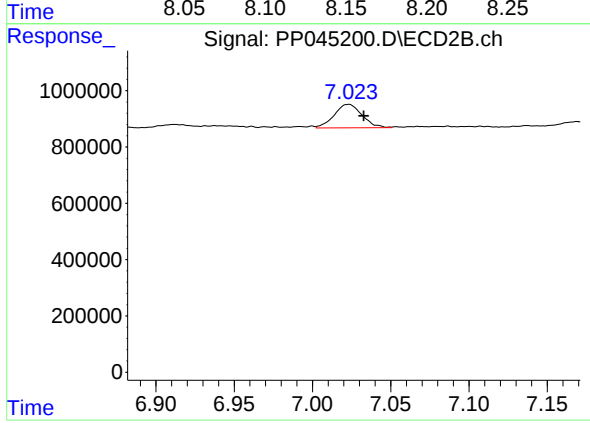

#35 AR-1260-5

R.T.: 7.023 min
Delta R.T.: -0.010 min
Response: 1027992
Conc: 6.58 ng/ml