

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032522\
 Data File : PP045201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2022 19:47
 Operator : YP\AJ
 Sample : N2141-04 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-39B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 21:12:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.890	3.150	2993860	3102244	1.643m	2.354m#
2) SA Decachlor...	10.016	8.506	3327524	3149768	2.585m	2.424
Target Compounds						
26) L6 AR-1254-1	6.068	5.144	311999	508396	4.699	5.879 #
27) L6 AR-1254-2	6.305	5.303	699016	598114	6.996	8.038m
28) L6 AR-1254-3	6.705	5.735	510363	652719	4.990	5.681m
29) L6 AR-1254-4	7.023	5.983	406834	422178	5.593	5.663
30) L6 AR-1254-5	7.480	6.434	633221	942219	8.187	9.150

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032522\
Data File : PP045201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2022 19:47
Operator : YP\AJ
Sample : N2141-04 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CLI-2022-39B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 21:12:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

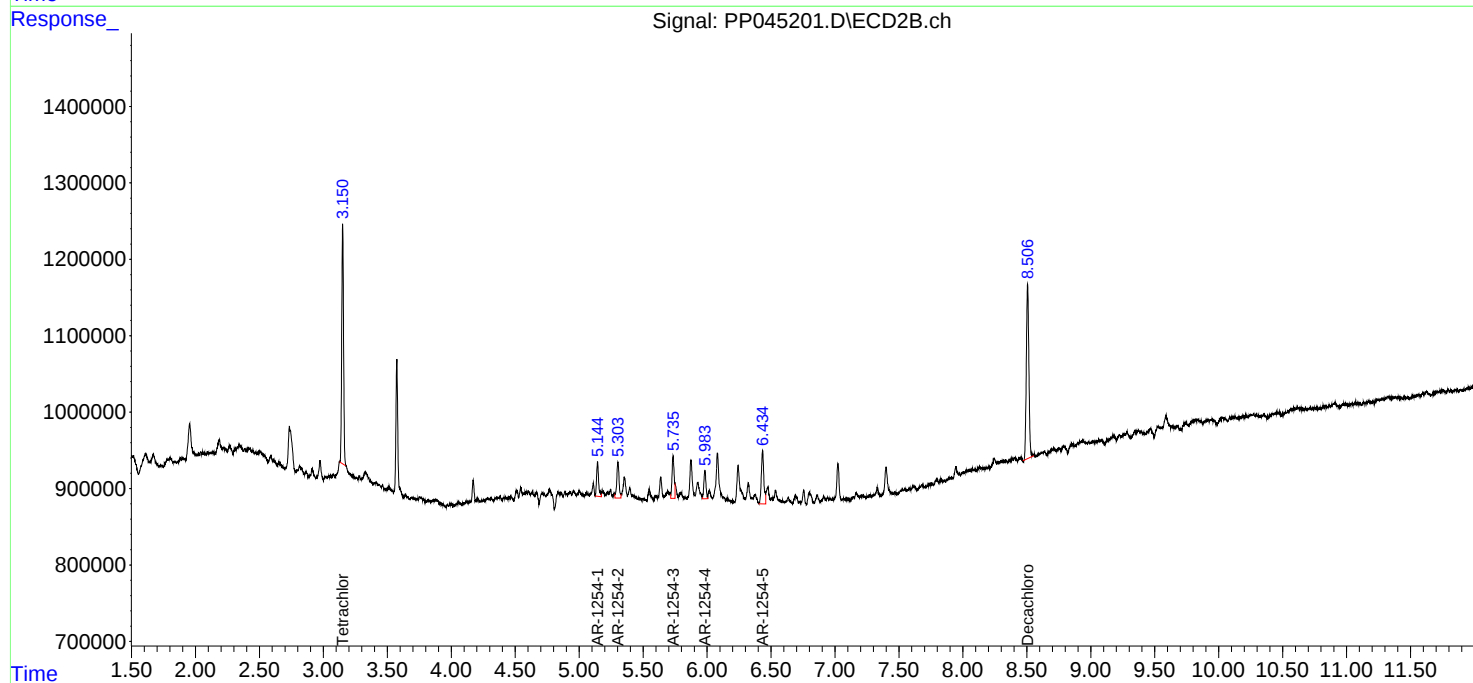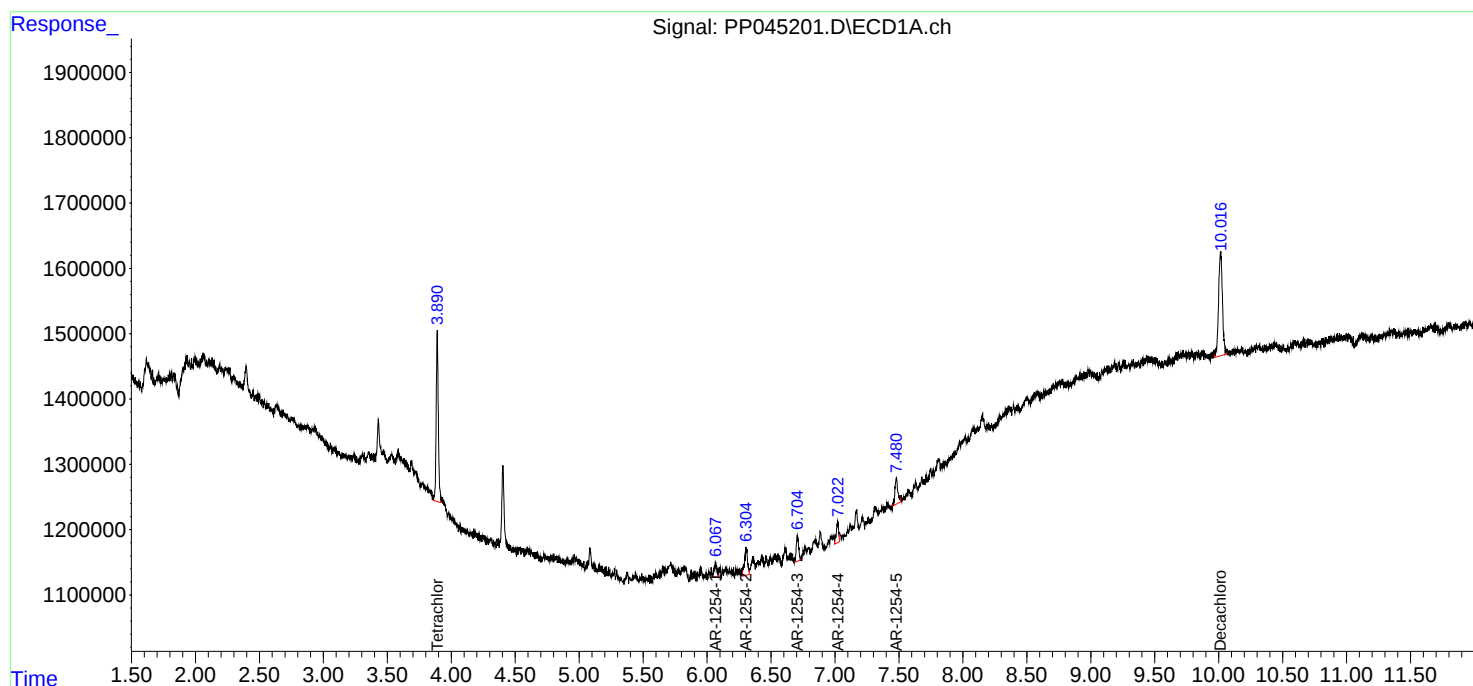

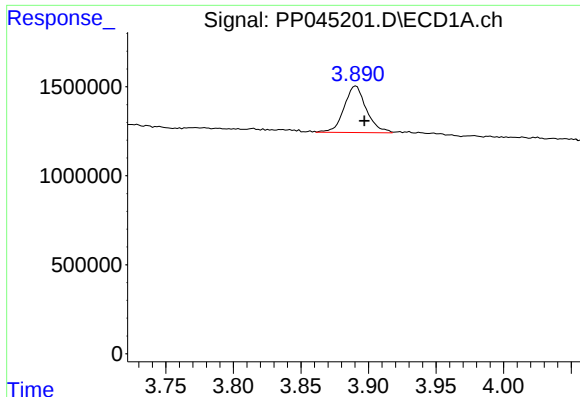


#1 Tetrachloro-m-xylene

R.T.: 3.890 min
Delta R.T.: -0.007 min
Response: 2993860
Conc: 1.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-39B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

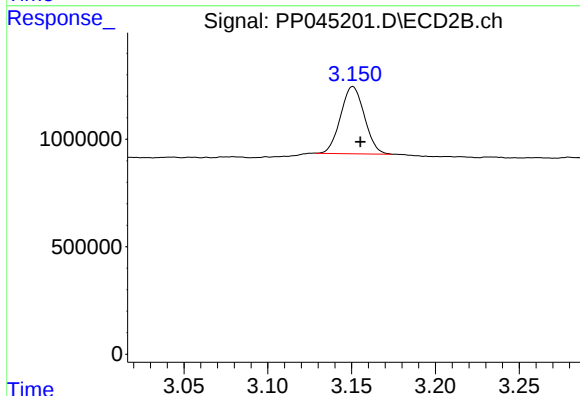


#1 Tetrachloro-m-xylene

R.T.: 3.150 min
Delta R.T.: -0.005 min
Response: 3102244
Conc: 2.35 ng/ml m

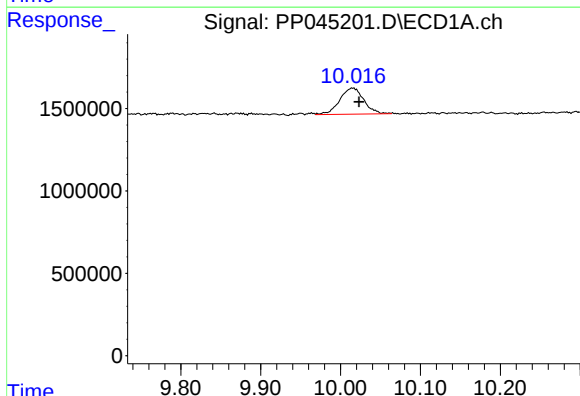


#2 Decachlorobiphenyl

R.T.: 10.016 min
Delta R.T.: -0.007 min
Response: 3327524
Conc: 2.58 ng/ml m

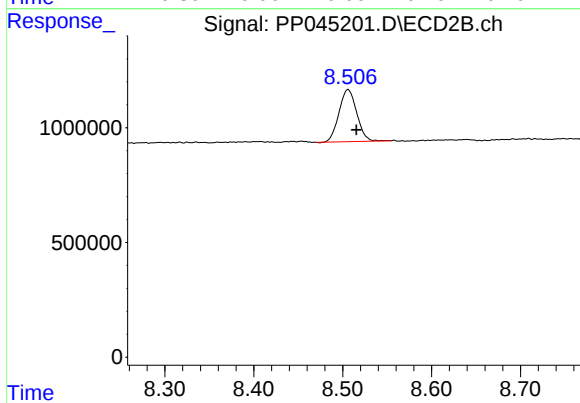

#2 Decachlorobiphenyl

R.T.: 8.506 min
Delta R.T.: -0.009 min
Response: 3149768
Conc: 2.42 ng/ml

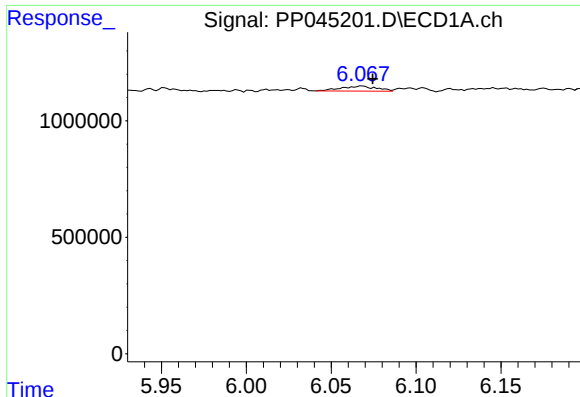


#26 AR-1254-1

R.T.: 6.068 min
Delta R.T.: -0.006 min
Response: 311999
Conc: 4.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-39B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

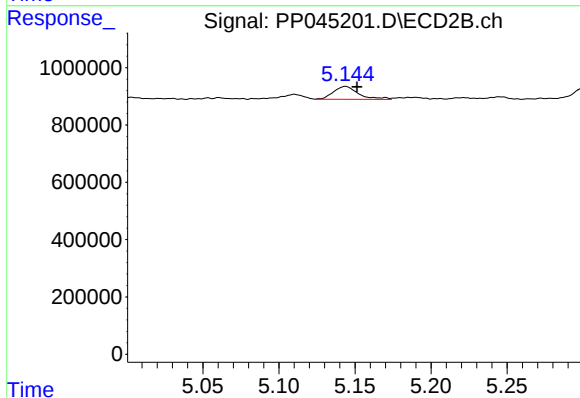


#26 AR-1254-1

R.T.: 5.144 min
Delta R.T.: -0.008 min
Response: 508396
Conc: 5.88 ng/ml

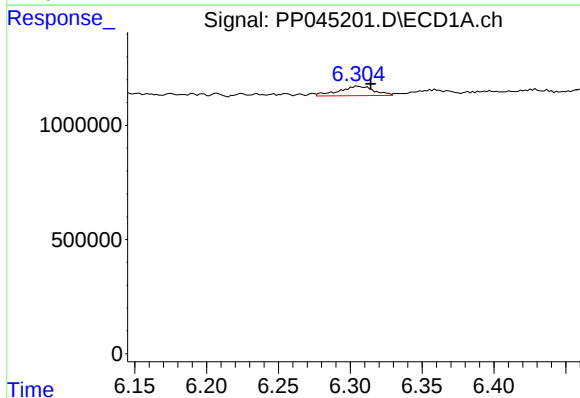


#27 AR-1254-2

R.T.: 6.305 min
Delta R.T.: -0.009 min
Response: 699016
Conc: 7.00 ng/ml

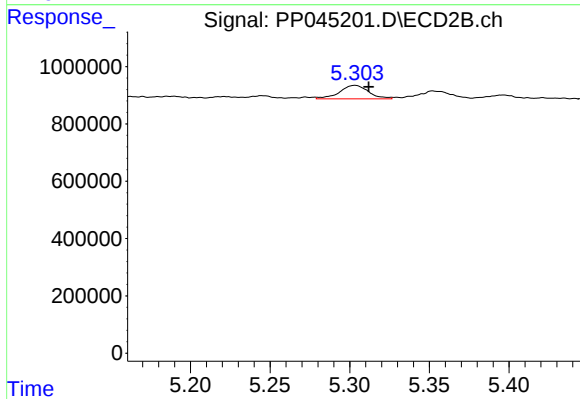

#27 AR-1254-2

R.T.: 5.303 min
Delta R.T.: -0.009 min
Response: 598114
Conc: 8.04 ng/ml m

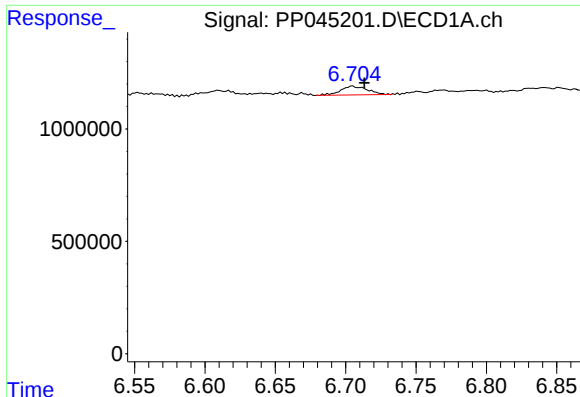


#28 AR-1254-3

R.T.: 6.705 min
Delta R.T.: -0.008 min
Response: 510363
Conc: 4.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-39B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

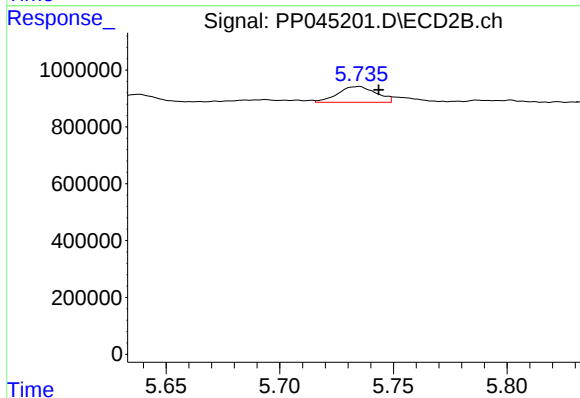


#28 AR-1254-3

R.T.: 5.735 min
Delta R.T.: -0.009 min
Response: 652719
Conc: 5.68 ng/ml m

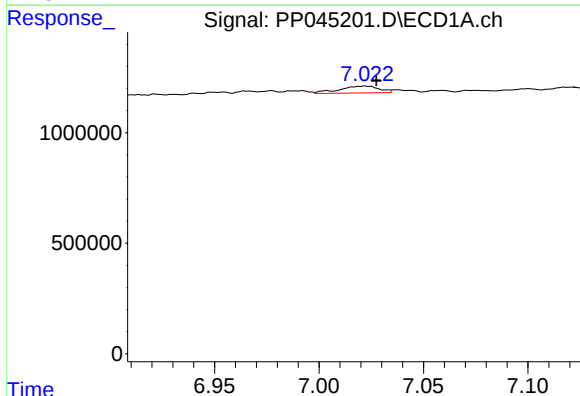


#29 AR-1254-4

R.T.: 7.023 min
Delta R.T.: -0.005 min
Response: 406834
Conc: 5.59 ng/ml

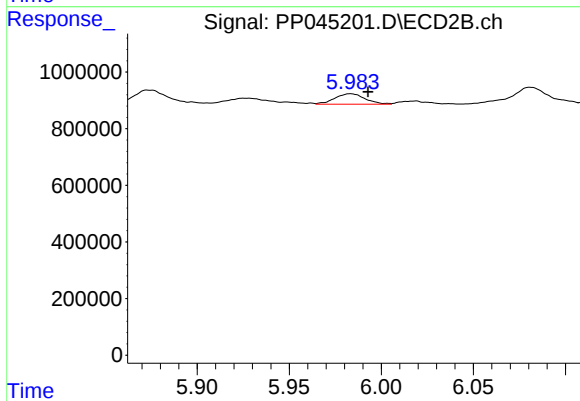

#29 AR-1254-4

R.T.: 5.983 min
Delta R.T.: -0.009 min
Response: 422178
Conc: 5.66 ng/ml

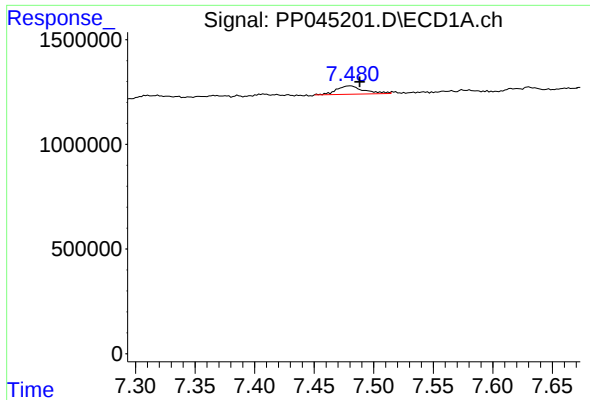


#30 AR-1254-5

R.T.: 7.480 min
Delta R.T.: -0.008 min
Response: 633221
Conc: 8.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-39B

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

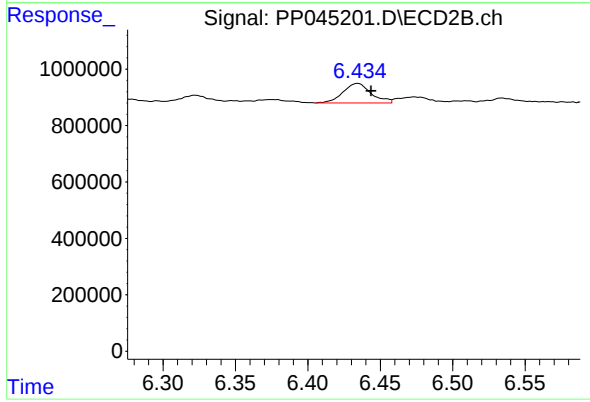

#30 AR-1254-5

R.T.: 6.434 min
Delta R.T.: -0.009 min
Response: 942219
Conc: 9.15 ng/ml