

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032522\
 Data File : PP045224.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2022 06:23
 Operator : YP\AJ
 Sample : N2095-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-06-4.0-5.0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 01:06:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.890	3.151	47186725	34154870	25.898	25.917
2) SA Decachlor...	10.009	8.502	29579169	25690544	22.978	19.771

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032522\
Data File : PP045224.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2022 06:23
Operator : YP\AJ
Sample : N2095-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SB-06-4.0-5.0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 01:06:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

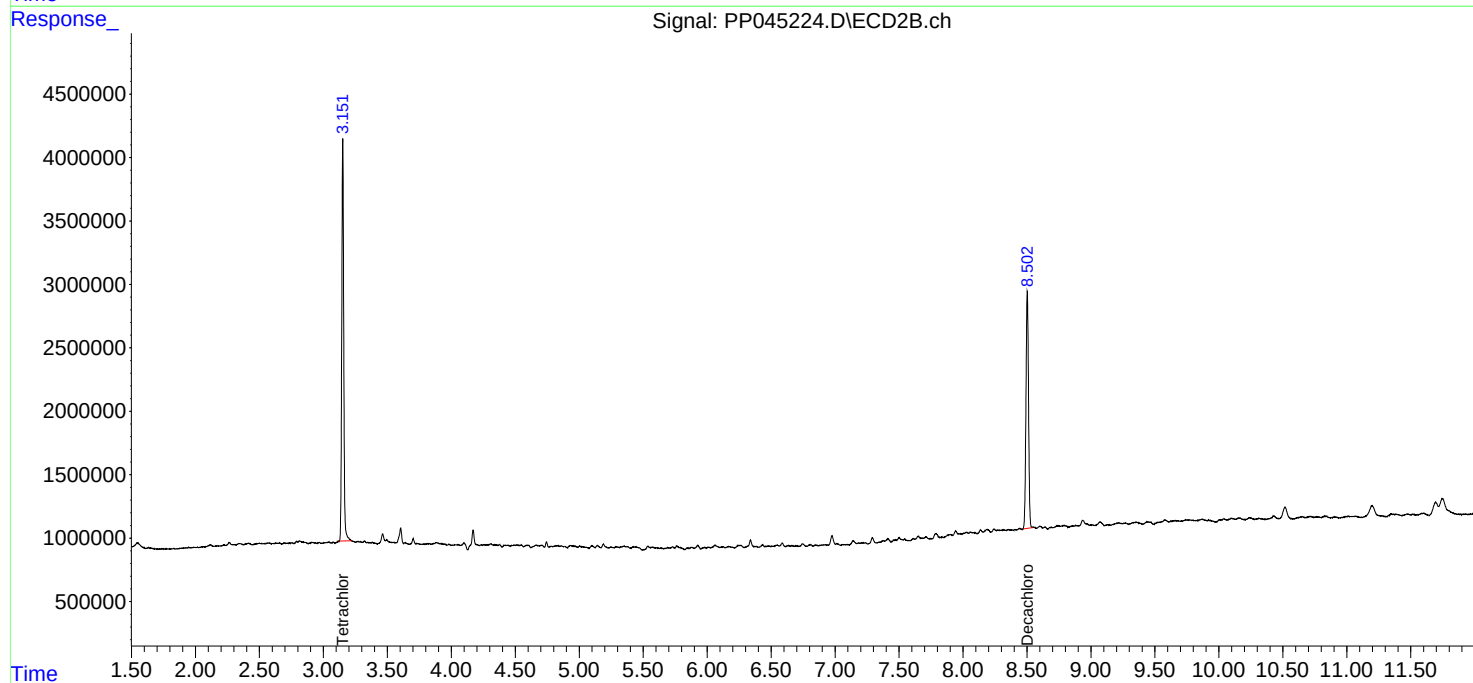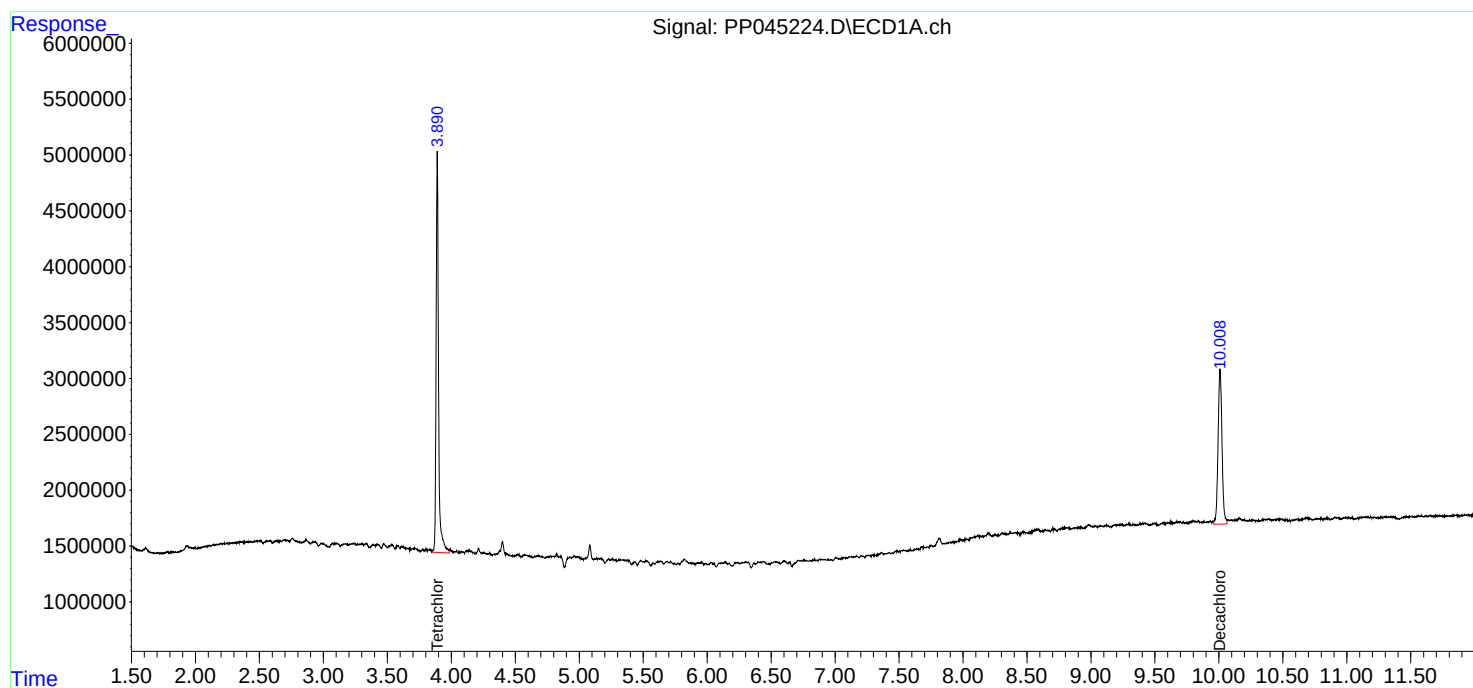


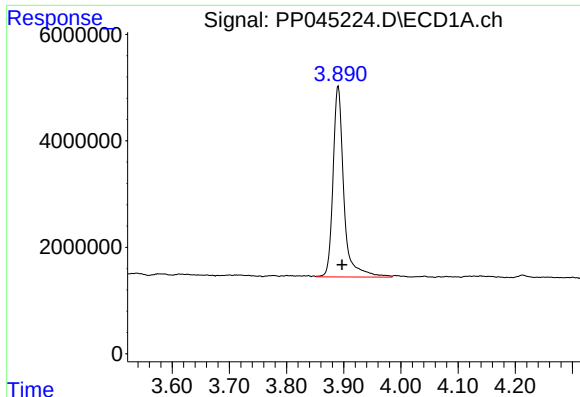

#1 Tetrachloro-m-xylene


R.T.: 3.890 min
Delta R.T.: -0.007 min
Response: 47186725
Conc: 25.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-06-4.0-5.0

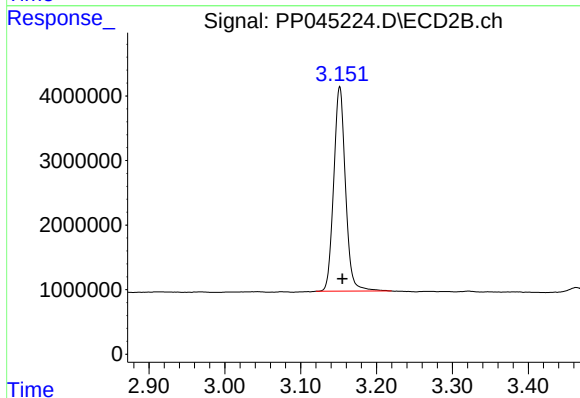


#1 Tetrachloro-m-xylene

R.T.: 3.151 min
Delta R.T.: -0.004 min
Response: 34154870
Conc: 25.92 ng/ml

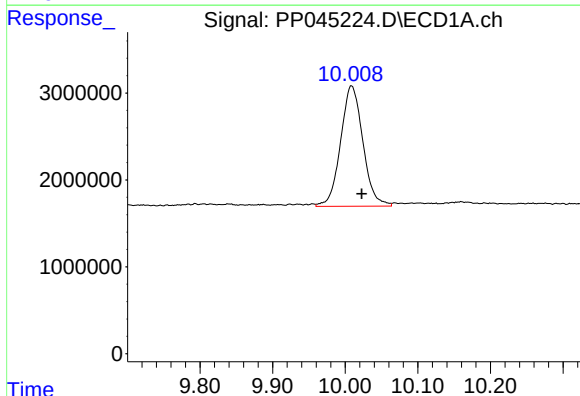

#2 Decachlorobiphenyl

R.T.: 10.009 min
Delta R.T.: -0.014 min
Response: 29579169
Conc: 22.98 ng/ml

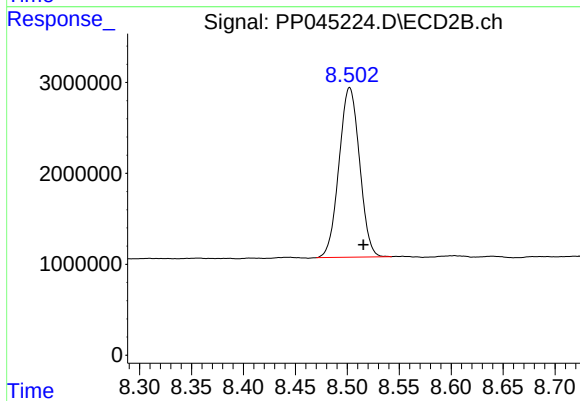

#2 Decachlorobiphenyl

R.T.: 8.502 min
Delta R.T.: -0.013 min
Response: 25690544
Conc: 19.77 ng/ml