

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032522\
 Data File : PP045244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2022 13:26
 Operator : YP\AJ
 Sample : N2125-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RO-124030

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 01:43:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.890	3.152	26618194	23589633	14.609m	17.900m
2) SA Decachlor...	10.008f	8.501	17395858	18150387	13.514m	13.969m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032522\
Data File : PP045244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2022 13:26
Operator : YP\AJ
Sample : N2125-01
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RO-124030


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 01:43:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

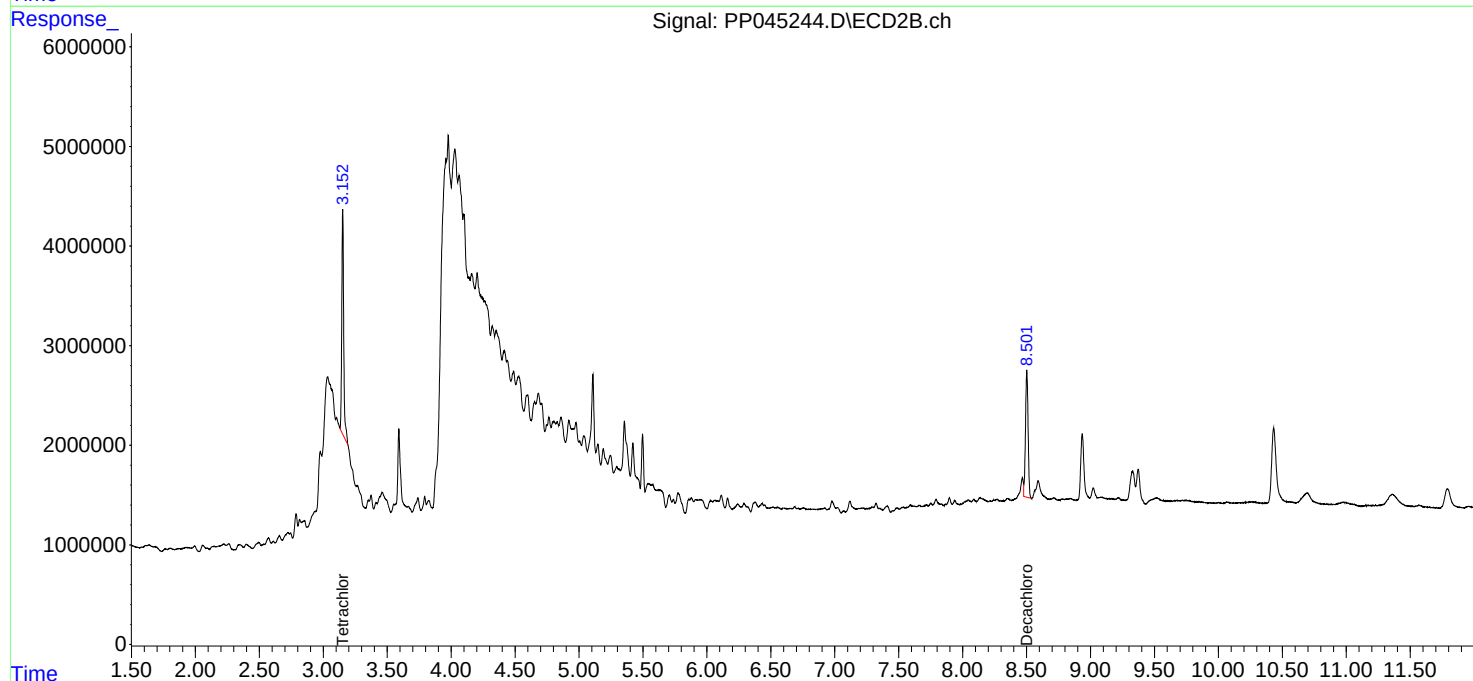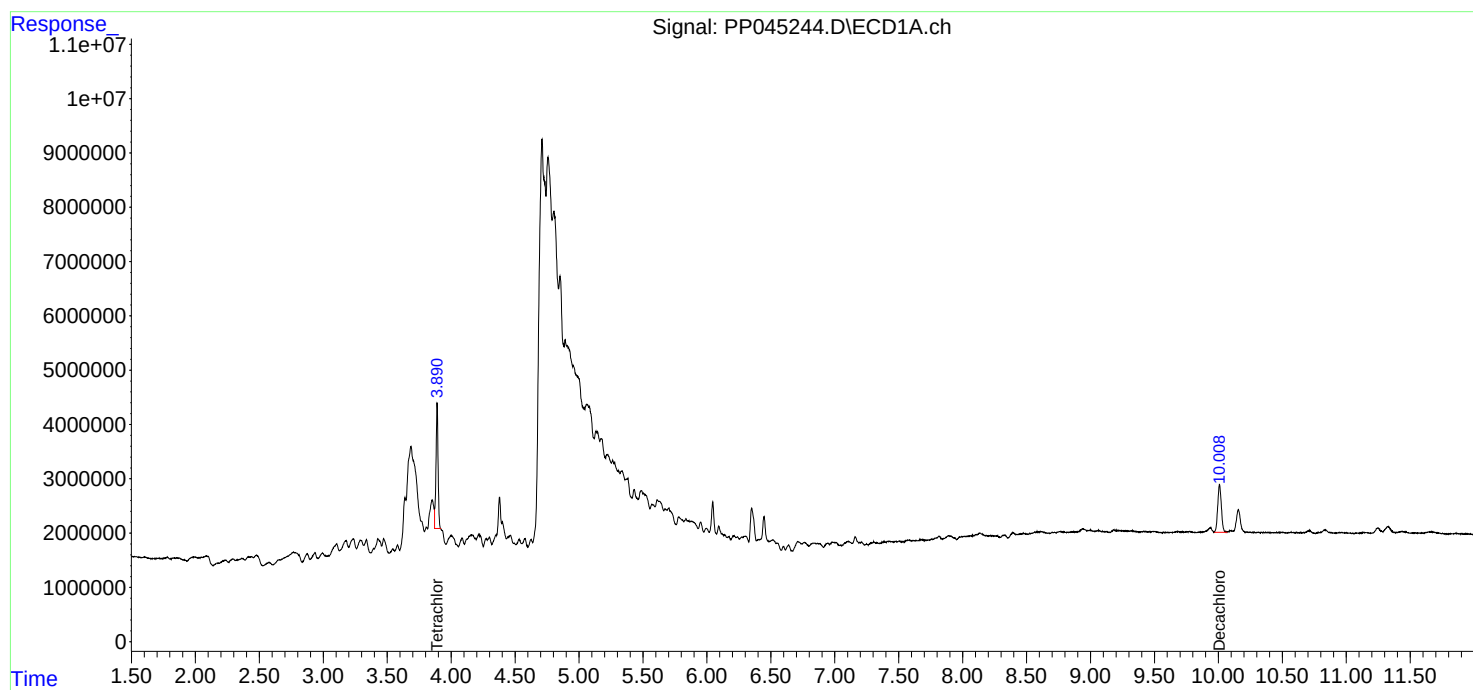

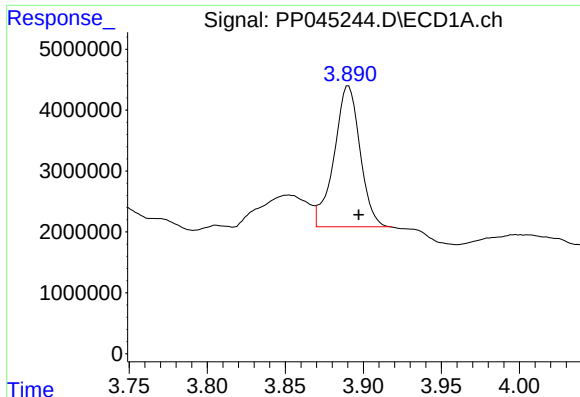


#1 Tetrachloro-m-xylene

R.T.: 3.890 min
Delta R.T.: -0.007 min
Response: 26618194
Conc: 14.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
RO-124030


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

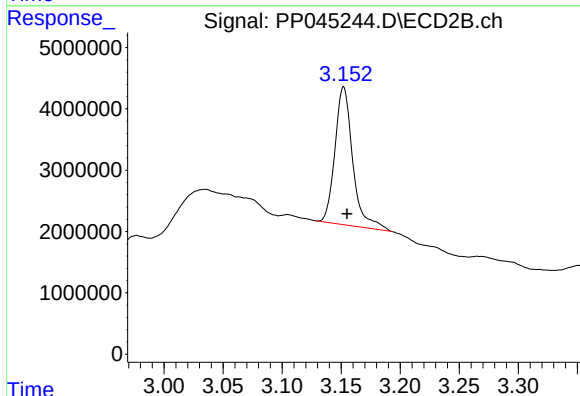


#1 Tetrachloro-m-xylene

R.T.: 3.152 min
Delta R.T.: -0.003 min
Response: 23589633
Conc: 17.90 ng/ml m

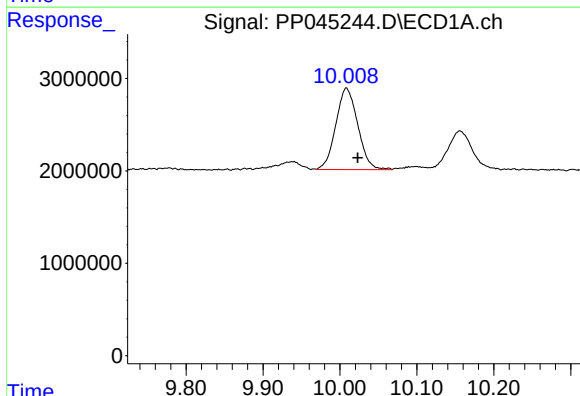

#2 Decachlorobiphenyl

R.T.: 10.008 min
Delta R.T.: -0.015 min
Response: 17395858
Conc: 13.51 ng/ml m

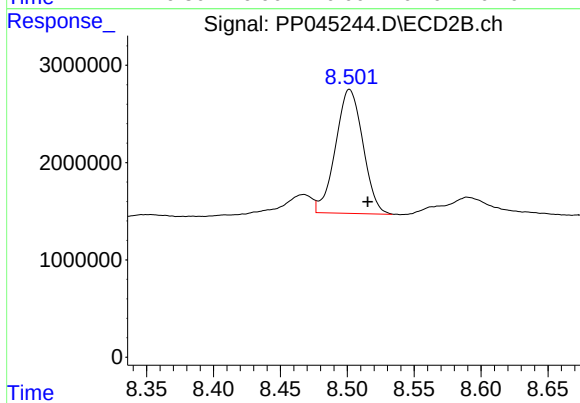

#2 Decachlorobiphenyl

R.T.: 8.501 min
Delta R.T.: -0.014 min
Response: 18150387
Conc: 13.97 ng/ml m