

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032522\
 Data File : PP045256.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2022 18:28
 Operator : YP\AJ
 Sample : N2123-04 10X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20220344-MODIFIED-ELUTRIATE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 01:50:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 17 04:32:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.889	3.151	2820888	2307844	1.548m	1.751
2) SA Decachlor...	10.006f	8.502	1211468	883769	0.941m	0.680 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032522\
Data File : PP045256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2022 18:28
Operator : YP\AJ
Sample : N2123-04 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 01:50:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031722.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 17 04:32:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

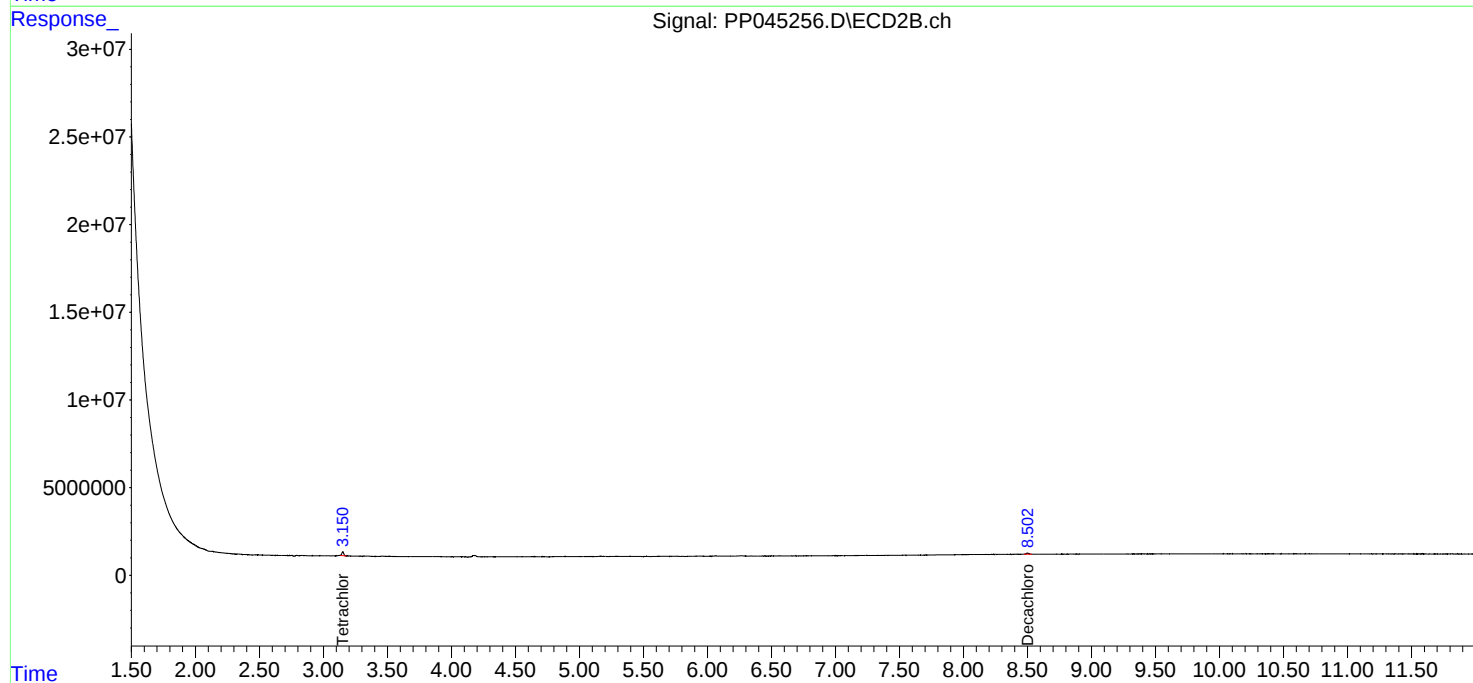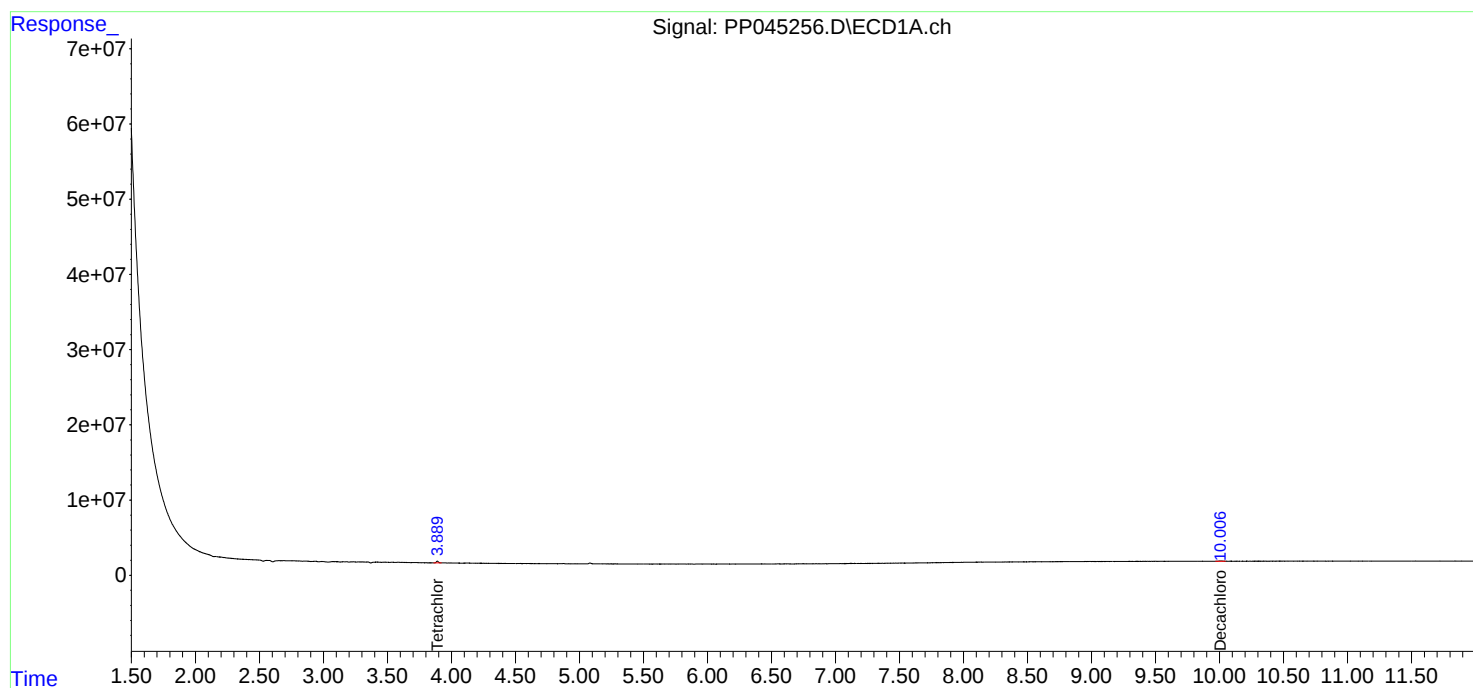

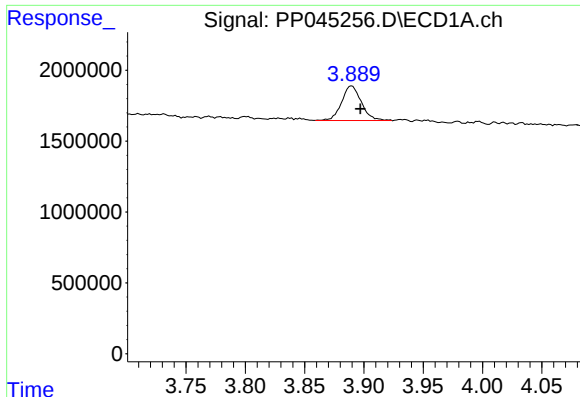


#1 Tetrachloro-m-xylene

R.T.: 3.889 min
Delta R.T.: -0.008 min
Response: 2820888
Conc: 1.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
20220344-MODIFIED-ELUTRIATE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

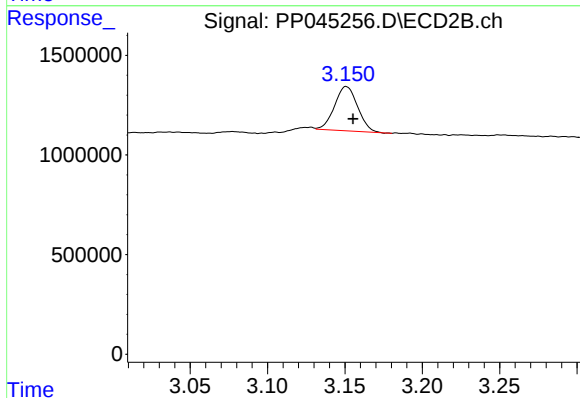


#1 Tetrachloro-m-xylene

R.T.: 3.151 min
Delta R.T.: -0.004 min
Response: 2307844
Conc: 1.75 ng/ml

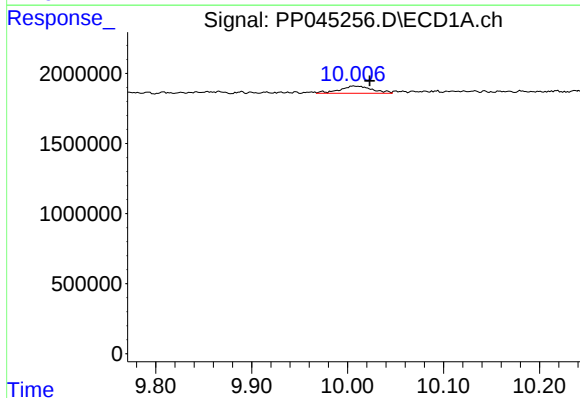

#2 Decachlorobiphenyl

R.T.: 10.006 min
Delta R.T.: -0.017 min
Response: 1211468
Conc: 0.94 ng/ml m

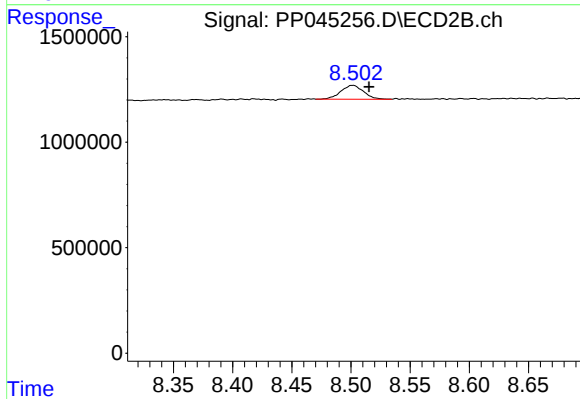

#2 Decachlorobiphenyl

R.T.: 8.502 min
Delta R.T.: -0.014 min
Response: 883769
Conc: 0.68 ng/ml