

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032525\
 Data File : PP070851.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2025 12:39
 Operator : YP\AJ
 Sample : Q1634-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HR-01-032425

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/26/2025
 Supervised By :mohammad ahmed 03/27/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 12:55:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 05:25:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.517	3.821	23066286	19367668	14.830m	19.324 #
2) SA Decachlor...	10.238	8.865	22216022	16426432	20.912	16.790

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032525\
Data File : PP070851.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2025 12:39
Operator : YP\AJ
Sample : Q1634-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HR-01-032425


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/26/2025
Supervised By :mohammad ahmed 03/27/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 12:55:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 05:25:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

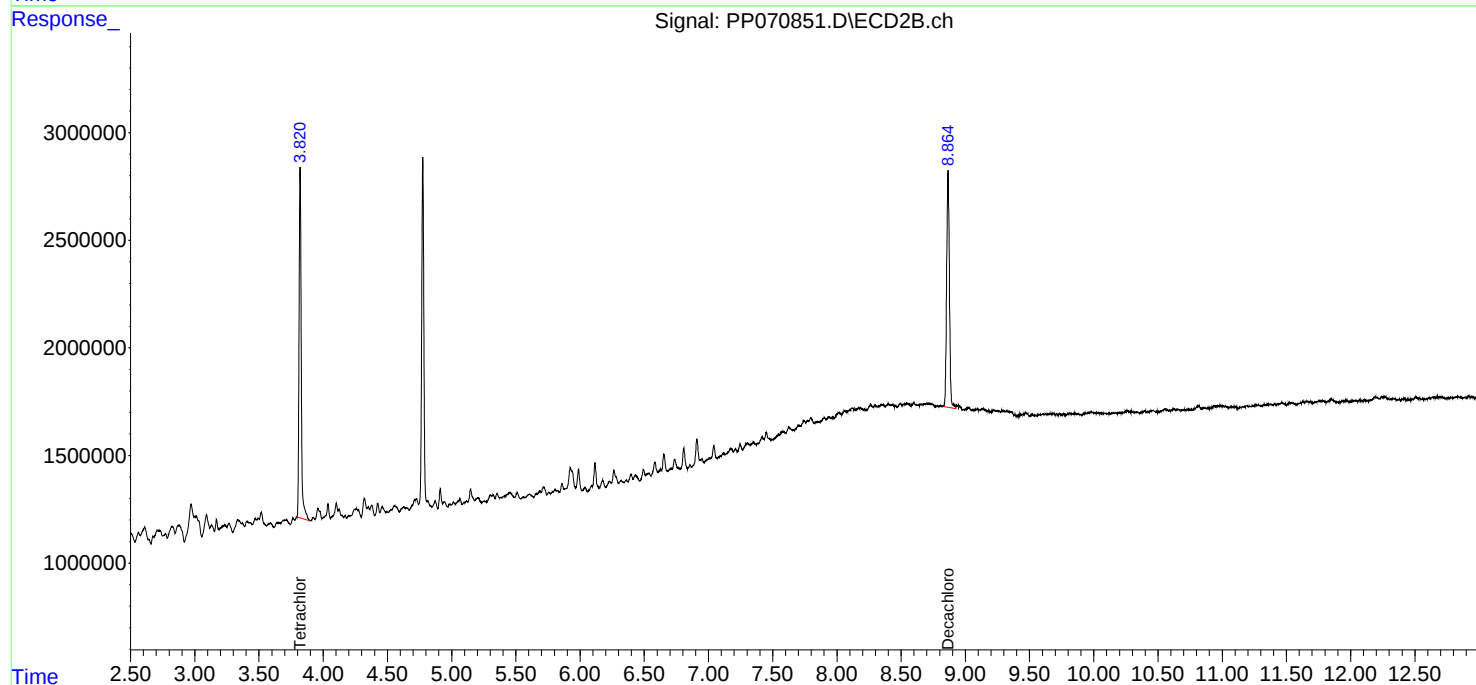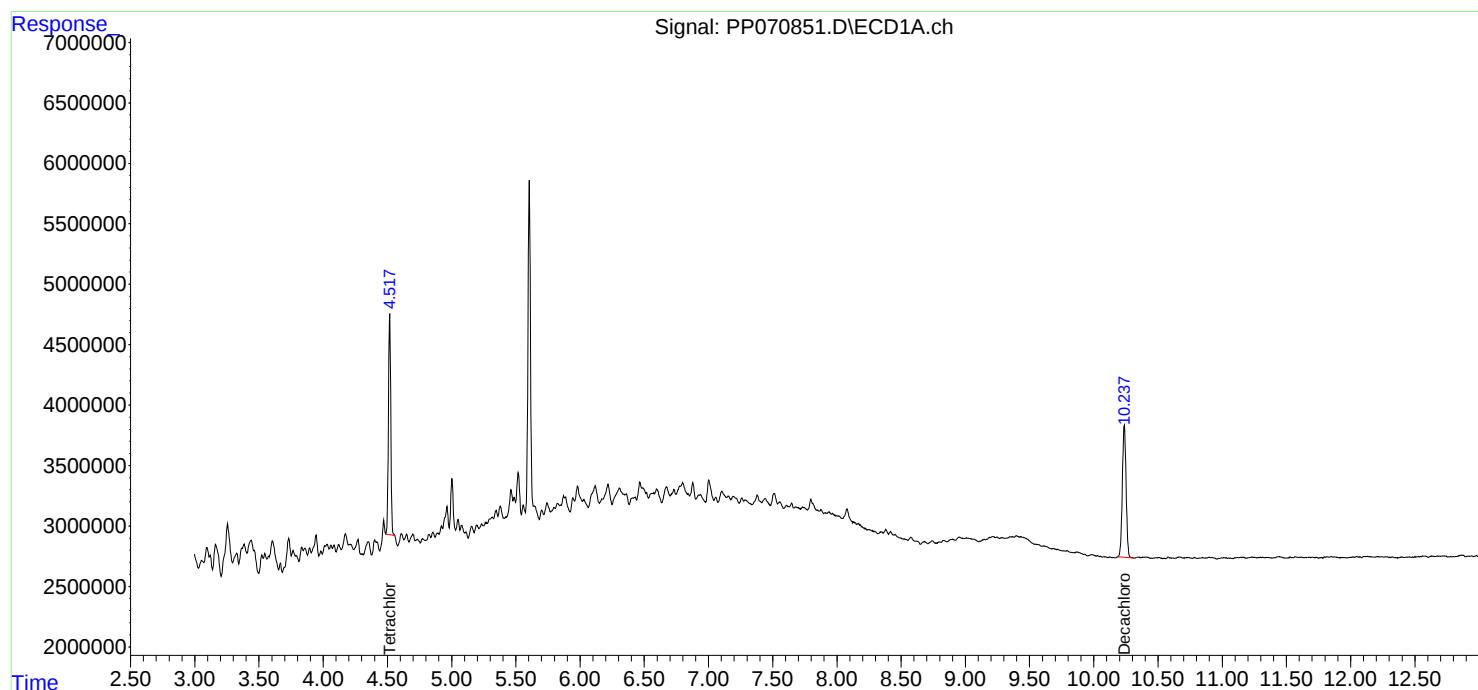

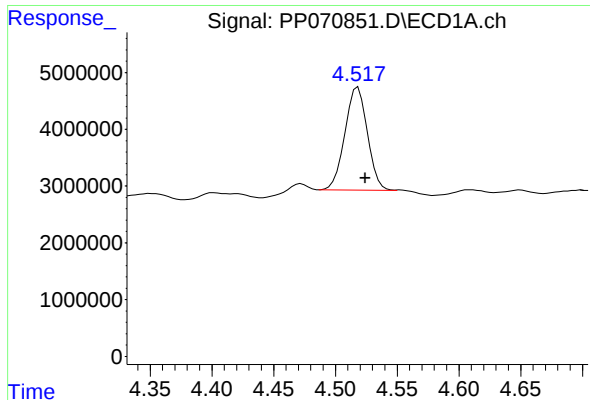


#1 Tetrachloro-m-xylene

R.T.: 4.517 min
Delta R.T.: -0.007 min
Response: 23066286
Conc: 14.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
HR-01-032425


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/26/2025
Supervised By :mohammad ahmed 03/27/2025

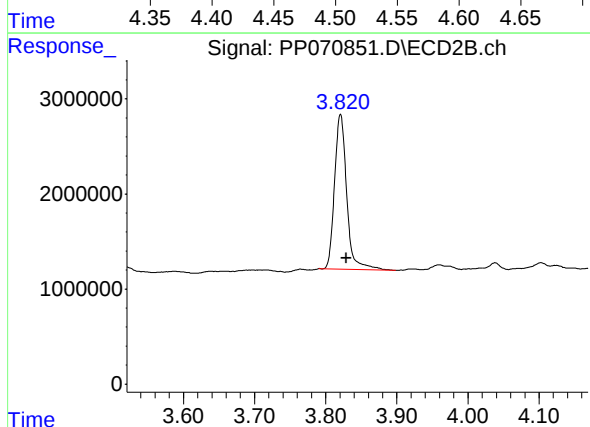


#1 Tetrachloro-m-xylene

R.T.: 3.821 min
Delta R.T.: -0.008 min
Response: 19367668
Conc: 19.32 ng/ml

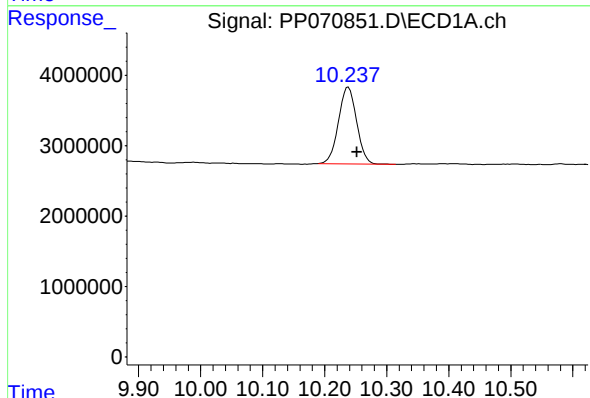

#2 Decachlorobiphenyl

R.T.: 10.238 min
Delta R.T.: -0.014 min
Response: 22216022
Conc: 20.91 ng/ml

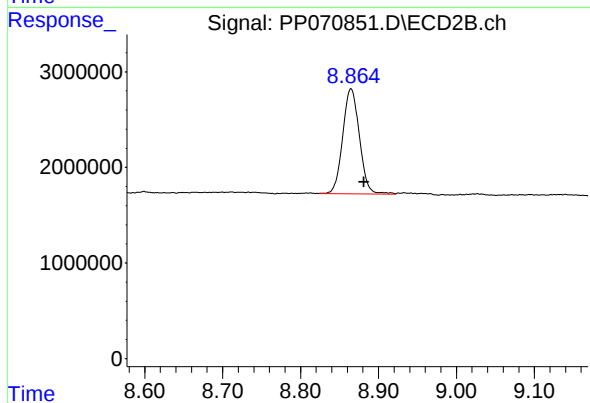

#2 Decachlorobiphenyl

R.T.: 8.865 min
Delta R.T.: -0.016 min
Response: 16426432
Conc: 16.79 ng/ml