

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032525\
 Data File : PP070873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2025 21:30
 Operator : YP\AJ
 Sample : Q1638-03 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC208062LOK-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/26/2025
 Supervised By :mohammad ahmed 03/27/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 02:37:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 05:25:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.517	3.820	2644195	1992258	1.700m	1.988m
2) SA Decachlor...	10.238	8.863	1905300	1386689	1.793	1.417m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032525\
Data File : PP070873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2025 21:30
Operator : YP\AJ
Sample : Q1638-03 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC208062LOK-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/26/2025
Supervised By :mohammad ahmed 03/27/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 02:37:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 05:25:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

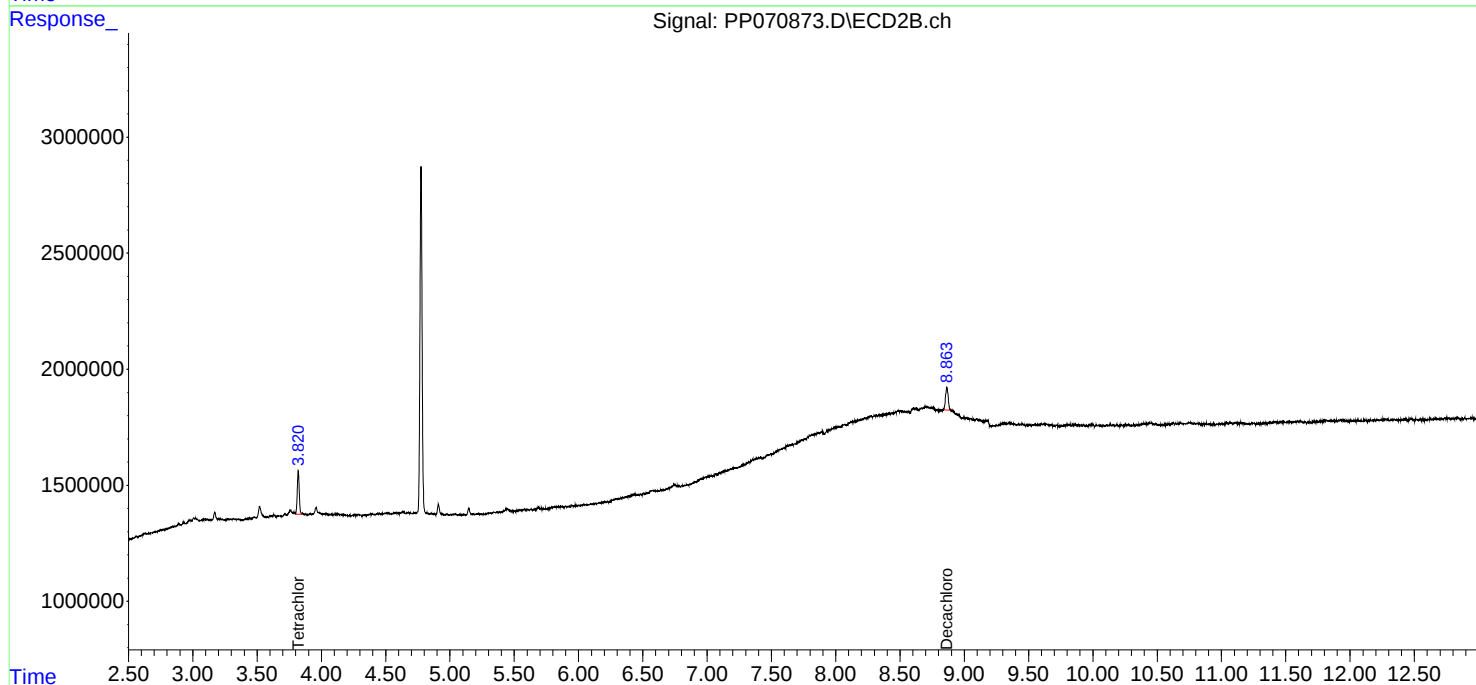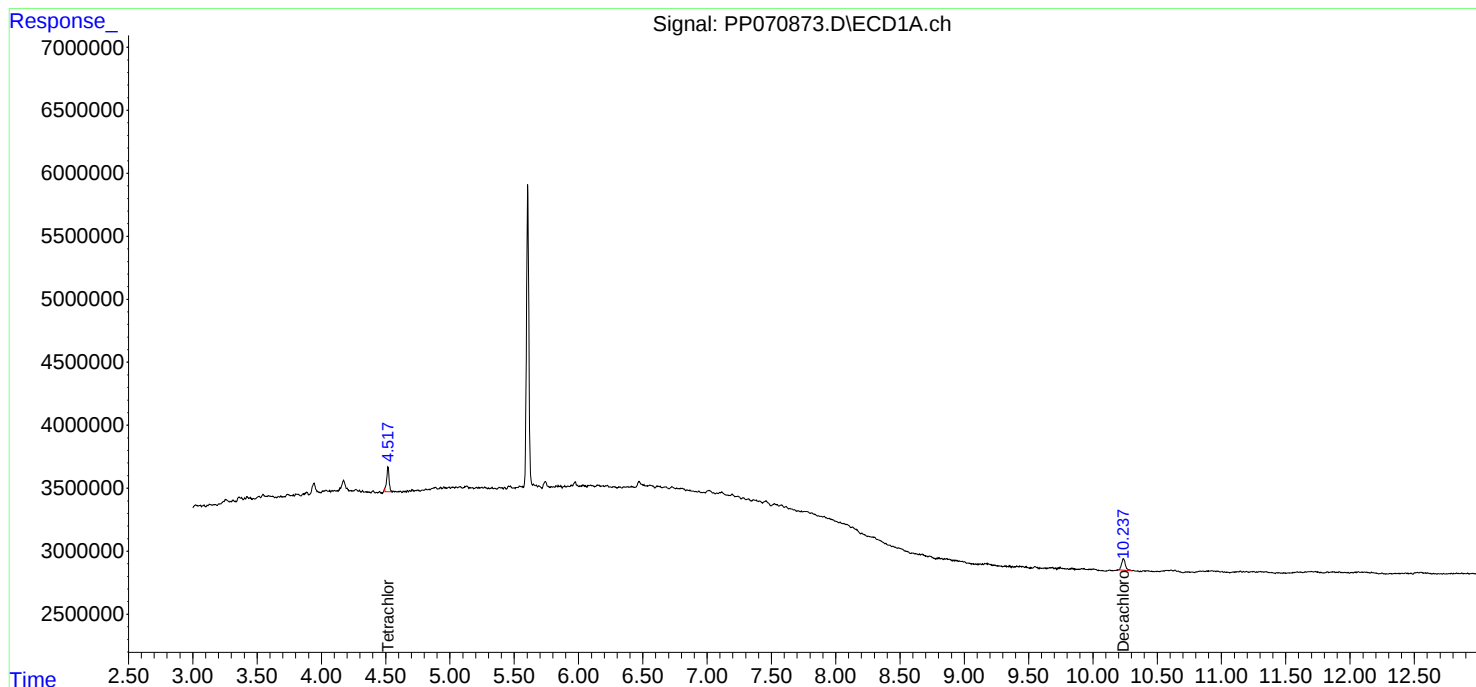

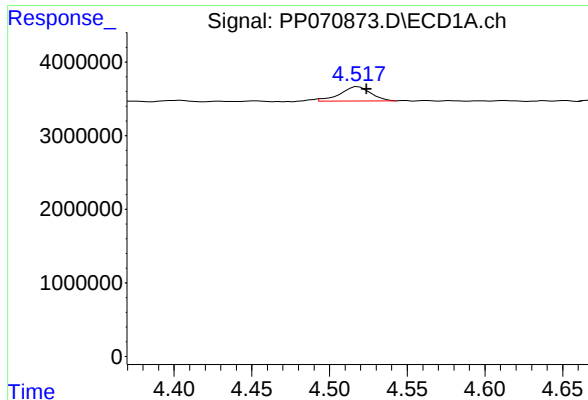


#1 Tetrachloro-m-xylene

R.T.: 4.517 min
Delta R.T.: -0.007 min
Response: 2644195
Conc: 1.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC208062LOK-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/26/2025
Supervised By :mohammad ahmed 03/27/2025

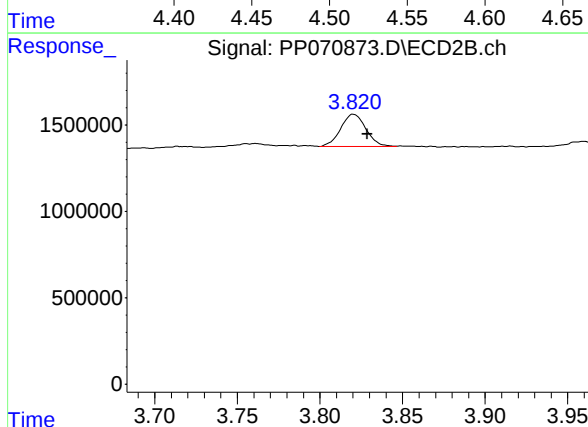


#1 Tetrachloro-m-xylene

R.T.: 3.820 min
Delta R.T.: -0.009 min
Response: 1992258
Conc: 1.99 ng/ml m

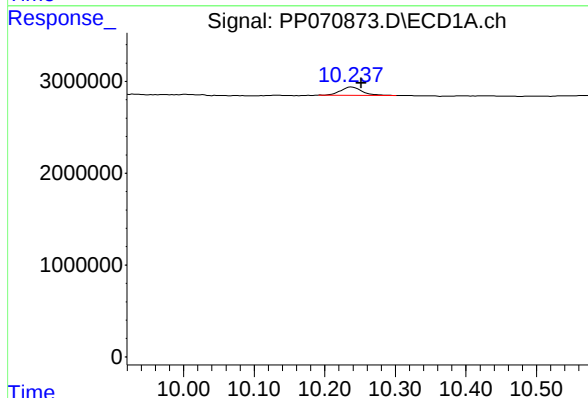

#2 Decachlorobiphenyl

R.T.: 10.238 min
Delta R.T.: -0.014 min
Response: 1905300
Conc: 1.79 ng/ml

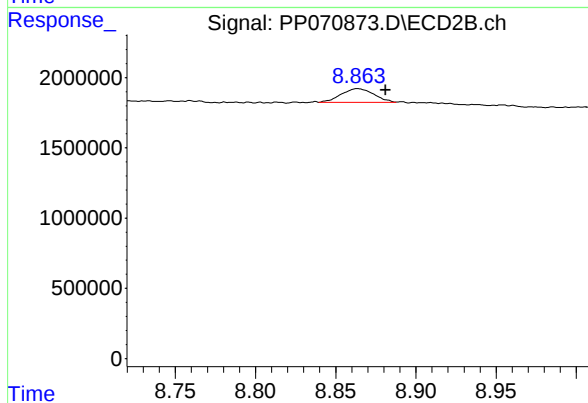

#2 Decachlorobiphenyl

R.T.: 8.863 min
Delta R.T.: -0.019 min
Response: 1386689
Conc: 1.42 ng/ml m