

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
 Data File : PP029520.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2019 12:00
 Operator : EI\MA
 Sample : PB118241TB
 Misc : hexane
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB118241TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 03:33:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.118	32287605	31963291	986.936	744.348
Target Compounds							
5) T	DICAMBA	12.266	0.000	301637	0	2.041	N.D. #
8) T	DICHLORPROP	0.000	13.552	0	1091176	N.D.	26.945 #
9) T	2,4-D	13.822	0.000	31064	0	0.803	N.D. #
12) T	2,4,5-T	15.439	15.848	499584	1038367	2.205	6.264 #
13) T	2,4-DB	16.220	0.000	635731	0	30.573	N.D. #
14) T	DINOSEB	17.680	0.000	72222	0	0.429	N.D. #
15) T	Picloram	17.459	18.239	860631	3735048	2.627	15.671 #
16) T	DCPA	18.044	0.000	520636	0	1.641	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
Data File : PP029520.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2019 12:00
Operator : EI\MA
Sample : PB118241TB
Misc : hexane
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB118241TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 03:33:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

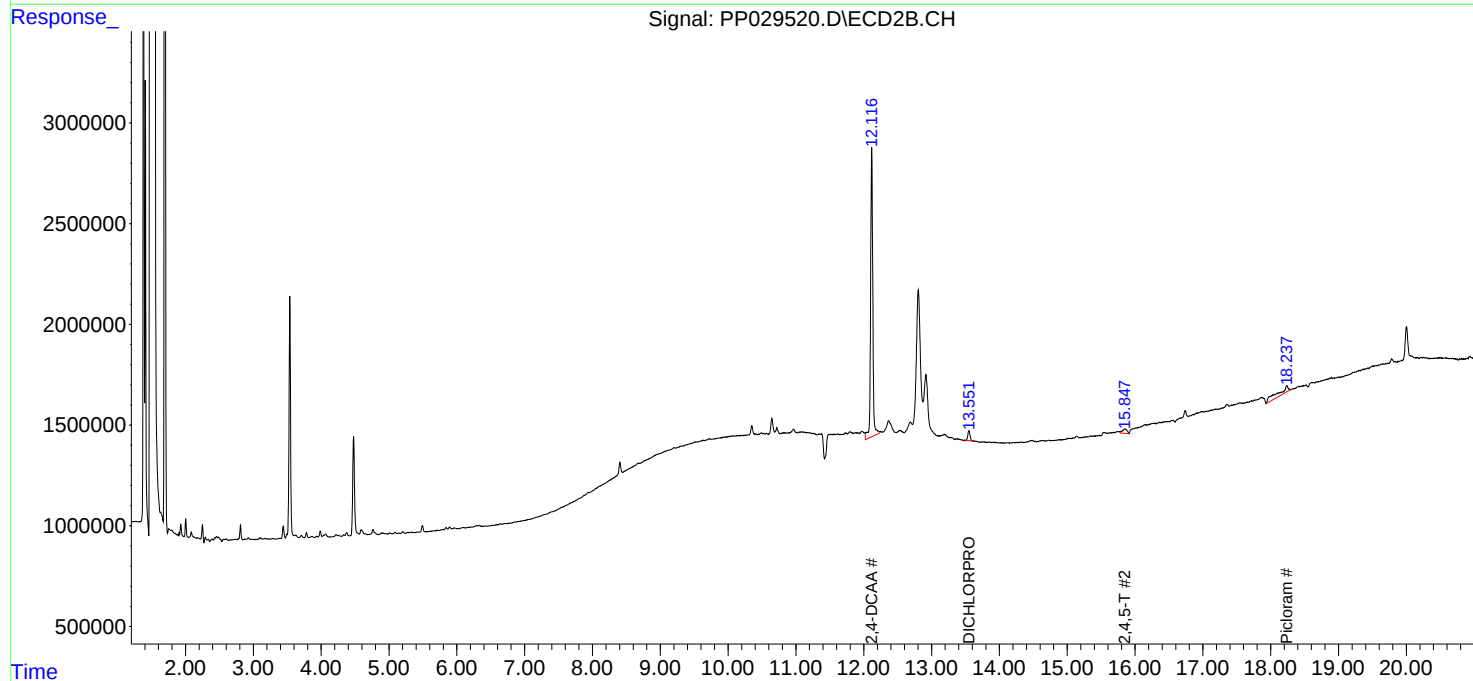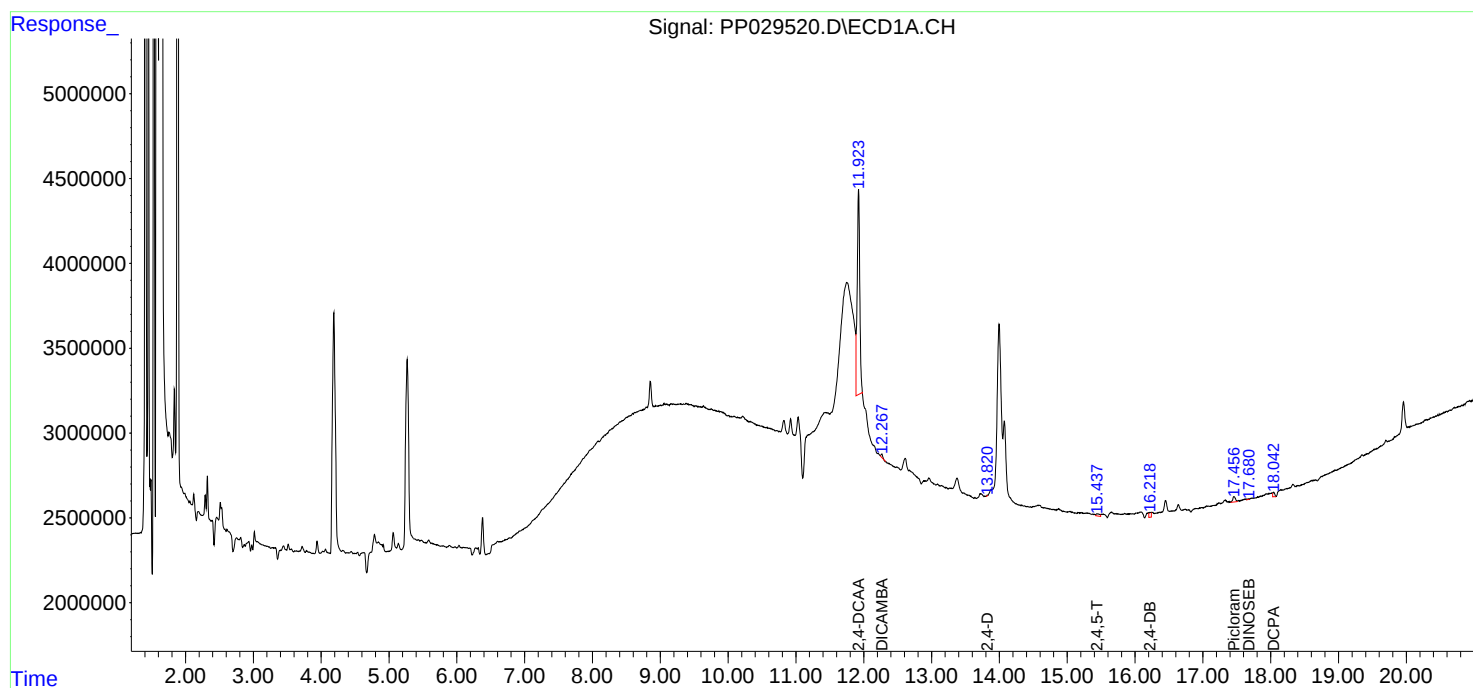


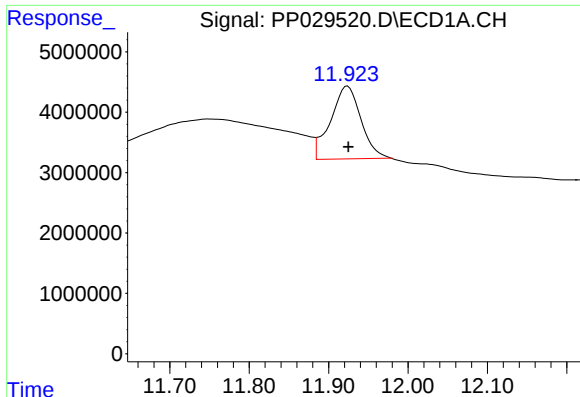

#4 2,4-DCAA


R.T.: 11.924 min
Delta R.T.: -0.001 min
Response: 32287605
Conc: 986.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118241TB

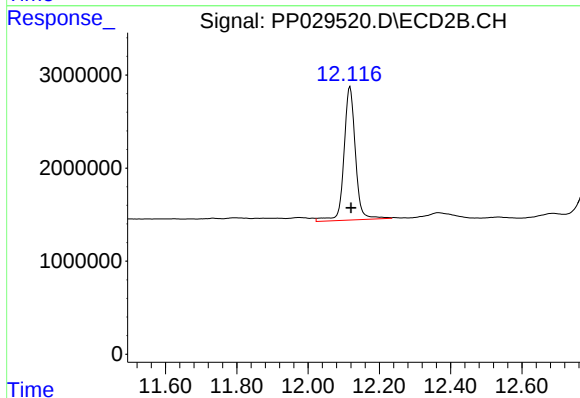


#4 2,4-DCAA

R.T.: 12.118 min
Delta R.T.: -0.003 min
Response: 31963291
Conc: 744.35 ng/ml

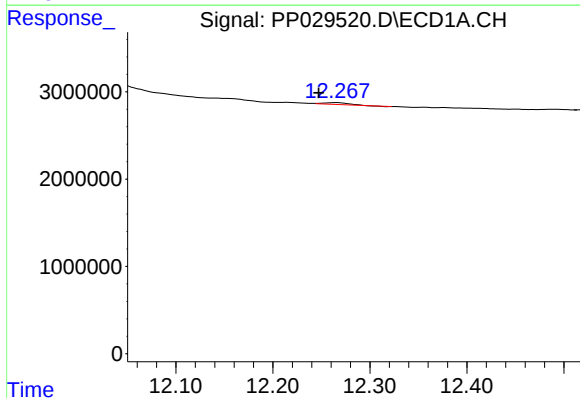


#5 DICAMBA

R.T.: 12.266 min
Delta R.T.: 0.019 min
Response: 301637
Conc: 2.04 ng/ml

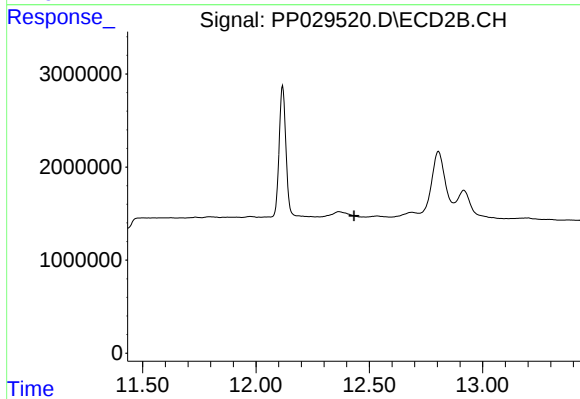

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.433 min
Response: 0
Conc: N.D.

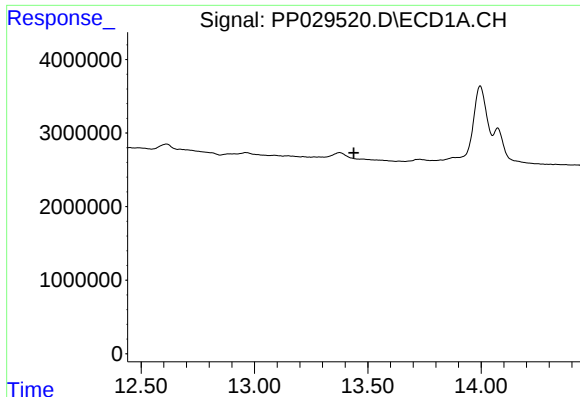

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB118241TB

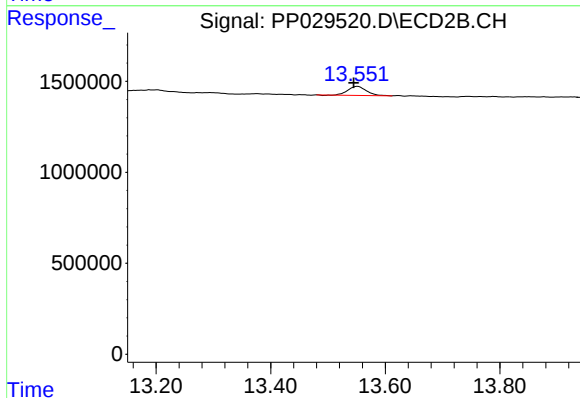


#8 DICHLORPROP

R.T.: 13.552 min
Delta R.T.: 0.007 min
Response: 1091176
Conc: 26.94 ng/ml

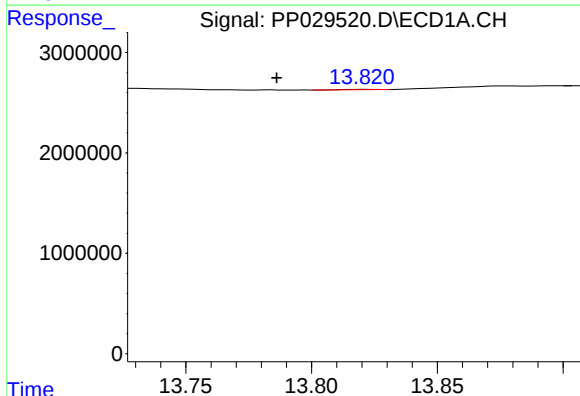


#9 2,4-D

R.T.: 13.822 min
Delta R.T.: 0.036 min
Response: 31064
Conc: 0.80 ng/ml

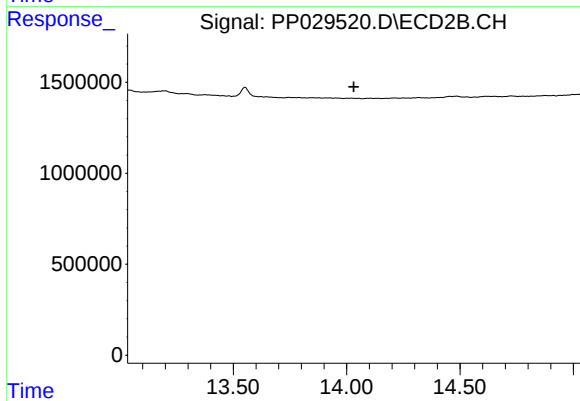

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 14.031 min
Response: 0
Conc: N.D.

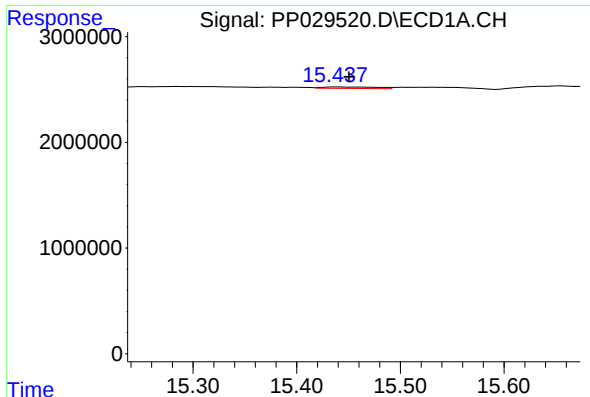

#12 2,4,5-T


R.T.: 15.439 min
Delta R.T.: -0.012 min
Response: 499584
Conc: 2.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118241TB

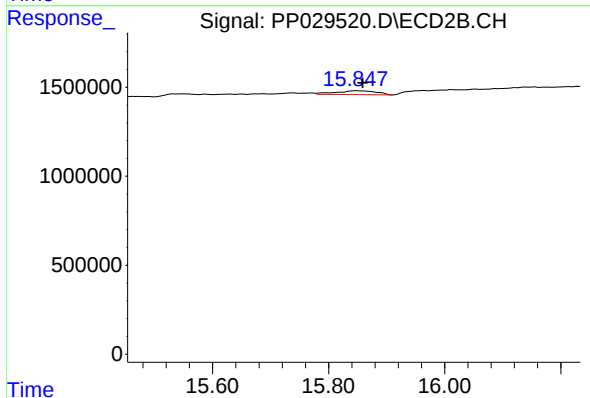


#12 2,4,5-T

R.T.: 15.848 min
Delta R.T.: -0.011 min
Response: 1038367
Conc: 6.26 ng/ml

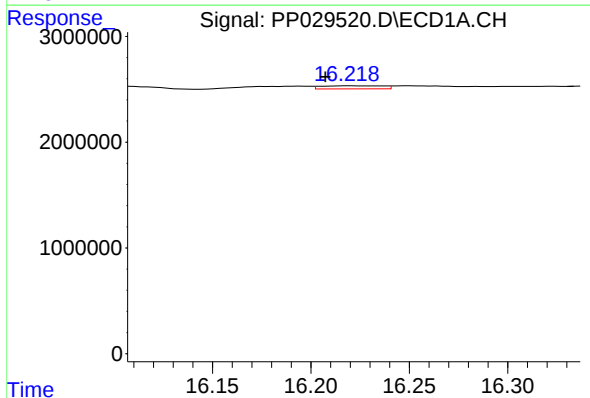


#13 2,4-DB

R.T.: 16.220 min
Delta R.T.: 0.013 min
Response: 635731
Conc: 30.57 ng/ml

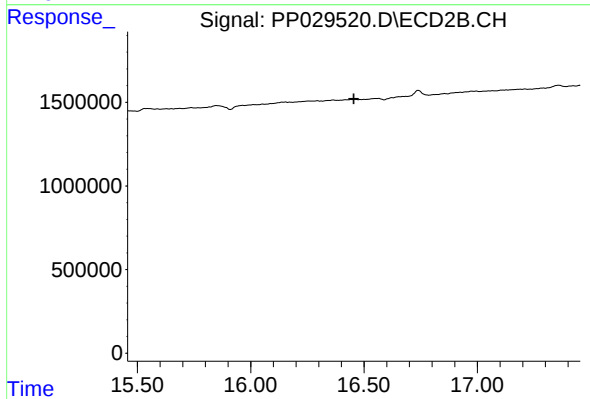

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.455 min
Response: 0
Conc: N.D.

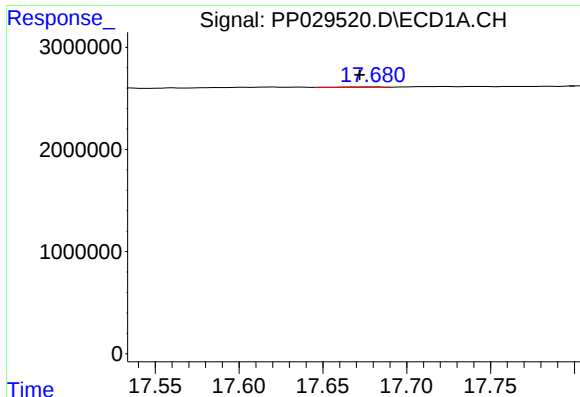

#14 DINoseb


R.T.: 17.680 min
Delta R.T.: 0.008 min
Response: 72222
Conc: 0.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118241TB

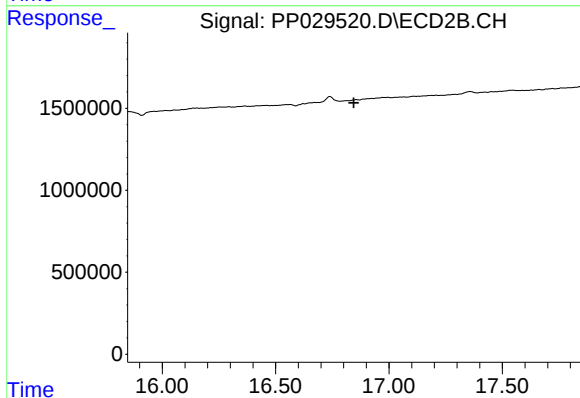


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 16.845 min
Response: 0
Conc: N.D.

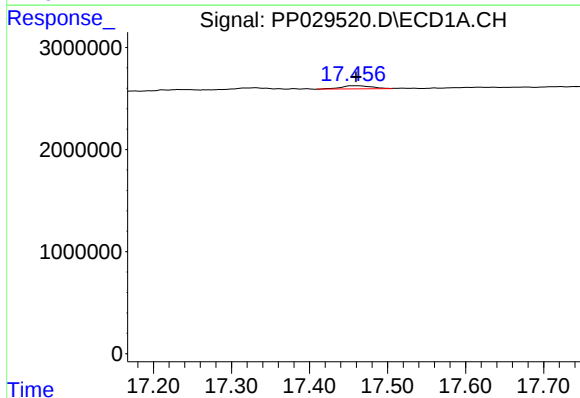


#15 Picloram

R.T.: 17.459 min
Delta R.T.: -0.001 min
Response: 860631
Conc: 2.63 ng/ml

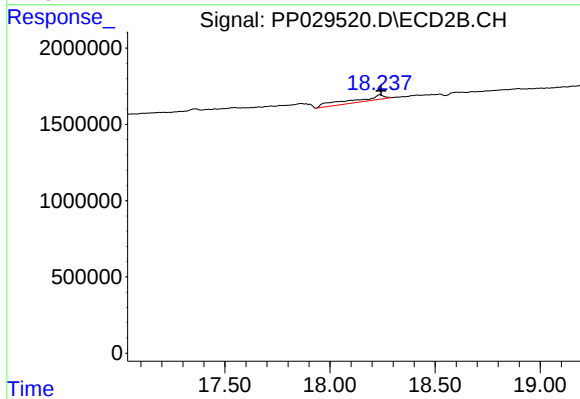

#15 Picloram


R.T.: 18.239 min
Delta R.T.: -0.003 min
Response: 3735048
Conc: 15.67 ng/ml

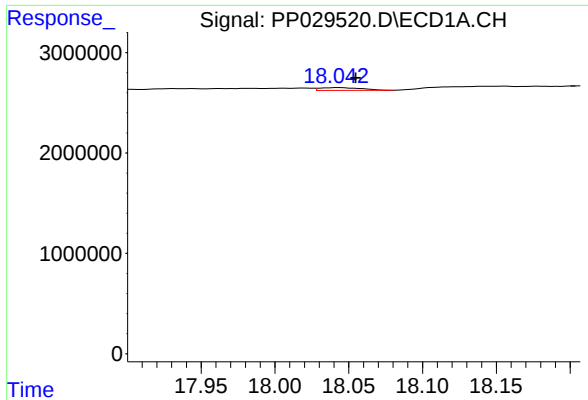

#16 DCPA

R.T.: 18.044 min
Delta R.T.: -0.011 min
Response: 520636
Conc: 1.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118241TB

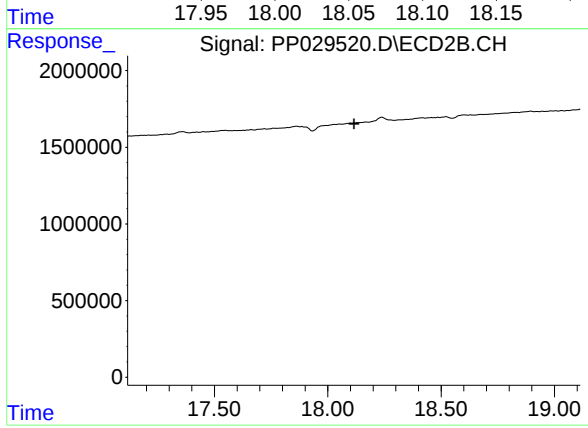

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.116 min
Response: 0
Conc: N.D.