

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
 Data File : PP029525.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2019 14:07
 Operator : EI\MA
 Sample : K2040-06
 Misc : hexane
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S4B(22-28)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 03:35:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.118	24019303	29381542	734.199	684.225
Target Compounds							
8) T	DICHLORPROP	0.000	13.550	0	636177	N.D.	15.709 #
9) T	2,4-D	13.718	0.000	571120	0	14.768	N.D. #
10) T	Pentachlo...	0.000	14.629	0	337382	N.D.	0.617 #
11) T	2,4,5-TP ...	0.000	15.194	0	1570478	N.D.	7.587 #
13) T	2,4-DB	16.216	0.000	468387	0	22.525	N.D. #
14) T	DINOSEB	17.674	16.812	49456	78865	0.293	0.522 #
15) T	Picloram	17.459	18.257	199331	1826496	0.608	7.663 #
16) T	DCPA	18.050	0.000	803109	0	2.531	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
Data File : PP029525.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2019 14:07
Operator : EI\MA
Sample : K2040-06
Misc : hexane
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
S4B(22-28)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 03:35:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

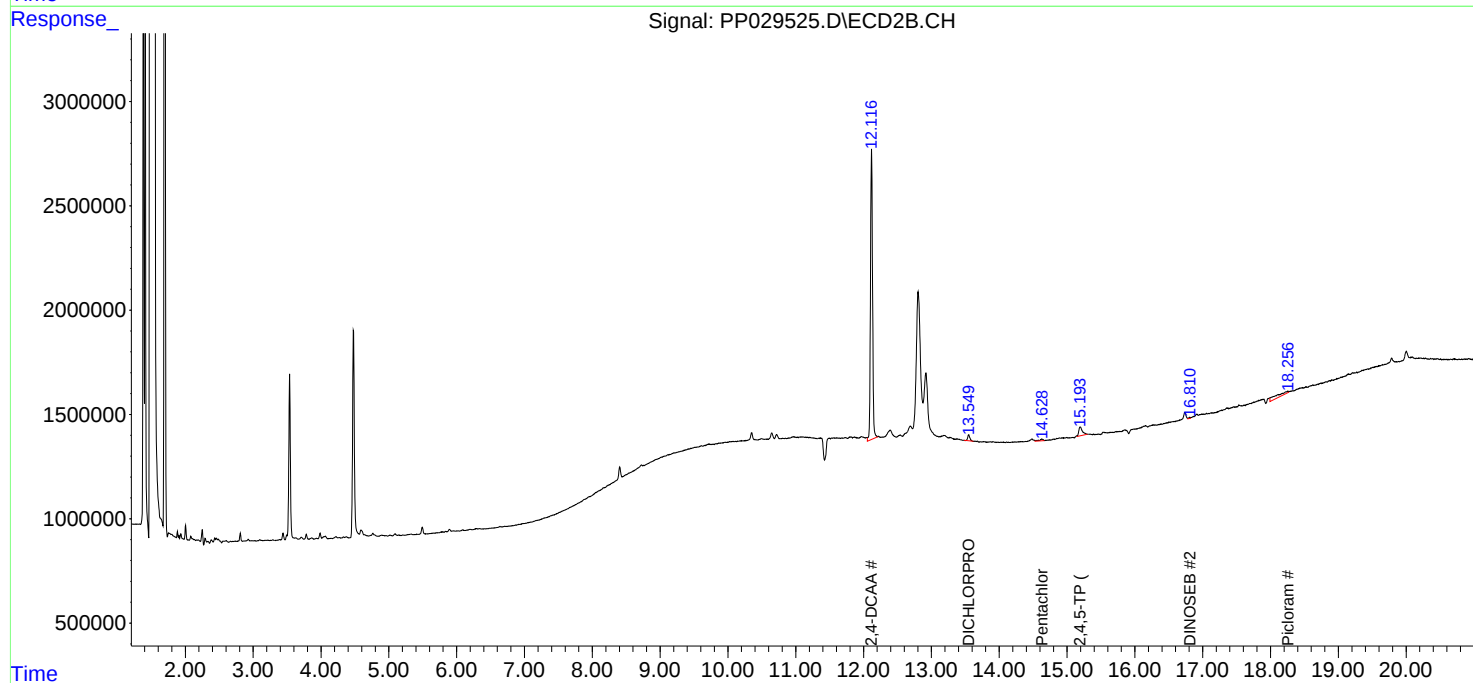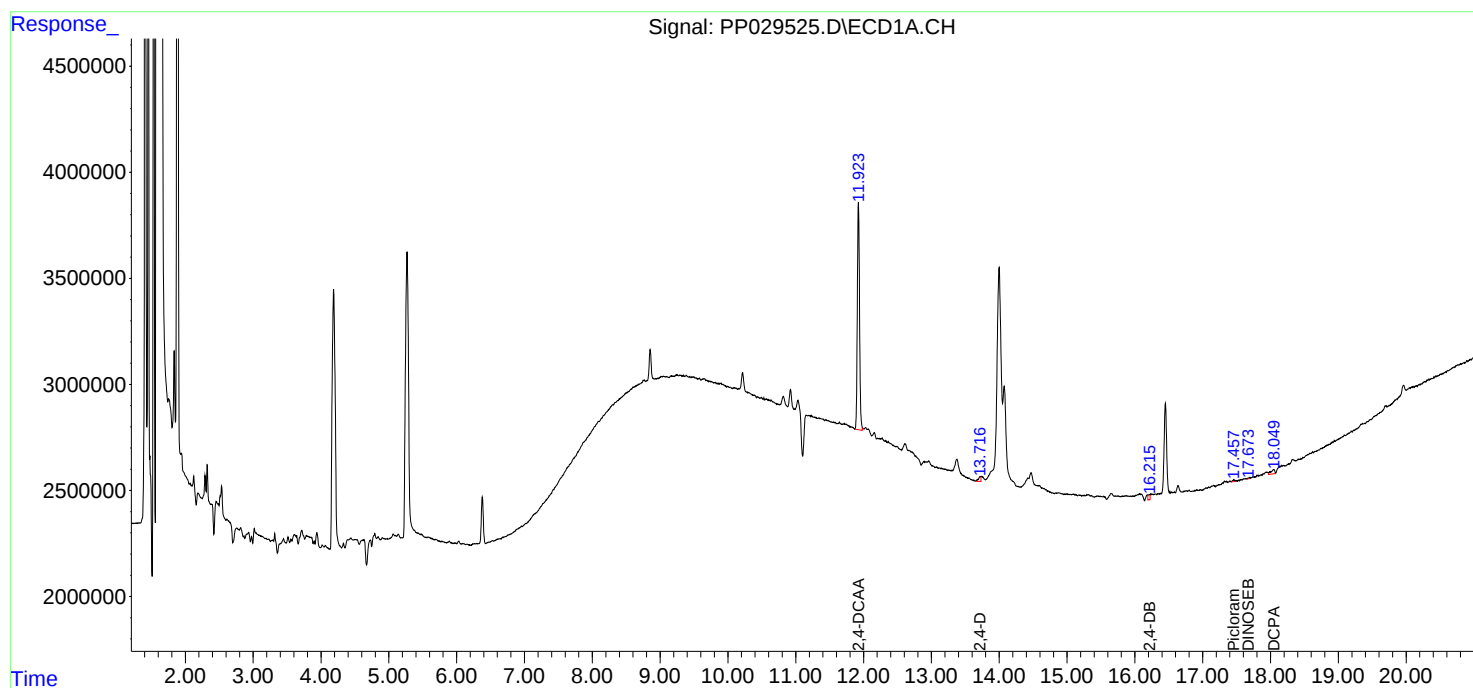


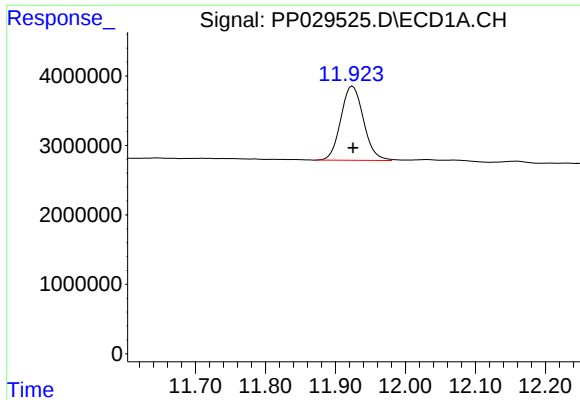

#4 2,4-DCAA


R.T.: 11.924 min
Delta R.T.: 0.000 min
Response: 24019303
Conc: 734.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
S4B(22-28)

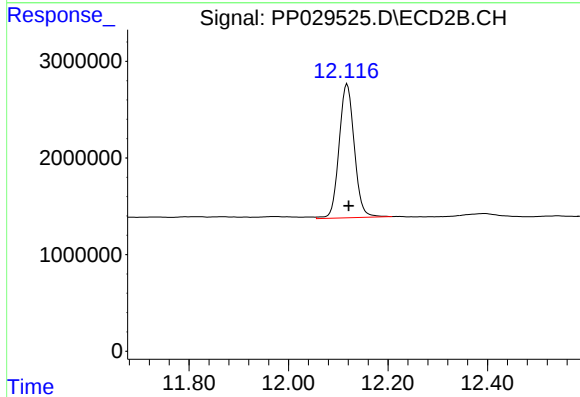


#4 2,4-DCAA

R.T.: 12.118 min
Delta R.T.: -0.003 min
Response: 29381542
Conc: 684.23 ng/ml

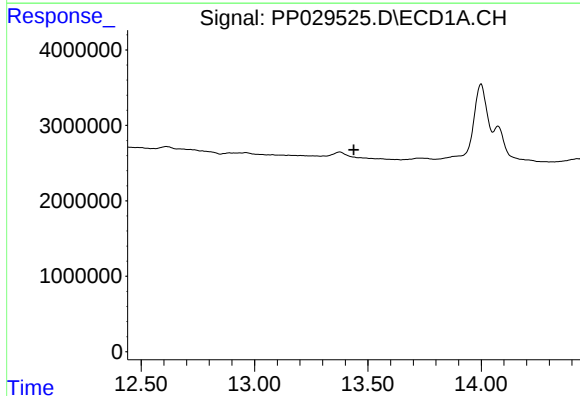


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.438 min
Response: 0
Conc: N.D.

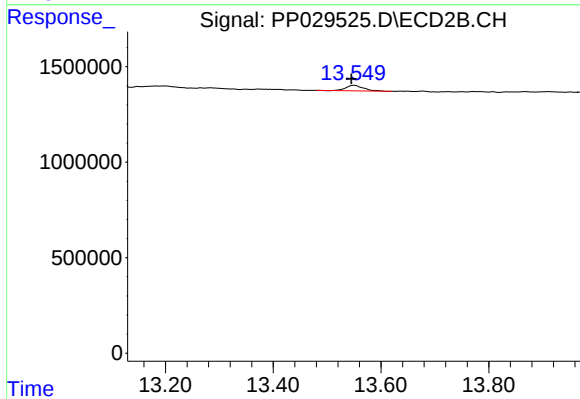

#8 DICHLORPROP


R.T.: 13.550 min
Delta R.T.: 0.005 min
Response: 636177
Conc: 15.71 ng/ml

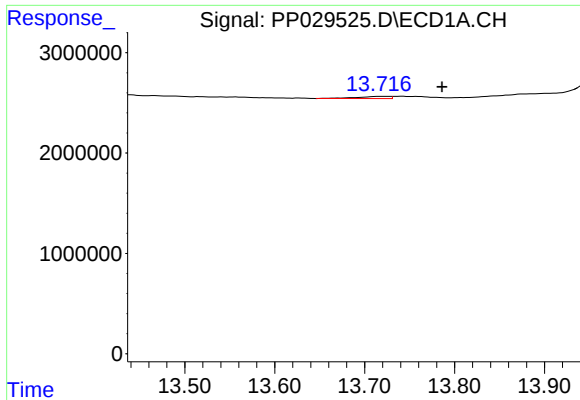

#9 2,4-D


R.T.: 13.718 min
Delta R.T.: -0.068 min
Response: 571120
Conc: 14.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
S4B(22-28)

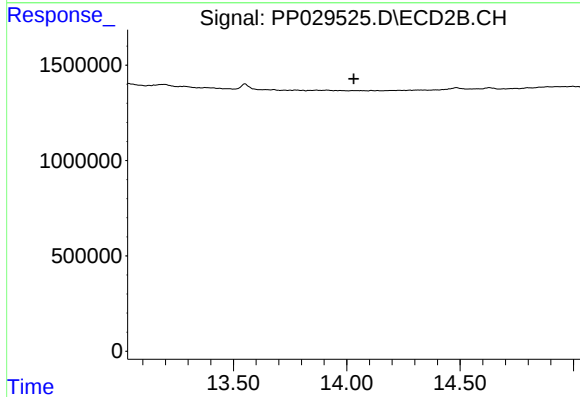


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 14.031 min
Response: 0
Conc: N.D.

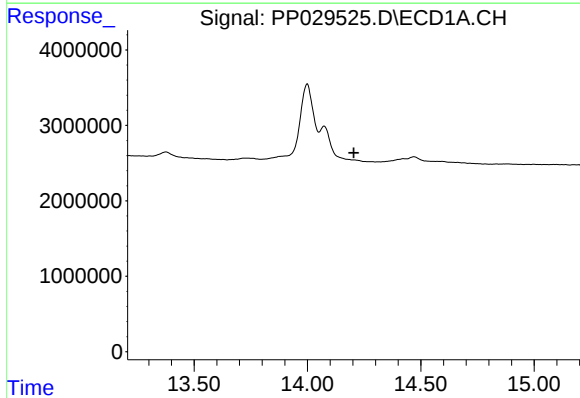


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 14.205 min
Response: 0
Conc: N.D.

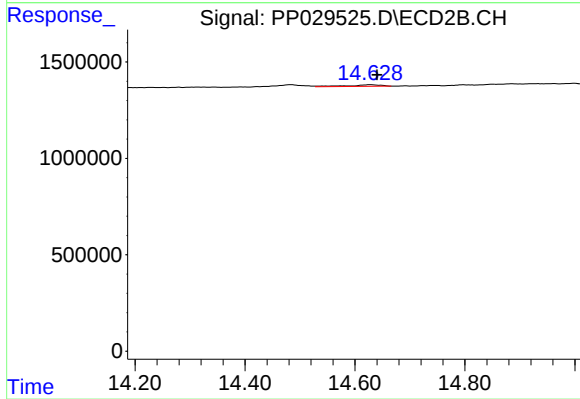

#10 Pentachlorophenol


R.T.: 14.629 min
Delta R.T.: -0.011 min
Response: 337382
Conc: 0.62 ng/ml

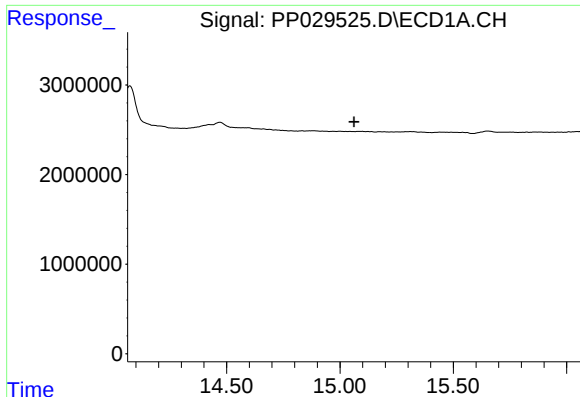

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S4B(22-28)

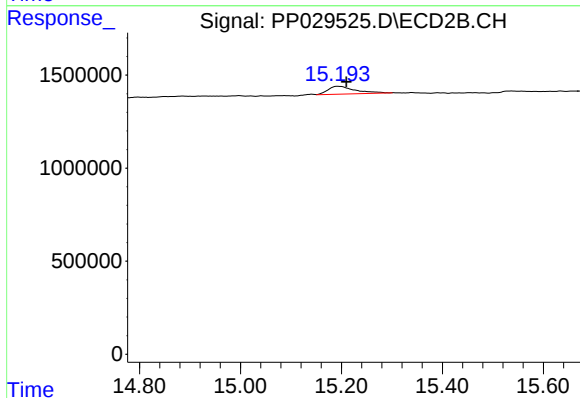


#11 2,4,5-TP (SILVEX)

R.T.: 15.194 min
Delta R.T.: -0.016 min
Response: 1570478
Conc: 7.59 ng/ml

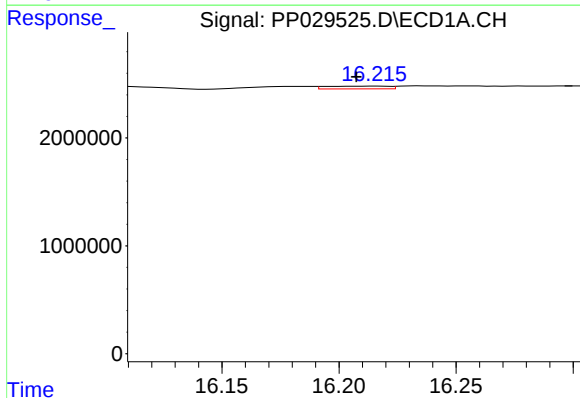


#13 2,4-DB

R.T.: 16.216 min
Delta R.T.: 0.009 min
Response: 468387
Conc: 22.53 ng/ml

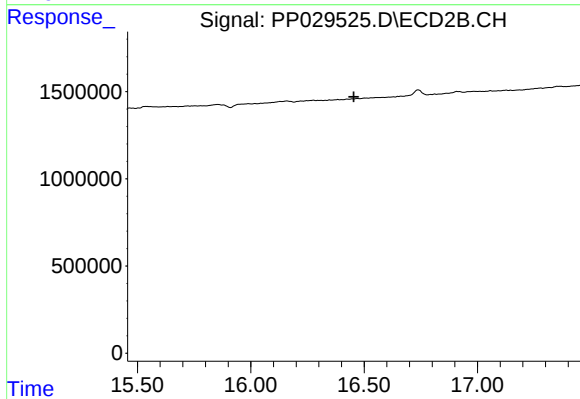

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.455 min
Response: 0
Conc: N.D.

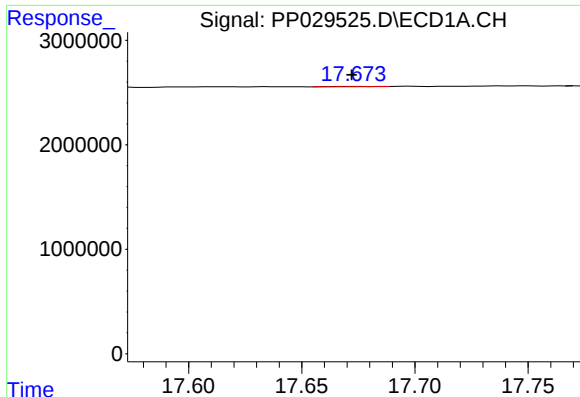

#14 DINOSEB


R.T.: 17.674 min
Delta R.T.: 0.002 min
Response: 49456
Conc: 0.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
S4B(22-28)

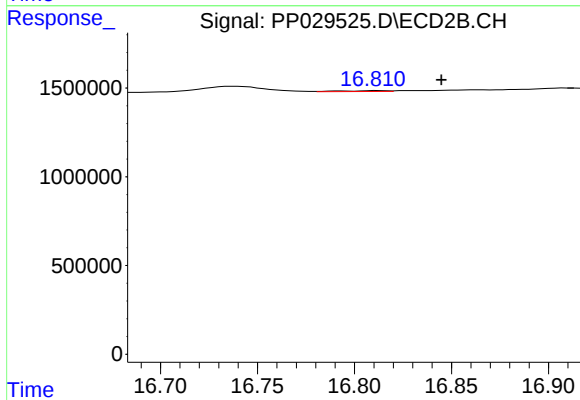


#14 DINOSEB

R.T.: 16.812 min
Delta R.T.: -0.033 min
Response: 78865
Conc: 0.52 ng/ml

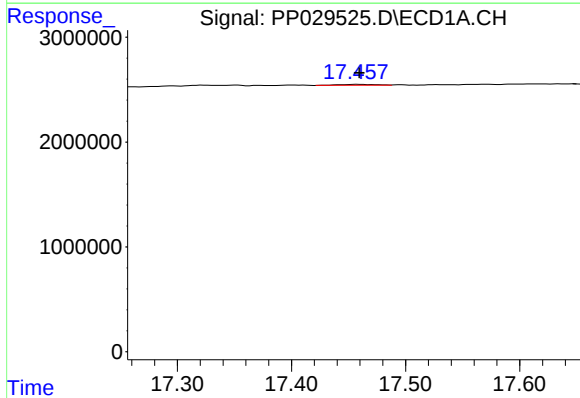


#15 Picloram

R.T.: 17.459 min
Delta R.T.: -0.001 min
Response: 199331
Conc: 0.61 ng/ml

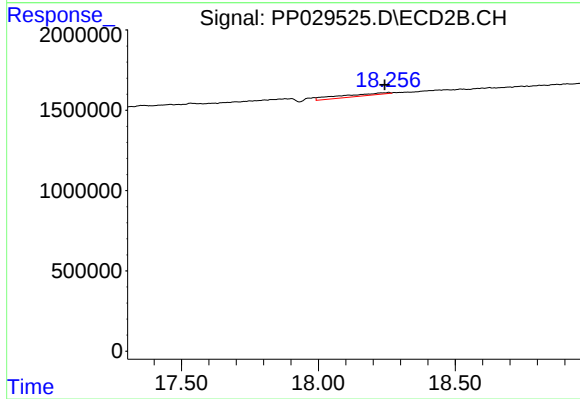

#15 Picloram


R.T.: 18.257 min
Delta R.T.: 0.015 min
Response: 1826496
Conc: 7.66 ng/ml

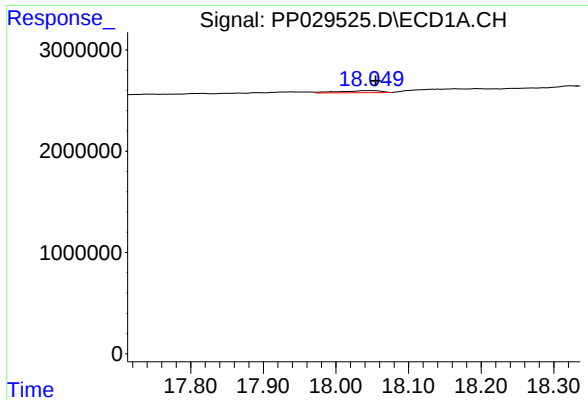

#16 DCPA

R.T.: 18.050 min
Delta R.T.: -0.005 min
Response: 803109
Conc: 2.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
S4B(22-28)

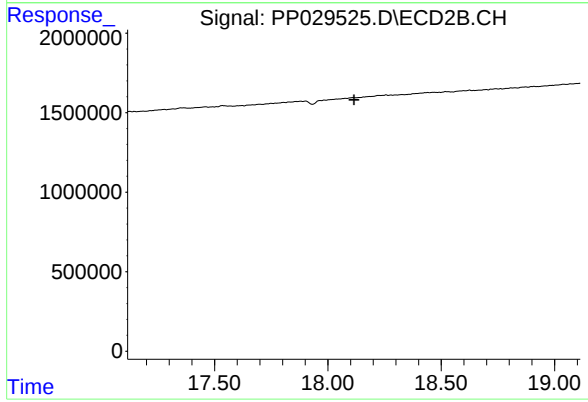

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.116 min
Response: 0
Conc: N.D.