

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
 Data File : PP029526.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2019 14:33
 Operator : EI\MA
 Sample : K2050-07
 Misc : hexane
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CS-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 03:35:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.926	12.118	21170162	26228975	647.109	610.809
Target Compounds							
5) T	DICAMBA	12.264	0.000	146440	0	0.991	N.D. #
8) T	DICHLORPROP	0.000	13.554	0	540496	N.D.	13.347 #
11) T	2,4,5-TP ...	0.000	15.199	0	961595	N.D.	4.646 #
12) T	2,4,5-T	0.000	15.861	0	1269352	N.D.	7.657 #
13) T	2,4-DB	16.202	0.000	1165478	0	56.049	N.D. #
14) T	DINOSEB	0.000	16.904	0	447838	N.D.	2.964 #
15) T	Picloram	17.466	18.257	266556	1131438	0.814	4.747 #
16) T	DCPA	18.039	18.112	1354046	343659	4.268	1.310 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
Data File : PP029526.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2019 14:33
Operator : EI\MA
Sample : K2050-07
Misc : hexane
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CS-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 03:35:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

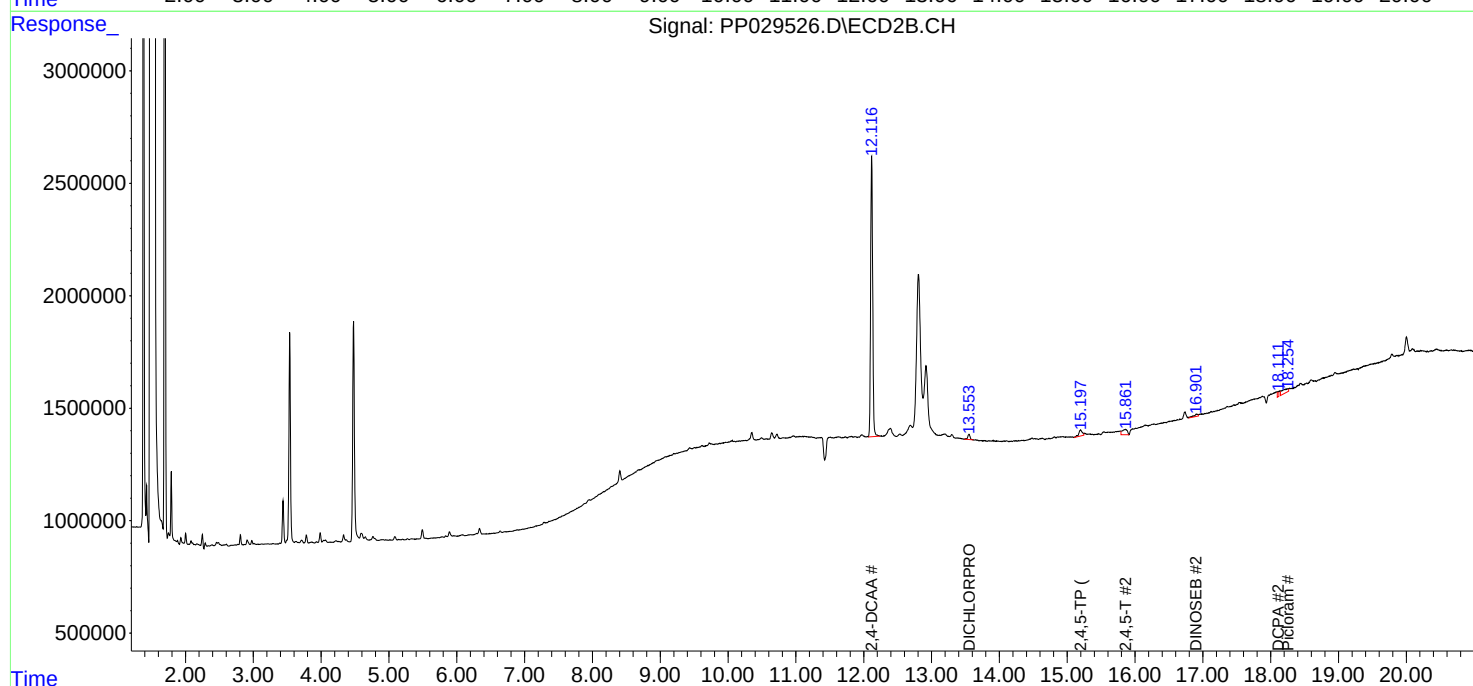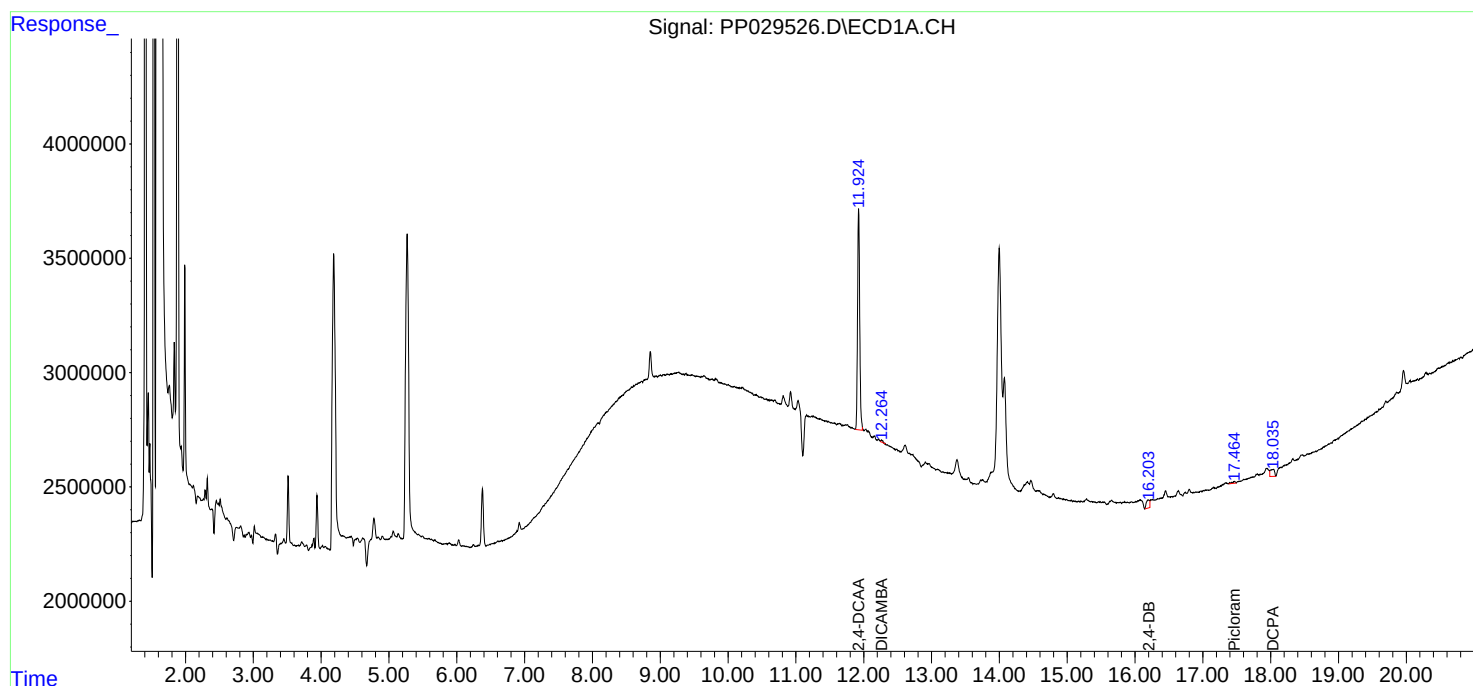


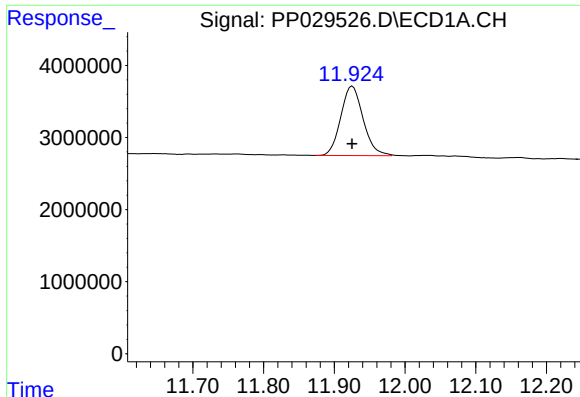

#4 2,4-DCAA


R.T.: 11.926 min
Delta R.T.: 0.000 min
Response: 21170162
Conc: 647.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
CS-5

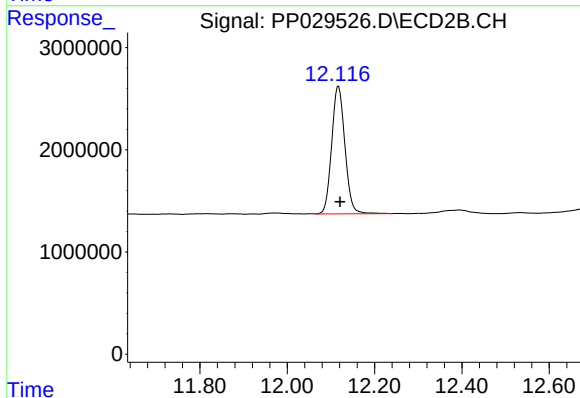


#4 2,4-DCAA

R.T.: 12.118 min
Delta R.T.: -0.003 min
Response: 26228975
Conc: 610.81 ng/ml

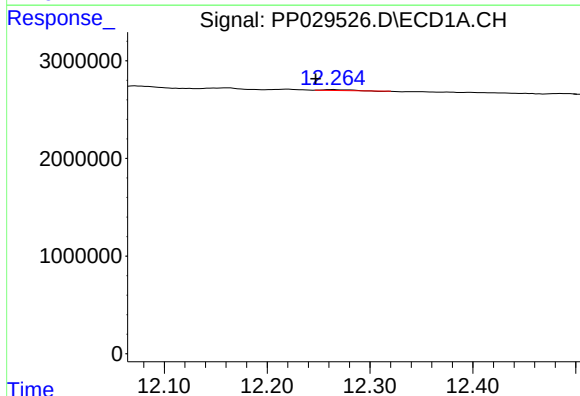


#5 DICAMBA

R.T.: 12.264 min
Delta R.T.: 0.017 min
Response: 146440
Conc: 0.99 ng/ml

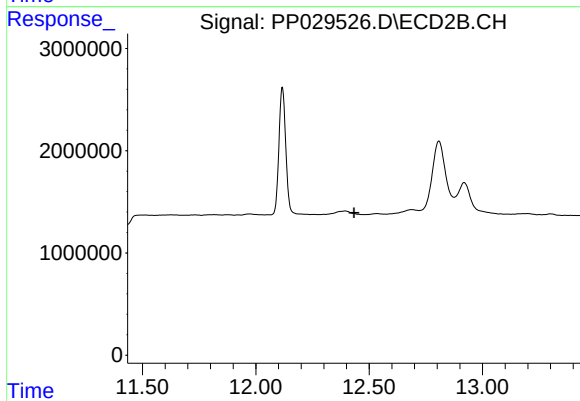

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.433 min
Response: 0
Conc: N.D.

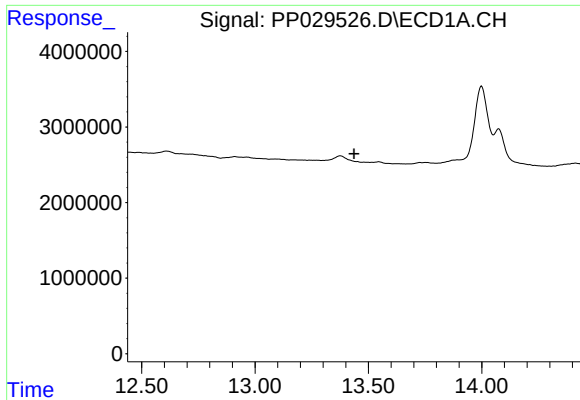

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CS-5

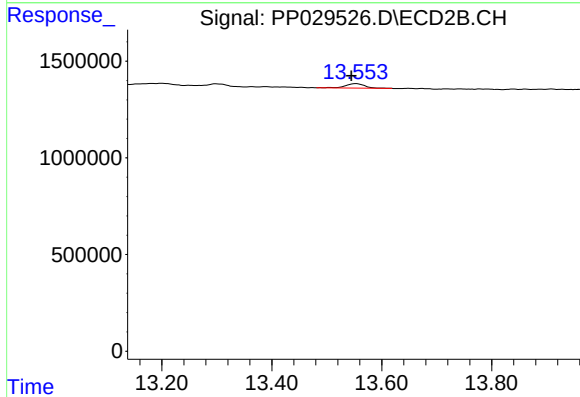


#8 DICHLORPROP

R.T.: 13.554 min
Delta R.T.: 0.009 min
Response: 540496
Conc: 13.35 ng/ml

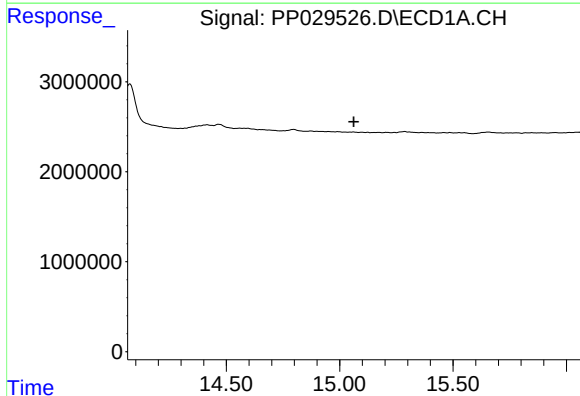


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 15.062 min
Response: 0
Conc: N.D.

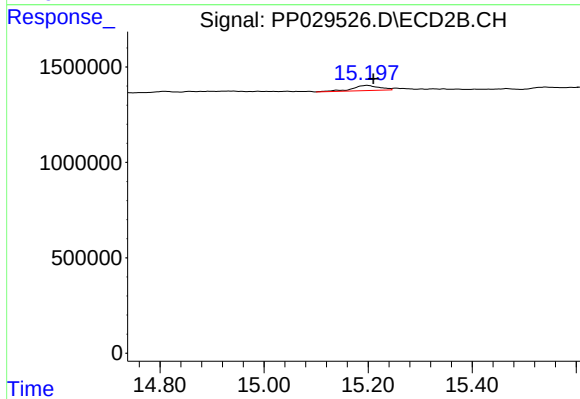

#11 2,4,5-TP (SILVEX)


R.T.: 15.199 min
Delta R.T.: -0.011 min
Response: 961595
Conc: 4.65 ng/ml

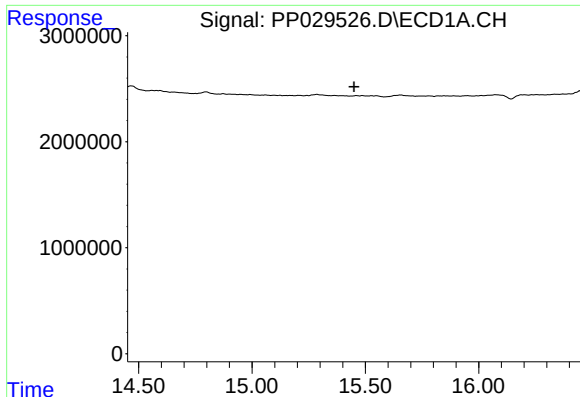

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CS-5

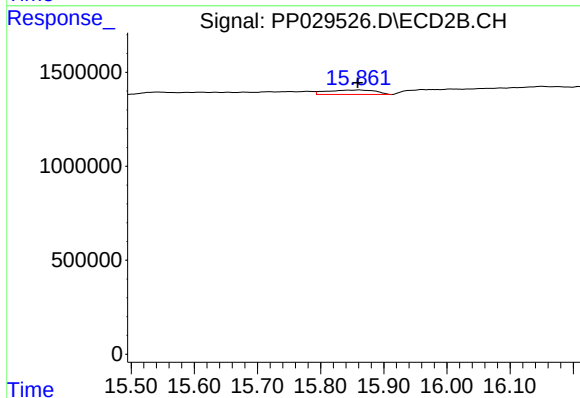


#12 2,4,5-T

R.T.: 15.861 min
Delta R.T.: 0.003 min
Response: 1269352
Conc: 7.66 ng/ml

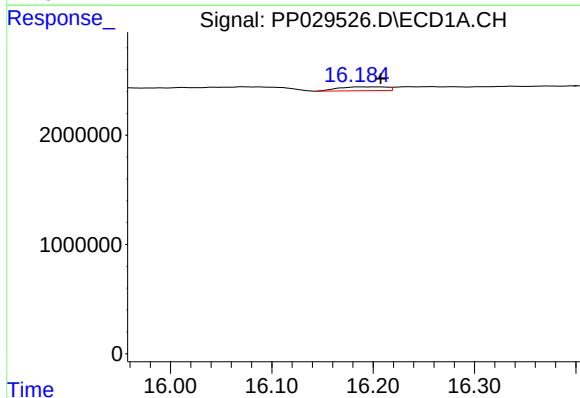


#13 2,4-DB

R.T.: 16.202 min
Delta R.T.: -0.005 min
Response: 1165478
Conc: 56.05 ng/ml

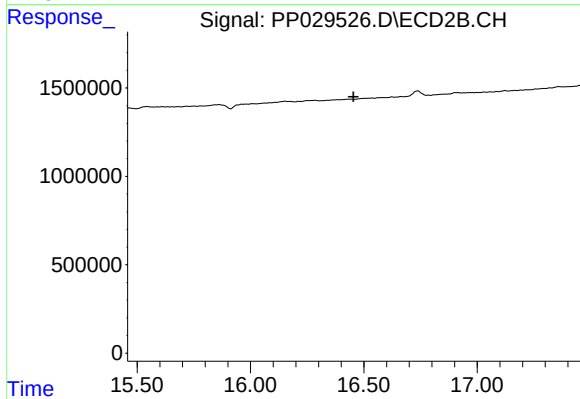

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.455 min
Response: 0
Conc: N.D.

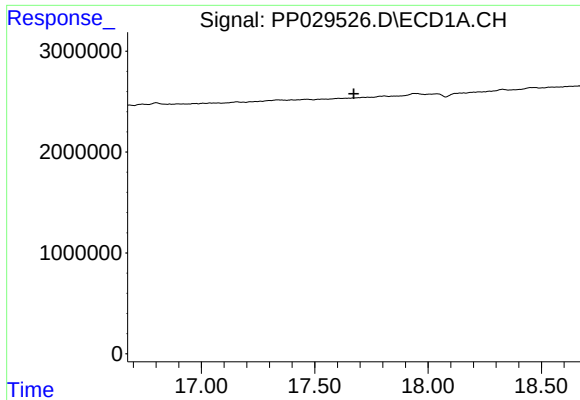

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.672 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CS-5

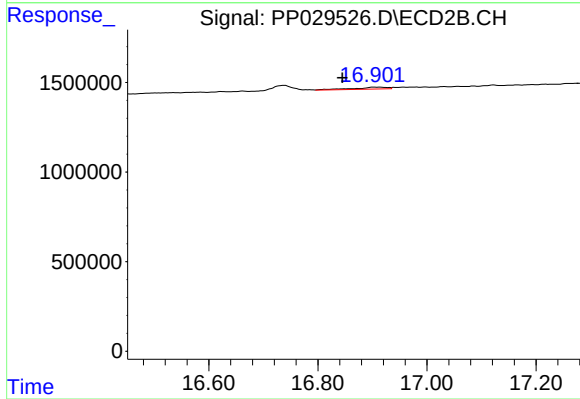


#14 DINOSEB

R.T.: 16.904 min
Delta R.T.: 0.059 min
Response: 447838
Conc: 2.96 ng/ml

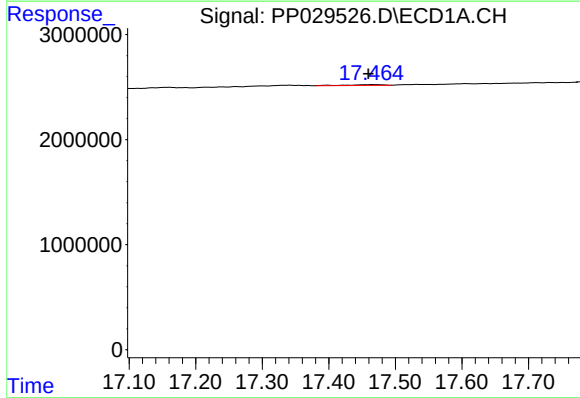


#15 Picloram

R.T.: 17.466 min
Delta R.T.: 0.007 min
Response: 266556
Conc: 0.81 ng/ml

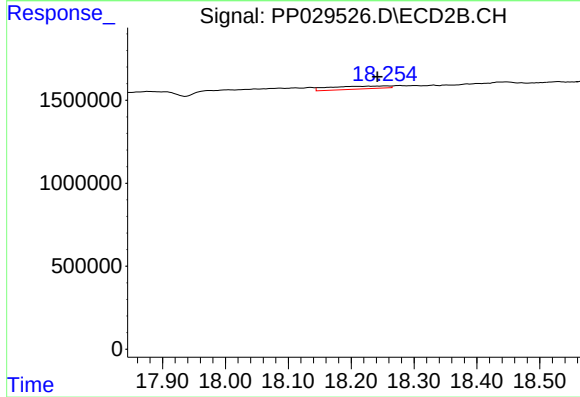

#15 Picloram


R.T.: 18.257 min
Delta R.T.: 0.015 min
Response: 1131438
Conc: 4.75 ng/ml

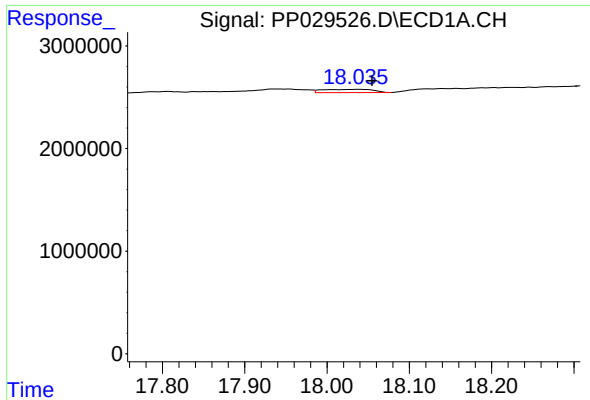

#16 DCPA

R.T.: 18.039 min
Delta R.T.: -0.016 min
Response: 1354046
Conc: 4.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
CS-5

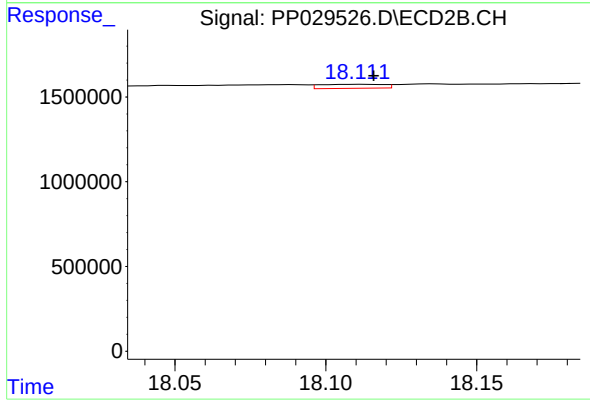

#16 DCPA

R.T.: 18.112 min
Delta R.T.: -0.004 min
Response: 343659
Conc: 1.31 ng/ml