

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
 Data File : PP029531.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2019 16:40
 Operator : EI\MA
 Sample : K2050-10
 Misc : hexane
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CS-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 03:36:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.925	12.118	18924227	23584379	578.457	549.223
Target Compounds							
5) T	DICAMBA	12.260	0.000	358898	0	2.429	N.D. #
8) T	DICHLORPROP	13.373	13.551	-134798	913356	N.D.	22.554
9) T	2,4-D	13.759	0.000	387933	0	10.031	N.D. #
11) T	2,4,5-TP ...	0.000	15.194	0	74660	N.D.	0.361 #
12) T	2,4,5-T	0.000	15.852	0	1705919	N.D.	10.290 #
13) T	2,4-DB	16.232	0.000	1239261	0	59.597	N.D. #
14) T	DINOSEB	17.661	0.000	38030	0	0.226	N.D. #
15) T	Picloram	17.470	0.000	112563	0	0.344	N.D. #
16) T	DCPA	18.050	0.000	742773	0	2.341	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
Data File : PP029531.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2019 16:40
Operator : EI\MA
Sample : K2050-10
Misc : hexane
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
CS-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 03:36:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

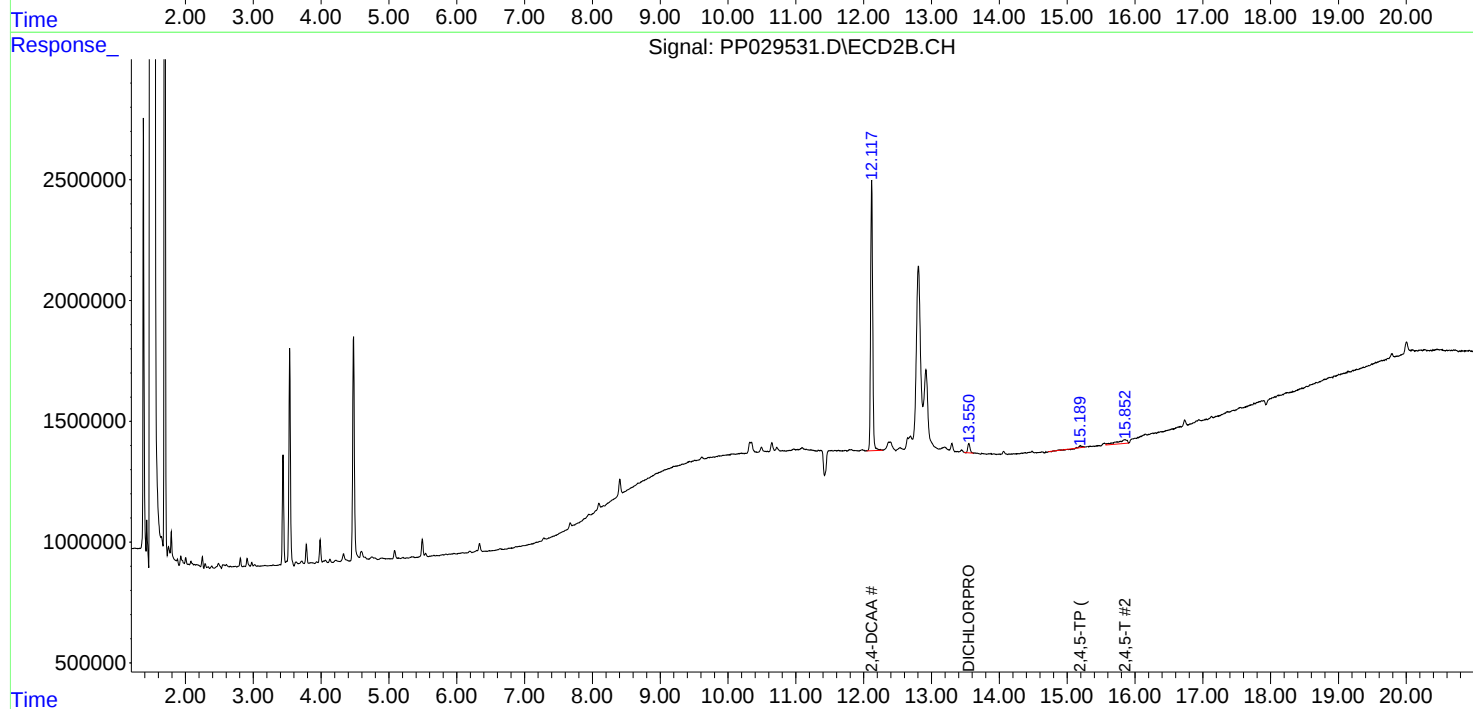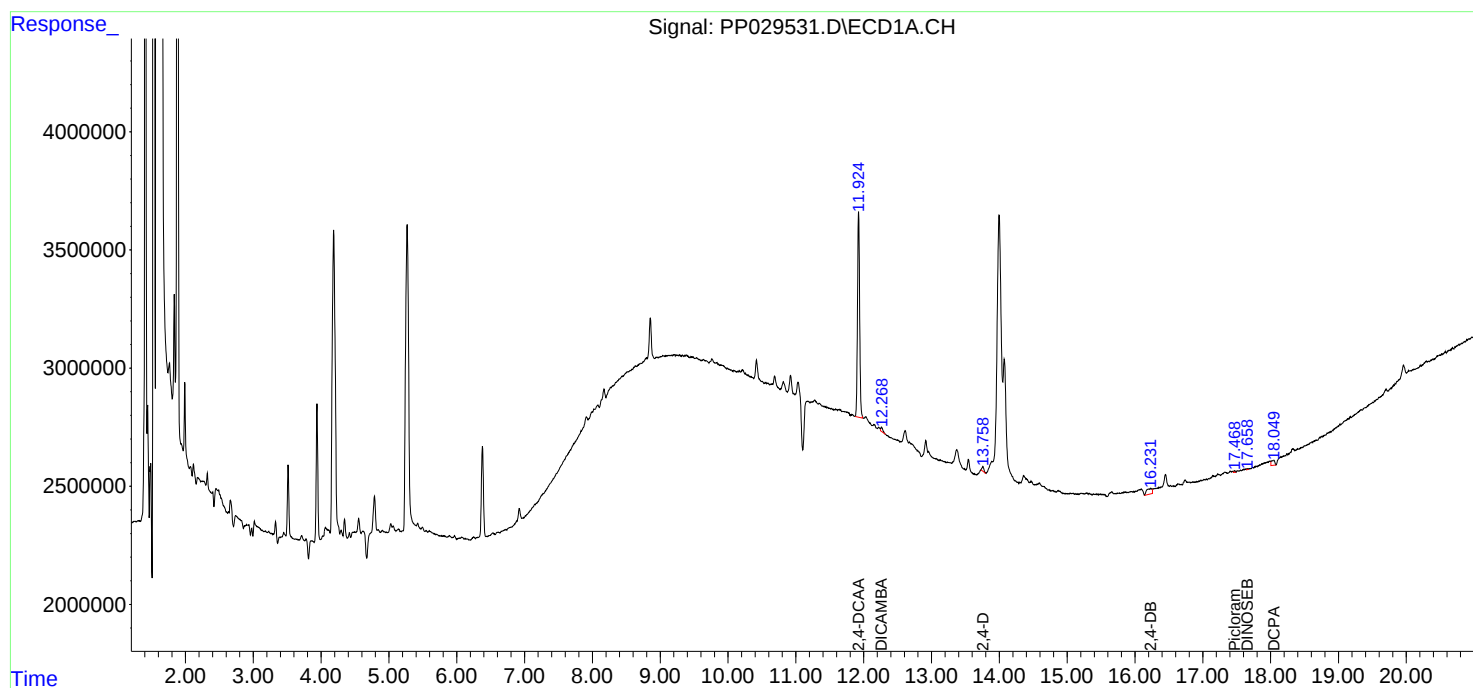


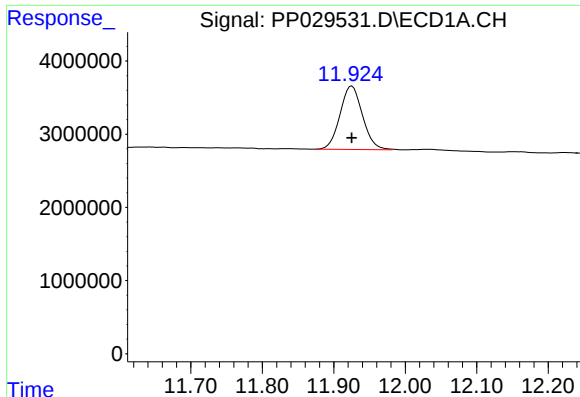

#4 2,4-DCAA


R.T.: 11.925 min
Delta R.T.: 0.000 min
Response: 18924227
Conc: 578.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
CS-2

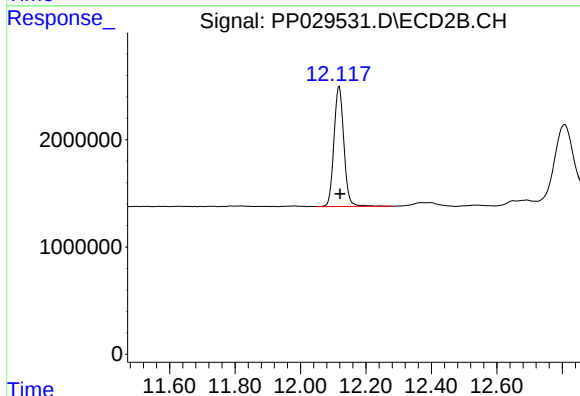


#4 2,4-DCAA

R.T.: 12.118 min
Delta R.T.: -0.003 min
Response: 23584379
Conc: 549.22 ng/ml

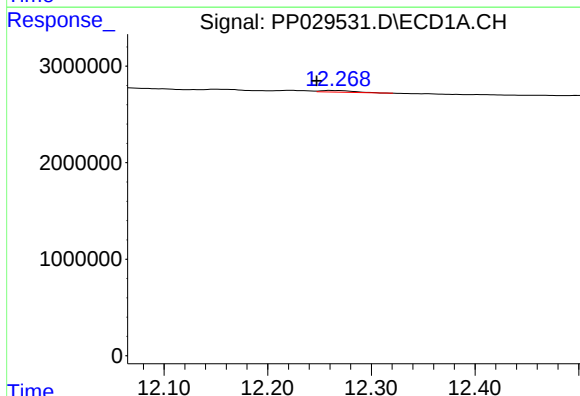


#5 DICAMBA

R.T.: 12.260 min
Delta R.T.: 0.013 min
Response: 358898
Conc: 2.43 ng/ml

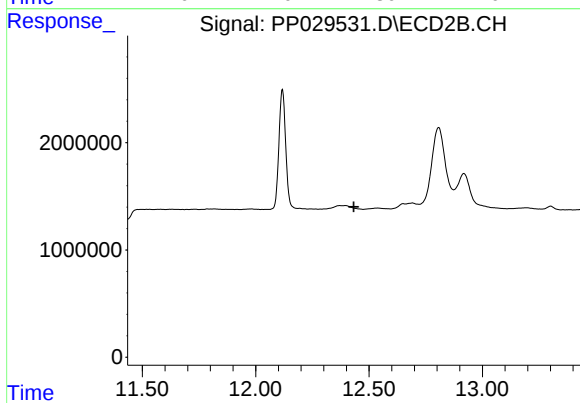

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.433 min
Response: 0
Conc: N.D.

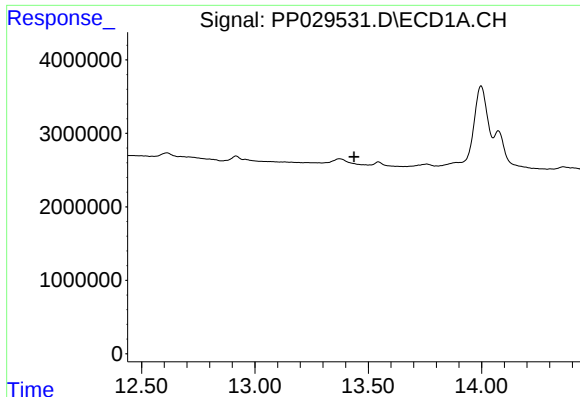

#8 DICHLORPROP


R.T.: 13.373 min
Delta R.T.: -0.064 min
Response: -134798
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CS-2

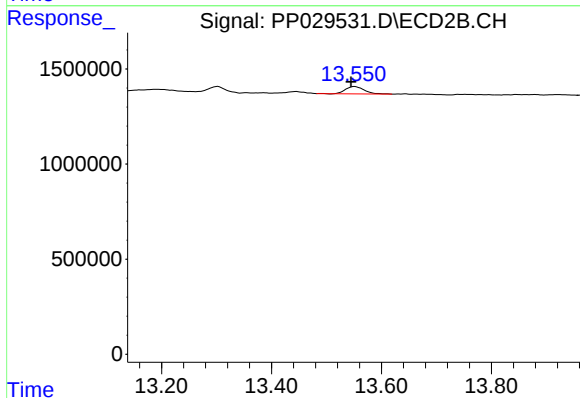


#8 DICHLORPROP

R.T.: 13.551 min
Delta R.T.: 0.007 min
Response: 913356
Conc: 22.55 ng/ml

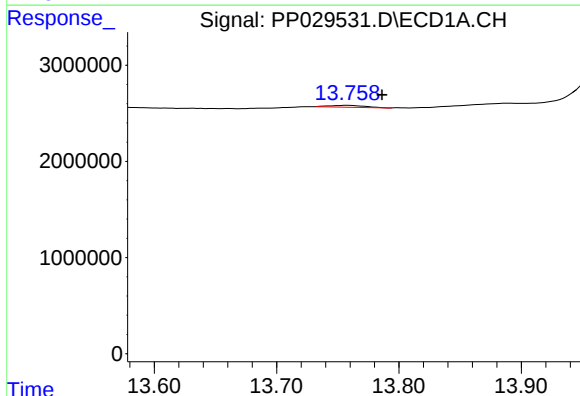


#9 2,4-D

R.T.: 13.759 min
Delta R.T.: -0.028 min
Response: 387933
Conc: 10.03 ng/ml

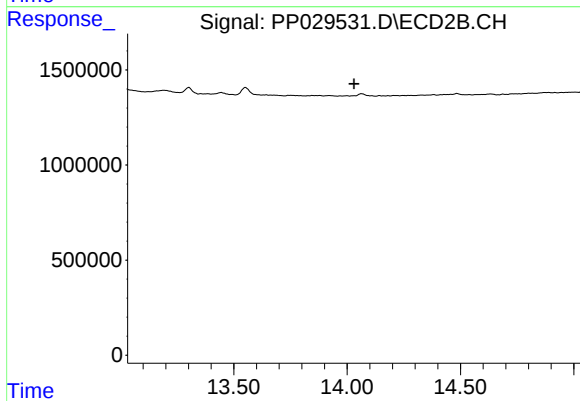

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 14.031 min
Response: 0
Conc: N.D.

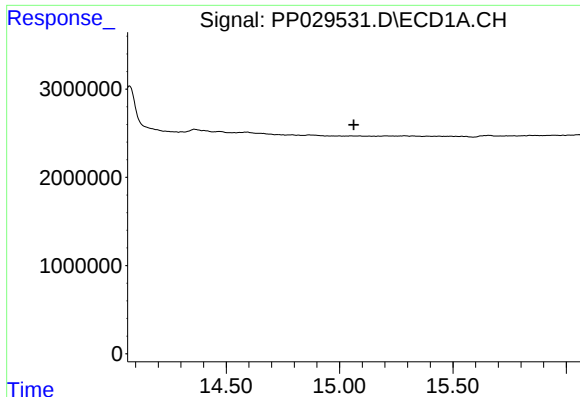

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CS-2

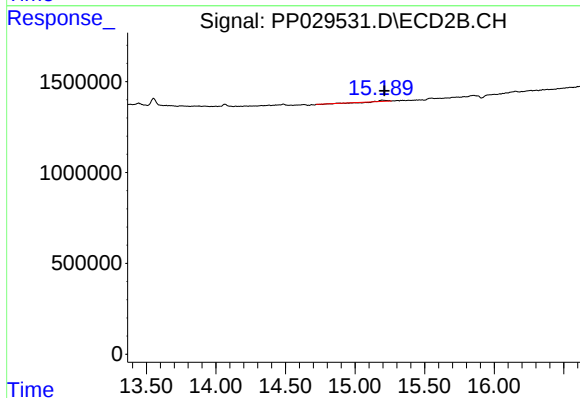


#11 2,4,5-TP (SILVEX)

R.T.: 15.194 min
Delta R.T.: -0.016 min
Response: 74660
Conc: 0.36 ng/ml

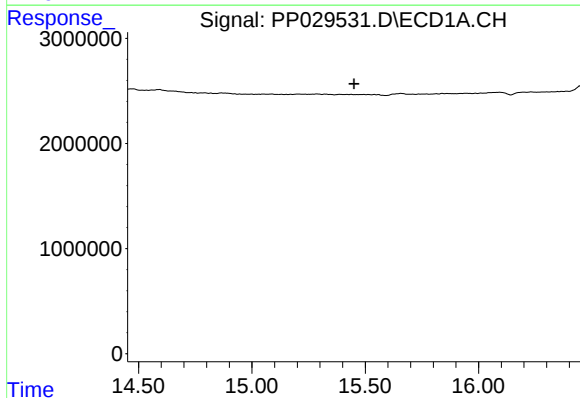


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

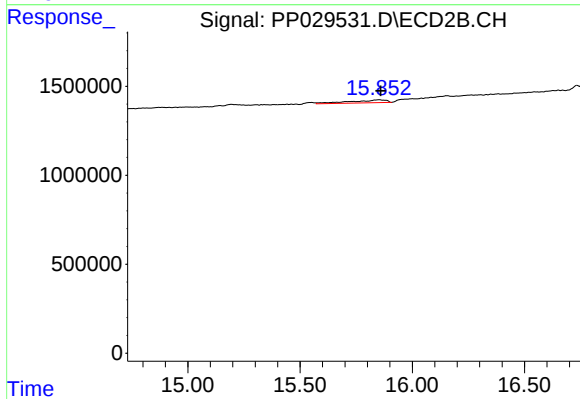

#12 2,4,5-T


R.T.: 15.852 min
Delta R.T.: -0.007 min
Response: 1705919
Conc: 10.29 ng/ml

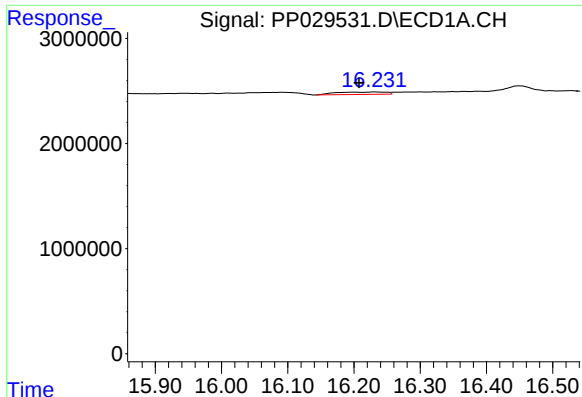

#13 2,4-DB


R.T.: 16.232 min
Delta R.T.: 0.024 min
Response: 1239261
Conc: 59.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
CS-2

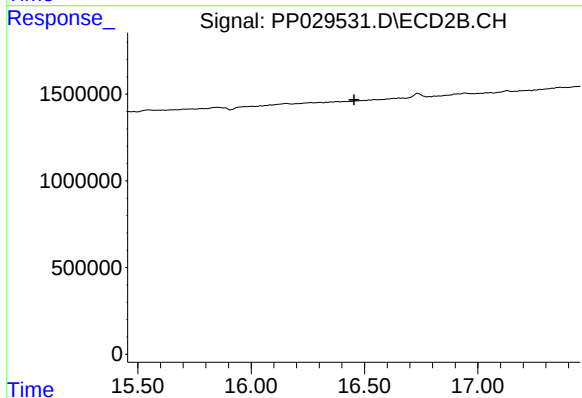


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

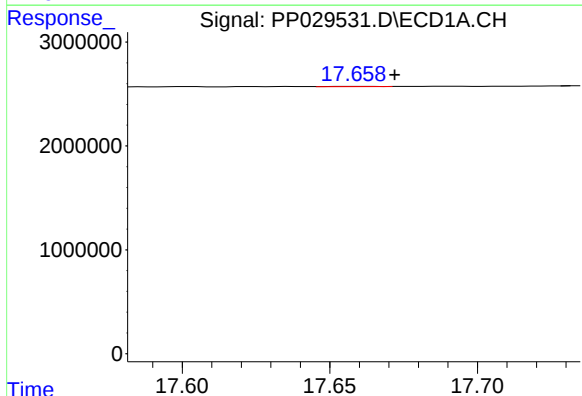


#14 DINOSEB

R.T.: 17.661 min
Delta R.T.: -0.011 min
Response: 38030
Conc: 0.23 ng/ml

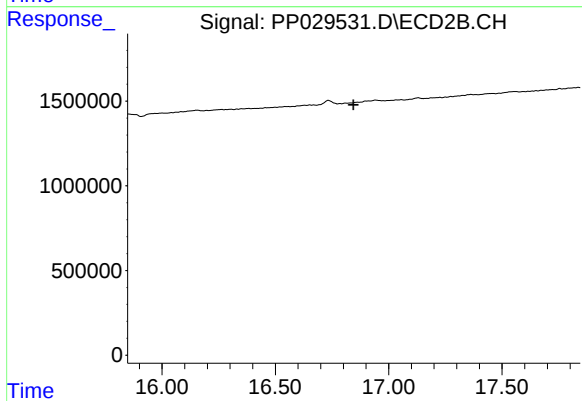

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.845 min
Response: 0
Conc: N.D.

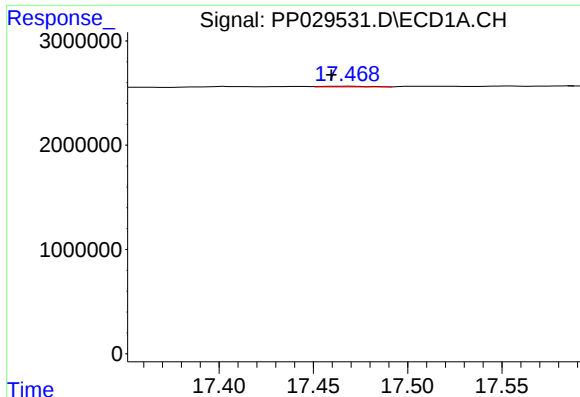

#15 Picloram


R.T.: 17.470 min
Delta R.T.: 0.010 min
Response: 112563
Conc: 0.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
CS-2

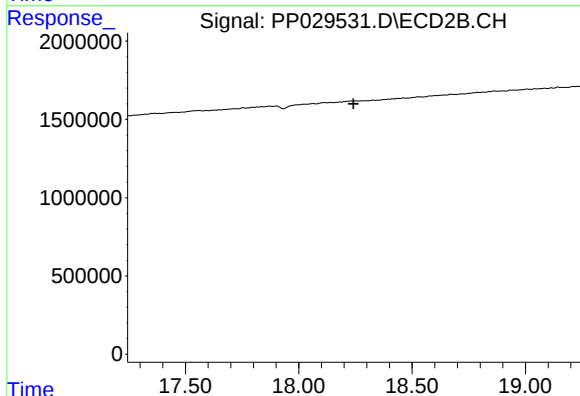


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.242 min
Response: 0
Conc: N.D.

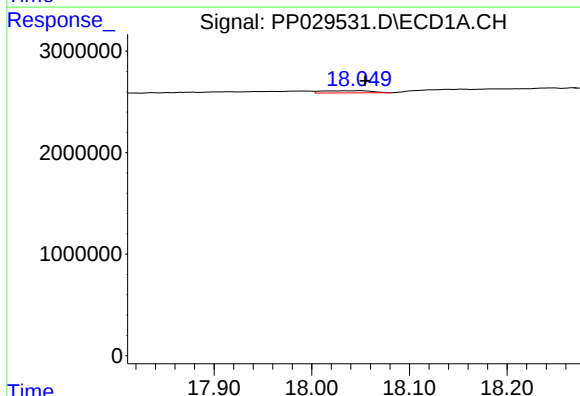

#16 DCPA

R.T.: 18.050 min
Delta R.T.: -0.005 min
Response: 742773
Conc: 2.34 ng/ml

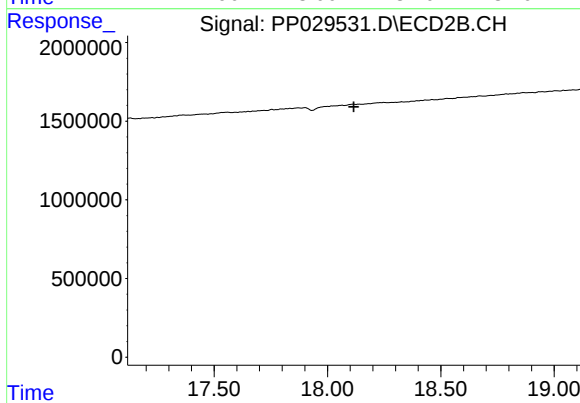

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.116 min
Response: 0
Conc: N.D.