

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
 Data File : PP029532.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2019 17:06
 Operator : EI\MA
 Sample : K2050-11
 Misc : hexane
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CS-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 03:37:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.118	22199844	27897208	678.583	649.659
Target Compounds							
1) T	Dalapon	0.000	2.979	0	19590	N.D.	0.358 #
8) T	DICHLORPROP	0.000	13.552	0	749663	N.D.	18.512 #
9) T	2,4-D	13.760	0.000	176490	0	4.564	N.D. #
12) T	2,4,5-T	0.000	15.844	0	1015253	N.D.	6.124 #
13) T	2,4-DB	16.220	0.000	803872	0	38.659	N.D. #
14) T	DINOSEB	17.670	0.000	184537	0	1.095	N.D. #
15) T	Picloram	17.466	18.248	79618	3482972	0.243	14.613 #
16) T	DCPA	18.044	0.000	901881	0	2.843	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
Data File : PP029532.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2019 17:06
Operator : EI\MA
Sample : K2050-11
Misc : hexane
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
CS-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 03:37:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

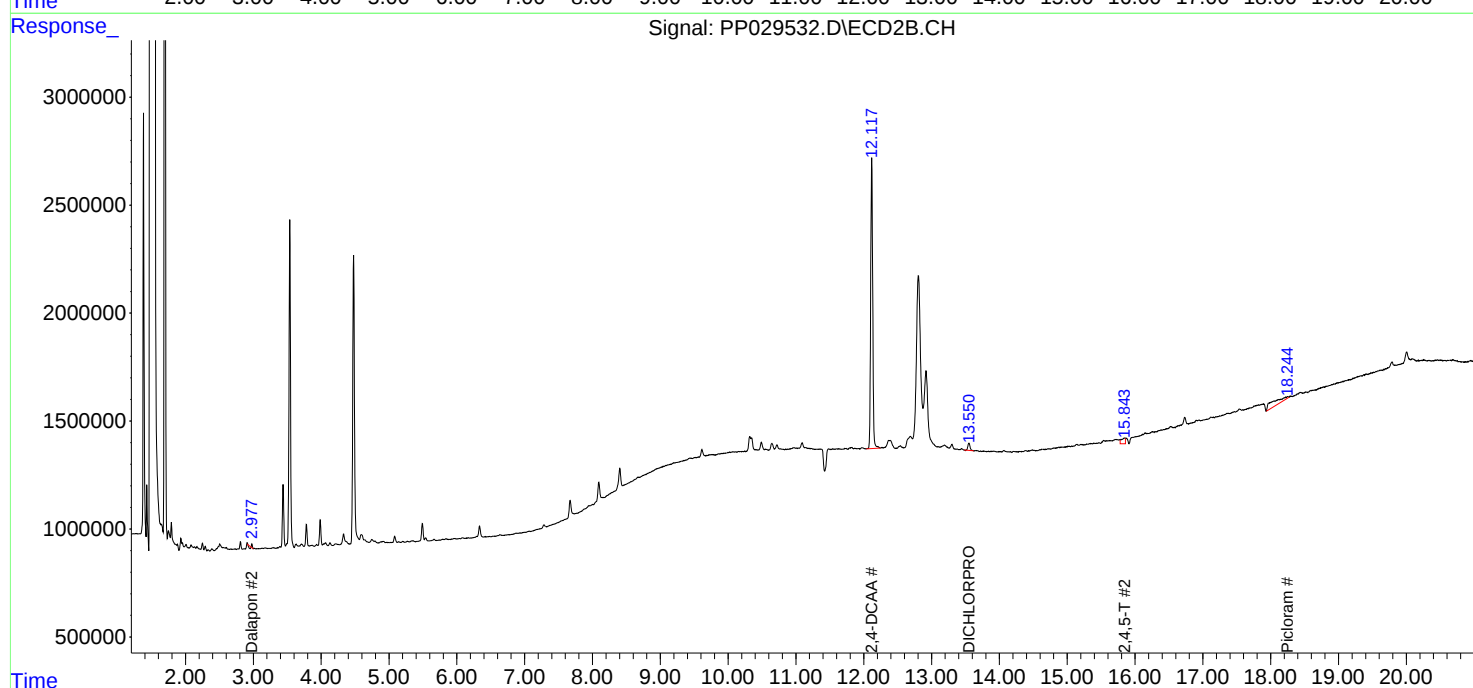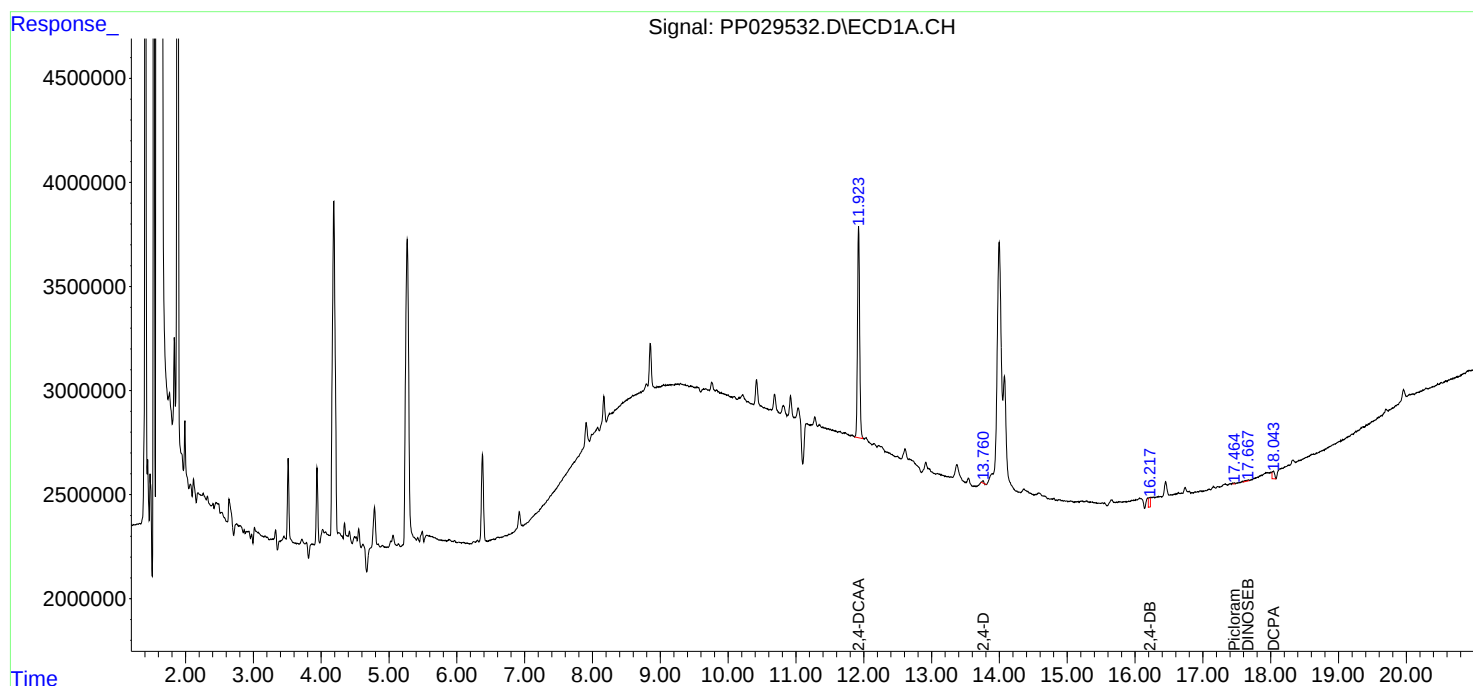


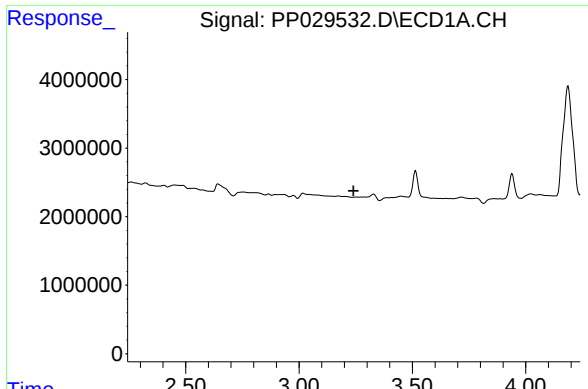

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CS-1

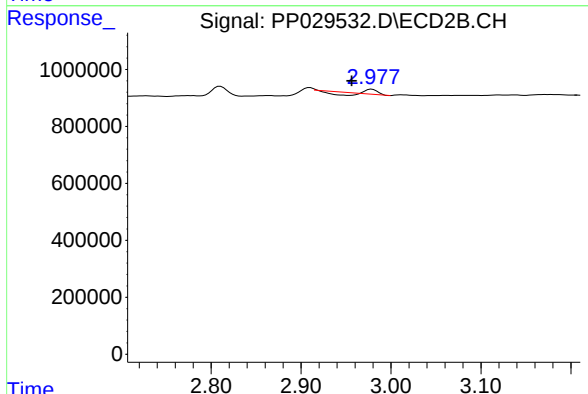


#1 Dalapon

R.T.: 2.979 min
Delta R.T.: 0.022 min
Response: 19590
Conc: 0.36 ng/ml

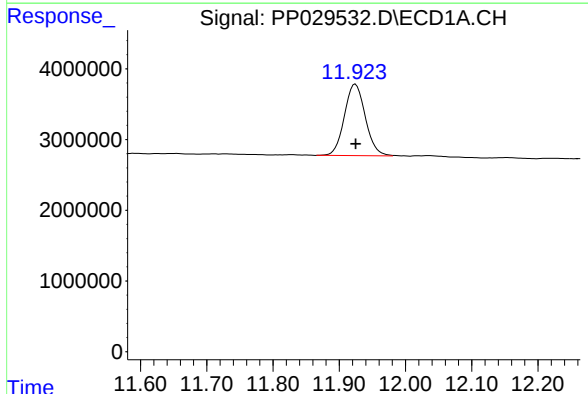


#4 2,4-DCAA

R.T.: 11.924 min
Delta R.T.: 0.000 min
Response: 22199844
Conc: 678.58 ng/ml

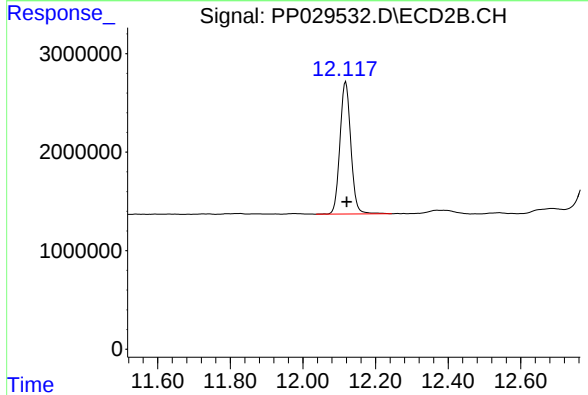

#4 2,4-DCAA


R.T.: 12.118 min
Delta R.T.: -0.003 min
Response: 27897208
Conc: 649.66 ng/ml

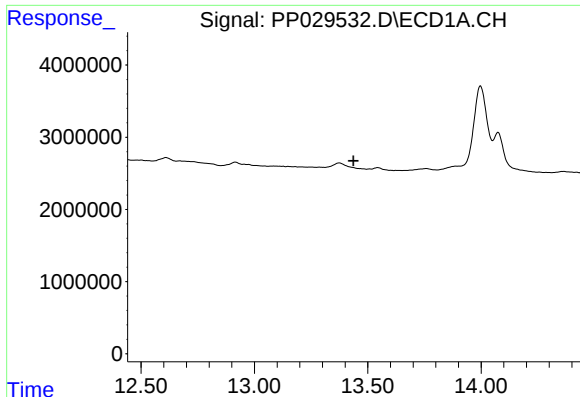

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CS-1

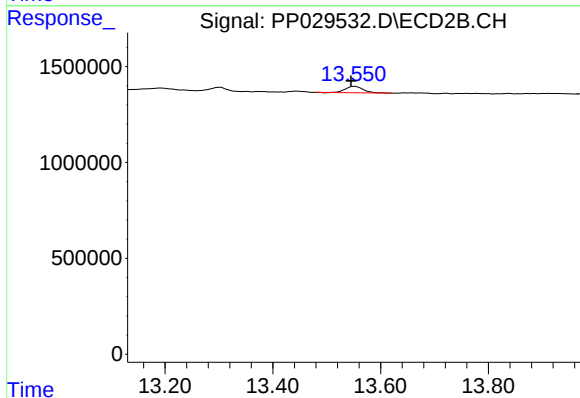


#8 DICHLORPROP

R.T.: 13.552 min
Delta R.T.: 0.007 min
Response: 749663
Conc: 18.51 ng/ml

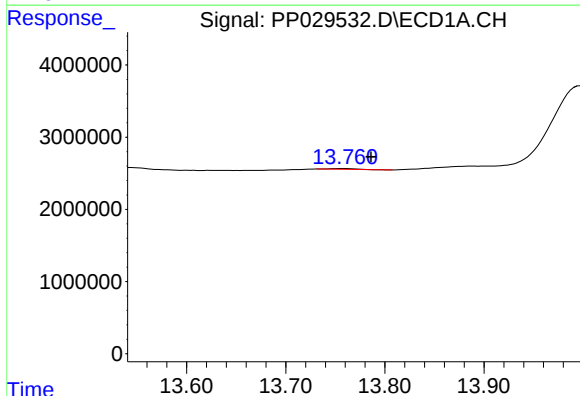


#9 2,4-D

R.T.: 13.760 min
Delta R.T.: -0.026 min
Response: 176490
Conc: 4.56 ng/ml

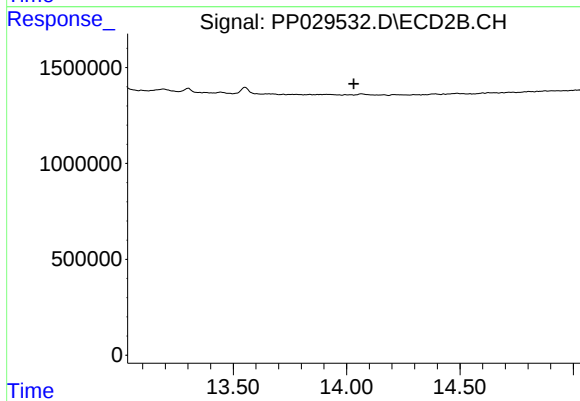

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 14.031 min
Response: 0
Conc: N.D.

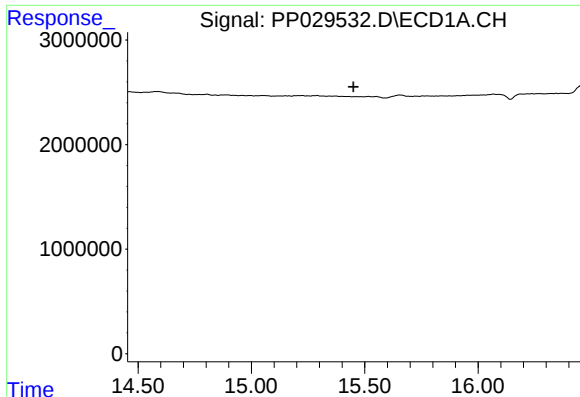

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CS-1

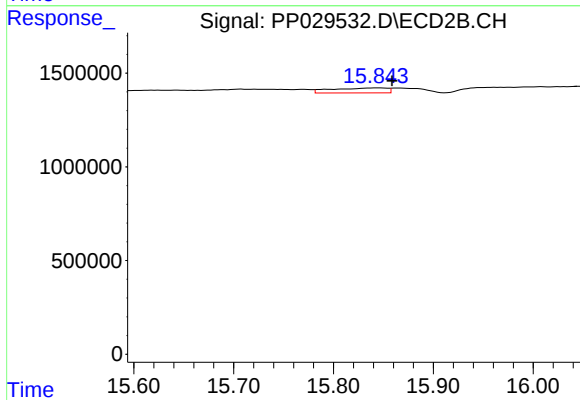


#12 2,4,5-T

R.T.: 15.844 min
Delta R.T.: -0.014 min
Response: 1015253
Conc: 6.12 ng/ml

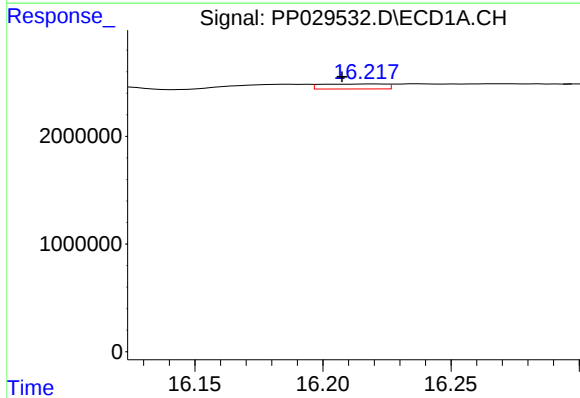


#13 2,4-DB

R.T.: 16.220 min
Delta R.T.: 0.012 min
Response: 803872
Conc: 38.66 ng/ml

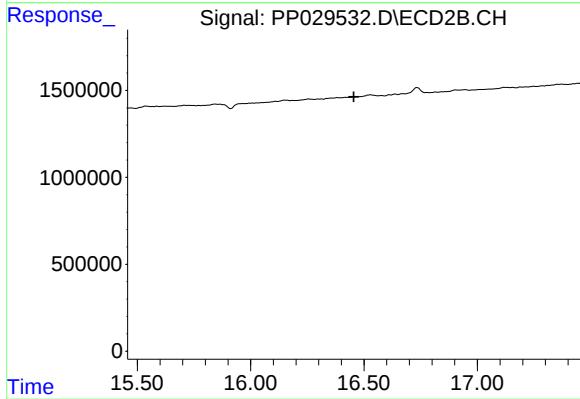

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.455 min
Response: 0
Conc: N.D.

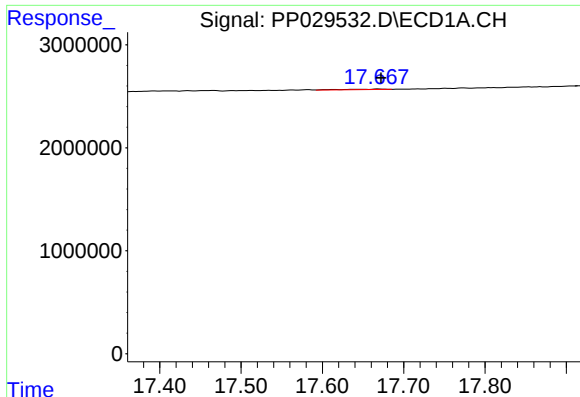

#14 DINOSEB


R.T.: 17.670 min
Delta R.T.: -0.002 min
Response: 184537
Conc: 1.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
CS-1

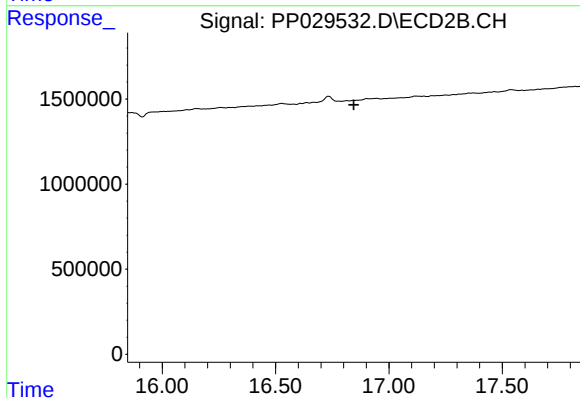


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.845 min
Response: 0
Conc: N.D.

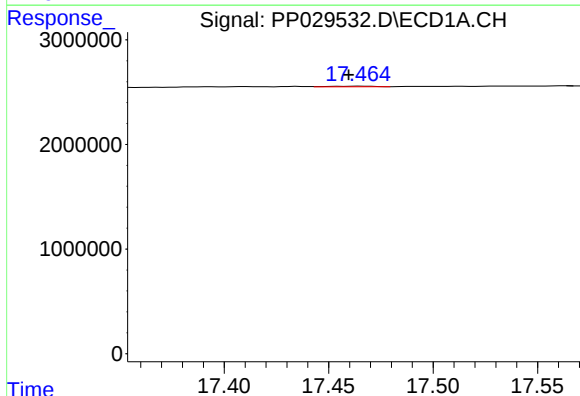


#15 Picloram

R.T.: 17.466 min
Delta R.T.: 0.006 min
Response: 79618
Conc: 0.24 ng/ml

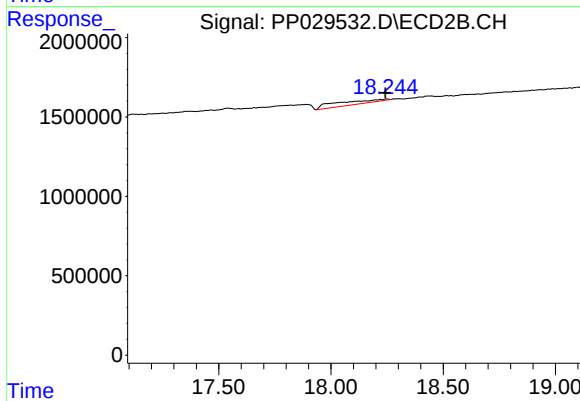

#15 Picloram


R.T.: 18.248 min
Delta R.T.: 0.006 min
Response: 3482972
Conc: 14.61 ng/ml

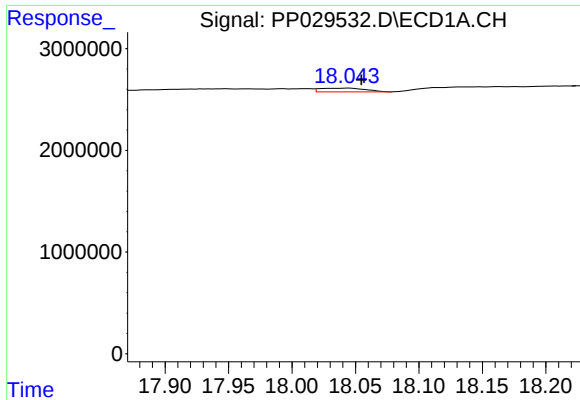

#16 DCPA

R.T.: 18.044 min
Delta R.T.: -0.010 min
Response: 901881
Conc: 2.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
CS-1

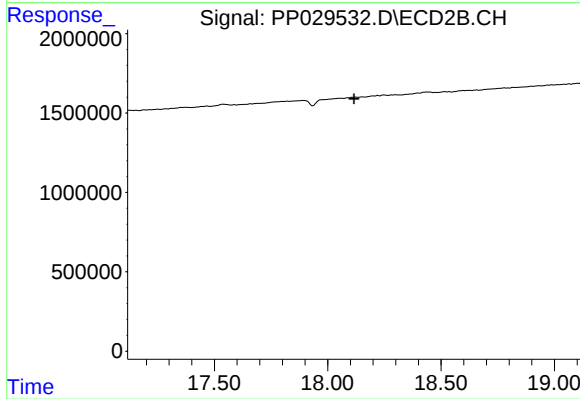

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.116 min
Response: 0
Conc: N.D.