

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
 Data File : PP029533.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2019 17:31
 Operator : EI\MA
 Sample : K2058-02
 Misc : hexane
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S3B(5-15)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 03:37:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.925	12.118	22207916	27870144	678.830	649.028
Target Compounds							
1) T	Dalapon	0.000	2.979	0	121669	N.D.	2.224 #
8) T	DICHLORPROP	13.369	13.552	-90231	862346	N.D.	21.294
11) T	2,4,5-TP ...	0.000	15.141	0	190640	N.D.	0.921 #
12) T	2,4,5-T	0.000	15.840	0	973522	N.D.	5.873 #
13) T	2,4-DB	16.202	16.395	1128633	61180	54.277	2.579 #
14) T	DINOSEB	0.000	16.810	0	72454	N.D.	0.480 #
15) T	Picloram	17.480	18.193	144535	851004	0.441	3.570 #
16) T	DCPA	18.040	18.110	3114210	953453	9.816	3.634 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
Data File : PP029533.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2019 17:31
Operator : EI\MA
Sample : K2058-02
Misc : hexane
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
S3B(5-15)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 03:37:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

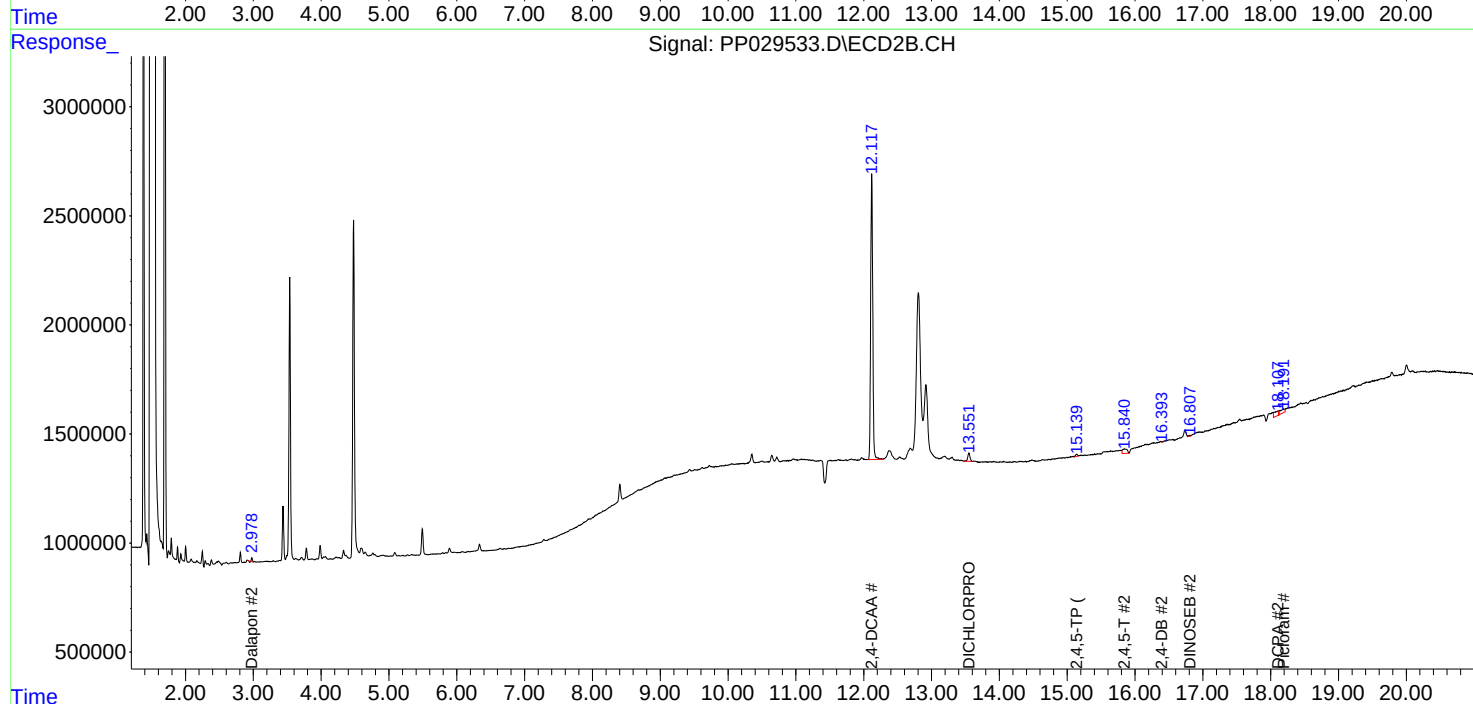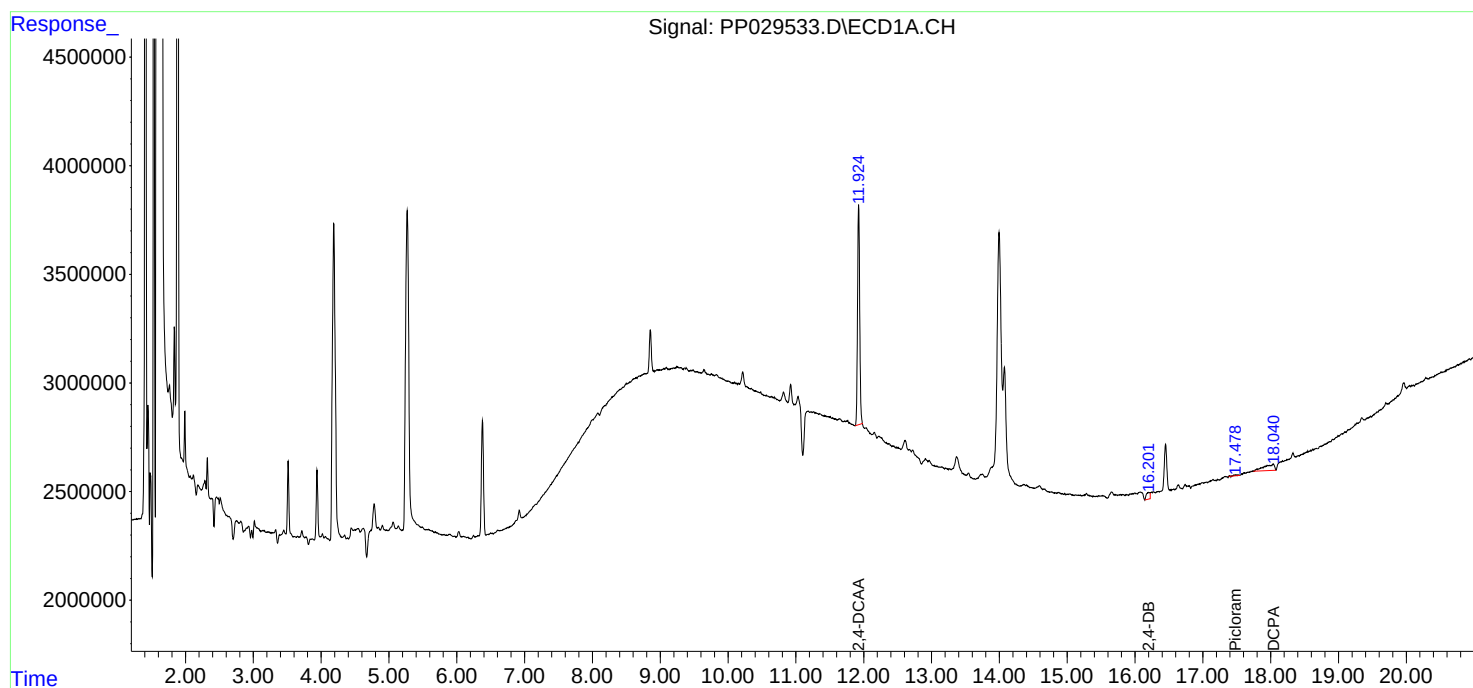


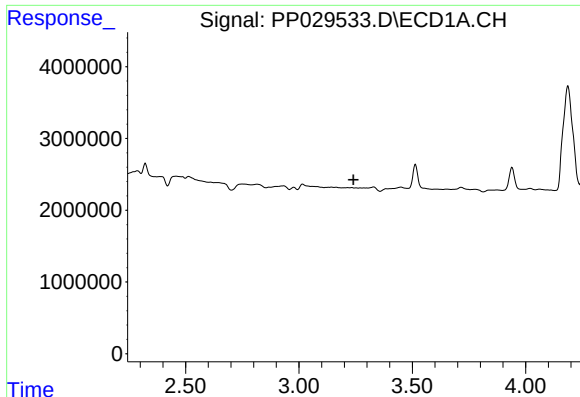

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S3B(5-15)COMP

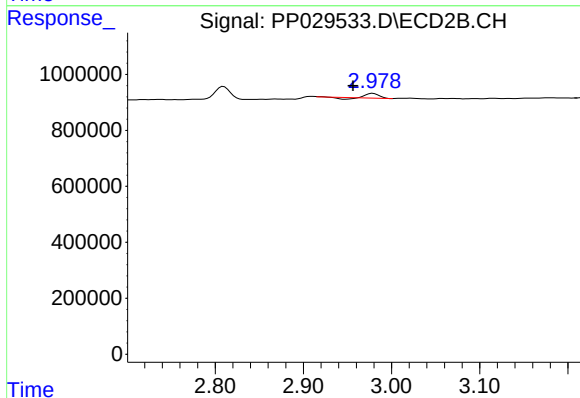


#1 Dalapon

R.T.: 2.979 min
Delta R.T.: 0.023 min
Response: 121669
Conc: 2.22 ng/ml

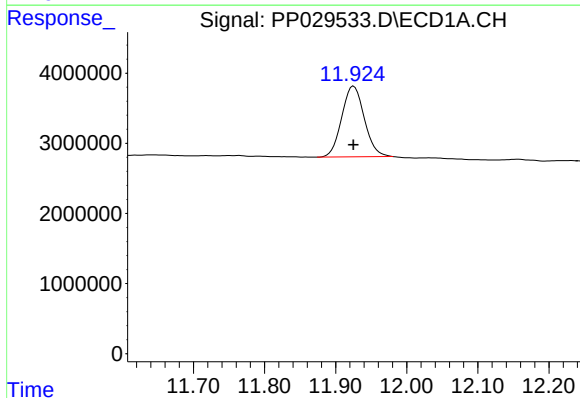


#4 2,4-DCAA

R.T.: 11.925 min
Delta R.T.: 0.000 min
Response: 22207916
Conc: 678.83 ng/ml

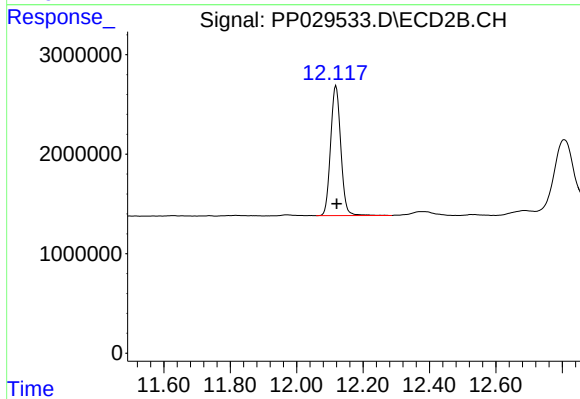

#4 2,4-DCAA


R.T.: 12.118 min
Delta R.T.: -0.003 min
Response: 27870144
Conc: 649.03 ng/ml

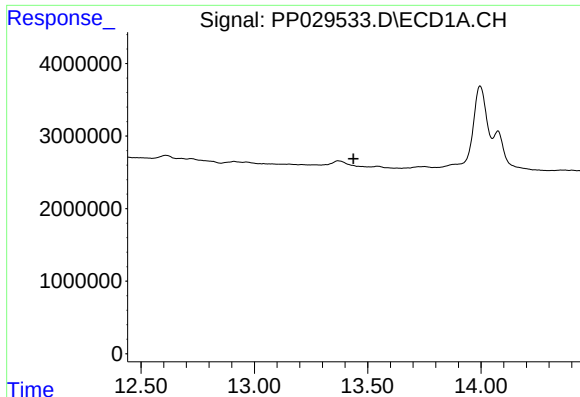

#8 DICHLORPROP


R.T.: 13.369 min
Delta R.T.: -0.069 min
Response: -90231
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S3B(5-15)COMP

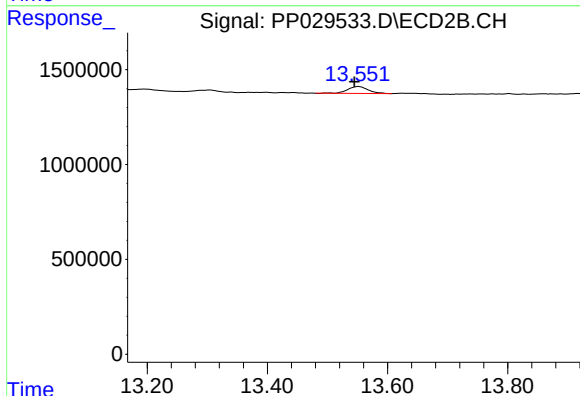


#8 DICHLORPROP

R.T.: 13.552 min
Delta R.T.: 0.007 min
Response: 862346
Conc: 21.29 ng/ml

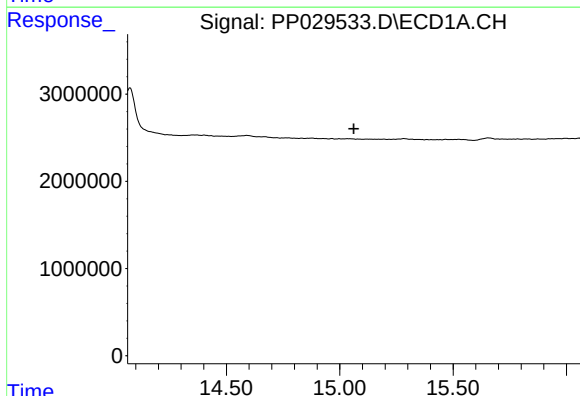


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 15.062 min
Response: 0
Conc: N.D.

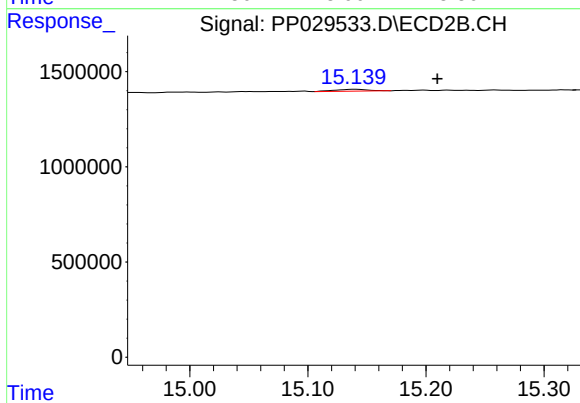

#11 2,4,5-TP (SILVEX)


R.T.: 15.141 min
Delta R.T.: -0.069 min
Response: 190640
Conc: 0.92 ng/ml

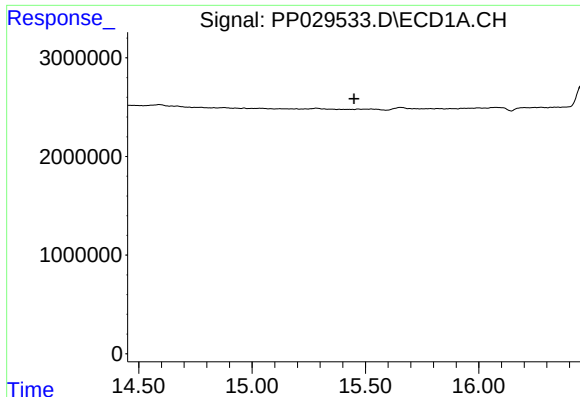

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S3B(5-15)COMP

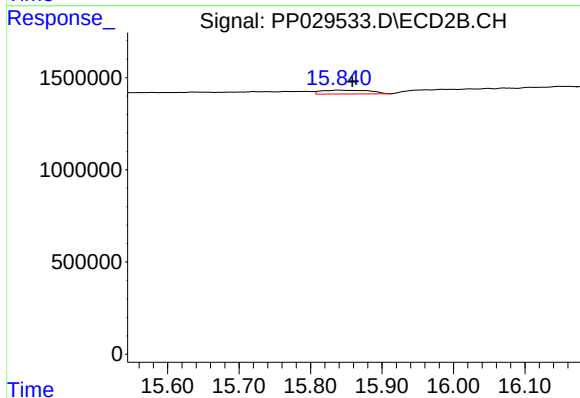


#12 2,4,5-T

R.T.: 15.840 min
Delta R.T.: -0.018 min
Response: 973522
Conc: 5.87 ng/ml

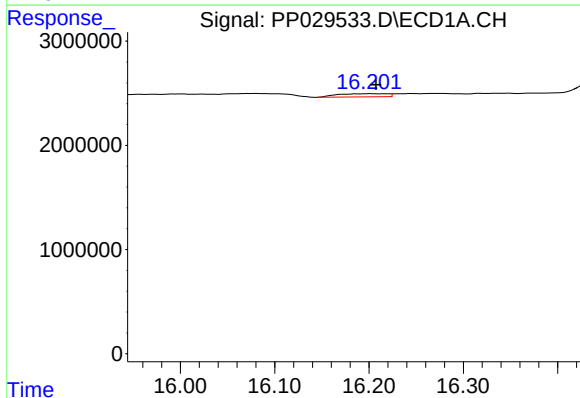


#13 2,4-DB

R.T.: 16.202 min
Delta R.T.: -0.005 min
Response: 1128633
Conc: 54.28 ng/ml

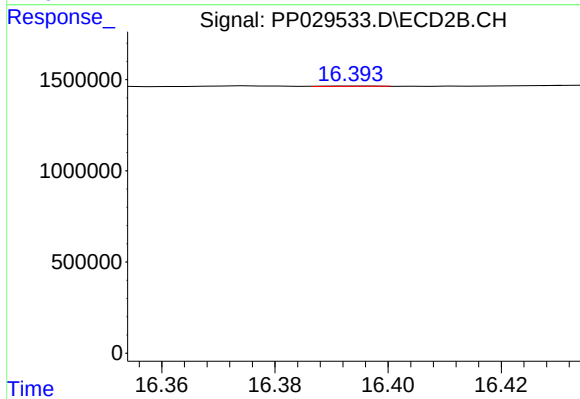

#13 2,4-DB


R.T.: 16.395 min
Delta R.T.: -0.060 min
Response: 61180
Conc: 2.58 ng/ml

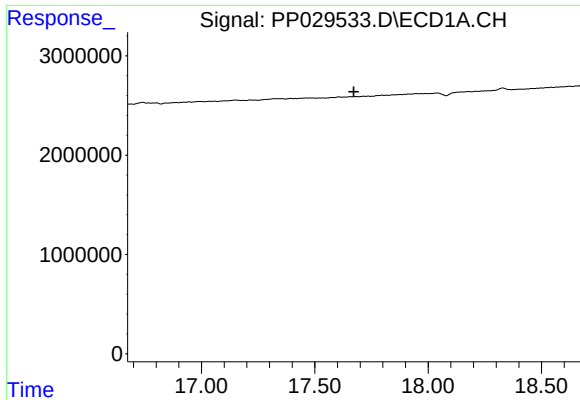

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.672 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S3B(5-15)COMP

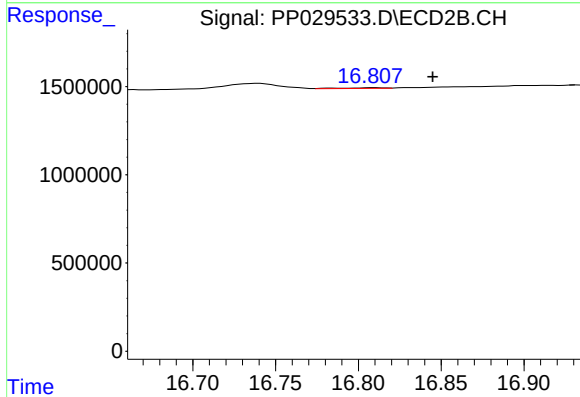


#14 DINOSEB

R.T.: 16.810 min
Delta R.T.: -0.035 min
Response: 72454
Conc: 0.48 ng/ml

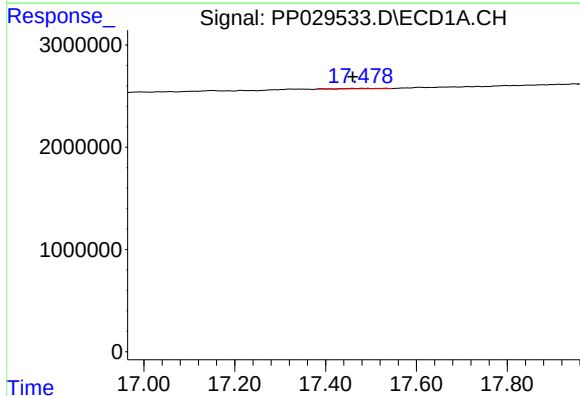


#15 Picloram

R.T.: 17.480 min
Delta R.T.: 0.020 min
Response: 144535
Conc: 0.44 ng/ml

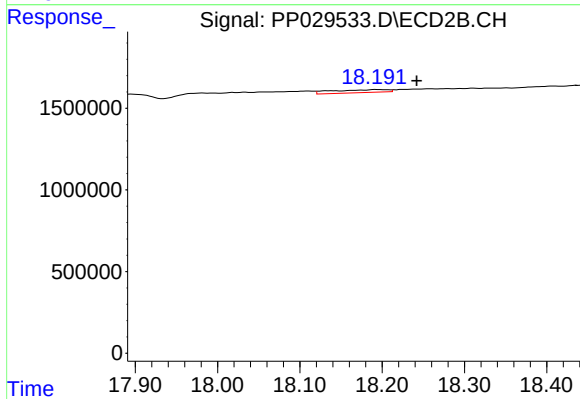

#15 Picloram


R.T.: 18.193 min
Delta R.T.: -0.049 min
Response: 851004
Conc: 3.57 ng/ml

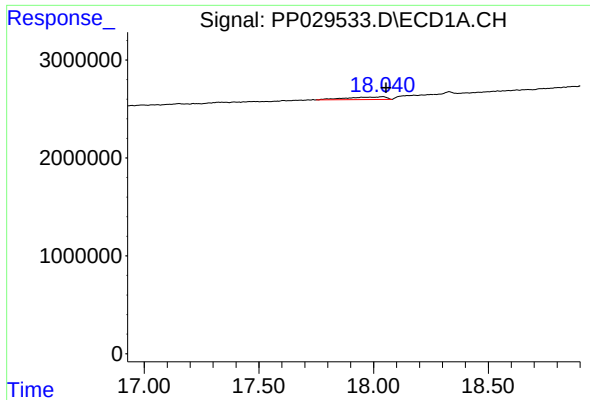

#16 DCPA

R.T.: 18.040 min
Delta R.T.: -0.015 min
Response: 3114210
Conc: 9.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
S3B(5-15)COMP

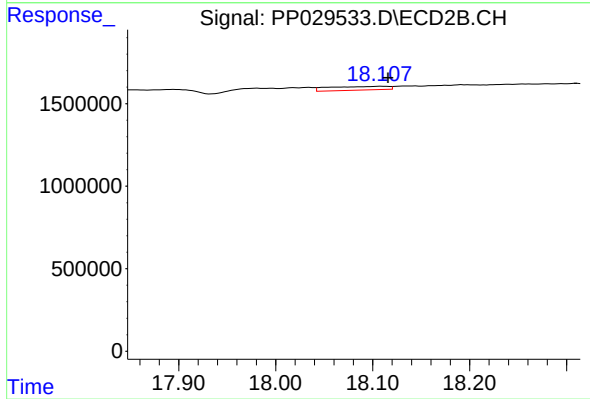

#16 DCPA

R.T.: 18.110 min
Delta R.T.: -0.006 min
Response: 953453
Conc: 3.63 ng/ml