

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
 Data File : PP029541.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2019 22:12
 Operator : EI\MA
 Sample : PB118291TB
 Misc : hexane
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB118291TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 03:39:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.118	24674591	26376422	754.229	614.243
Target Compounds							
5) T	DICAMBA	12.226	0.000	479607	0	3.246	N.D. #
8) T	DICHLORPROP	13.375	13.552	966121	973294	28.224	24.034
11) T	2,4,5-TP ...	0.000	15.142	0	397568	N.D.	1.921 #
12) T	2,4,5-T	0.000	15.849	0	1434744	N.D.	8.655 #
13) T	2,4-DB	16.194	0.000	572958	0	27.554	N.D. #
14) T	DINOSEB	17.664	16.915	80855	762787	0.480	5.049 #
15) T	Picloram	17.460	18.237	404423	582390	1.234	2.443 #
16) T	DCPA	18.040	18.095	556796	554745	1.755	2.114



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
Data File : PP029541.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2019 22:12
Operator : EI\MA
Sample : PB118291TB
Misc : hexane
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB118291TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 03:39:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

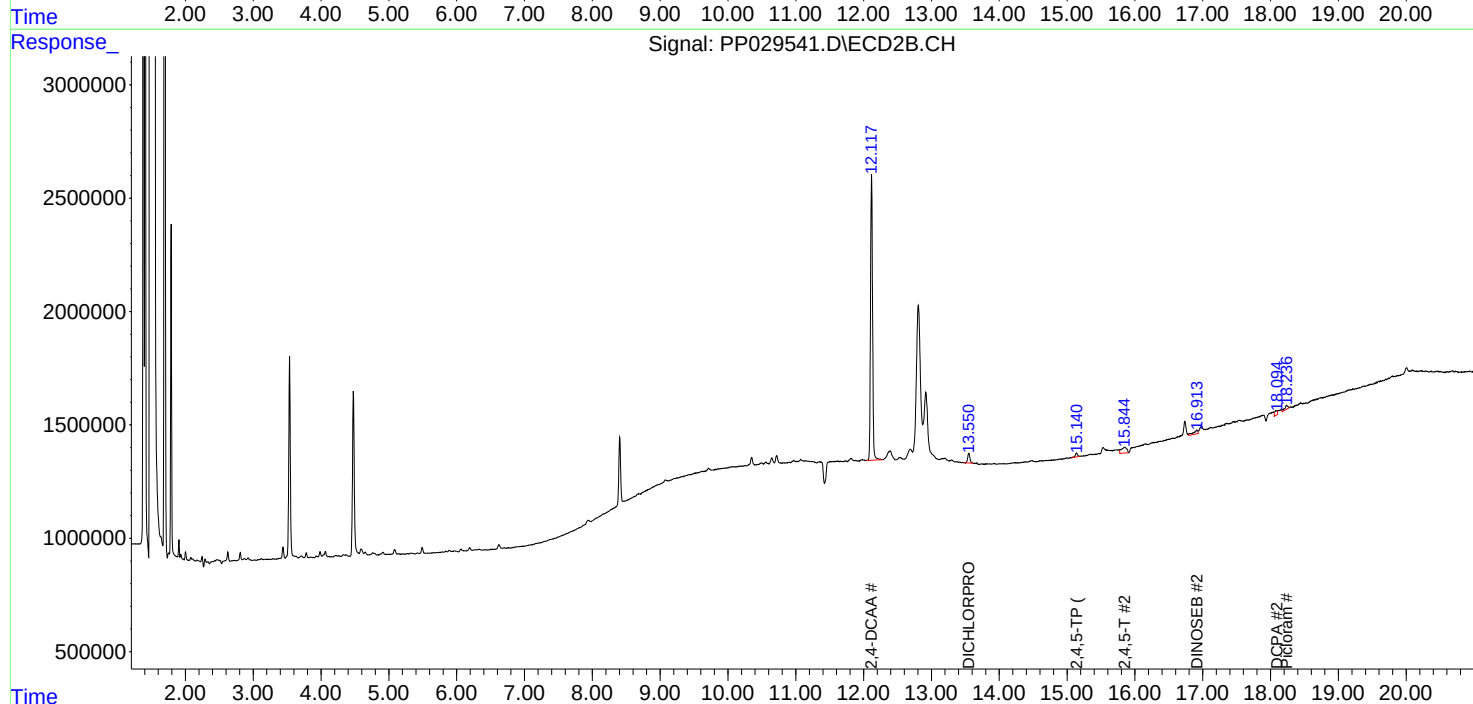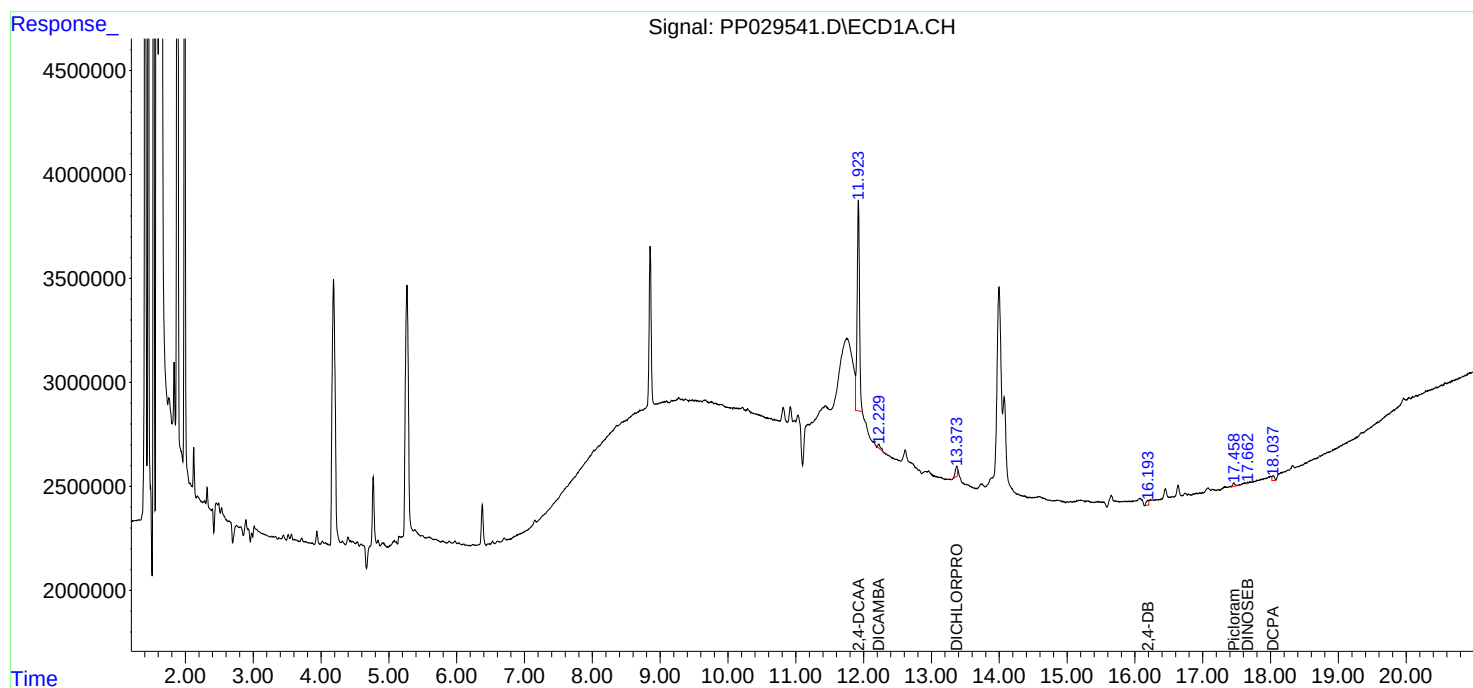


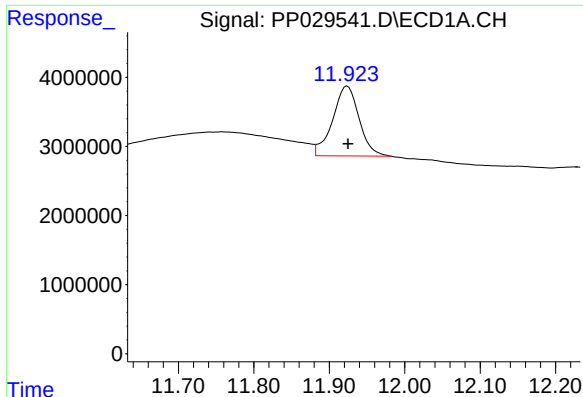

#4 2,4-DCAA


R.T.: 11.924 min
Delta R.T.: -0.001 min
Response: 24674591
Conc: 754.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118291TB

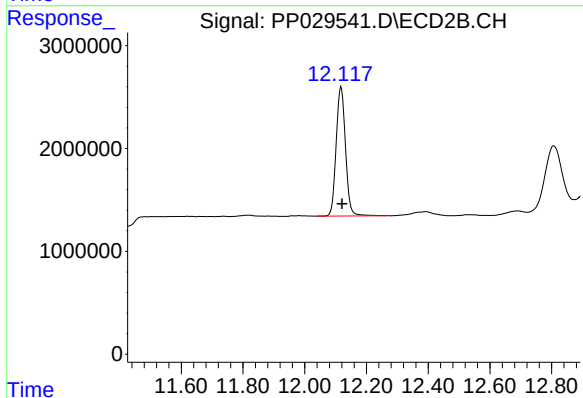


#4 2,4-DCAA

R.T.: 12.118 min
Delta R.T.: -0.003 min
Response: 26376422
Conc: 614.24 ng/ml

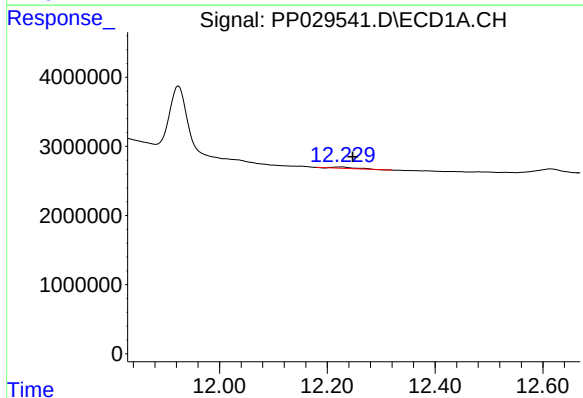


#5 DICAMBA

R.T.: 12.226 min
Delta R.T.: -0.021 min
Response: 479607
Conc: 3.25 ng/ml

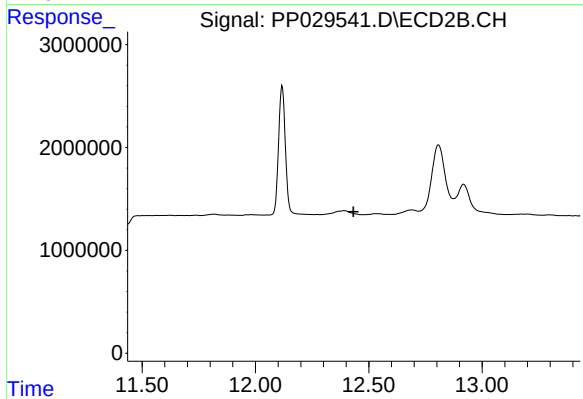

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.433 min
Response: 0
Conc: N.D.

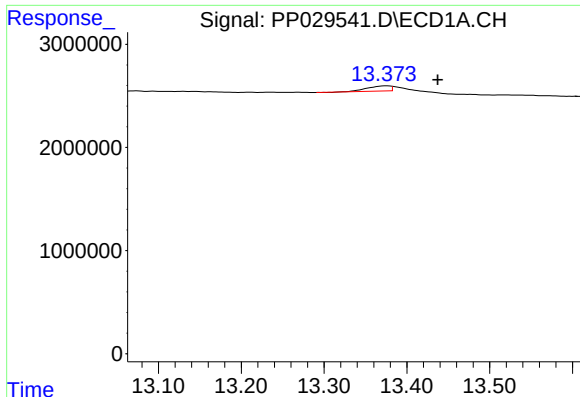

#8 DICHLORPROP


R.T.: 13.375 min
Delta R.T.: -0.062 min
Response: 966121
Conc: 28.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118291TB

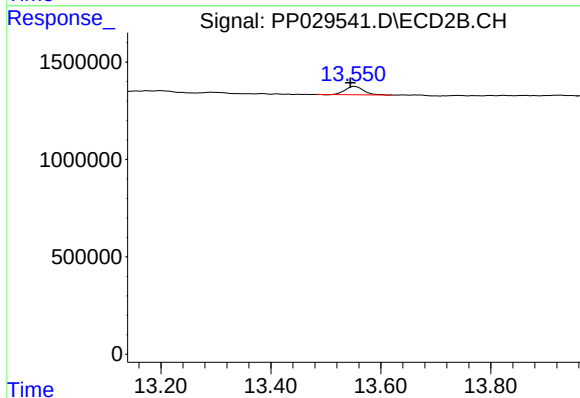


#8 DICHLORPROP

R.T.: 13.552 min
Delta R.T.: 0.007 min
Response: 973294
Conc: 24.03 ng/ml

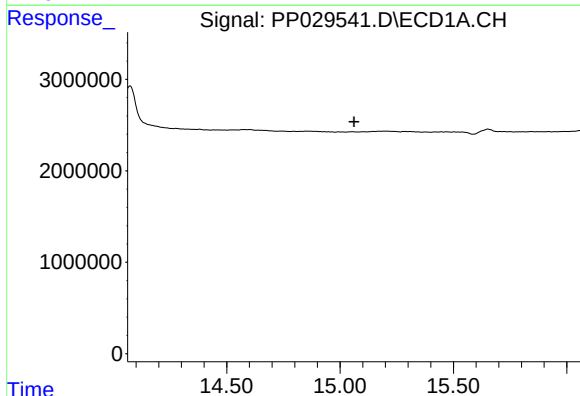


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 15.062 min
Response: 0
Conc: N.D.

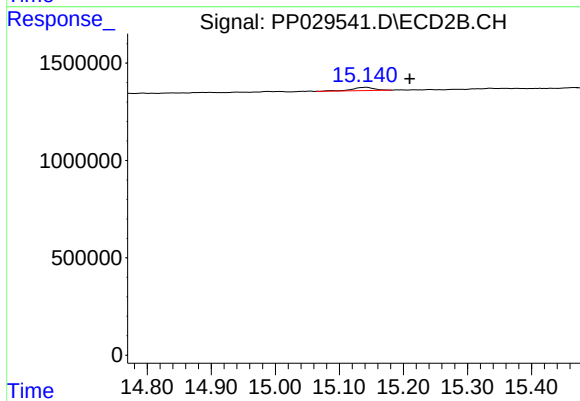

#11 2,4,5-TP (SILVEX)


R.T.: 15.142 min
Delta R.T.: -0.068 min
Response: 397568
Conc: 1.92 ng/ml

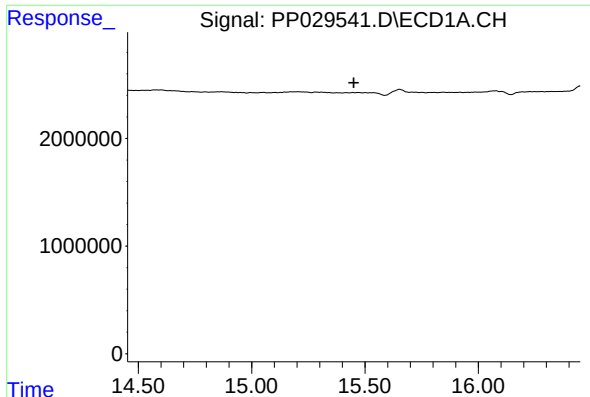

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB118291TB

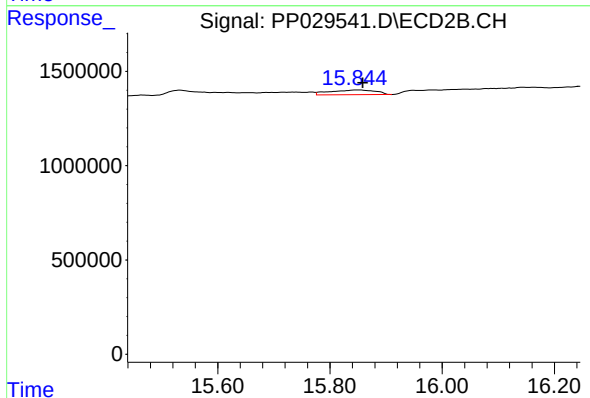


#12 2,4,5-T

R.T.: 15.849 min
Delta R.T.: -0.010 min
Response: 1434744
Conc: 8.65 ng/ml

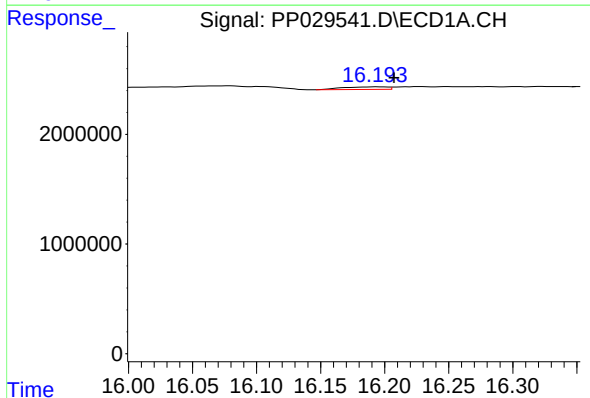


#13 2,4-DB

R.T.: 16.194 min
Delta R.T.: -0.013 min
Response: 572958
Conc: 27.55 ng/ml

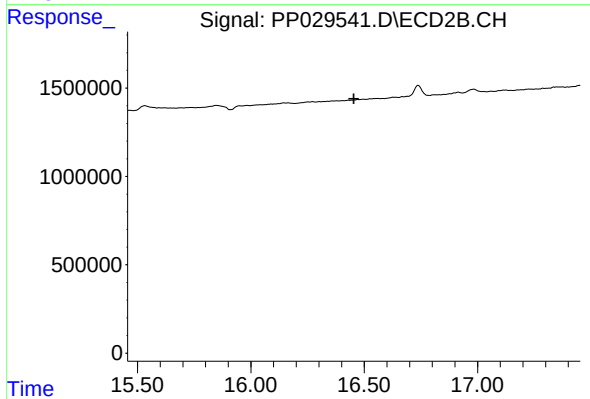

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.455 min
Response: 0
Conc: N.D.

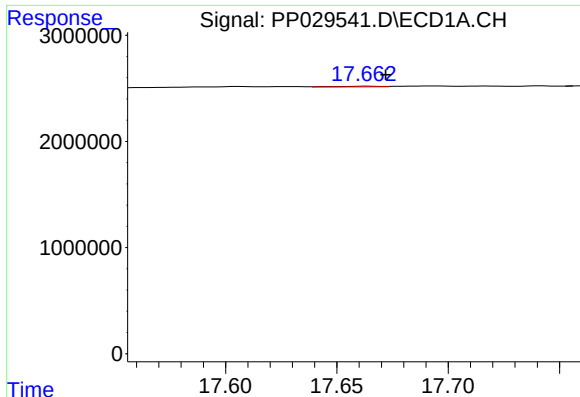

#14 DINOSEB


R.T.: 17.664 min
Delta R.T.: -0.008 min
Response: 80855
Conc: 0.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118291TB

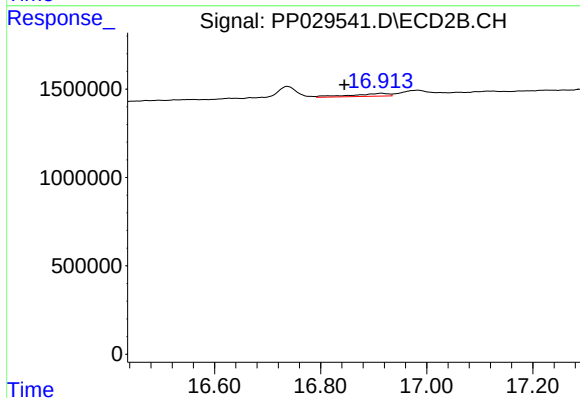


#14 DINOSEB

R.T.: 16.915 min
Delta R.T.: 0.070 min
Response: 762787
Conc: 5.05 ng/ml

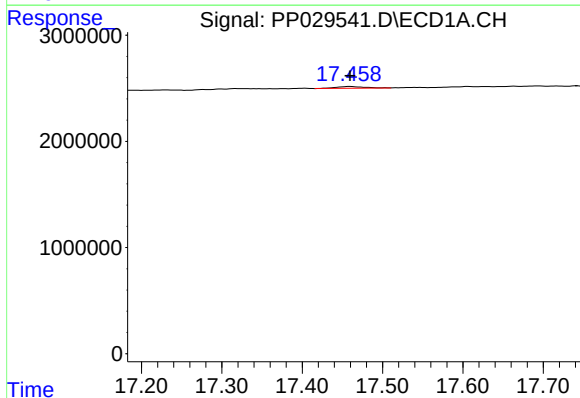


#15 Picloram

R.T.: 17.460 min
Delta R.T.: 0.000 min
Response: 404423
Conc: 1.23 ng/ml

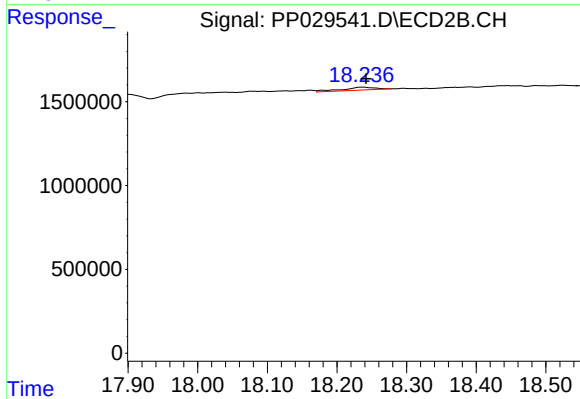

#15 Picloram


R.T.: 18.237 min
Delta R.T.: -0.005 min
Response: 582390
Conc: 2.44 ng/ml

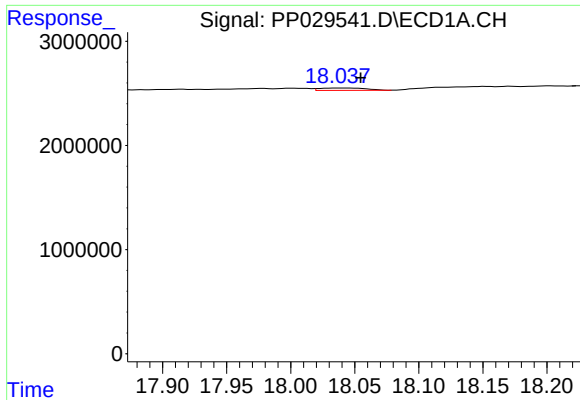

#16 DCPA

R.T.: 18.040 min
Delta R.T.: -0.015 min
Response: 556796
Conc: 1.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118291TB

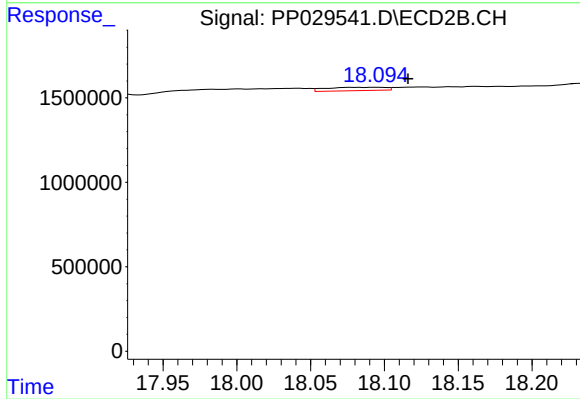

#16 DCPA

R.T.: 18.095 min
Delta R.T.: -0.021 min
Response: 554745
Conc: 2.11 ng/ml