

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
 Data File : PP029548.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 1:10
 Operator : EI\MA
 Sample : K2081-15
 Misc : hexane
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S3A(22-28)-SB(27)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 03:41:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.119	17263086	21453192	527.681	499.593
Target Compounds							
5) T	DICAMBA	12.230	0.000	4371	0	0.030	N.D. #
8) T	DICHLORPROP	13.373	13.552	-83390	603007	N.D.	14.890
10) T	Pentachlo...	0.000	14.632	0	333817	N.D.	0.610 #
11) T	2,4,5-TP ...	0.000	15.197	0	933614	N.D.	4.511 #
12) T	2,4,5-T	0.000	15.843	0	559211	N.D.	3.373 #
13) T	2,4-DB	16.221	0.000	287120	0	13.808	N.D. #
14) T	DINOSEB	17.662	16.808	64210	75069	0.381	0.497 #
15) T	Picloram	17.456	18.243	125481	1146508	0.383	4.810 #
16) T	DCPA	18.044	0.000	476688	0	1.502	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
Data File : PP029548.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 1:10
Operator : EI\MA
Sample : K2081-15
Misc : hexane
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
S3A(22-28)-SB(27)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 03:41:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

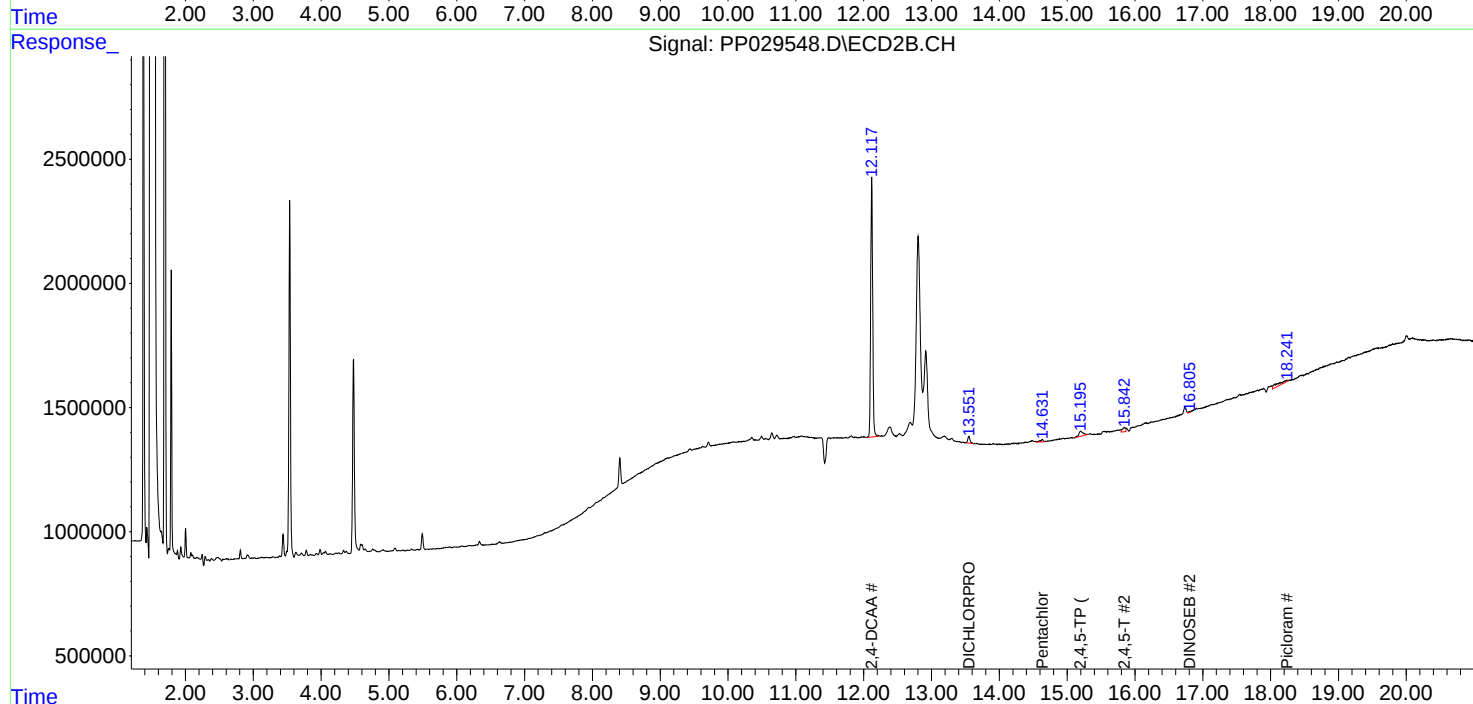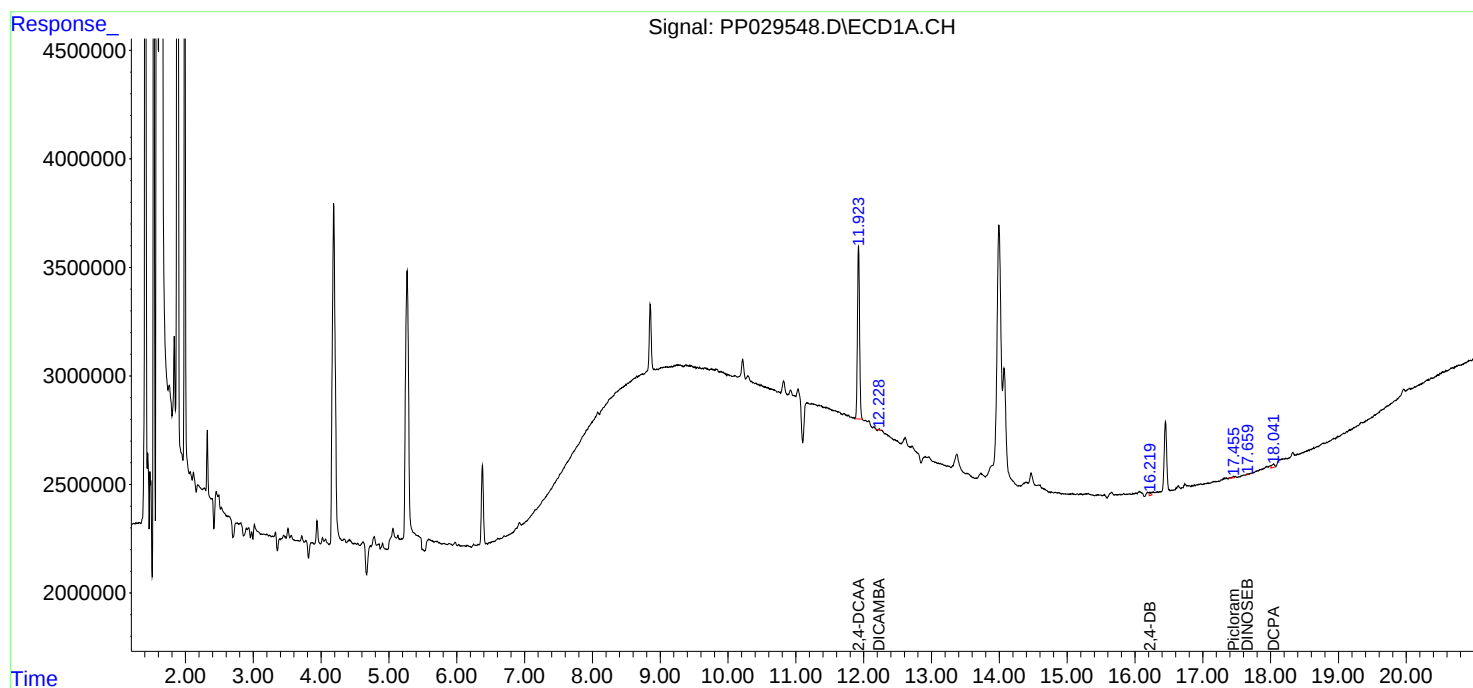


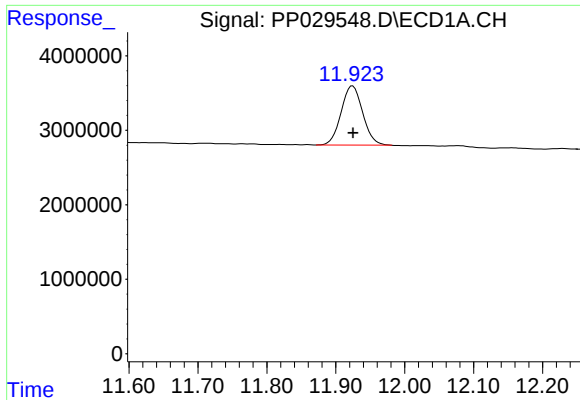

#4 2,4-DCAA


R.T.: 11.924 min
Delta R.T.: 0.000 min
Response: 17263086
Conc: 527.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
S3A(22-28)-SB(27)COMP

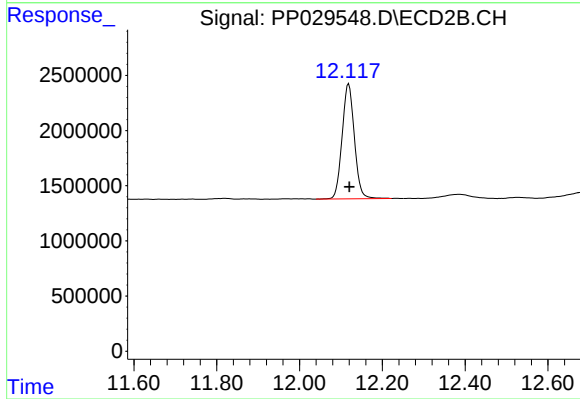


#4 2,4-DCAA

R.T.: 12.119 min
Delta R.T.: -0.002 min
Response: 21453192
Conc: 499.59 ng/ml

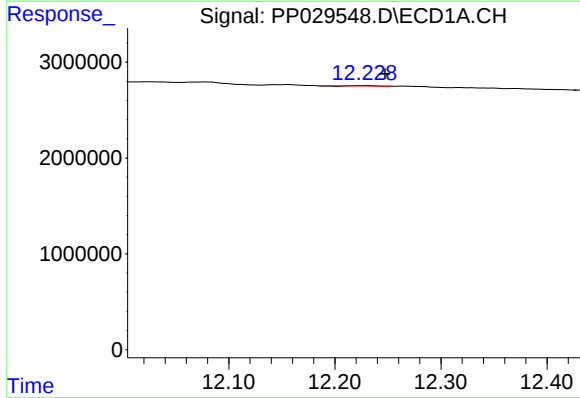


#5 DICAMBA

R.T.: 12.230 min
Delta R.T.: -0.017 min
Response: 4371
Conc: 0.03 ng/ml

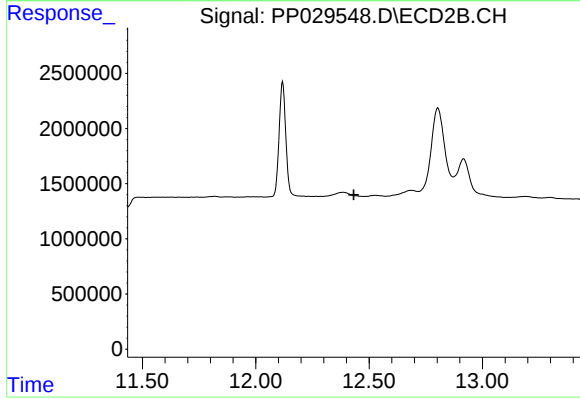

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 12.433 min
Response: 0
Conc: N.D.

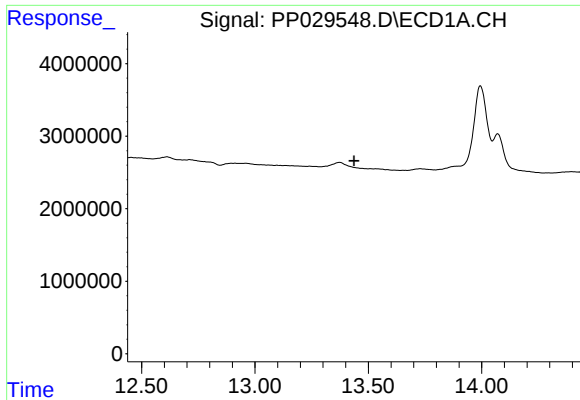

#8 DICHLORPROP


R.T.: 13.373 min
Delta R.T.: -0.064 min
Response: -83390
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S3A(22-28)-SB(27)COMP

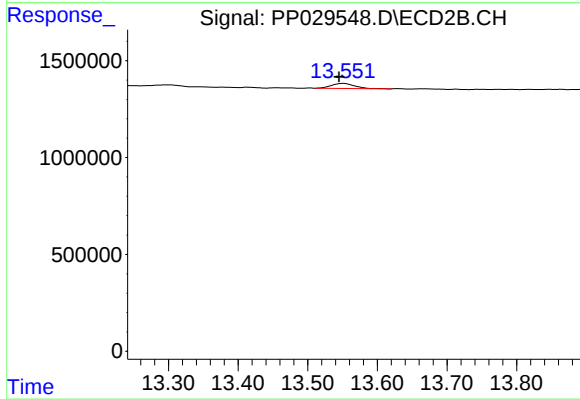


#8 DICHLORPROP

R.T.: 13.552 min
Delta R.T.: 0.007 min
Response: 603007
Conc: 14.89 ng/ml

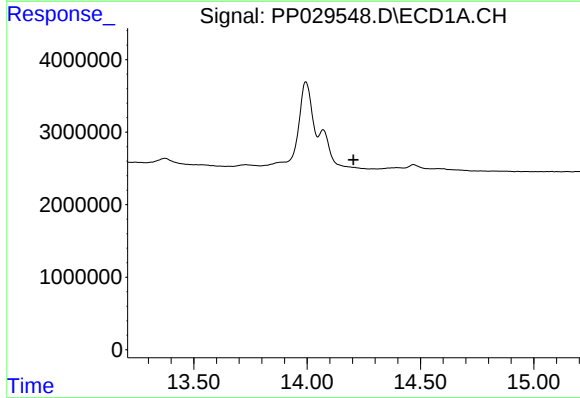


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 14.205 min
Response: 0
Conc: N.D.

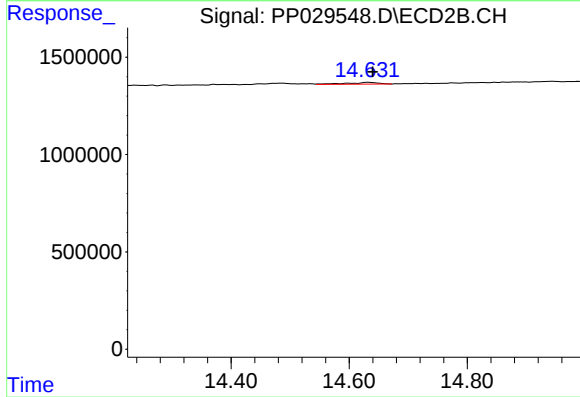

#10 Pentachlorophenol


R.T.: 14.632 min
Delta R.T.: -0.007 min
Response: 333817
Conc: 0.61 ng/ml

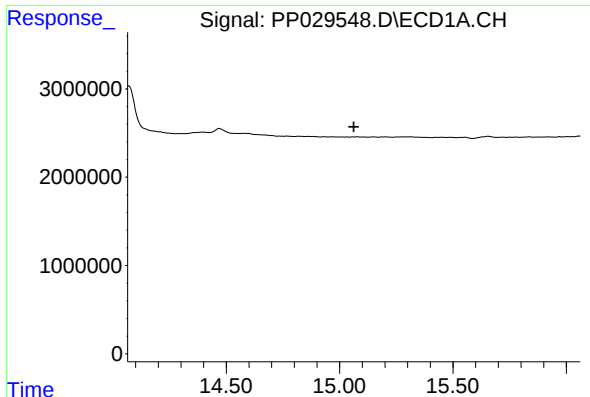

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S3A(22-28)-SB(27)COMP

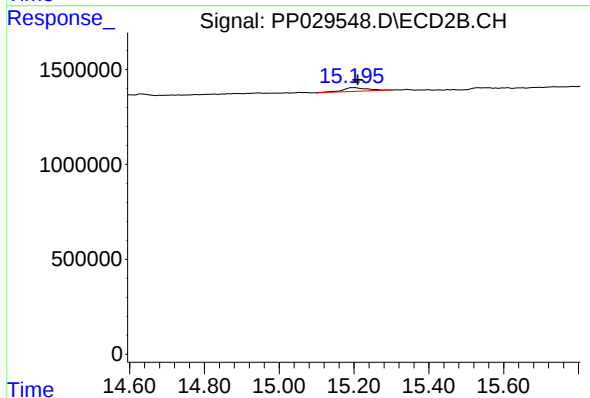


#11 2,4,5-TP (SILVEX)

R.T.: 15.197 min
Delta R.T.: -0.013 min
Response: 933614
Conc: 4.51 ng/ml

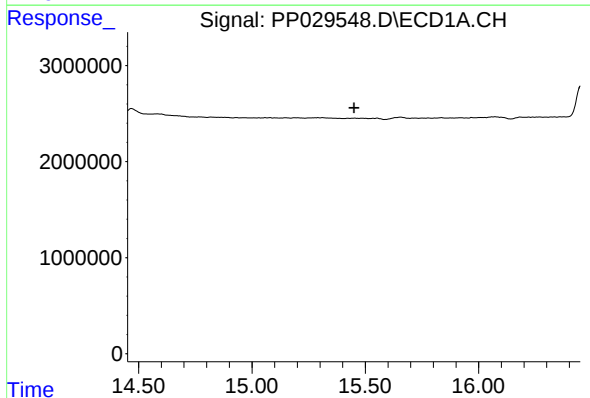


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

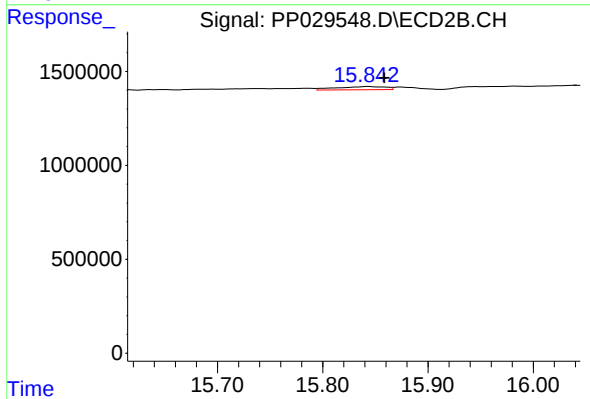

#12 2,4,5-T


R.T.: 15.843 min
Delta R.T.: -0.015 min
Response: 559211
Conc: 3.37 ng/ml

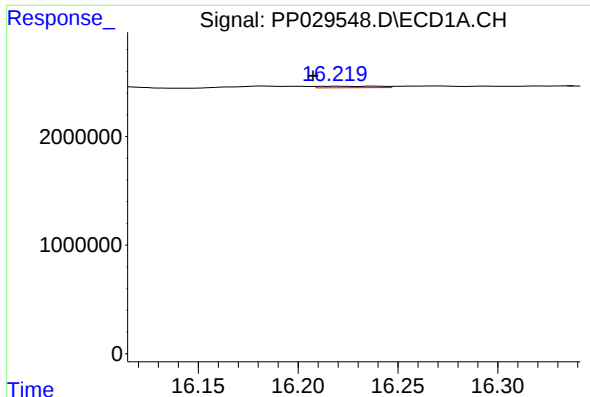

#13 2,4-DB


R.T.: 16.221 min
Delta R.T.: 0.013 min
Response: 287120
Conc: 13.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
S3A(22-28)-SB(27)COMP

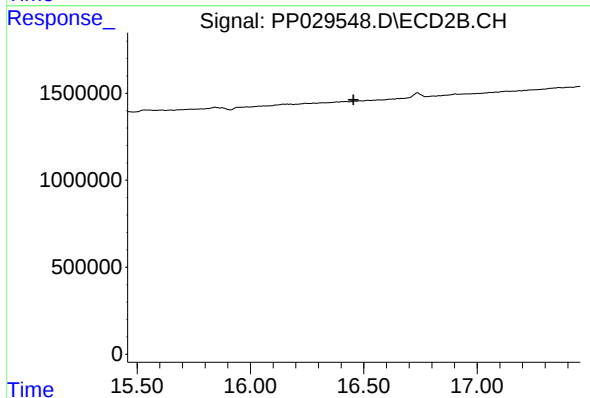


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

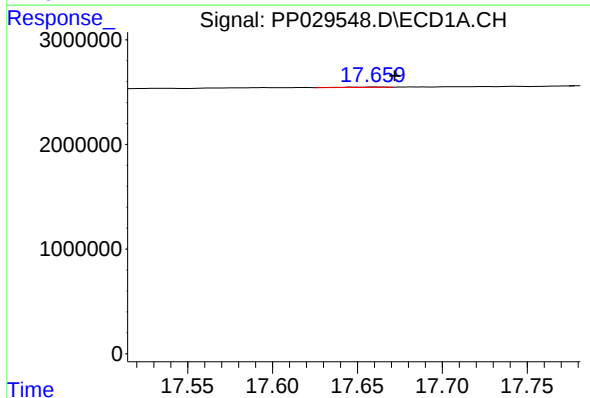


#14 DINOSEB

R.T.: 17.662 min
Delta R.T.: -0.011 min
Response: 64210
Conc: 0.38 ng/ml

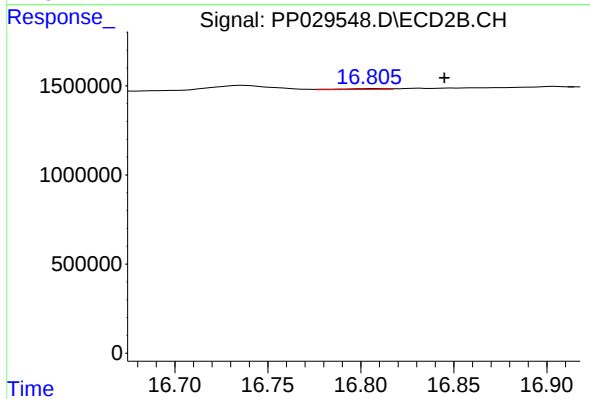

#14 DINOSEB


R.T.: 16.808 min
Delta R.T.: -0.037 min
Response: 75069
Conc: 0.50 ng/ml

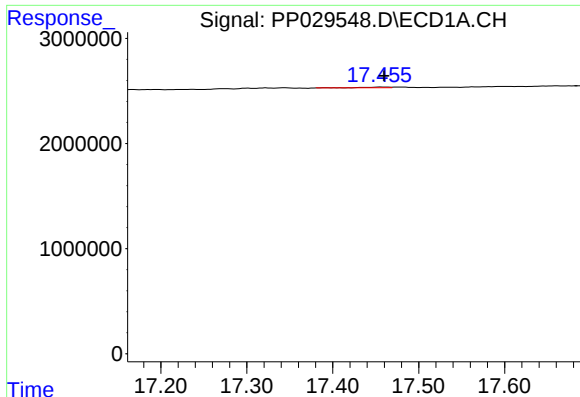

#15 Picloram


R.T.: 17.456 min
Delta R.T.: -0.003 min
Response: 125481
Conc: 0.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
S3A(22-28)-SB(27)COMP

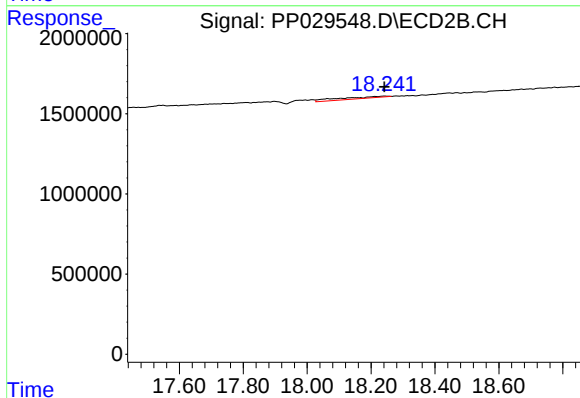


#15 Picloram

R.T.: 18.243 min
Delta R.T.: 0.000 min
Response: 1146508
Conc: 4.81 ng/ml

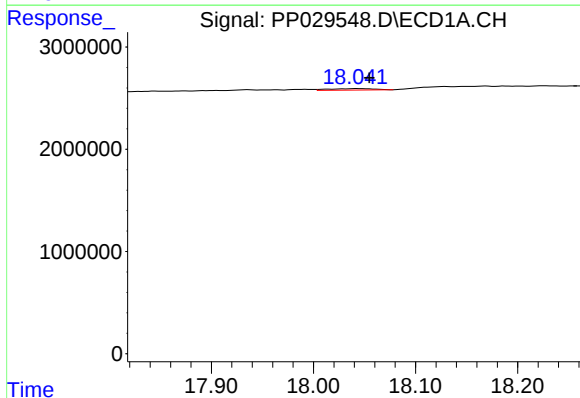

#16 DCPA

R.T.: 18.044 min
Delta R.T.: -0.011 min
Response: 476688
Conc: 1.50 ng/ml

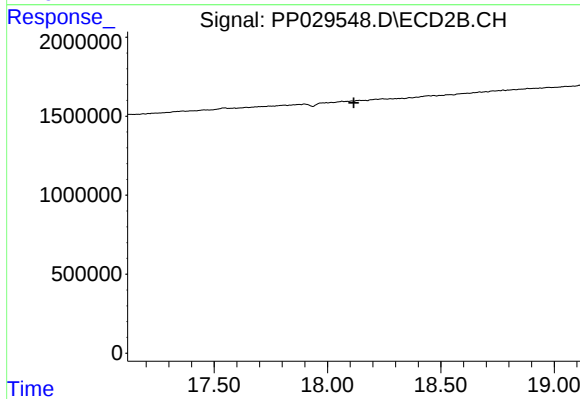

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.116 min
Response: 0
Conc: N.D.