

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
 Data File : PP029549.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 1:36
 Operator : EI\MA
 Sample : K2081-17
 Misc : hexane
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S4C(6-18)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 03:41:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.119	18173083	24471150	555.497	569.874
Target Compounds							
1) T	Dalapon	3.270	0.000	78645	0	1.173	N.D. #
8) T	DICHLORPROP	13.371	13.552	286796	3393418	8.378	83.795 #
11) T	2,4,5-TP ...	0.000	15.197	0	736571	N.D.	3.559 #
12) T	2,4,5-T	0.000	15.847	0	926339	N.D.	5.588 #
13) T	2,4-DB	16.187	0.000	421262	0	20.259	N.D. #
14) T	DINOSEB	17.697	16.907	129768	493699	0.770	3.268 #
15) T	Picloram	17.469	18.247	1850801	505915	5.649	2.123 #
16) T	DCPA	18.045	18.119	263885	144839	0.832	0.552 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032619\
Data File : PP029549.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 1:36
Operator : EI\MA
Sample : K2081-17
Misc : hexane
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
S4C(6-18)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 03:41:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

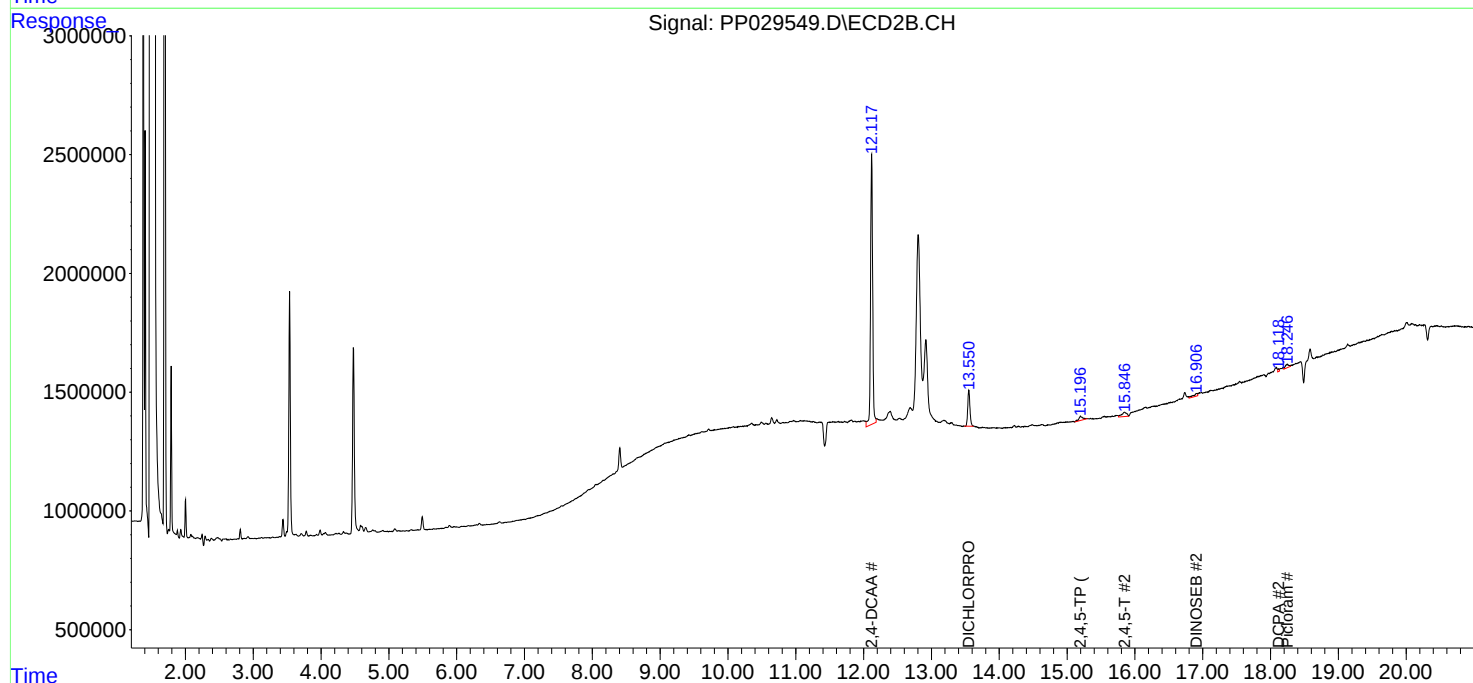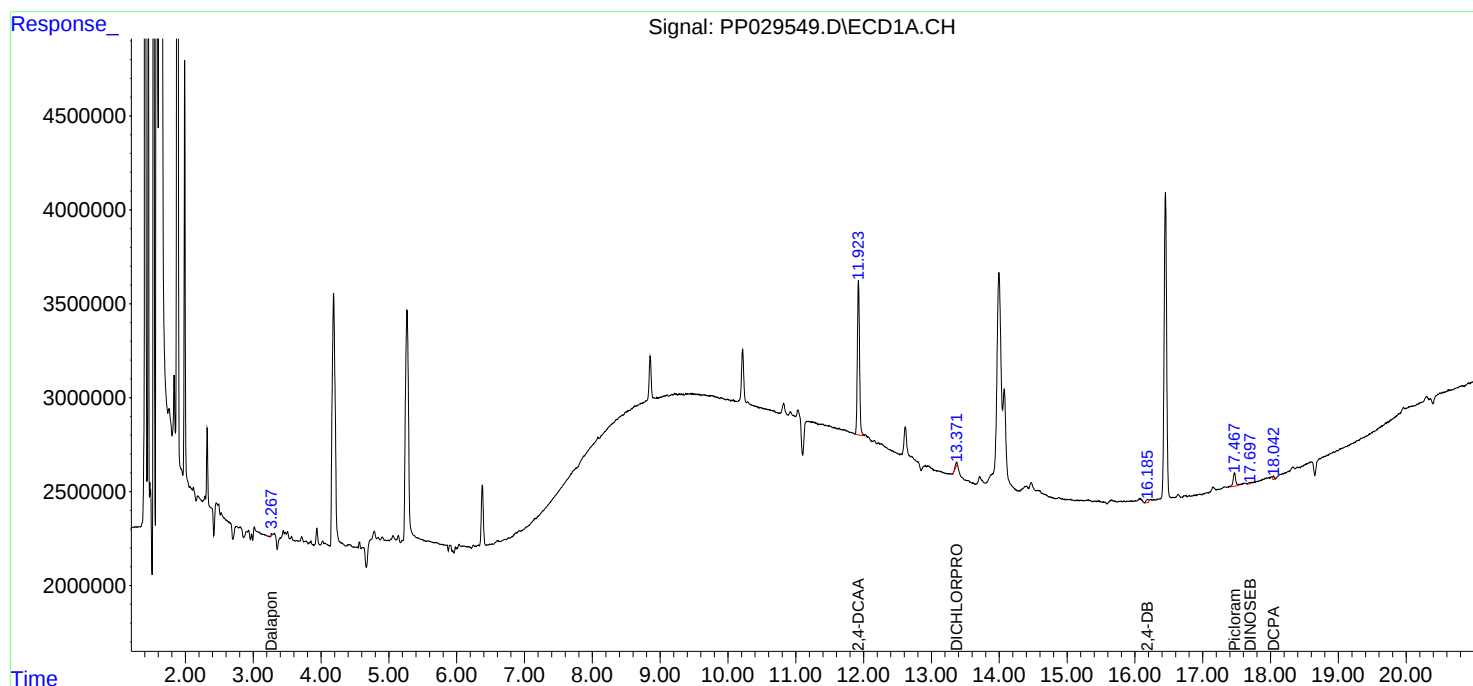


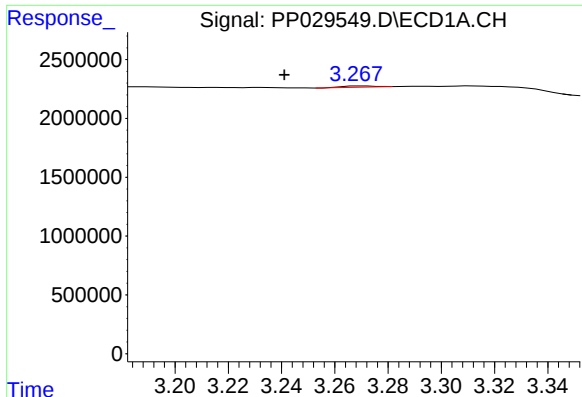

#1 Dalapon


R.T.: 3.270 min
Delta R.T.: 0.029 min
Response: 78645
Conc: 1.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
S4C(6-18)COMP

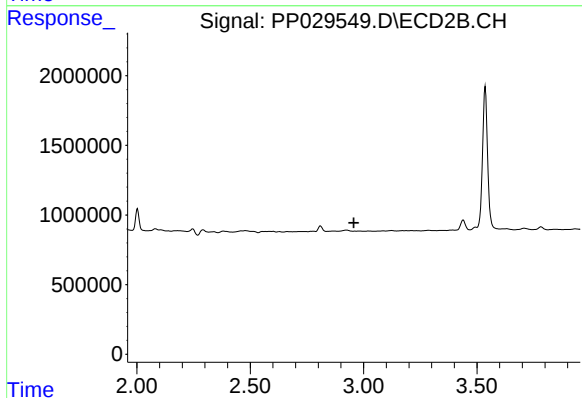


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.956 min
Response: 0
Conc: N.D.

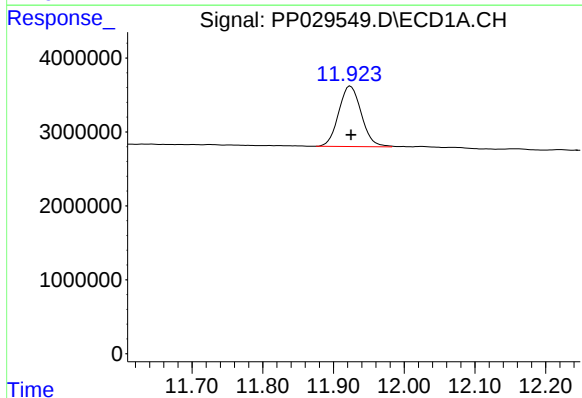


#4 2,4-DCAA

R.T.: 11.924 min
Delta R.T.: 0.000 min
Response: 18173083
Conc: 555.50 ng/ml

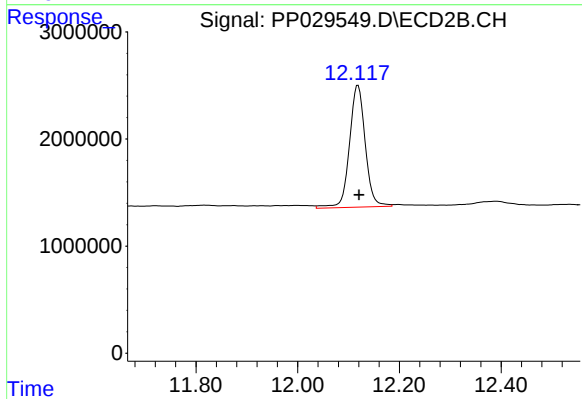

#4 2,4-DCAA


R.T.: 12.119 min
Delta R.T.: -0.002 min
Response: 24471150
Conc: 569.87 ng/ml

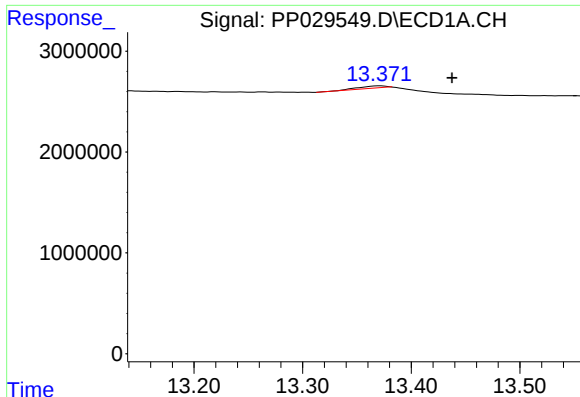

#8 DICHLORPROP


R.T.: 13.371 min
Delta R.T.: -0.066 min
Response: 286796
Conc: 8.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
S4C(6-18)COMP

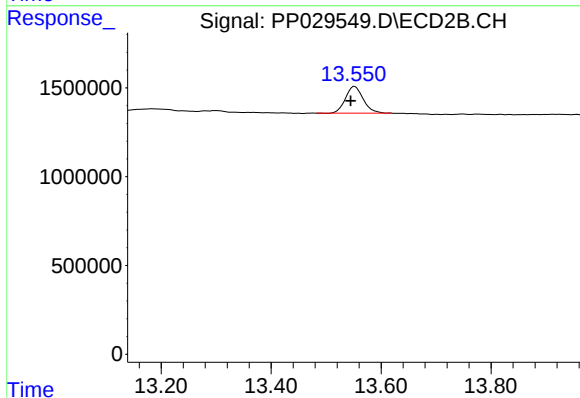


#8 DICHLORPROP

R.T.: 13.552 min
Delta R.T.: 0.007 min
Response: 3393418
Conc: 83.80 ng/ml

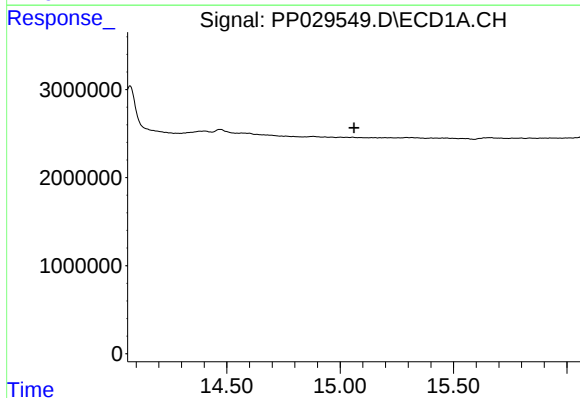


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 15.062 min
Response: 0
Conc: N.D.

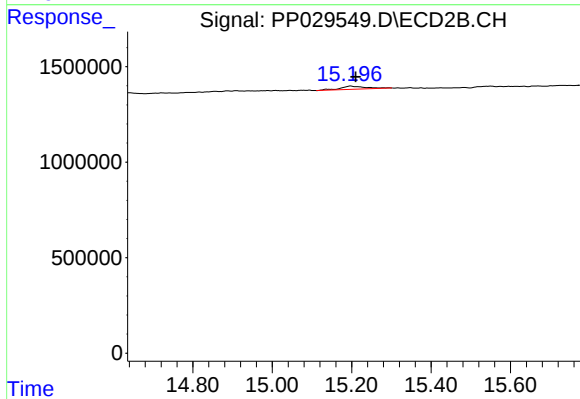

#11 2,4,5-TP (SILVEX)


R.T.: 15.197 min
Delta R.T.: -0.013 min
Response: 736571
Conc: 3.56 ng/ml

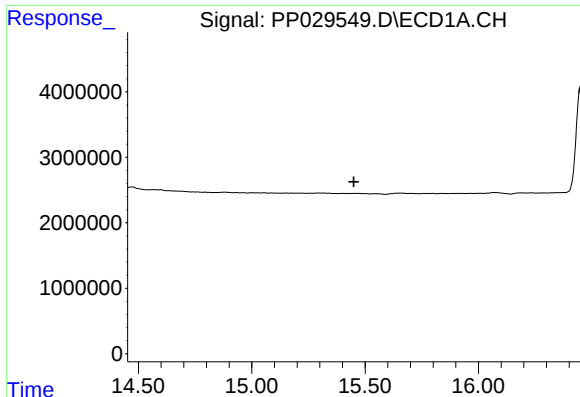

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
S4C(6-18)COMP

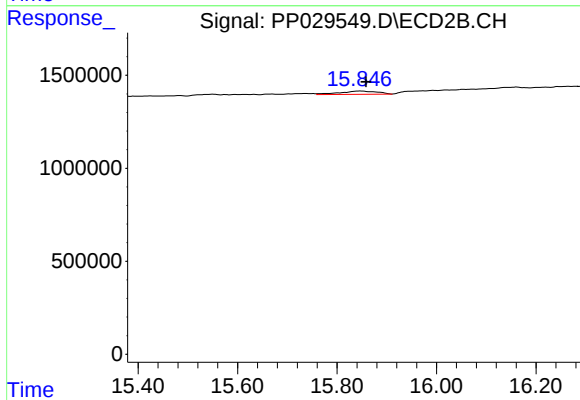


#12 2,4,5-T

R.T.: 15.847 min
Delta R.T.: -0.012 min
Response: 926339
Conc: 5.59 ng/ml

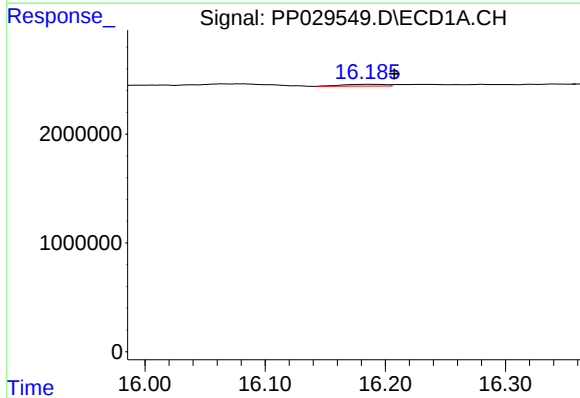


#13 2,4-DB

R.T.: 16.187 min
Delta R.T.: -0.021 min
Response: 421262
Conc: 20.26 ng/ml

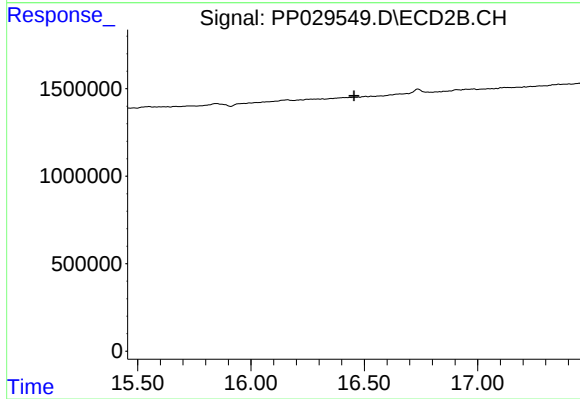

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.455 min
Response: 0
Conc: N.D.

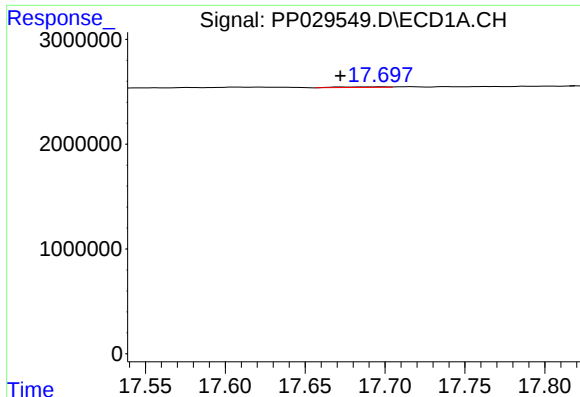

#14 DINOSEB


R.T.: 17.697 min
Delta R.T.: 0.025 min
Response: 129768
Conc: 0.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
S4C(6-18)COMP

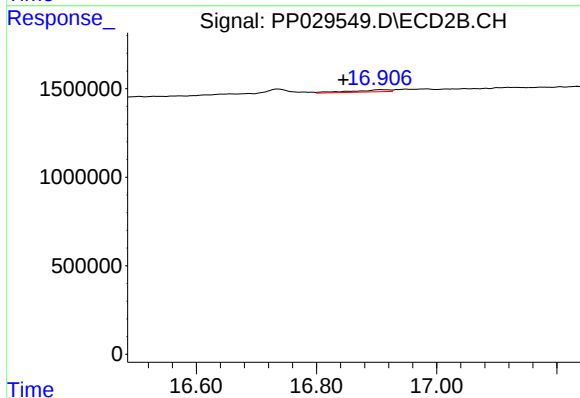


#14 DINOSEB

R.T.: 16.907 min
Delta R.T.: 0.062 min
Response: 493699
Conc: 3.27 ng/ml

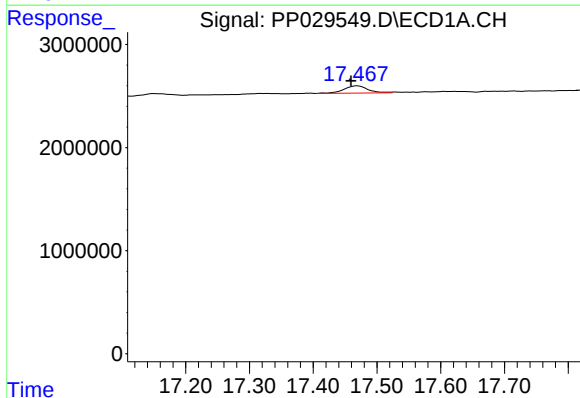


#15 Picloram

R.T.: 17.469 min
Delta R.T.: 0.009 min
Response: 1850801
Conc: 5.65 ng/ml

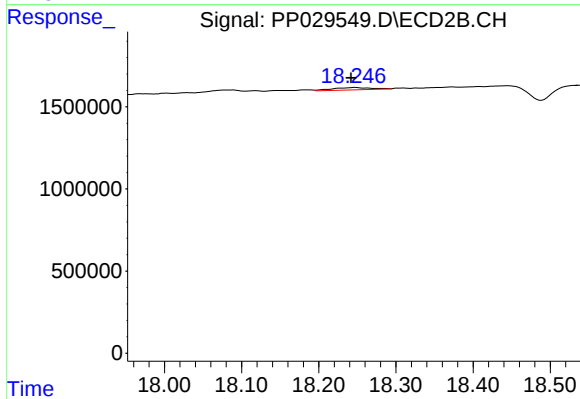

#15 Picloram


R.T.: 18.247 min
Delta R.T.: 0.005 min
Response: 505915
Conc: 2.12 ng/ml

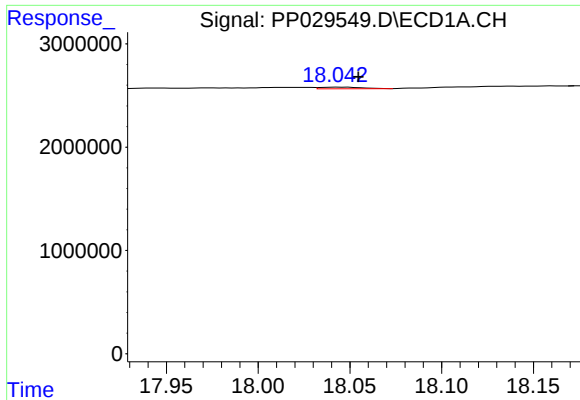

#16 DCPA

R.T.: 18.045 min
Delta R.T.: -0.009 min
Response: 263885
Conc: 0.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
S4C(6-18)COMP

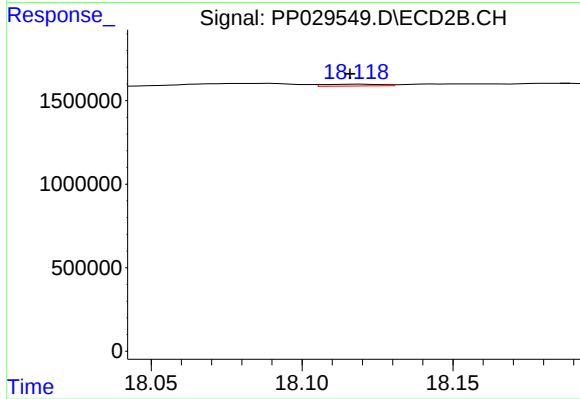

#16 DCPA

R.T.: 18.119 min
Delta R.T.: 0.003 min
Response: 144839
Conc: 0.55 ng/ml