

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032621\
 Data File : PP034403.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2021 9:57
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 00:02:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.853	4.259	1645186	925676	19.584	20.918
2)	SA Decachlor...	10.780	9.574	1798640	652448	22.919	24.724
Target Compounds							
9)	L2 AR-1221-2	5.202	4.614	20296	13115	29.491	36.982 #
30)	L6 AR-1254-5	0.000	7.650f	0	5135	N.D.	2.781 #
31)	L7 AR-1260-1	7.854	0.000	9742	0	3.057	N.D. #
32)	L7 AR-1260-2	8.088f	0.000	76127	0	20.257	N.D. #
36)	L8 AR-1262-1	0.000	7.650f	0	5135	N.D.	5.086 #
40)	L8 AR-1262-5	0.000	9.047f	0	89434	N.D.	85.066 #
44)	L9 AR-1268-4	0.000	9.047f	0	89434	N.D.	74.319 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032621\
Data File : PP034403.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2021 9:57
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 00:02:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

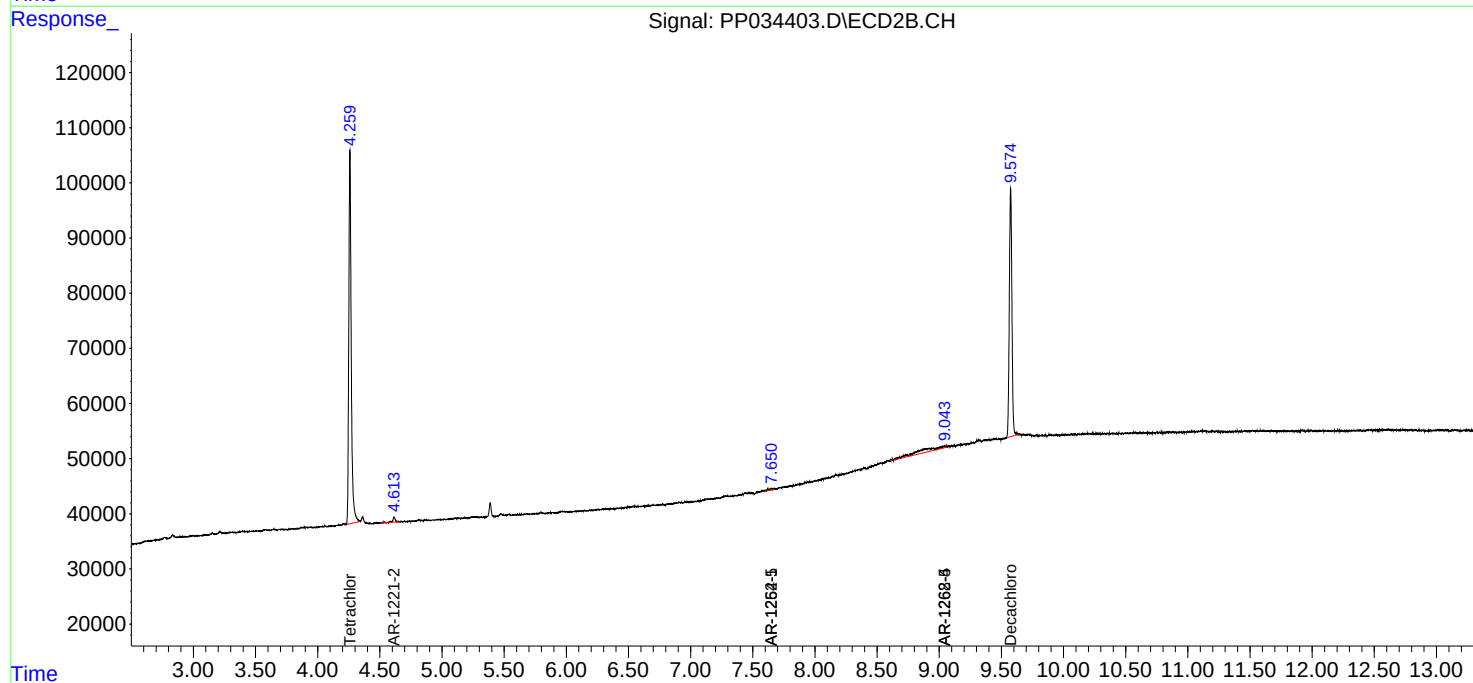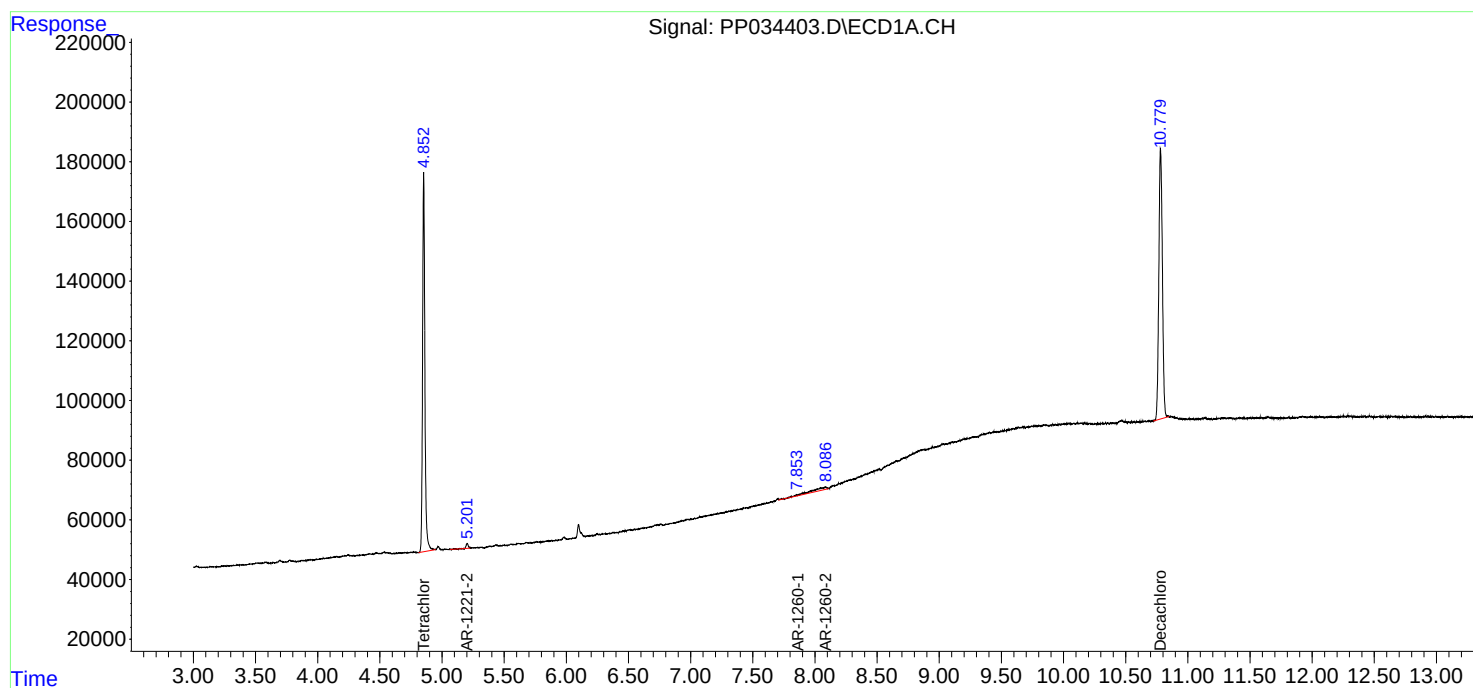


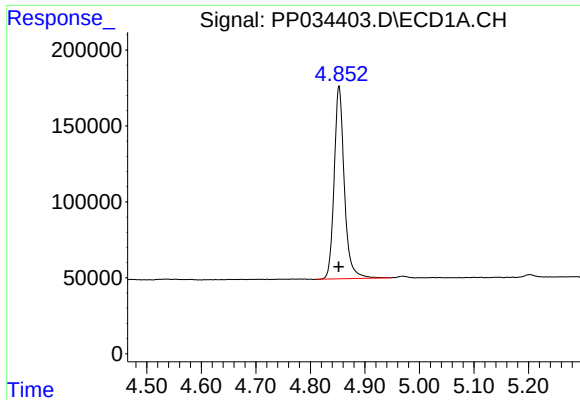

#1 Tetrachloro-m-xylene


R.T.: 4.853 min
Delta R.T.: 0.000 min
Response: 1645186
Conc: 19.58 ng/ml

Instrument :
ECD_P
ClientSampleId :

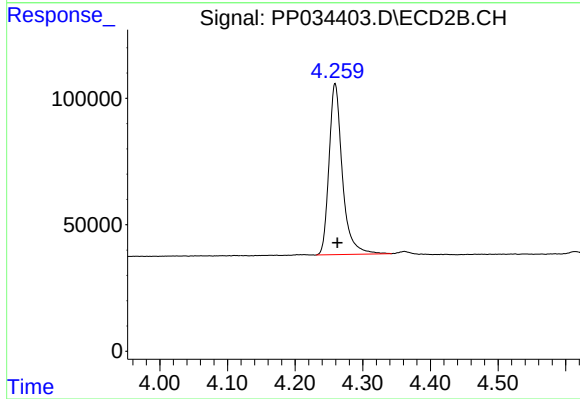


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: -0.004 min
Response: 925676
Conc: 20.92 ng/ml

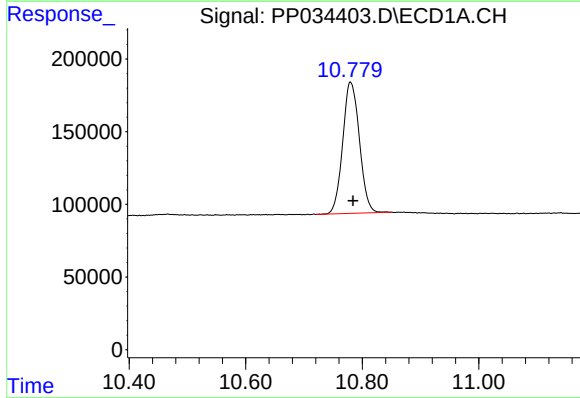


#2 Decachlorobiphenyl

R.T.: 10.780 min
Delta R.T.: -0.004 min
Response: 1798640
Conc: 22.92 ng/ml

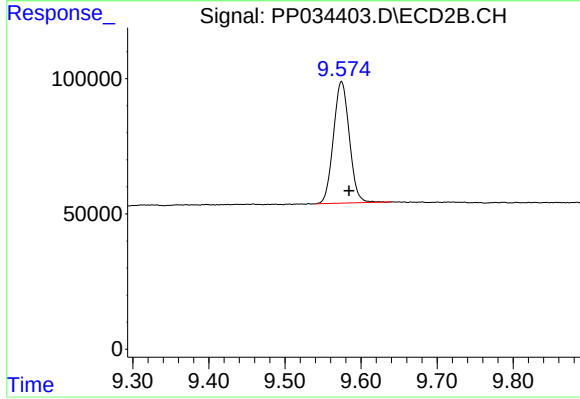

#2 Decachlorobiphenyl


R.T.: 9.574 min
Delta R.T.: -0.010 min
Response: 652448
Conc: 24.72 ng/ml

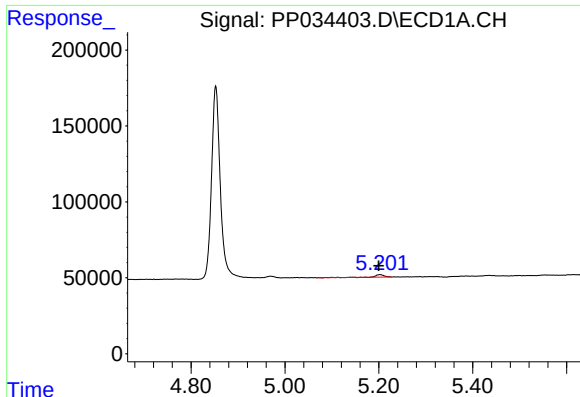

#9 AR-1221-2


R.T.: 5.202 min
Delta R.T.: 0.003 min
Response: 20296
Conc: 29.49 ng/ml

Instrument :
ECD_P
ClientSampleId :

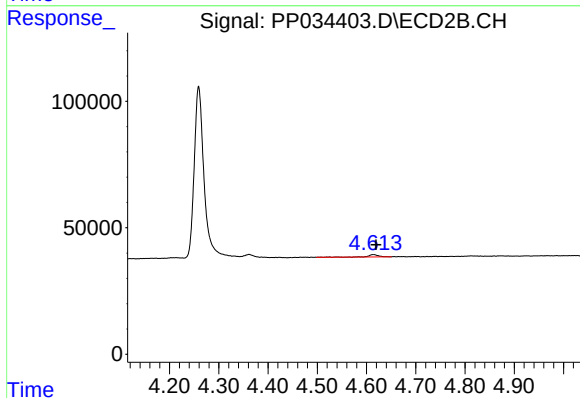


#9 AR-1221-2

R.T.: 4.614 min
Delta R.T.: -0.005 min
Response: 13115
Conc: 36.98 ng/ml

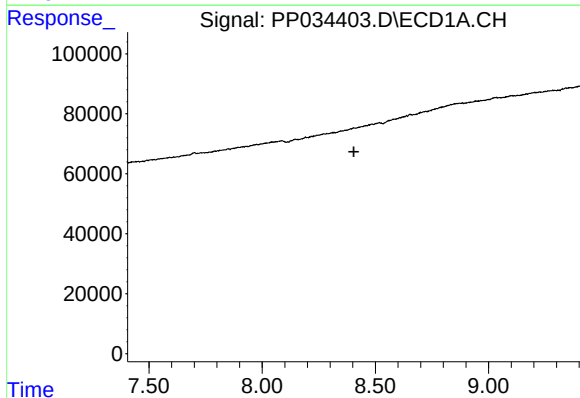


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 8.405 min
Response: 0
Conc: N.D.

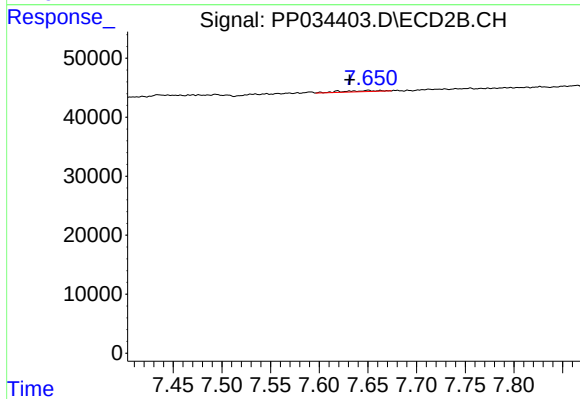

#30 AR-1254-5


R.T.: 7.650 min
Delta R.T.: 0.019 min
Response: 5135
Conc: 2.78 ng/ml

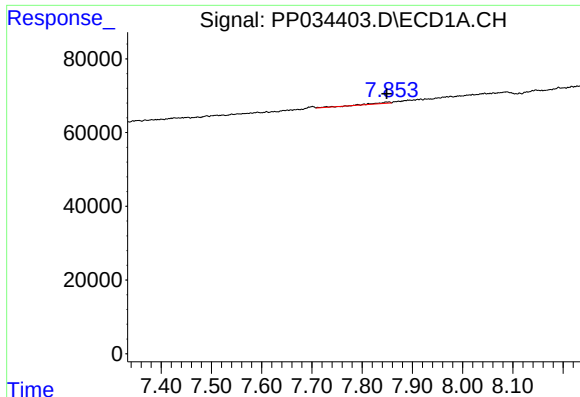

#31 AR-1260-1


R.T.: 7.854 min
Delta R.T.: 0.005 min
Response: 9742
Conc: 3.06 ng/ml

Instrument :
ECD_P
ClientSampleId :

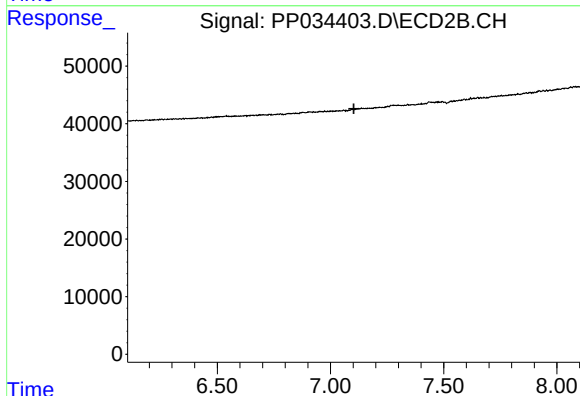


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.103 min
Response: 0
Conc: N.D.

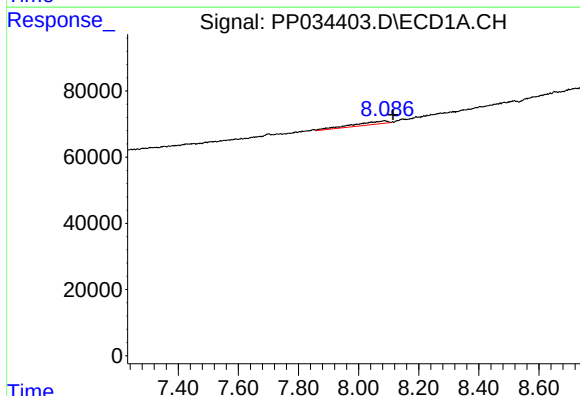


#32 AR-1260-2

R.T.: 8.088 min
Delta R.T.: -0.026 min
Response: 76127
Conc: 20.26 ng/ml

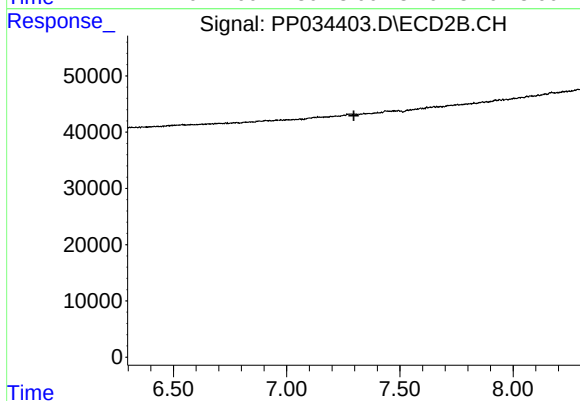

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.297 min
Response: 0
Conc: N.D.

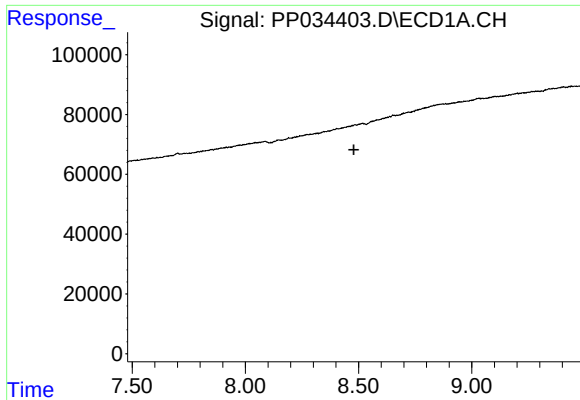

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 8.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

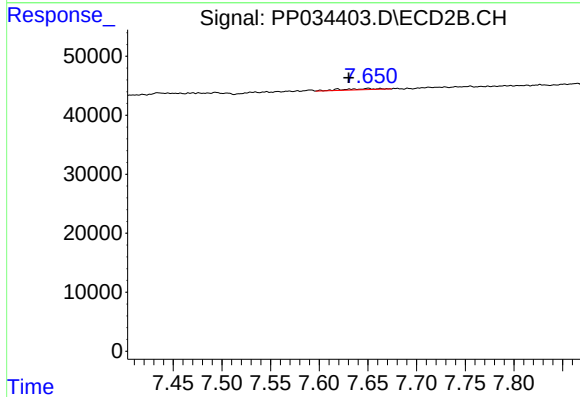


#36 AR-1262-1

R.T.: 7.650 min
Delta R.T.: 0.020 min
Response: 5135
Conc: 5.09 ng/ml

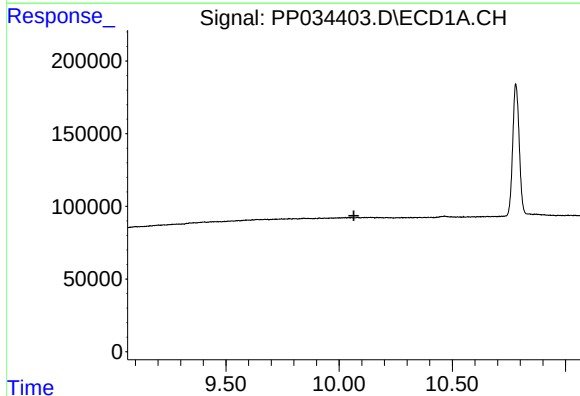


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 10.065 min
Response: 0
Conc: N.D.

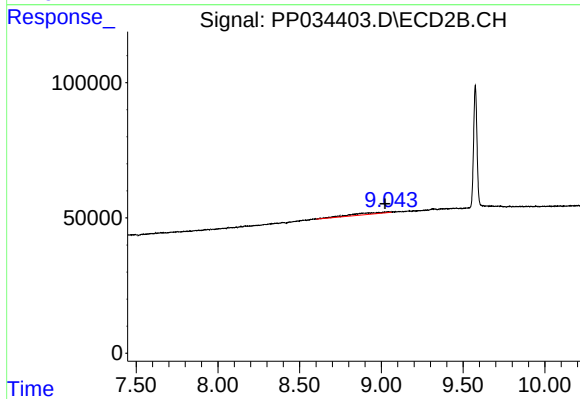

#40 AR-1262-5


R.T.: 9.047 min
Delta R.T.: 0.023 min
Response: 89434
Conc: 85.07 ng/ml

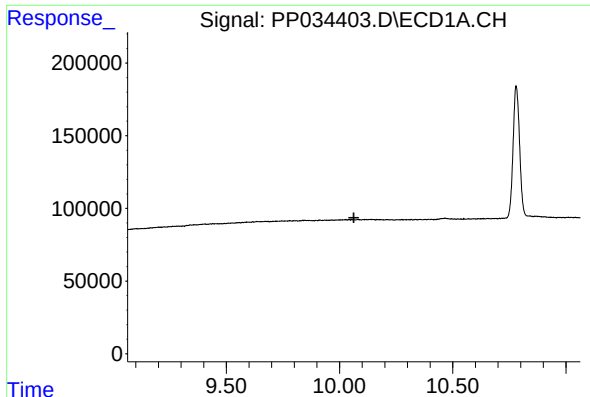

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 10.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

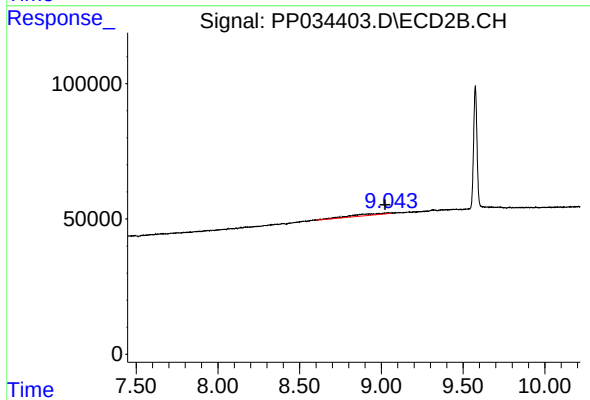

#44 AR-1268-4

R.T.: 9.047 min
Delta R.T.: 0.023 min
Response: 89434
Conc: 74.32 ng/ml