

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032621\
 Data File : PP034405.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2021 10:31
 Operator : DD\AJ
 Sample : M1792-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-5

Manual Integrations
 APPROVED

Ankita
 3/30/2021 2:10:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 00:03:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.847	4.259	1590482	766597	18.933	17.323
2) SA Decachlor...	10.776	9.573	849253	300226	10.822	11.377
Target Compounds						
16) L4 AR-1242-1	6.161	5.513	2202012	1080041	1105.053	1185.754m
17) L4 AR-1242-2	6.185	5.534	1657691	659477	557.527	502.414m
18) L4 AR-1242-3	6.254	5.729	496794	416922	266.974	573.398 #
19) L4 AR-1242-4	6.355	5.820	754981	843802	500.811	1164.801 #
20) L4 AR-1242-5	7.136	6.383	1137034	578137	745.822m	736.623m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032621\
Data File : PP034405.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2021 10:31
Operator : DD\AJ
Sample : M1792-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
TP-5


Manual Integrations
APPROVED

Ankita
3/30/2021 2:10:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 00:03:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

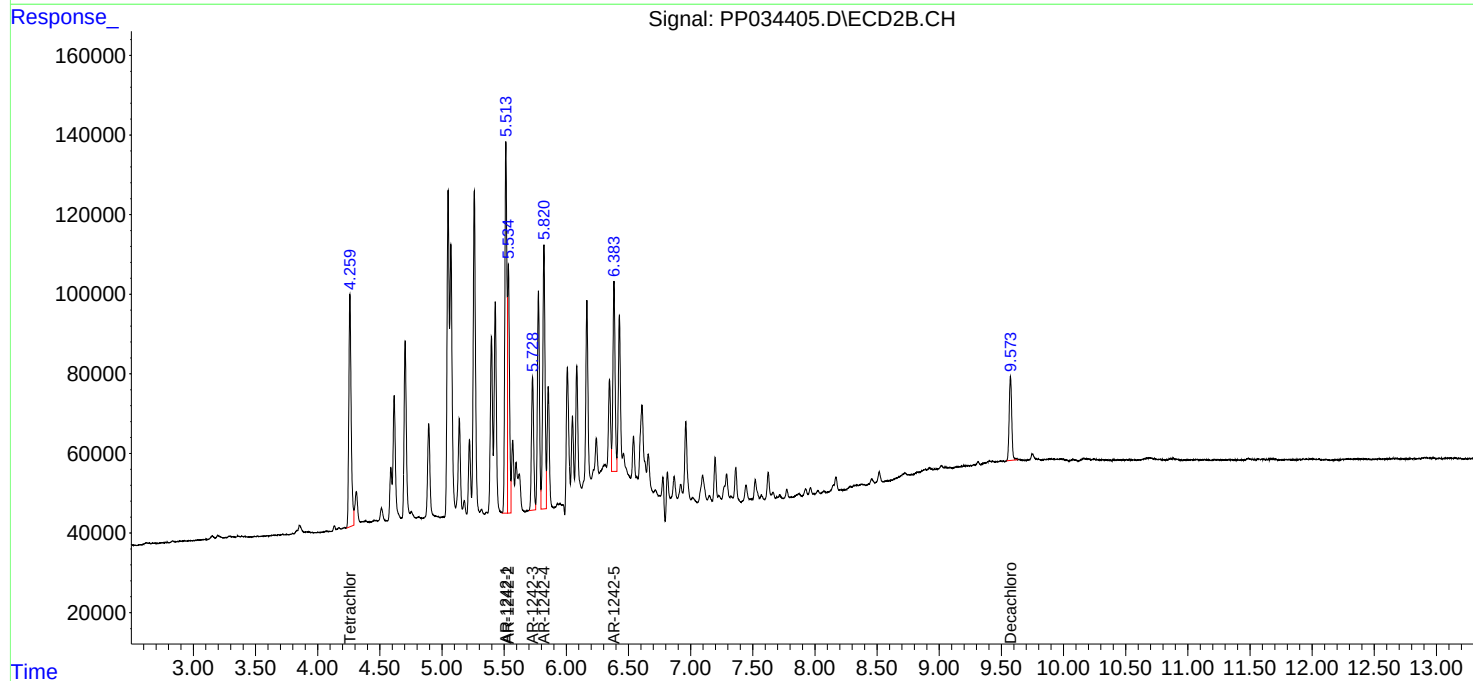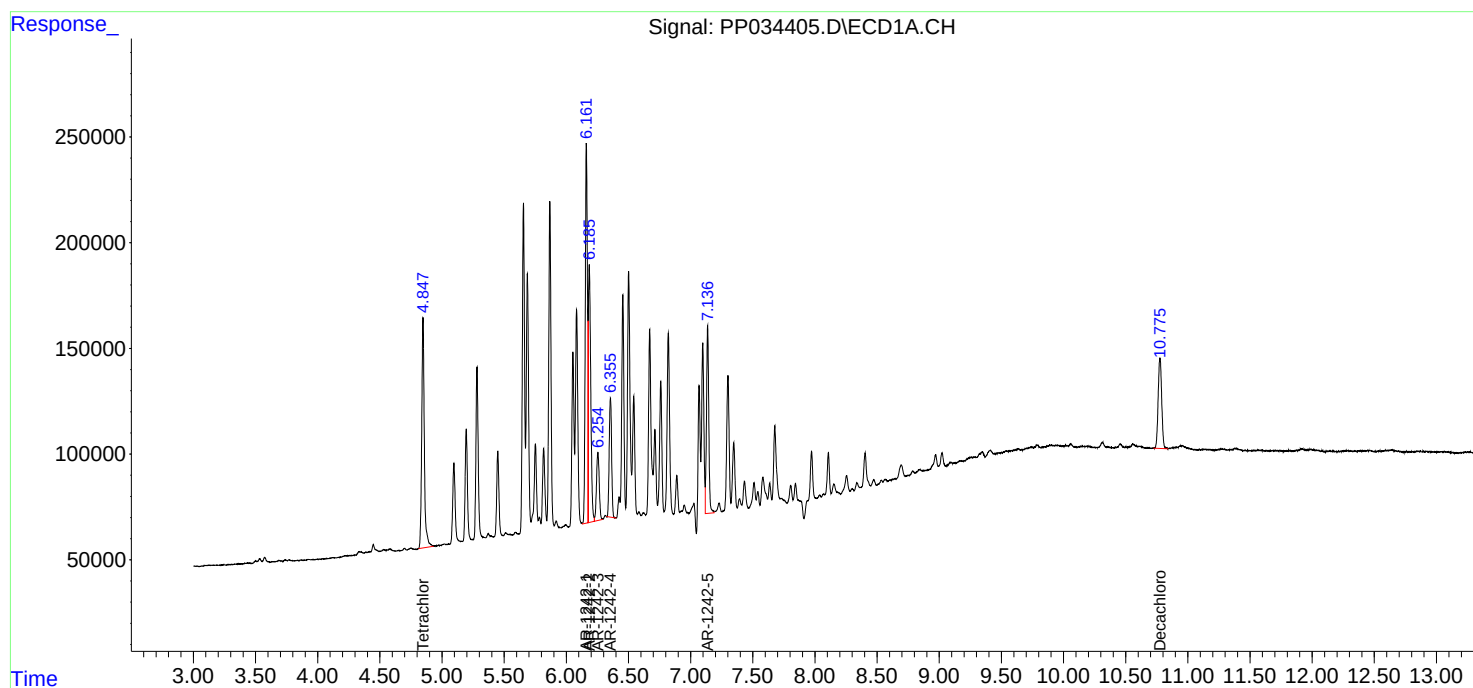

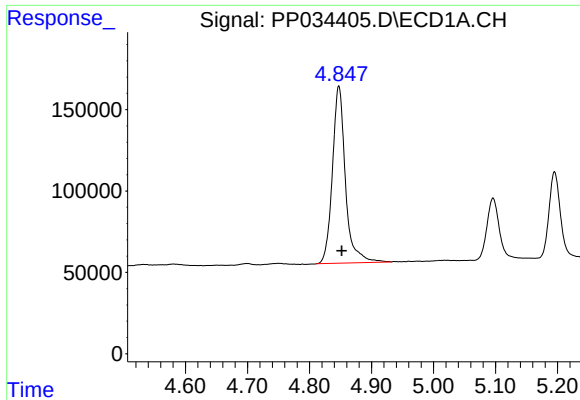


#1 Tetrachloro-m-xylene

R.T.: 4.847 min
Delta R.T.: -0.005 min
Response: 1590482
Conc: 18.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
3/30/2021 2:10:32 PM

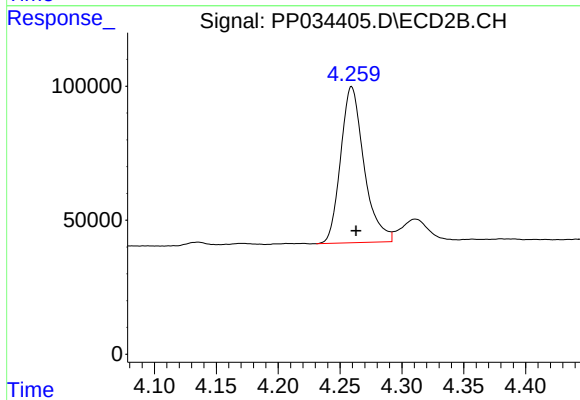


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: -0.003 min
Response: 766597
Conc: 17.32 ng/ml

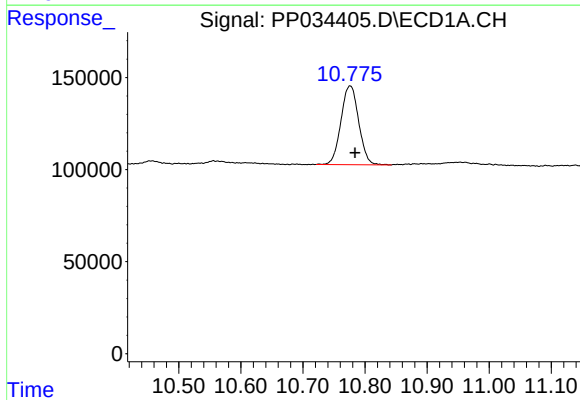


#2 Decachlorobiphenyl

R.T.: 10.776 min
Delta R.T.: -0.008 min
Response: 849253
Conc: 10.82 ng/ml

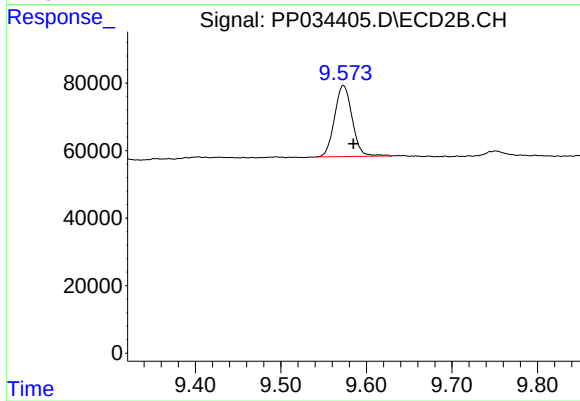

#2 Decachlorobiphenyl

R.T.: 9.573 min
Delta R.T.: -0.011 min
Response: 300226
Conc: 11.38 ng/ml

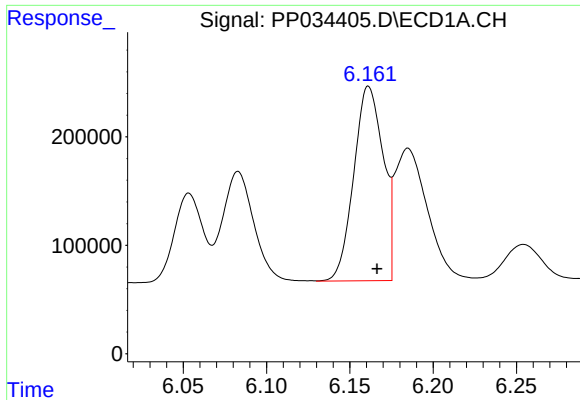


#16 AR-1242-1

R.T.: 6.161 min
Delta R.T.: -0.005 min
Response: 2202012
Conc: 1105.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
3/30/2021 2:10:32 PM

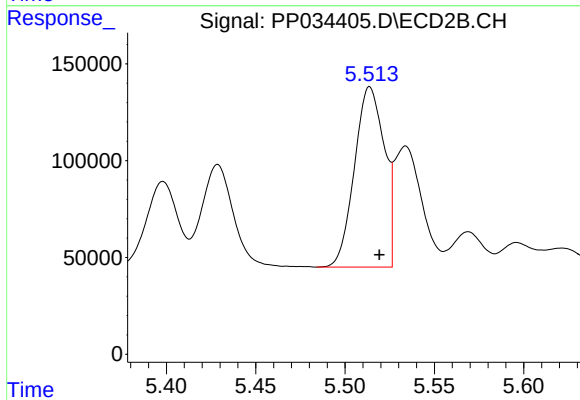


#16 AR-1242-1

R.T.: 5.513 min
Delta R.T.: -0.006 min
Response: 1080041
Conc: 1185.75 ng/ml m

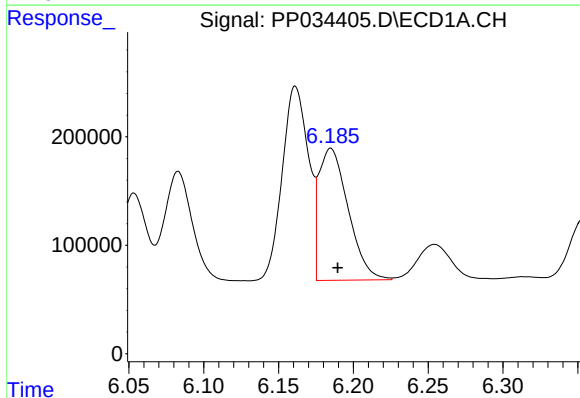


#17 AR-1242-2

R.T.: 6.185 min
Delta R.T.: -0.005 min
Response: 1657691
Conc: 557.53 ng/ml

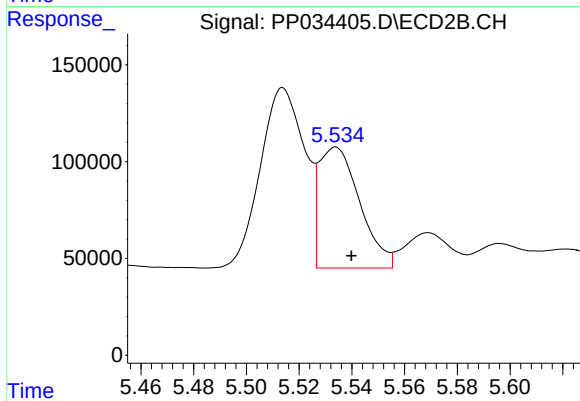

#17 AR-1242-2

R.T.: 5.534 min
Delta R.T.: -0.006 min
Response: 659477
Conc: 502.41 ng/ml m

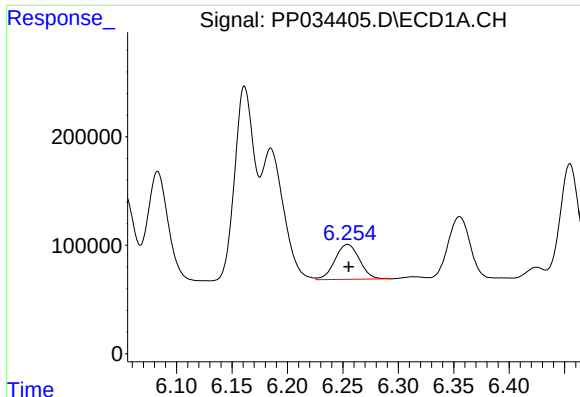


#18 AR-1242-3

R.T.: 6.254 min
Delta R.T.: 0.000 min
Response: 496794
Conc: 266.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
3/30/2021 2:10:32 PM

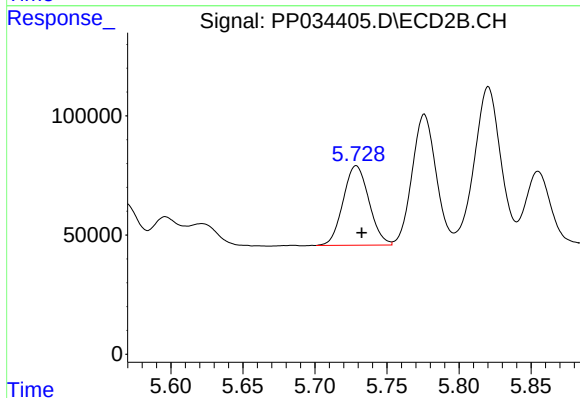


#18 AR-1242-3

R.T.: 5.729 min
Delta R.T.: -0.004 min
Response: 416922
Conc: 573.40 ng/ml

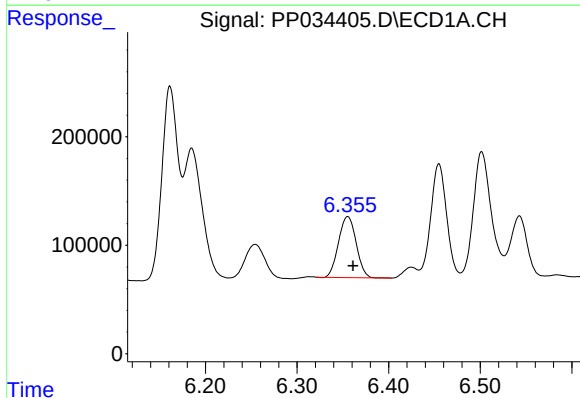


#19 AR-1242-4

R.T.: 6.355 min
Delta R.T.: -0.006 min
Response: 754981
Conc: 500.81 ng/ml

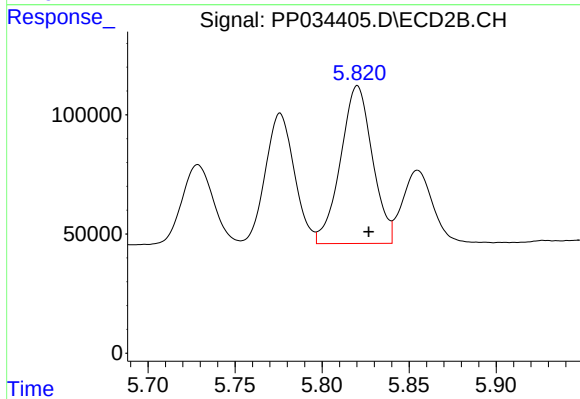

#19 AR-1242-4

R.T.: 5.820 min
Delta R.T.: -0.007 min
Response: 843802
Conc: 1164.80 ng/ml

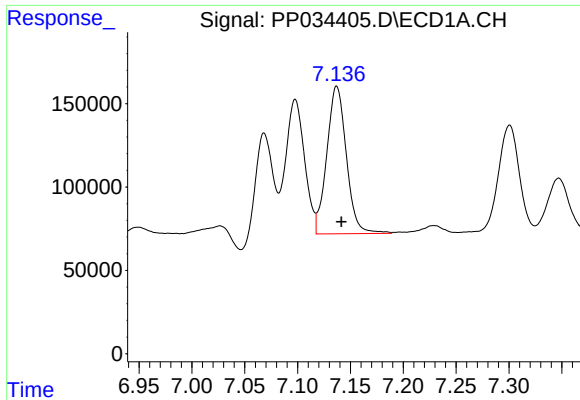


#20 AR-1242-5

R.T.: 7.136 min
Delta R.T.: -0.005 min
Response: 1137034
Conc: 745.82 ng/ml m

Instrument :
ECD_P
ClientSampleId :
TP-5

Manual Integrations
APPROVED

Ankita
3/30/2021 2:10:32 PM

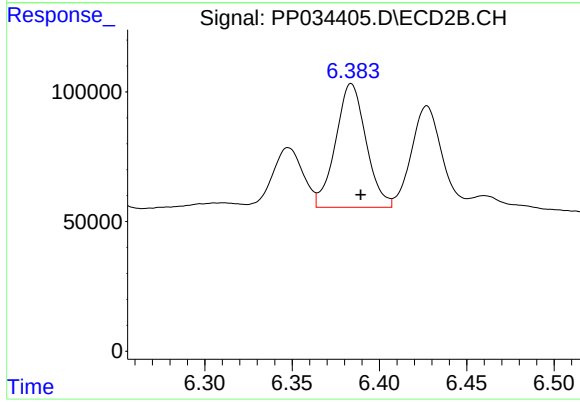

#20 AR-1242-5

R.T.: 6.383 min
Delta R.T.: -0.006 min
Response: 578137
Conc: 736.62 ng/ml m