

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032621\
 Data File : PP034418.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2021 15:22
 Operator : DD\AJ
 Sample : M1817-02DL 200X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PHC-326FB-003DL

Manual Integrations
 APPROVED

Ankita
 3/30/2021 2:10:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 05:52:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
36)	L8	AR-1262-1	8.475	7.631	3763096	88343 843.558 87.488 #
37)	L8	AR-1262-2	9.024	8.171	4361242	1758213 575.367 544.719
38)	L8	AR-1262-3	9.325	8.456	8102414	3116566 1519.798 2274.750 #
39)	L8	AR-1262-4	9.419	8.521	8445365	3375361 1959.648 1393.886 #
40)	L8	AR-1262-5	10.058	9.017	7162810	1928792 2522.061m 1834.586 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032621\
Data File : PP034418.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2021 15:22
Operator : DD\AJ
Sample : M1817-02DL 200X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleID :
PHC-326FB-003DL


Manual Integrations
APPROVED

Ankita
3/30/2021 2:10:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 05:52:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

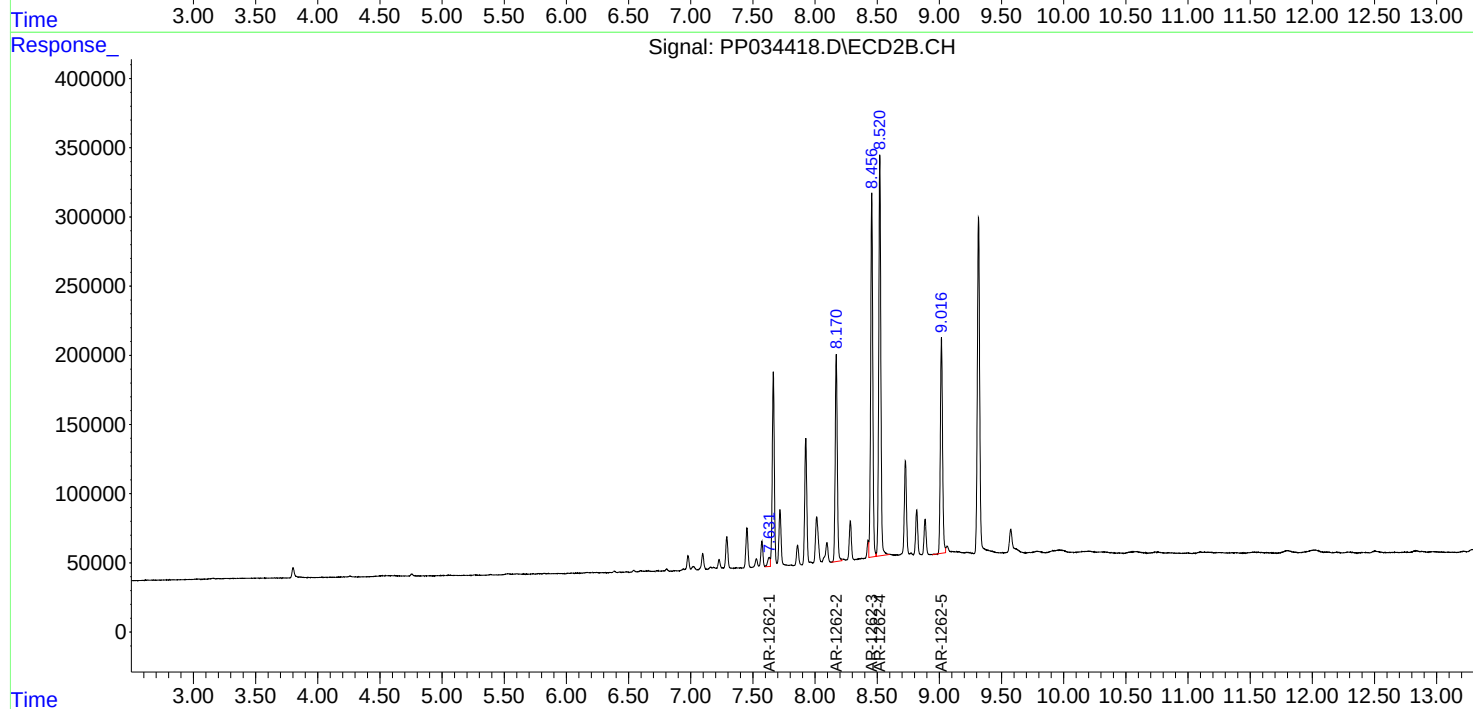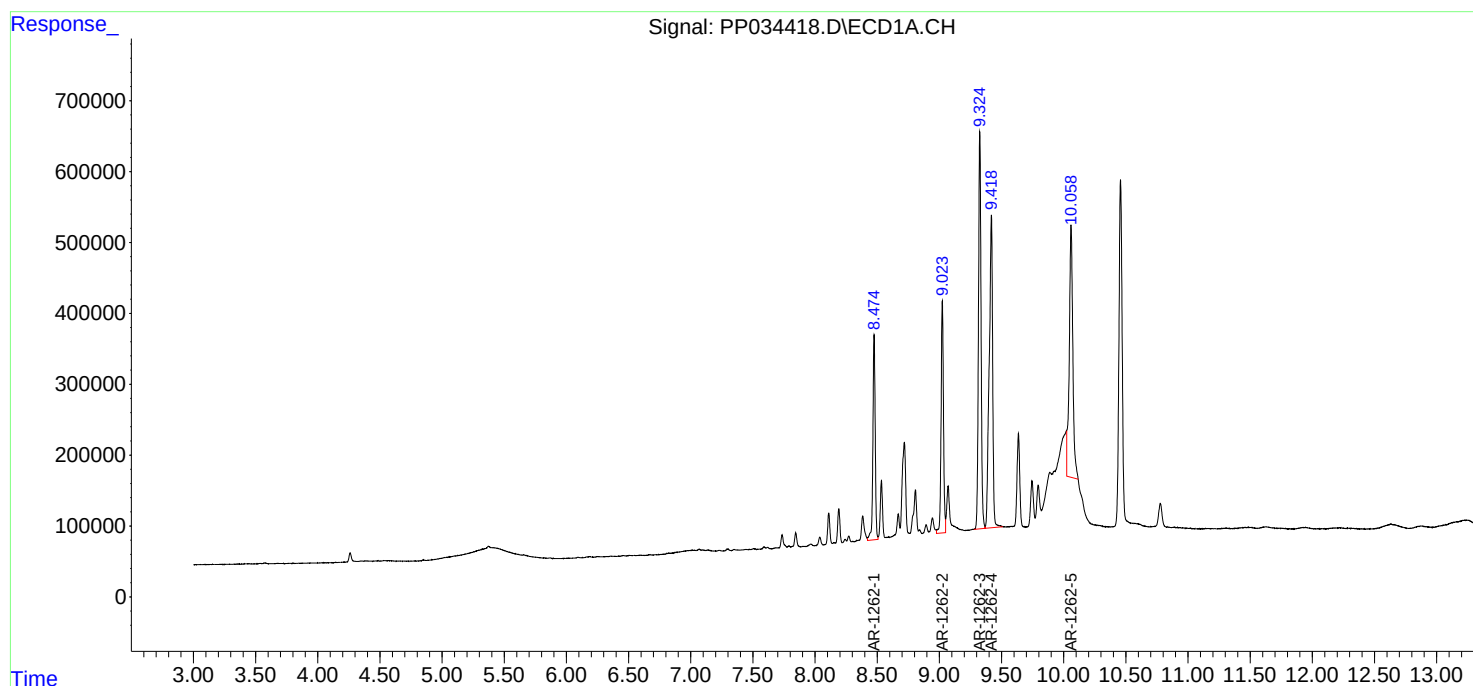

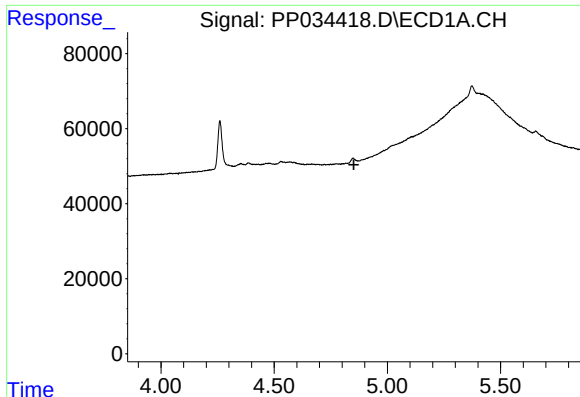


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PHC-326FB-003DL


Manual Integrations
APPROVED

Ankita
3/30/2021 2:10:39 PM

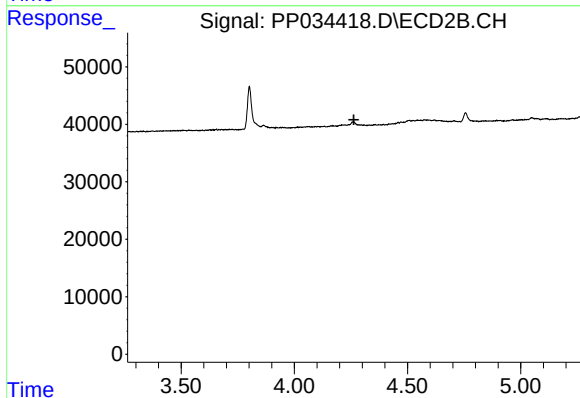


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.263 min
Response: 0
Conc: N.D.

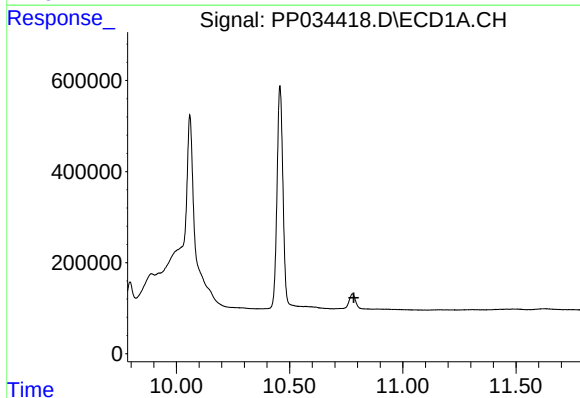


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.784 min
Response: 0
Conc: N.D.

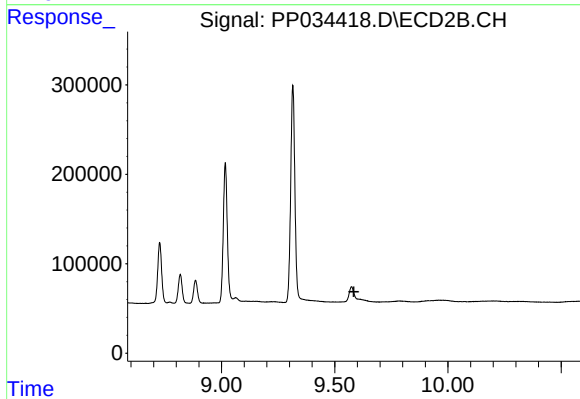

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.585 min
Response: 0
Conc: N.D.

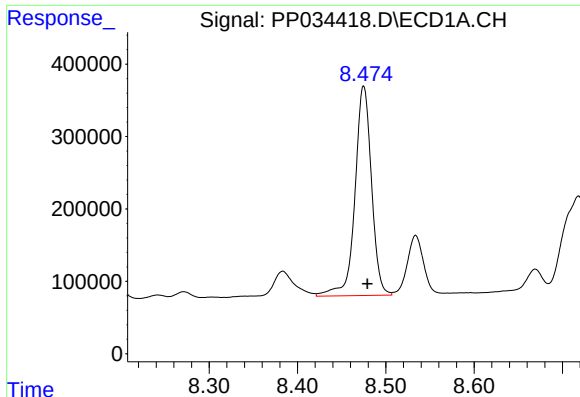


#36 AR-1262-1

R.T.: 8.475 min
Delta R.T.: -0.004 min
Response: 3763096
Conc: 843.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
PHC-326FB-003DL


Manual Integrations
APPROVED

Ankita
3/30/2021 2:10:39 PM

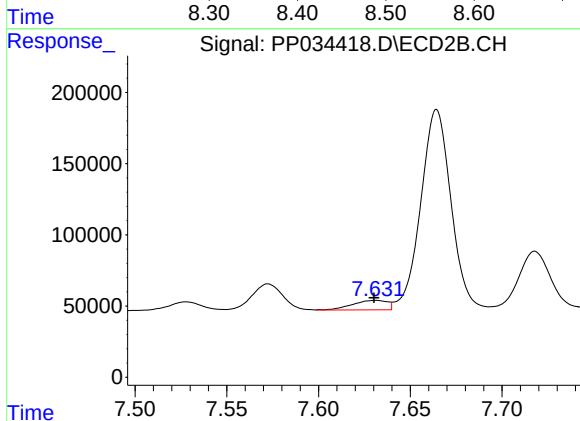


#36 AR-1262-1

R.T.: 7.631 min
Delta R.T.: 0.000 min
Response: 88343
Conc: 87.49 ng/ml

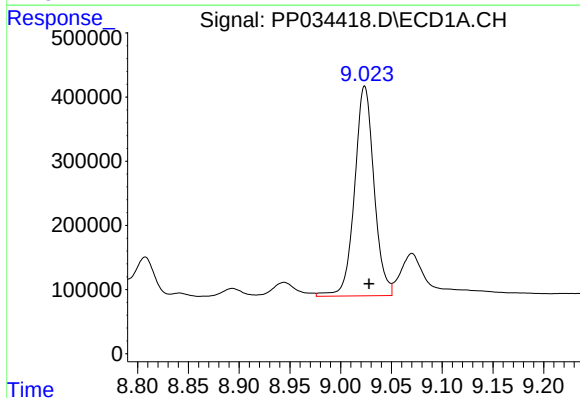


#37 AR-1262-2

R.T.: 9.024 min
Delta R.T.: -0.004 min
Response: 4361242
Conc: 575.37 ng/ml

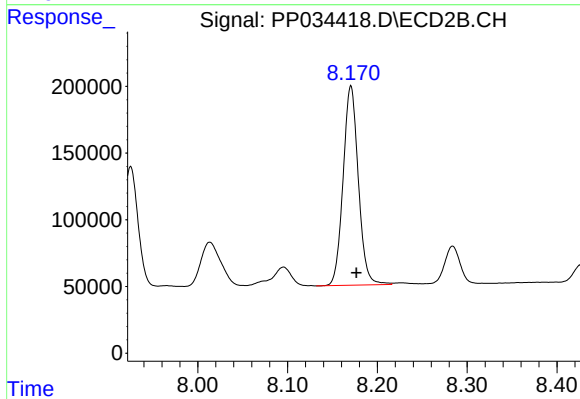

#37 AR-1262-2

R.T.: 8.171 min
Delta R.T.: -0.006 min
Response: 1758213
Conc: 544.72 ng/ml

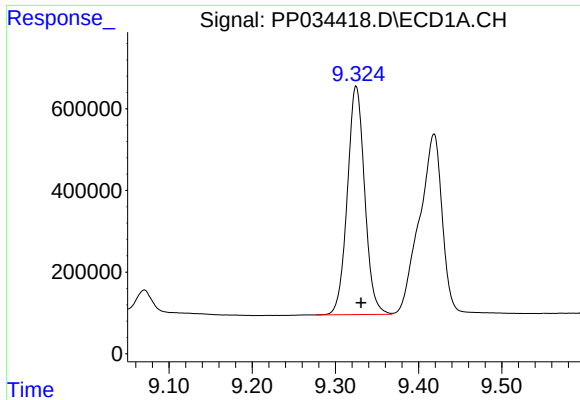


#38 AR-1262-3

R.T.: 9.325 min
Delta R.T.: -0.006 min
Response: 8102414
Conc: 1519.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
PHC-326FB-003DL


Manual Integrations
APPROVED

Ankita
3/30/2021 2:10:39 PM

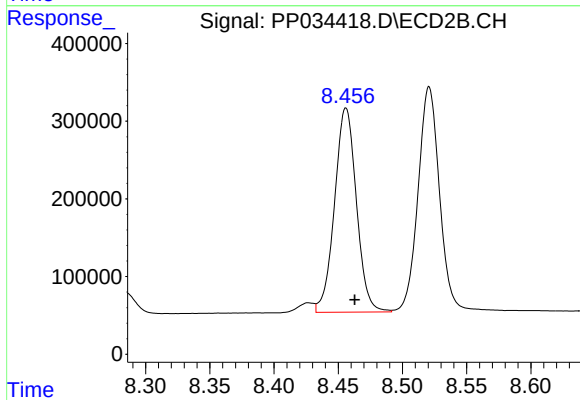


#38 AR-1262-3

R.T.: 8.456 min
Delta R.T.: -0.007 min
Response: 3116566
Conc: 2274.75 ng/ml

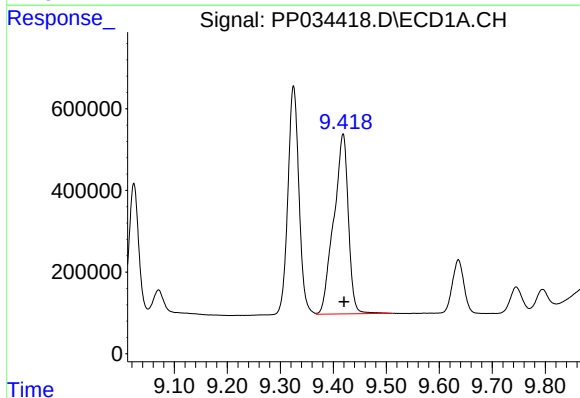


#39 AR-1262-4

R.T.: 9.419 min
Delta R.T.: -0.002 min
Response: 8445365
Conc: 1959.65 ng/ml

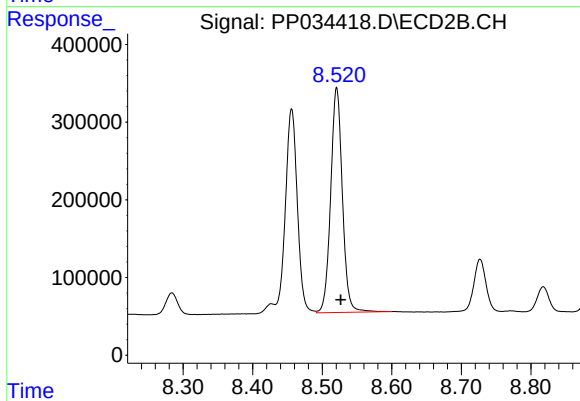

#39 AR-1262-4

R.T.: 8.521 min
Delta R.T.: -0.006 min
Response: 3375361
Conc: 1393.89 ng/ml

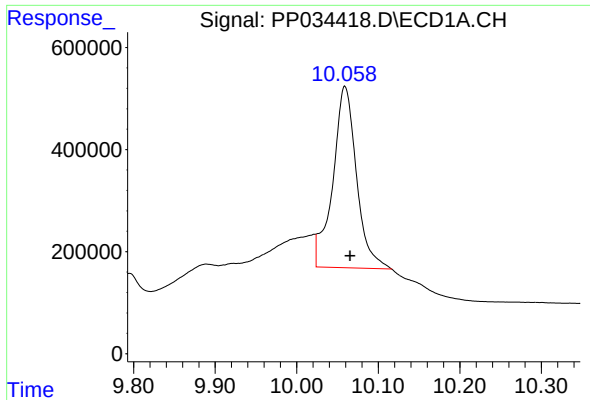


#40 AR-1262-5

R.T.: 10.058 min
Delta R.T.: -0.007 min
Response: 7162810
Conc: 2522.06 ng/ml m

Instrument :
ECD_P
ClientSampleId :
PHC-326FB-003DL

Manual Integrations
APPROVED

Ankita
3/30/2021 2:10:39 PM

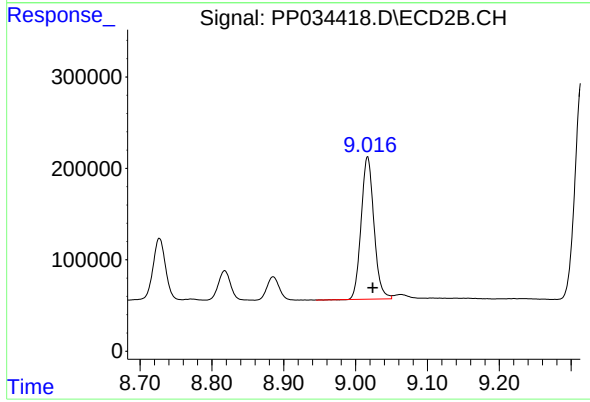

#40 AR-1262-5

R.T.: 9.017 min
Delta R.T.: -0.007 min
Response: 1928792
Conc: 1834.59 ng/ml