

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032621\
 Data File : PP034432.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Mar 2021 20:27
 Operator : DD\AJ
 Sample : M1811-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 031621-BIN-2

Manual Integrations
 APPROVED

Ankita
 3/30/2021 2:10:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 00:17:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 20 01:42:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.848	4.259	1669232	954100	19.870	21.560
2) SA Decachlor...	10.775	9.573	1792542	648189	22.842	24.563

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032621\
Data File : PP034432.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Mar 2021 20:27
Operator : DD\AJ
Sample : M1811-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
031621-BIN-2


Manual Integrations
APPROVED

Ankita
3/30/2021 2:10:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 00:17:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 20 01:42:16 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

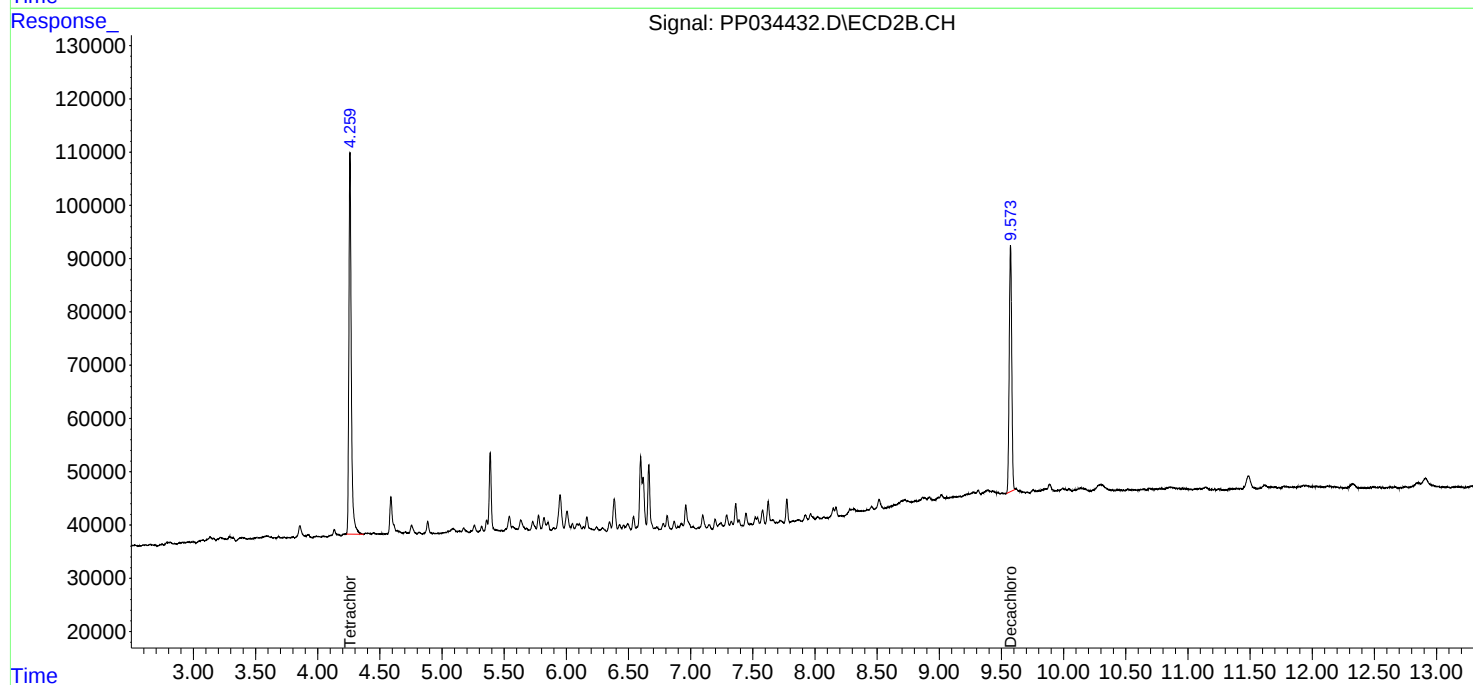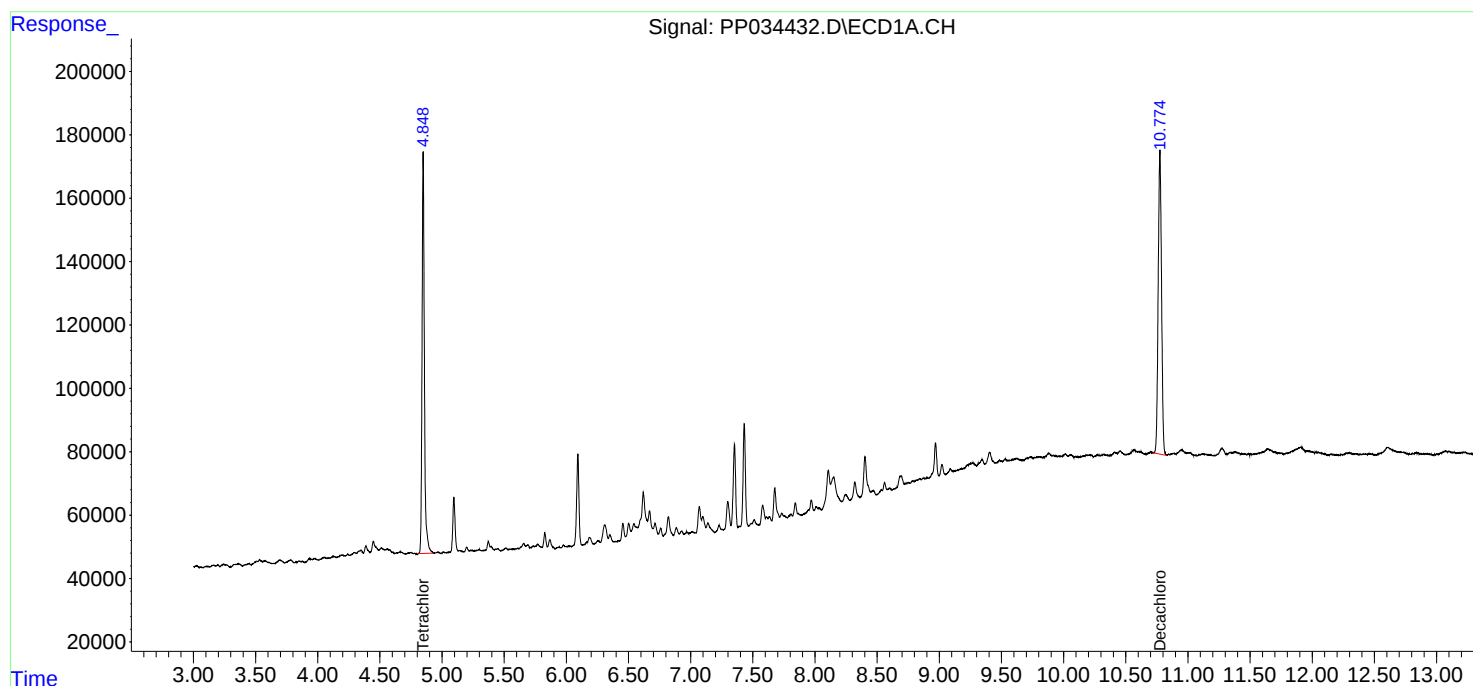

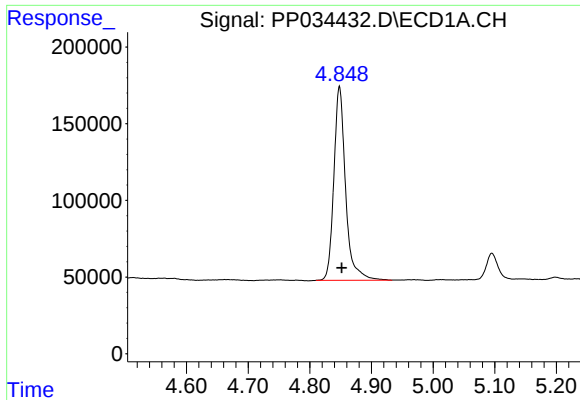


#1 Tetrachloro-m-xylene

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 1669232
Conc: 19.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
031621-BIN-2


Manual Integrations
APPROVED

Ankita
3/30/2021 2:10:44 PM

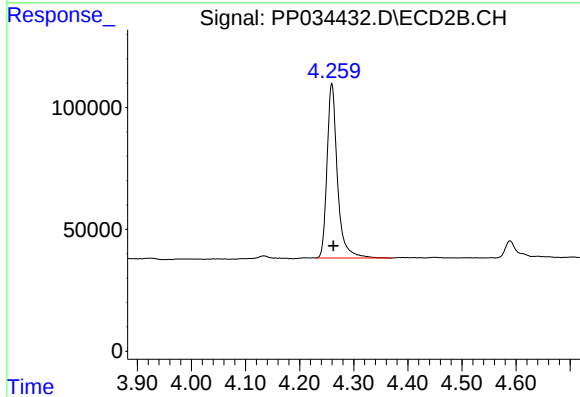


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: -0.003 min
Response: 954100
Conc: 21.56 ng/ml

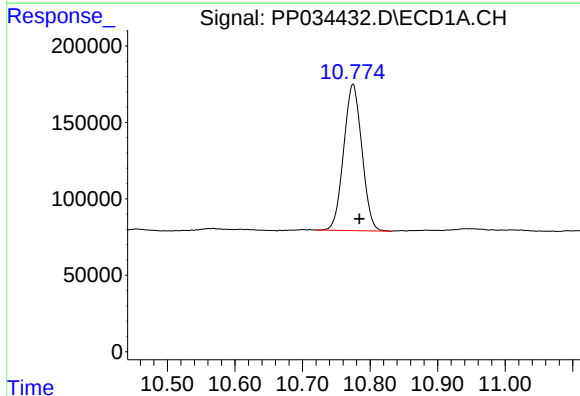

#2 Decachlorobiphenyl

R.T.: 10.775 min
Delta R.T.: -0.009 min
Response: 1792542
Conc: 22.84 ng/ml

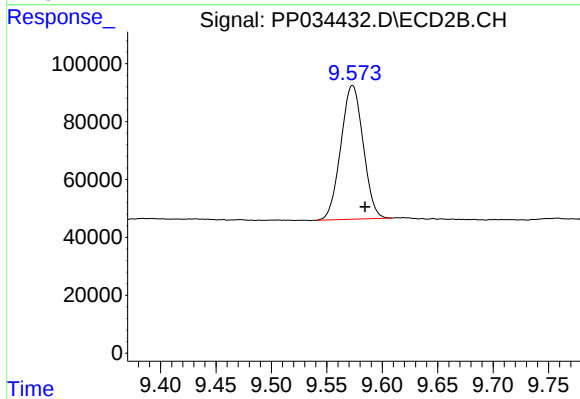

#2 Decachlorobiphenyl

R.T.: 9.573 min
Delta R.T.: -0.011 min
Response: 648189
Conc: 24.56 ng/ml