

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032719\
 Data File : PP029555.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 12:08
 Operator : EI\MA
 Sample : PB118277BL
 Misc : hexane
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB118277BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 14:42:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.927	12.119	34422810	43637279	1052.203	1016.207
Target Compounds							
5) T	DICAMBA	0.000	12.398	0	881992	N.D.	6.012 #
8) T	DICHLORPROP	0.000	13.554	0	1946519	N.D.	48.066 #
9) T	2,4-D	13.752	0.000	273521	0	7.073	N.D. #
11) T	2,4,5-TP ...	0.000	15.151	0	278144	N.D.	1.344 #
12) T	2,4,5-T	0.000	15.841	0	3373177	N.D.	20.348 #
13) T	2,4-DB	16.199	0.000	3373127	0	162.217	N.D. #
14) T	DINOSEB	17.676	16.910	36876	1708656	0.219	11.309 #
15) T	Picloram	17.473	0.000	214286	0	0.654	N.D. #
16) T	DCPA	18.036	0.000	1514724	0	4.774	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032719\
Data File : PP029555.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 12:08
Operator : EI\MA
Sample : PB118277BL
Misc : hexane
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB118277BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 14:42:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

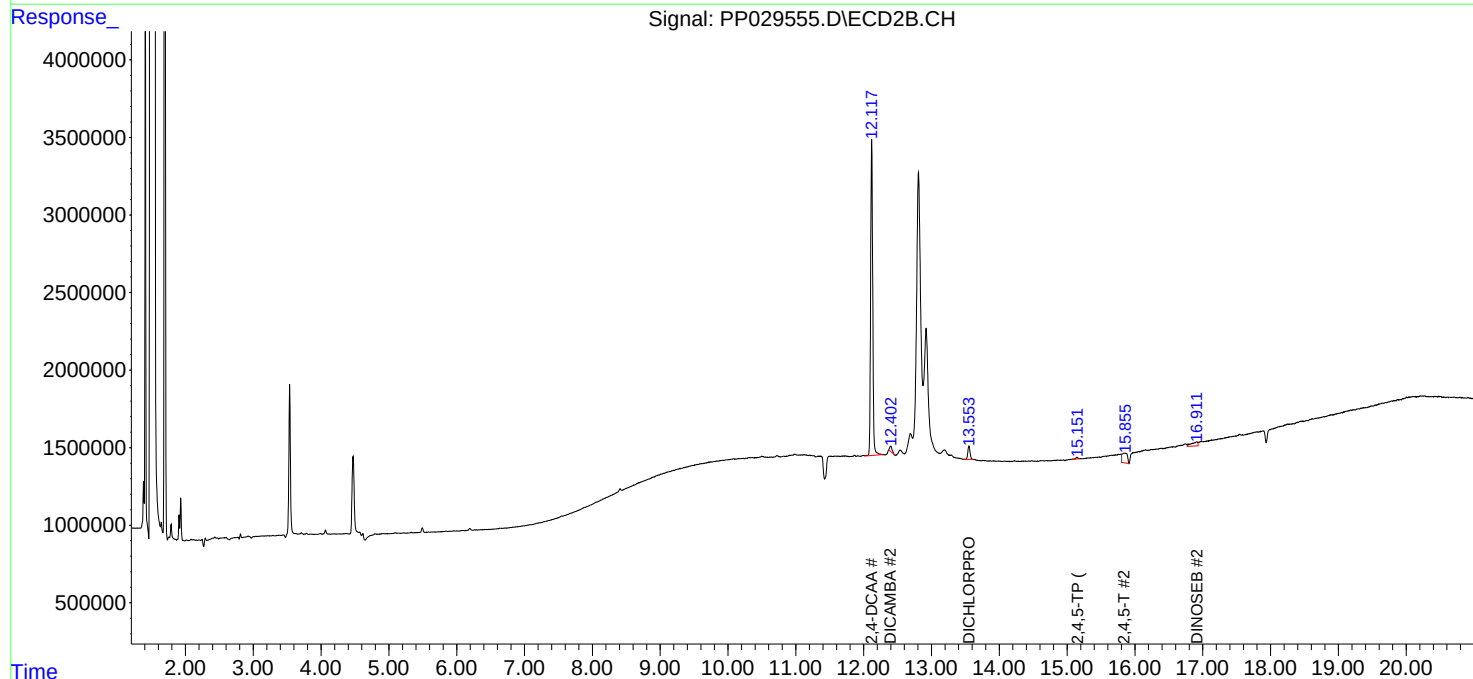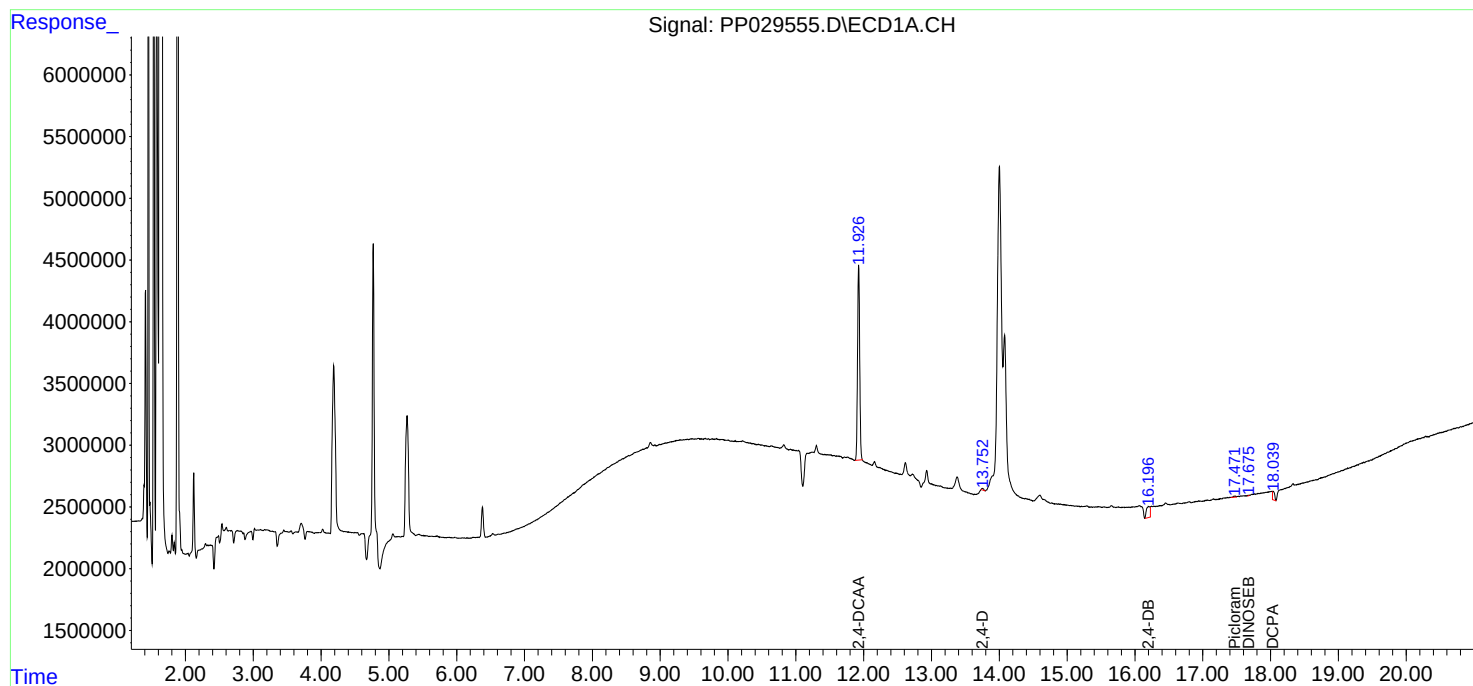


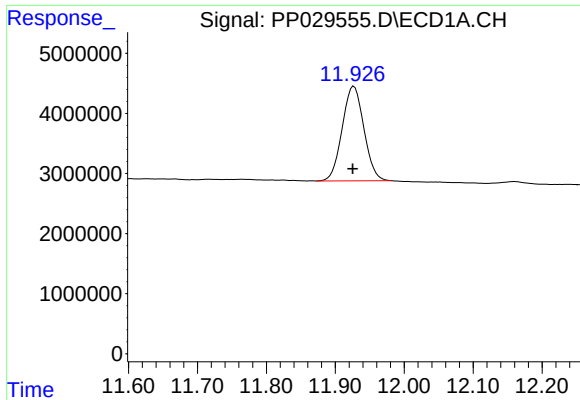

#4 2,4-DCAA


R.T.: 11.927 min
Delta R.T.: 0.002 min
Response: 34422810
Conc: 1052.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118277BL

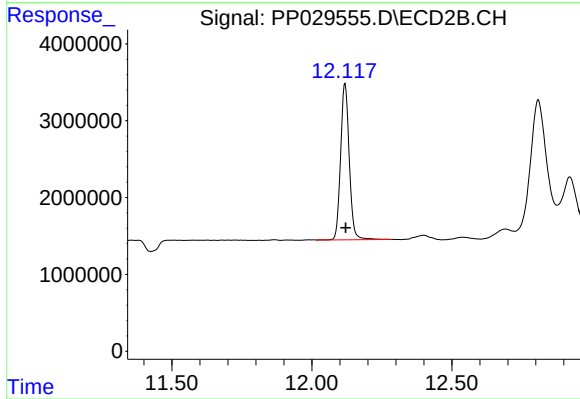


#4 2,4-DCAA

R.T.: 12.119 min
Delta R.T.: -0.002 min
Response: 43637279
Conc: 1016.21 ng/ml

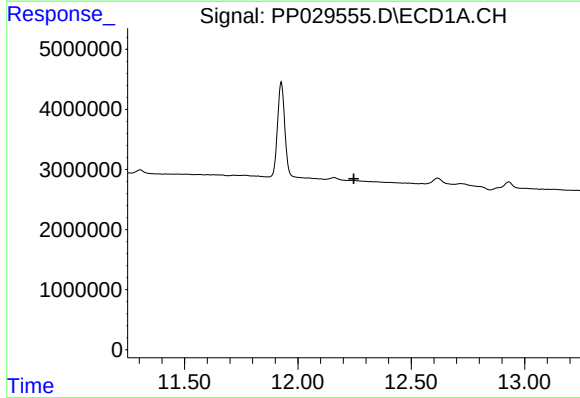


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.247 min
Response: 0
Conc: N.D.

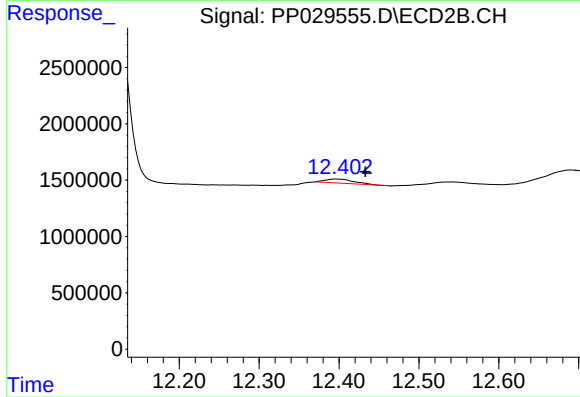

#5 DICAMBA


R.T.: 12.398 min
Delta R.T.: -0.035 min
Response: 881992
Conc: 6.01 ng/ml

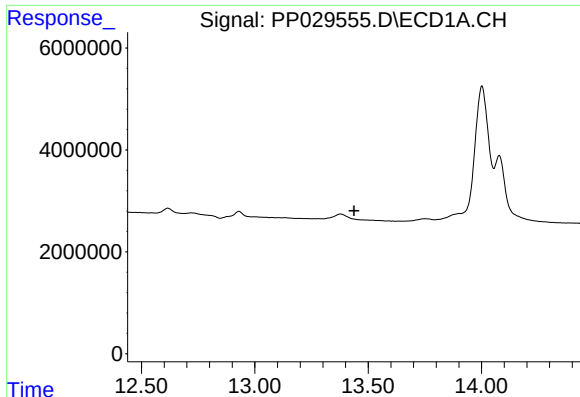

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB118277BL

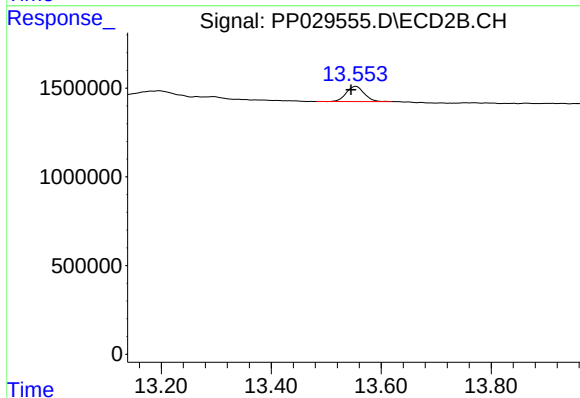


#8 DICHLORPROP

R.T.: 13.554 min
Delta R.T.: 0.009 min
Response: 1946519
Conc: 48.07 ng/ml

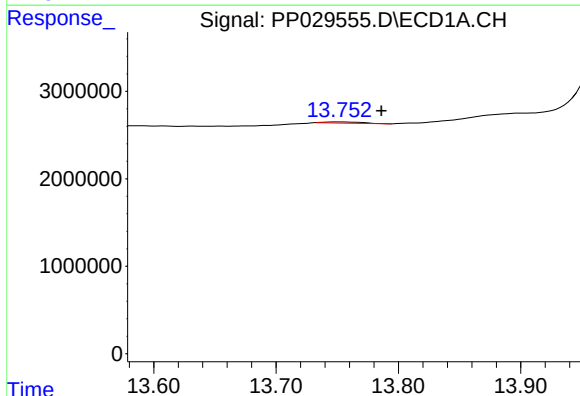


#9 2,4-D

R.T.: 13.752 min
Delta R.T.: -0.034 min
Response: 273521
Conc: 7.07 ng/ml

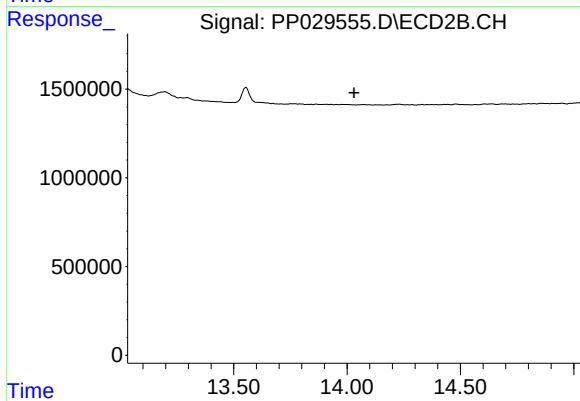

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 14.031 min
Response: 0
Conc: N.D.

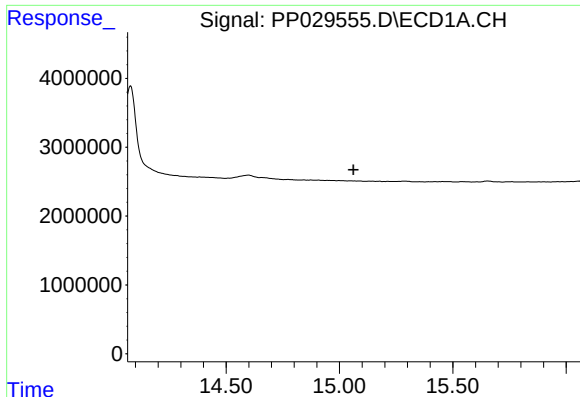

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 15.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB118277BL

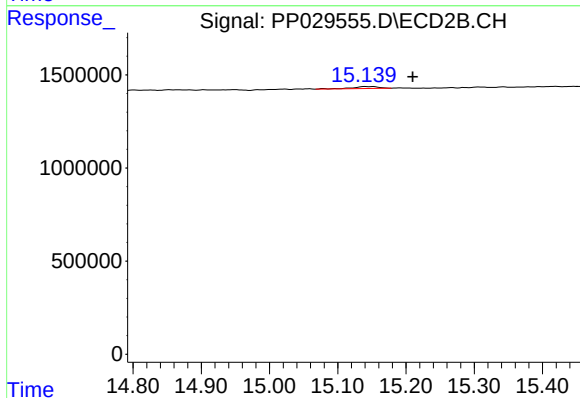


#11 2,4,5-TP (SILVEX)

R.T.: 15.151 min
Delta R.T.: -0.058 min
Response: 278144
Conc: 1.34 ng/ml

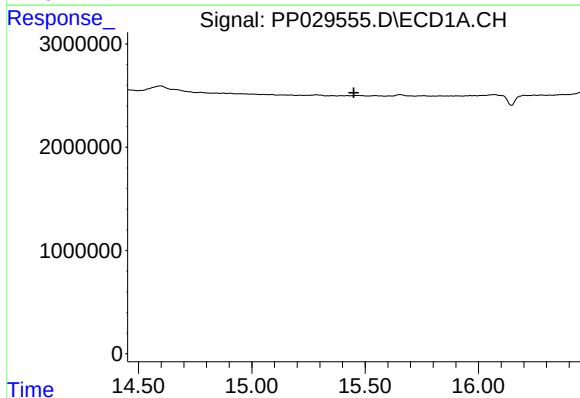


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.451 min
Response: 0
Conc: N.D.

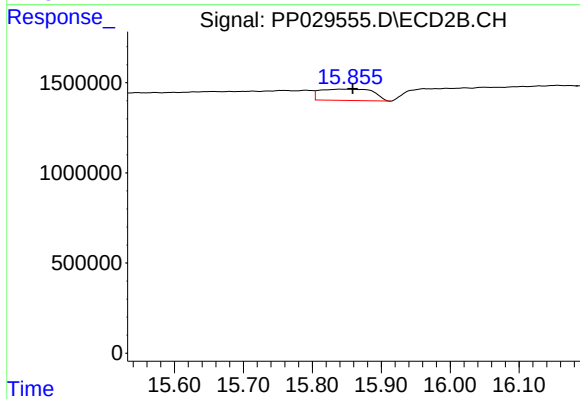

#12 2,4,5-T


R.T.: 15.841 min
Delta R.T.: -0.018 min
Response: 3373177
Conc: 20.35 ng/ml

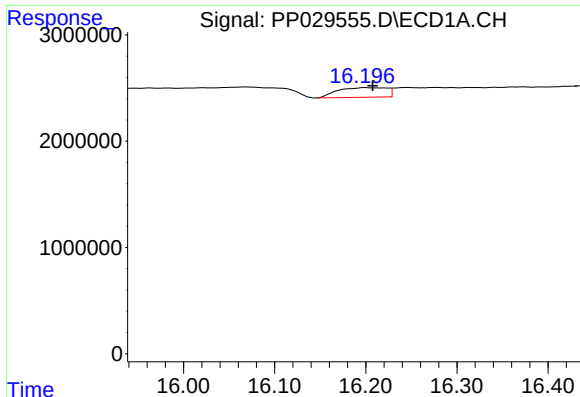

#13 2,4-DB


R.T.: 16.199 min
Delta R.T.: -0.008 min
Response: 3373127
Conc: 162.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118277BL

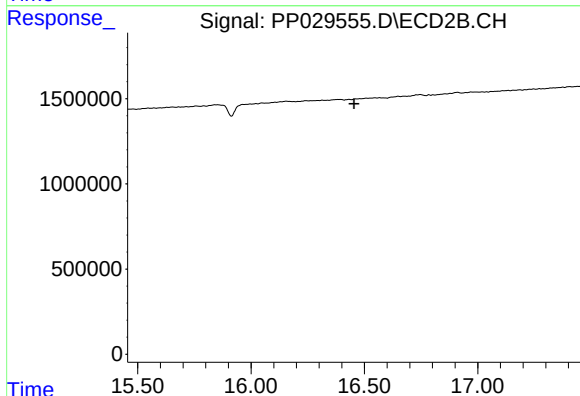


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.455 min
Response: 0
Conc: N.D.

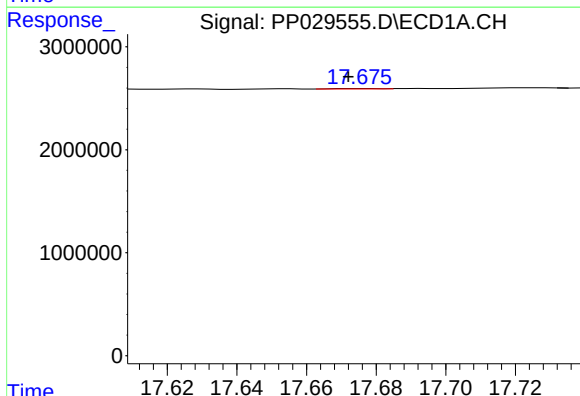


#14 DINOSEB

R.T.: 17.676 min
Delta R.T.: 0.004 min
Response: 36876
Conc: 0.22 ng/ml

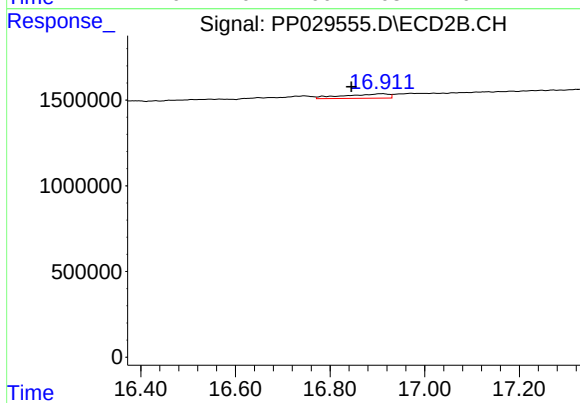

#14 DINOSEB


R.T.: 16.910 min
Delta R.T.: 0.065 min
Response: 1708656
Conc: 11.31 ng/ml

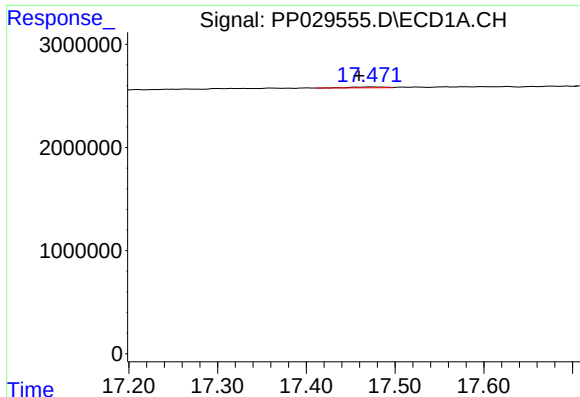

#15 Picloram


R.T.: 17.473 min
Delta R.T.: 0.014 min
Response: 214286
Conc: 0.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB118277BL

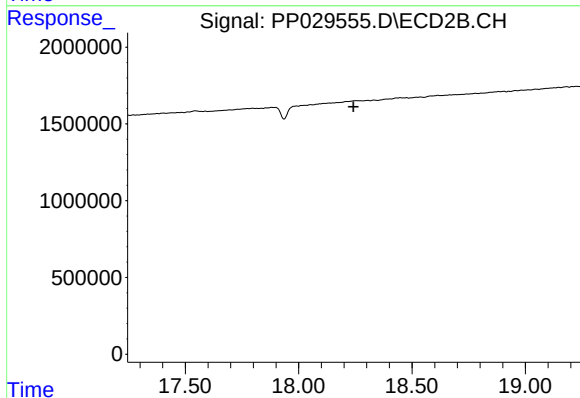


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.242 min
Response: 0
Conc: N.D.

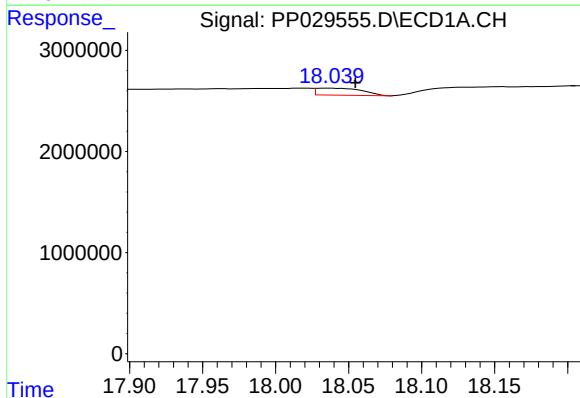

#16 DCPA

R.T.: 18.036 min
Delta R.T.: -0.019 min
Response: 1514724
Conc: 4.77 ng/ml

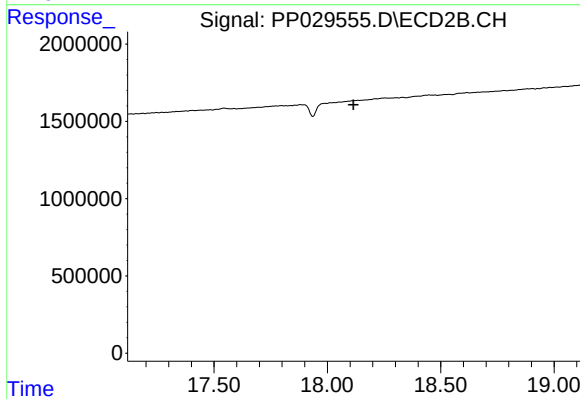

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.116 min
Response: 0
Conc: N.D.