

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032719\
 Data File : PP029563.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Mar 2019 15:32
 Operator : EI\MA
 Sample : K2078-01
 Misc : hexane
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-SF-01-005-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 16:04:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 22 09:23:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.924	12.118	12394351	15035705	378.858	350.145
Target Compounds							
2) T	3,5-DICHL...	10.386	0.000	451720	0	7.151	N.D. #
3) T	4-Nitroph...	11.431	0.000	49356	0	0.753	N.D. #
5) T	DICAMBA	0.000	12.396	0	433154	N.D.	2.953 #
8) T	DICHLORPROP	0.000	13.552	0	296646	N.D.	7.325 #
10) T	Pentachlo...	14.205	14.637	3179014	3142014	4.665	5.742
11) T	2,4,5-TP ...	15.064	0.000	403365	0	1.659	N.D. #
12) T	2,4,5-T	0.000	15.872	0	2551690	N.D.	15.392 #
13) T	2,4-DB	16.215	0.000	10196887	0	490.378	N.D. #
14) T	DINOSEB	17.679	16.907	137220	2449889	0.814	16.216 #
15) T	Picloram	17.474	18.244	83138	4663898	0.254	19.568 #
16) T	DCPA	18.003	0.000	6647083	0	20.951	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032719\
Data File : PP029563.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Mar 2019 15:32
Operator : EI\MA
Sample : K2078-01
Misc : hexane
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
FK-SF-01-005-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 16:04:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032119.M
Quant Title : 8080.M
QLast Update : Fri Mar 22 09:23:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

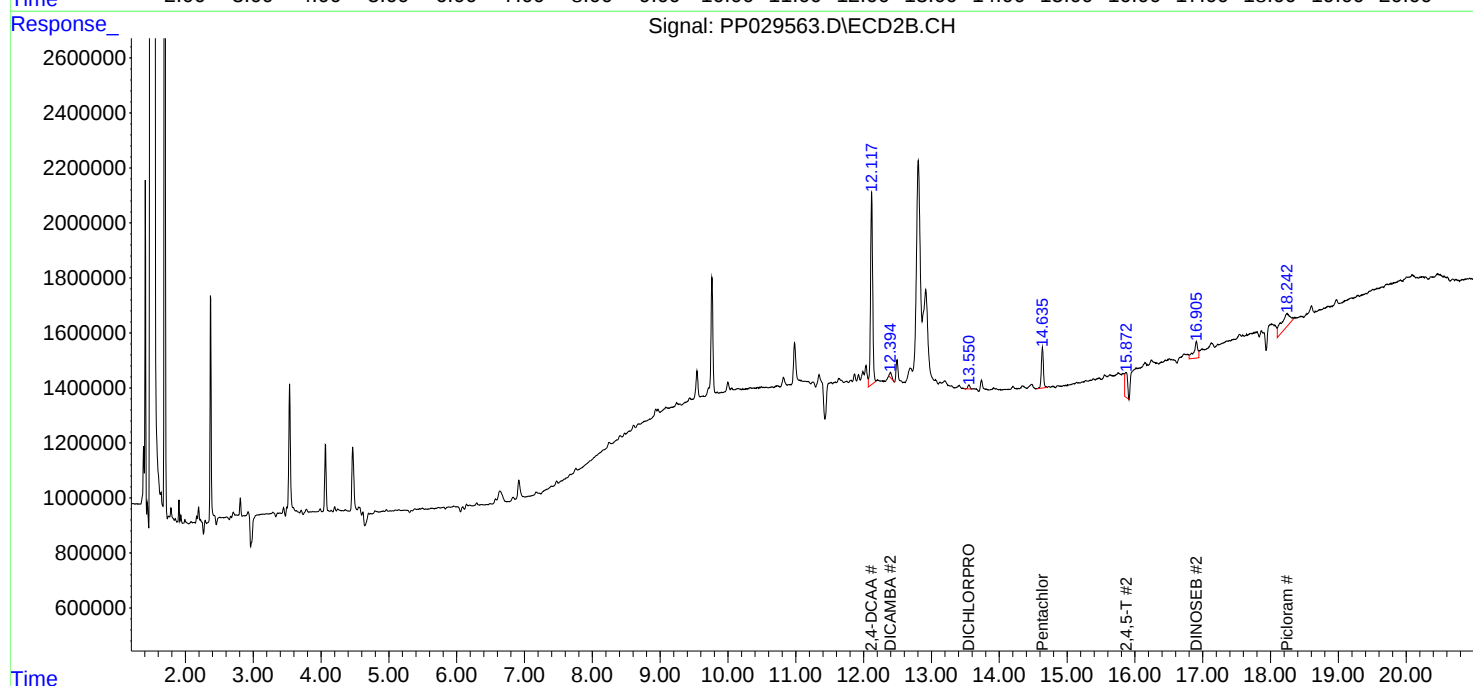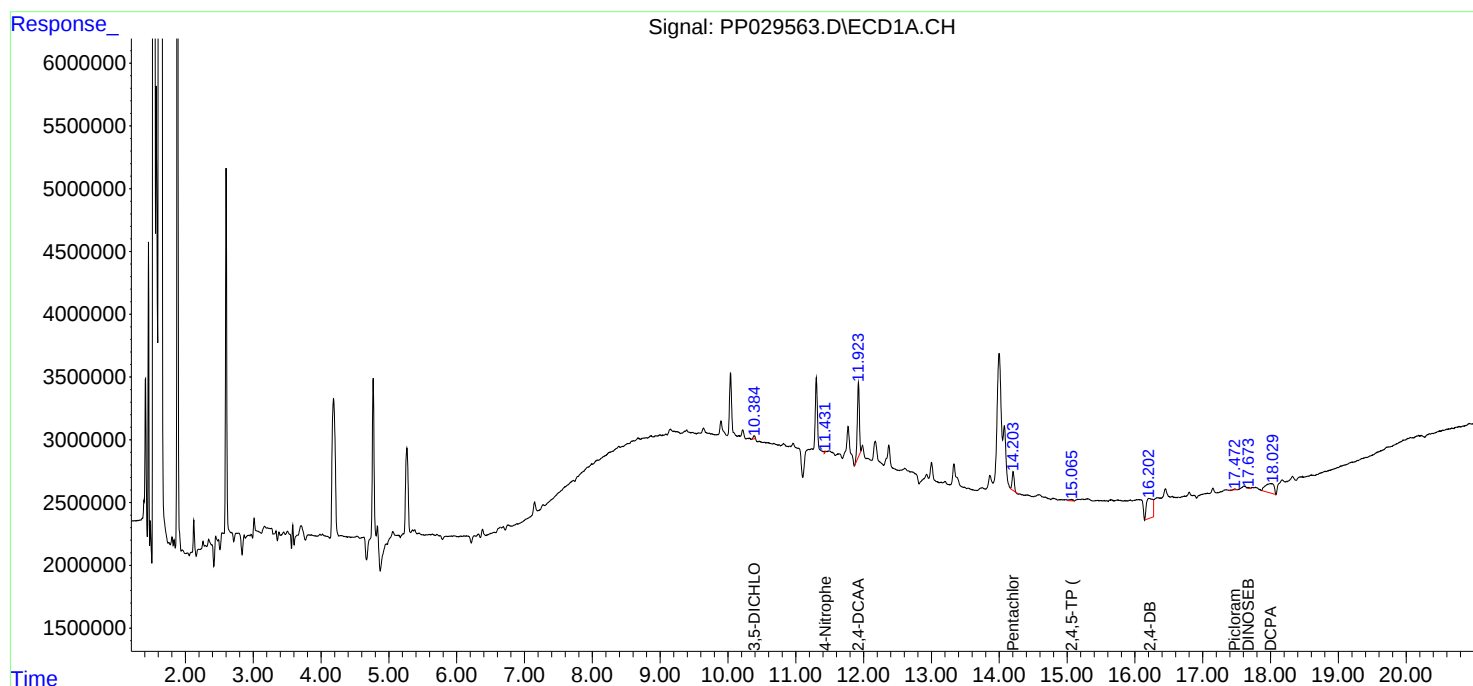


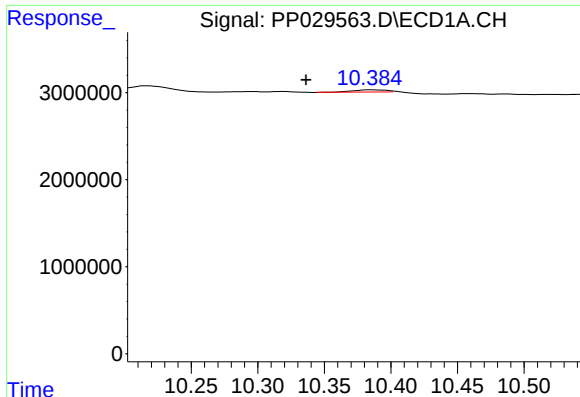

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 10.386 min
Delta R.T.: 0.050 min
Response: 451720
Conc: 7.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-01-005-A

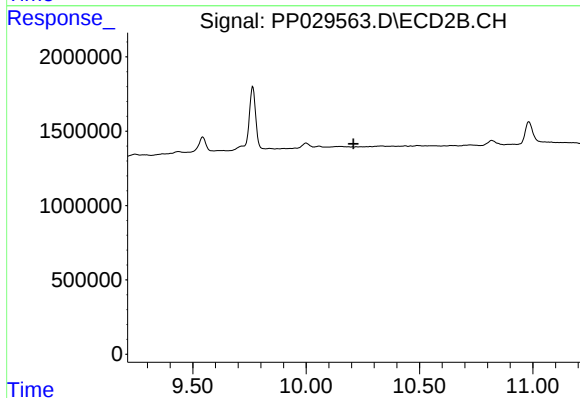


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.209 min
Response: 0
Conc: N.D.

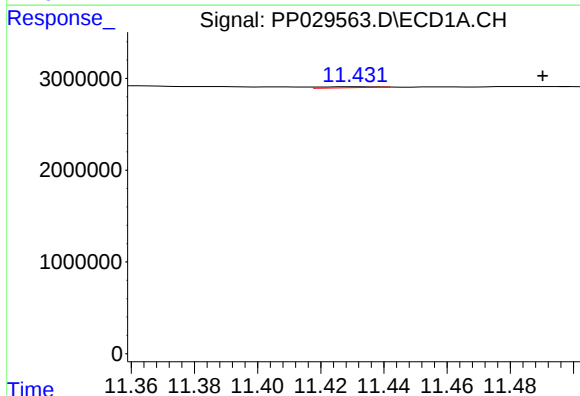


#3 4-Nitrophenol

R.T.: 11.431 min
Delta R.T.: -0.059 min
Response: 49356
Conc: 0.75 ng/ml

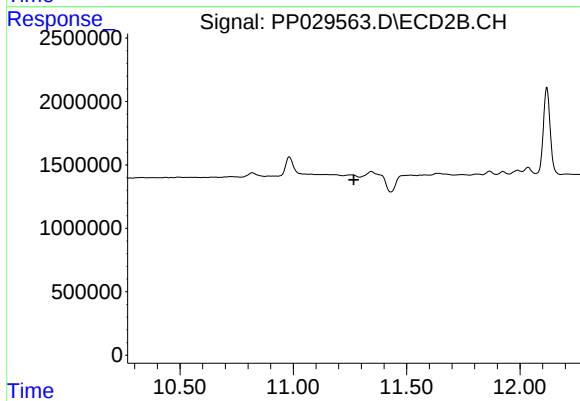

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 11.266 min
Response: 0
Conc: N.D.

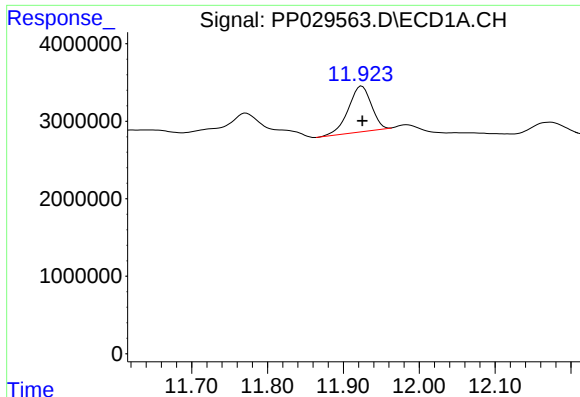

#4 2,4-DCAA


R.T.: 11.924 min
Delta R.T.: 0.000 min
Response: 12394351
Conc: 378.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-01-005-A

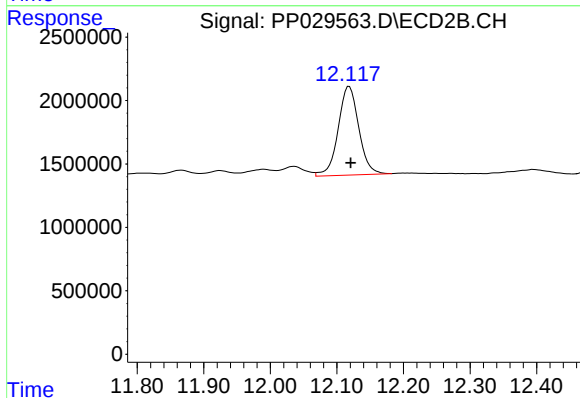


#4 2,4-DCAA

R.T.: 12.118 min
Delta R.T.: -0.002 min
Response: 15035705
Conc: 350.15 ng/ml

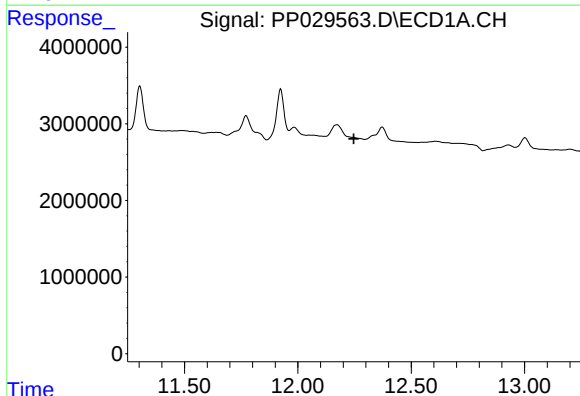


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.247 min
Response: 0
Conc: N.D.

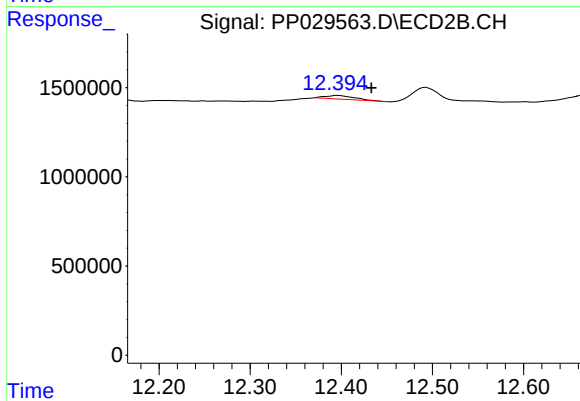

#5 DICAMBA


R.T.: 12.396 min
Delta R.T.: -0.037 min
Response: 433154
Conc: 2.95 ng/ml

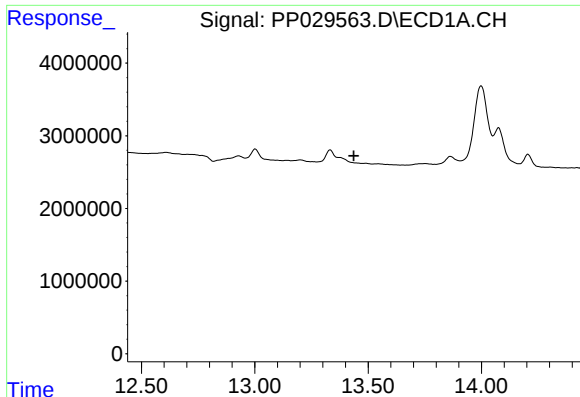

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-SF-01-005-A

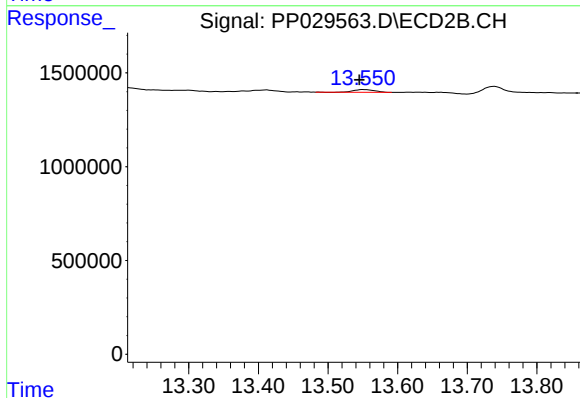


#8 DICHLORPROP

R.T.: 13.552 min
Delta R.T.: 0.007 min
Response: 296646
Conc: 7.33 ng/ml

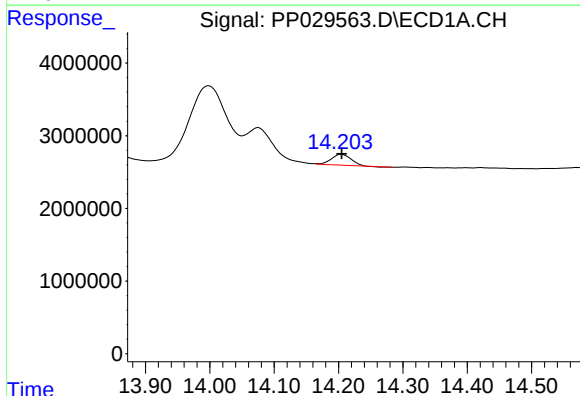


#10 Pentachlorophenol

R.T.: 14.205 min
Delta R.T.: 0.000 min
Response: 3179014
Conc: 4.66 ng/ml

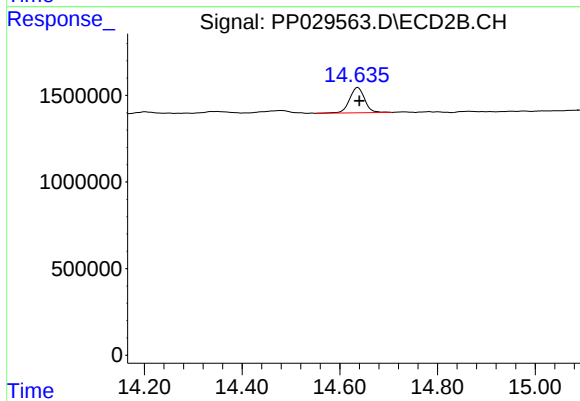

#10 Pentachlorophenol


R.T.: 14.637 min
Delta R.T.: -0.003 min
Response: 3142014
Conc: 5.74 ng/ml

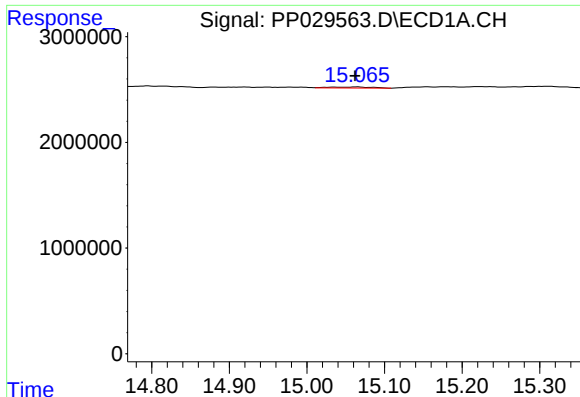

#11 2,4,5-TP (SILVEX)


R.T.: 15.064 min
Delta R.T.: 0.002 min
Response: 403365
Conc: 1.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-01-005-A

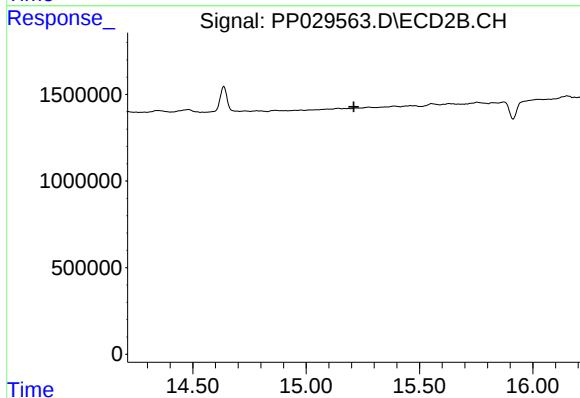


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 15.210 min
Response: 0
Conc: N.D.

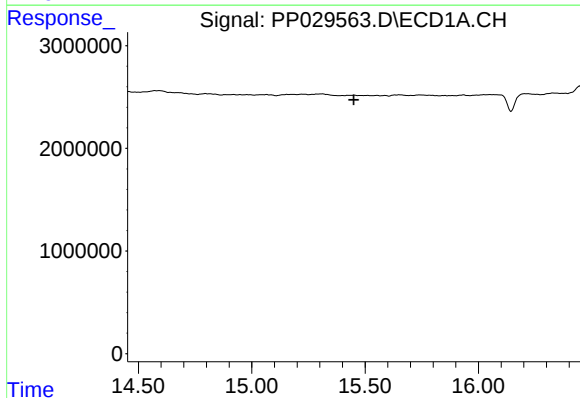


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.451 min
Response: 0
Conc: N.D.

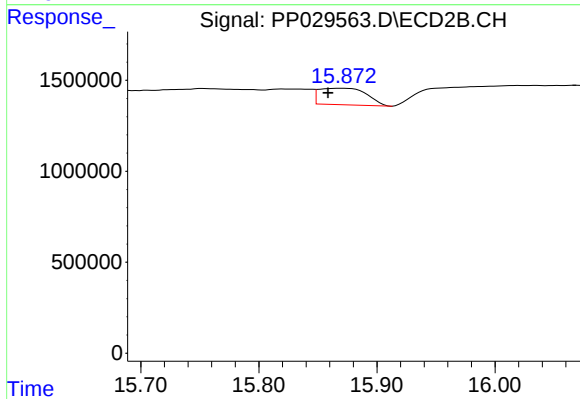

#12 2,4,5-T


R.T.: 15.872 min
Delta R.T.: 0.013 min
Response: 2551690
Conc: 15.39 ng/ml

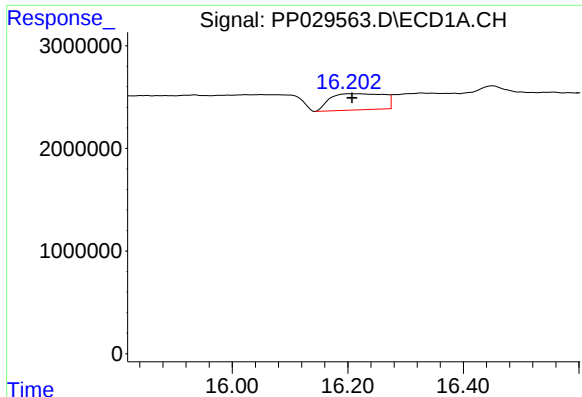

#13 2,4-DB


R.T.: 16.215 min
Delta R.T.: 0.008 min
Response: 10196887
Conc: 490.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-01-005-A

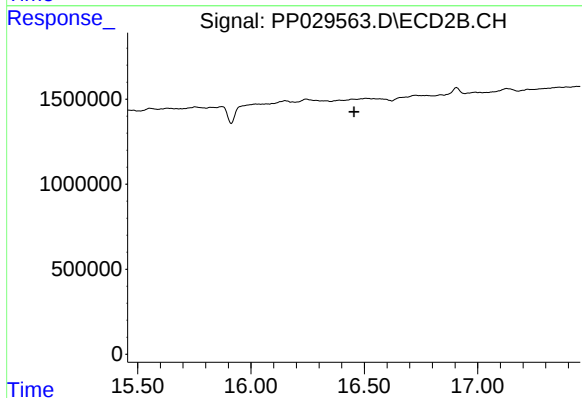


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 16.455 min
Response: 0
Conc: N.D.

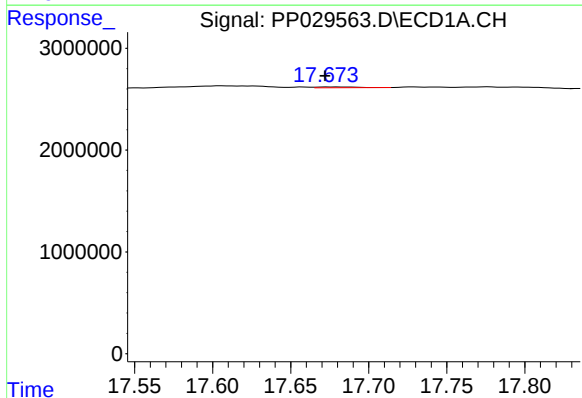


#14 DINOSEB

R.T.: 17.679 min
Delta R.T.: 0.007 min
Response: 137220
Conc: 0.81 ng/ml

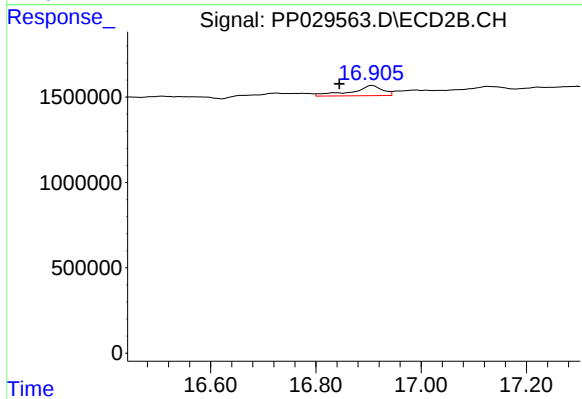

#14 DINOSEB


R.T.: 16.907 min
Delta R.T.: 0.062 min
Response: 2449889
Conc: 16.22 ng/ml

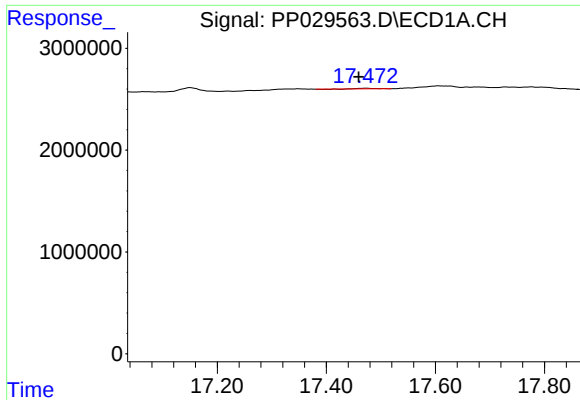

#15 Picloram


R.T.: 17.474 min
Delta R.T.: 0.014 min
Response: 83138
Conc: 0.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-SF-01-005-A

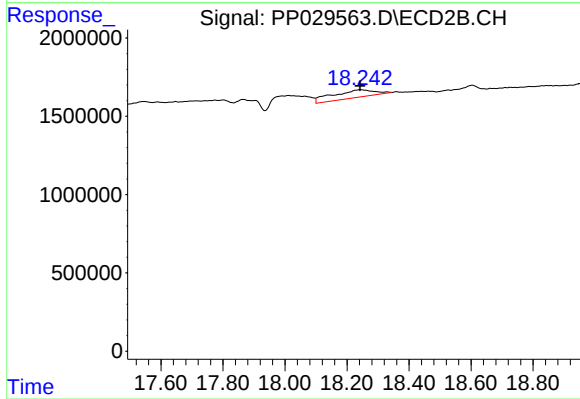


#15 Picloram

R.T.: 18.244 min
Delta R.T.: 0.002 min
Response: 4663898
Conc: 19.57 ng/ml

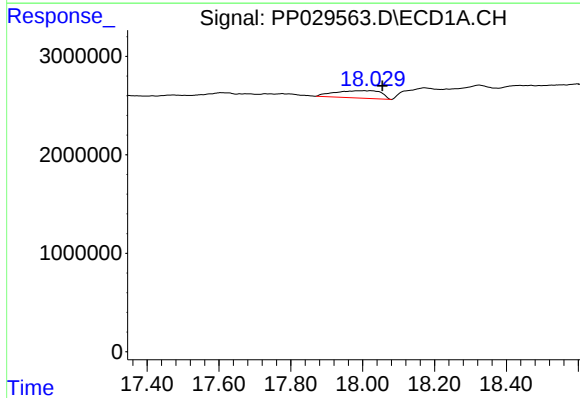

#16 DCPA

R.T.: 18.003 min
Delta R.T.: -0.051 min
Response: 6647083
Conc: 20.95 ng/ml

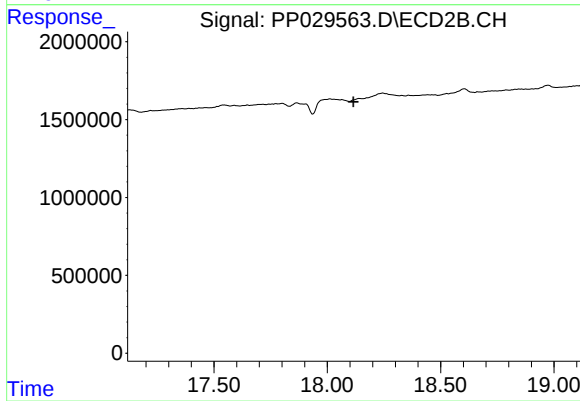

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.116 min
Response: 0
Conc: N.D.